

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013042.D
 Acq On : 10 Dec 2022 16:27
 Operator : CG/JU
 Sample : PB149527BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK527

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	39	rVB	183648	260817	1.46%	0.148%
2	3.781	97	101	125	rBV	2174200	3654974	20.53%	2.073%
3	4.111	154	157	163	rVB	35328	48189	0.27%	0.027%
4	7.128	662	670	685	rBV	2928086	4640194	26.06%	2.631%
5	7.299	692	699	711	rVB	2435425	3785761	21.26%	2.147%
6	7.499	726	733	746	rBV	2987709	4618433	25.94%	2.619%
7	7.969	804	813	826	rVB	2103369	3277627	18.41%	1.859%
8	8.675	925	933	949	rBV	3676100	5917245	33.23%	3.356%
9	9.140	1004	1012	1024	rBV	2864211	4638281	26.05%	2.630%
10	9.863	1125	1135	1147	rBV	2454197	3959763	22.24%	2.246%
11	10.399	1219	1226	1235	rBV	3802852	6234333	35.02%	3.535%
12	10.787	1284	1292	1300	rBV	3043785	5008674	28.13%	2.840%
13	10.922	1307	1315	1334	rBV	3626136	6147163	34.53%	3.486%
14	12.363	1555	1560	1568	rBV2	63496	106854	0.60%	0.061%
15	13.499	1747	1753	1759	rBV2	53629	88848	0.50%	0.050%
16	14.016	1834	1841	1851	rBV	7034921	9552476	53.65%	5.417%
17	14.304	1883	1890	1901	rBV	7811713	11551144	64.88%	6.551%
18	14.610	1934	1942	1951	rBV	4956960	7157063	40.20%	4.059%
19	14.798	1967	1974	1993	rBV	2915094	4547358	25.54%	2.579%
20	15.016	2008	2011	2016	rVB7	16794	23520	0.13%	0.013%
21	15.604	2103	2111	2124	rBV	10194424	14702581	82.58%	8.338%
22	15.716	2124	2130	2143	rVV	3078249	4284232	24.06%	2.430%
23	15.845	2147	2152	2160	rVB2	47176	87523	0.49%	0.050%
24	16.387	2239	2244	2250	rVB5	14541	19044	0.11%	0.011%
25	17.040	2351	2355	2362	rVB7	13131	25714	0.14%	0.015%
26	17.151	2370	2374	2380	rBV4	13336	20282	0.11%	0.012%
27	17.369	2404	2411	2420	rBV	6044871	8680254	48.75%	4.922%
28	17.469	2421	2428	2448	rVB	11162526	16182337	90.89%	9.177%
29	19.269	2730	2734	2740	rVB2	131439	179641	1.01%	0.102%
30	19.339	2741	2746	2750	rBV	123778	173151	0.97%	0.098%
31	19.698	2801	2807	2818	rBV	13096668	17804440	100.00%	10.097%
32	21.451	3100	3105	3113	rBV	6067169	7912925	44.44%	4.487%
33	23.780	3493	3501	3519	rVB2	6696484	14084754	79.11%	7.987%
34	23.939	3521	3528	3540	rVB2	3383515	6963711	39.11%	3.949%

Sum of corrected areas: 176339306




Instrument :
BNA_P
ClientSampleId :
SBLK527

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013042.D
Acq On : 10 Dec 2022 16:27
Operator : CG/JU
Sample : PB149527BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

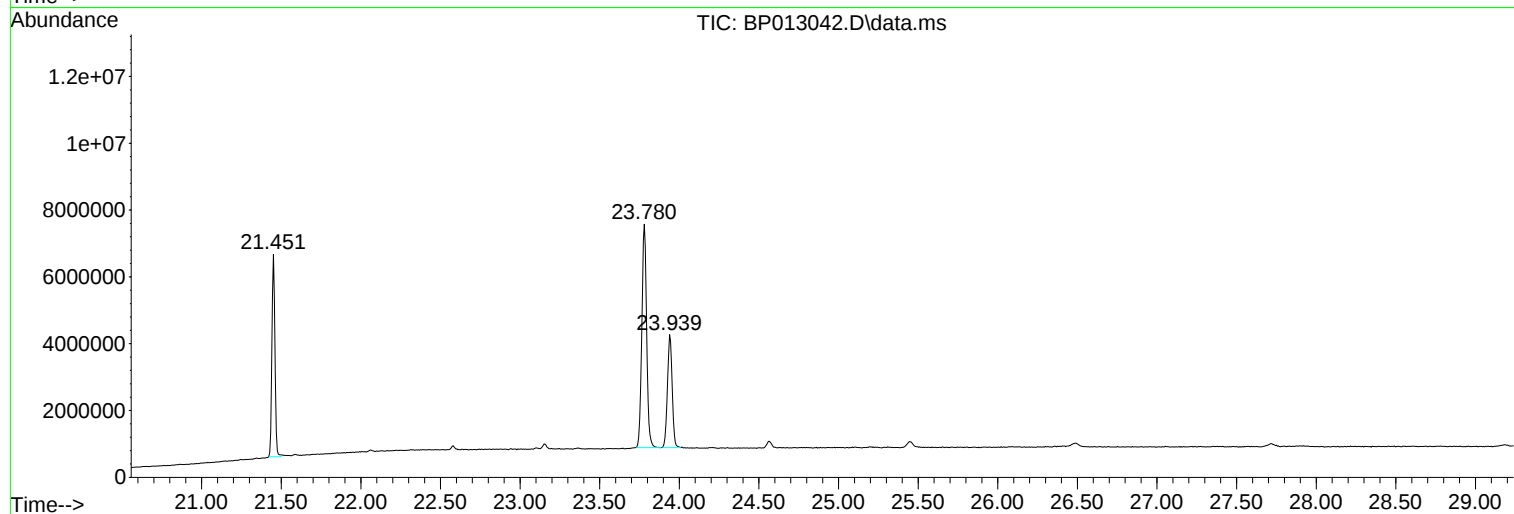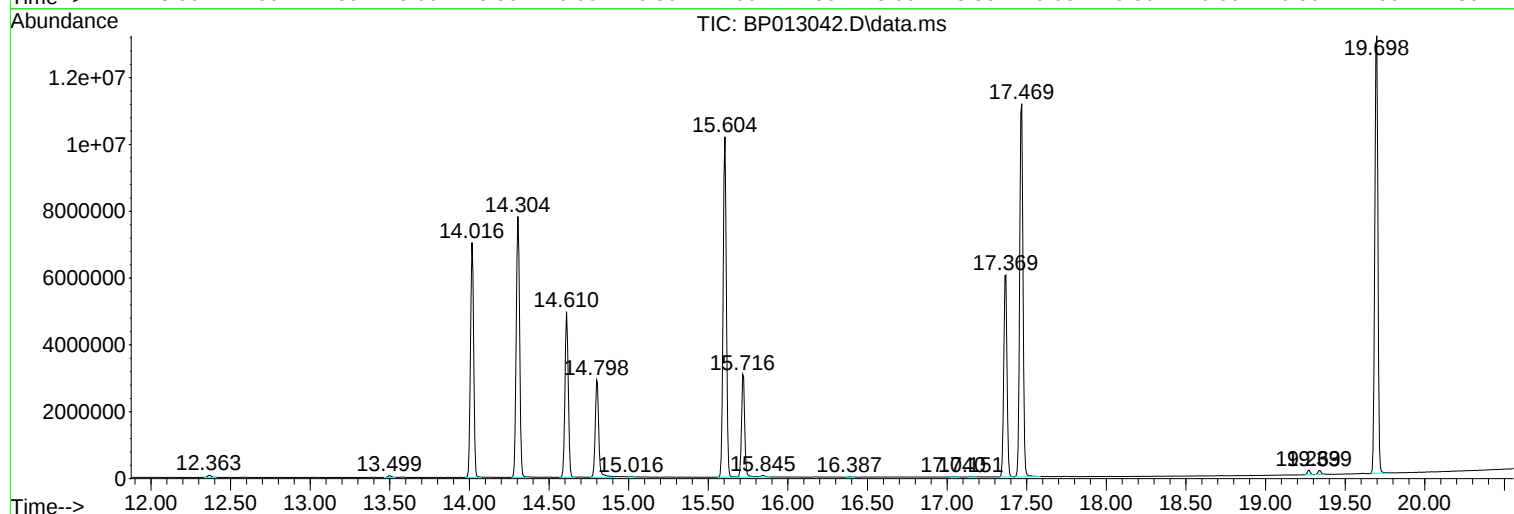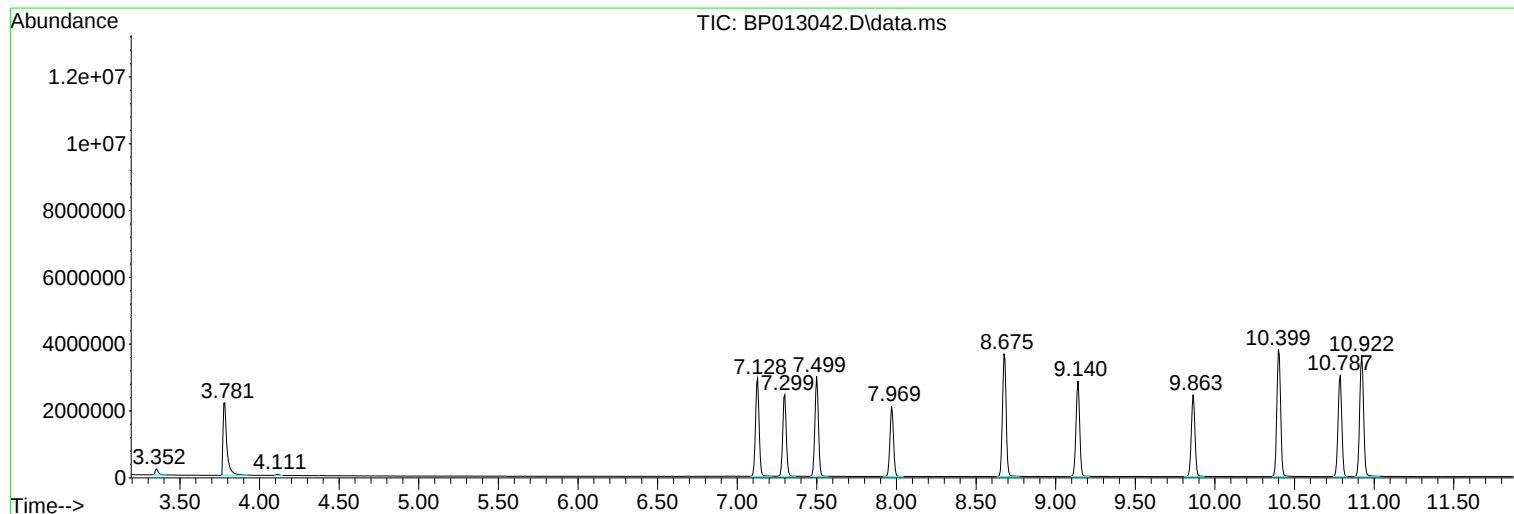

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013042.D
Acq On : 10 Dec 2022 16:27
Operator : CG/JU
Sample : PB149527BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013042.D
Acq On : 10 Dec 2022 16:27
Operator : CG/JU
Sample : PB149527BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK527

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc