

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013043.D
 Acq On : 10 Dec 2022 17:01
 Operator : CG/JU
 Sample : N5950-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	42	rVB	157952	237530	1.16%	0.129%
2	3.787	99	102	113	rBV	464497	754579	3.68%	0.411%
3	4.016	136	141	146	rVB	74557	107491	0.52%	0.059%
4	4.111	153	157	162	rBV	47722	67659	0.33%	0.037%
5	7.122	659	669	681	rVB	608997	1017619	4.97%	0.554%
6	7.293	691	698	705	rBV	2346904	3733057	18.23%	2.032%
7	7.352	705	708	717	rVB	120301	184217	0.90%	0.100%
8	7.499	726	733	743	rBV	2158947	3370471	16.46%	1.834%
9	7.969	806	813	820	rBV	2472311	3883392	18.96%	2.114%
10	8.028	820	823	827	rVV2	26882	39763	0.19%	0.022%
11	8.081	827	832	840	rVB	84807	140613	0.69%	0.077%
12	8.463	893	897	901	rVB4	19426	27181	0.13%	0.015%
13	8.610	914	922	926	rBV8	12441	27702	0.14%	0.015%
14	8.675	926	933	945	rVV	1789443	2908405	14.20%	1.583%
15	8.775	945	950	957	rVB2	37316	70382	0.34%	0.038%
16	8.981	979	985	995	rVB4	33862	57661	0.28%	0.031%
17	9.081	995	1002	1005	rBV	52742	88759	0.43%	0.048%
18	9.140	1005	1012	1024	rVB	2895912	4764564	23.26%	2.593%
19	9.316	1035	1042	1050	rVB	14965	44138	0.22%	0.024%
20	9.410	1053	1058	1065	rBV2	30548	57836	0.28%	0.031%
21	9.546	1076	1081	1086	rBV2	98572	155140	0.76%	0.084%
22	9.604	1086	1091	1097	rVV	60242	96109	0.47%	0.052%
23	9.663	1097	1101	1106	rVB	23748	36628	0.18%	0.020%
24	9.863	1126	1135	1149	rBV	2273467	3728239	18.20%	2.029%
25	9.975	1149	1154	1160	rVV3	24883	52078	0.25%	0.028%
26	10.063	1164	1169	1176	rVB7	15736	34907	0.17%	0.019%
27	10.181	1182	1189	1196	rVB2	99193	191091	0.93%	0.104%
28	10.399	1212	1226	1236	rBV	3270566	5472039	26.72%	2.978%
29	10.481	1237	1240	1249	rVB3	24758	40051	0.20%	0.022%
30	10.663	1262	1271	1274	rBV3	16329	36290	0.18%	0.020%
31	10.787	1282	1292	1306	rVV	3589655	6199758	30.27%	3.374%
32	10.922	1306	1315	1324	rVV	1789483	3116840	15.22%	1.696%
33	10.998	1324	1328	1332	rVB	25559	41770	0.20%	0.023%
34	11.146	1348	1353	1357	rBV6	14994	35854	0.18%	0.020%
35	11.187	1357	1360	1368	rVV9	17188	50211	0.25%	0.027%
36	11.404	1392	1397	1400	rBV5	14907	26766	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013043.D
 Acq On : 10 Dec 2022 17:01
 Operator : CG/JU
 Sample : N5950-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF48

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	11.446	1400	1404	1408	rVV3	22448	32919	0.16%	0.018%
38	11.498	1408	1413	1418	rVB3	38410	64767	0.32%	0.035%
39	11.557	1418	1423	1429	rBV7	17368	30480	0.15%	0.017%
40	11.757	1450	1457	1463	rBV2	88810	177615	0.87%	0.097%
41	11.810	1463	1466	1474	rVV2	39538	76781	0.37%	0.042%
42	11.893	1474	1480	1486	rVB2	41341	72053	0.35%	0.039%
43	12.040	1502	1505	1509	rVV4	23037	27667	0.14%	0.015%
44	12.093	1509	1514	1520	rVV6	33073	69595	0.34%	0.038%
45	12.193	1520	1531	1537	rVB3	48197	113880	0.56%	0.062%
46	12.275	1537	1545	1548	rBV10	13021	25592	0.12%	0.014%
47	12.363	1556	1560	1570	rVV	59248	104190	0.51%	0.057%
48	12.498	1578	1583	1588	rVB7	13213	24373	0.12%	0.013%
49	12.593	1594	1599	1604	rBV	76918	120995	0.59%	0.066%
50	12.704	1614	1618	1622	rBV5	29359	52170	0.25%	0.028%
51	12.822	1631	1638	1642	rBV9	22305	41267	0.20%	0.022%
52	12.940	1654	1658	1665	rVV9	17605	40962	0.20%	0.022%
53	13.004	1665	1669	1677	rVV10	20658	40748	0.20%	0.022%
54	13.081	1677	1682	1687	rVV5	22991	49603	0.24%	0.027%
55	13.145	1687	1693	1699	rVV3	46881	100629	0.49%	0.055%
56	13.216	1699	1705	1710	rVB9	12029	28652	0.14%	0.016%
57	13.428	1733	1741	1747	rBV	81873	135710	0.66%	0.074%
58	13.498	1747	1753	1758	rVV2	45020	97234	0.47%	0.053%
59	13.575	1761	1766	1772	rVV3	65586	113813	0.56%	0.062%
60	13.645	1774	1778	1784	rVB5	16551	31028	0.15%	0.017%
61	13.745	1791	1795	1797	rBV4	24417	36457	0.18%	0.020%
62	13.781	1797	1801	1811	rVB	67492	115361	0.56%	0.063%
63	13.934	1822	1827	1832	rBV9	16262	31984	0.16%	0.017%
64	14.016	1832	1841	1850	rBV	7487568	10392075	50.74%	5.656%
65	14.134	1856	1861	1865	rVB7	21758	31924	0.16%	0.017%
66	14.304	1883	1890	1907	rBV	8494311	12169216	59.41%	6.623%
67	14.428	1907	1911	1915	rVB6	17659	28243	0.14%	0.015%
68	14.492	1917	1922	1926	rBV2	21718	37417	0.18%	0.020%
69	14.610	1932	1942	1950	rBV	5919866	8882234	43.37%	4.834%
70	14.798	1966	1974	1987	rBV	568066	949594	4.64%	0.517%
71	15.016	2007	2011	2018	rVB6	51790	105176	0.51%	0.057%
72	15.234	2044	2048	2059	rVB6	14125	33355	0.16%	0.018%
73	15.404	2070	2077	2079	rVV	18395	33134	0.16%	0.018%
74	15.604	2104	2111	2124	rBV	11123826	15793168	77.11%	8.596%
75	15.722	2124	2131	2140	rBV	3531273	4912233	23.98%	2.674%
76	15.845	2147	2152	2158	rVB	54018	86779	0.42%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013043.D
 Acq On : 10 Dec 2022 17:01
 Operator : CG/JU
 Sample : N5950-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF48

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

77	15.969	2167	2173	2179	rBV	948926	1272739	6.21%	0.693%
78	16.392	2238	2245	2249	rBV7	15054	27353	0.13%	0.015%
79	16.745	2301	2305	2309	rBV4	28109	36581	0.18%	0.020%
80	17.039	2350	2355	2359	rVB6	15000	26002	0.13%	0.014%
81	17.157	2370	2375	2384	rVB2	21325	46487	0.23%	0.025%
82	17.369	2404	2411	2420	rBV	7450038	10707957	52.28%	5.828%
83	17.469	2421	2428	2445	rVV	12409921	17999713	87.88%	9.797%
84	17.645	2455	2458	2462	rBV	20095	26756	0.13%	0.015%
85	17.739	2470	2474	2478	rBV2	21518	32177	0.16%	0.018%
86	18.022	2519	2522	2526	rVB5	19979	27682	0.14%	0.015%
87	18.110	2534	2537	2541	rVV5	24380	28850	0.14%	0.016%
88	18.233	2553	2558	2567	rBV2	438411	575346	2.81%	0.313%
89	18.310	2567	2571	2580	rVB	41937	79034	0.39%	0.043%
90	18.645	2625	2628	2633	rVB3	39557	45791	0.22%	0.025%
91	19.275	2730	2735	2740	rBV	160771	227011	1.11%	0.124%
92	19.339	2741	2746	2750	rBV	166959	245565	1.20%	0.134%
93	19.463	2763	2767	2773	rBV2	112911	151520	0.74%	0.082%
94	19.610	2789	2792	2796	rVB4	65810	68471	0.33%	0.037%
95	19.698	2801	2807	2819	rVV	14818076	20481844	100.00%	11.148%
96	21.139	3048	3052	3061	rBV	829039	1259737	6.15%	0.686%
97	21.451	3100	3105	3114	rBV	7188807	9485006	46.31%	5.162%
98	22.727	3318	3322	3329	rVB	432322	603812	2.95%	0.329%
99	23.780	3493	3501	3516	rVB2	7641486	15813431	77.21%	8.607%
100	23.939	3521	3528	3540	rVB2	4101289	8257136	40.31%	4.494%




Sum of corrected areas: 183733864

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013043.D
Acq On : 10 Dec 2022 17:01
Operator : CG/JU
Sample : N5950-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF48

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

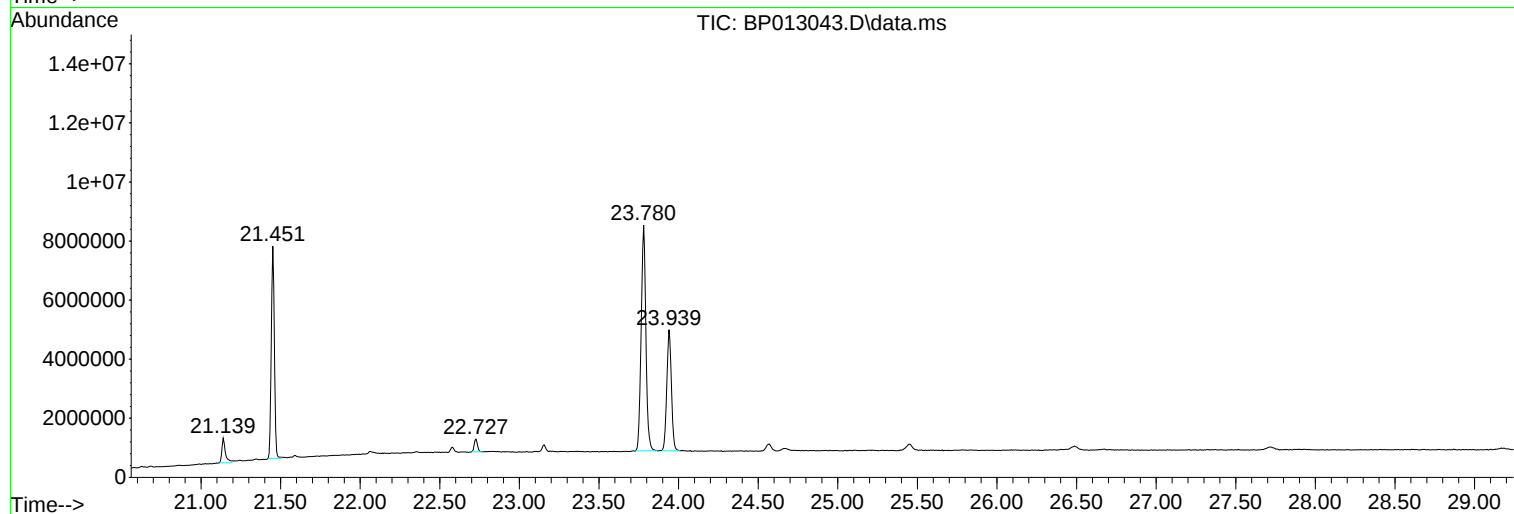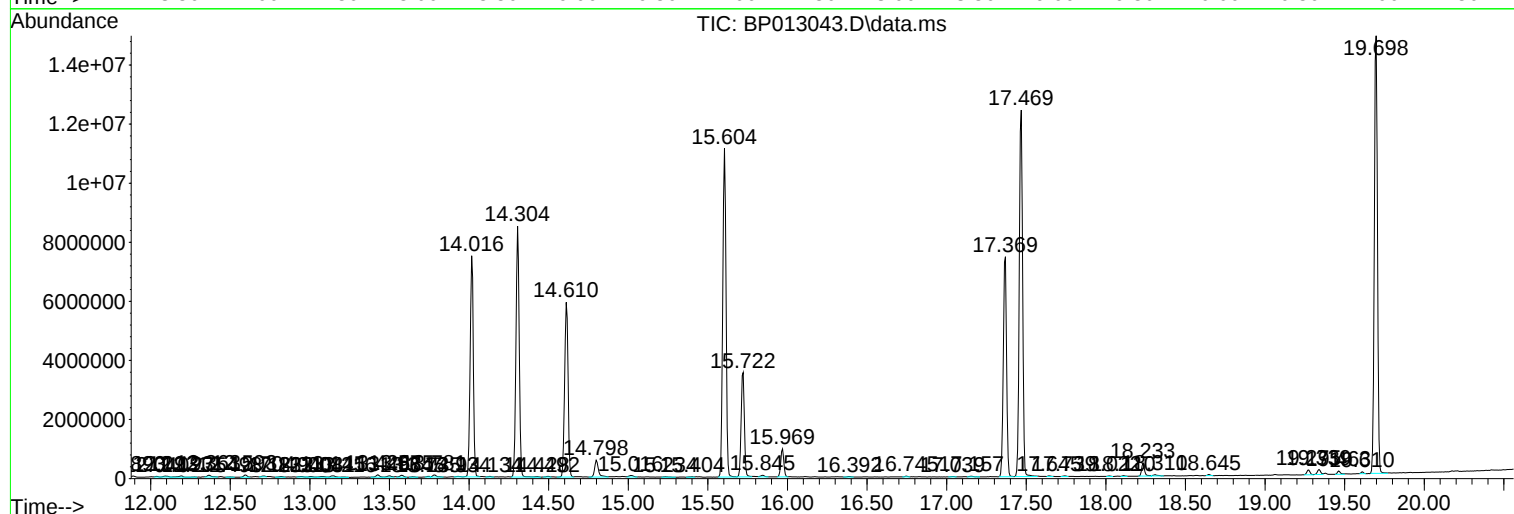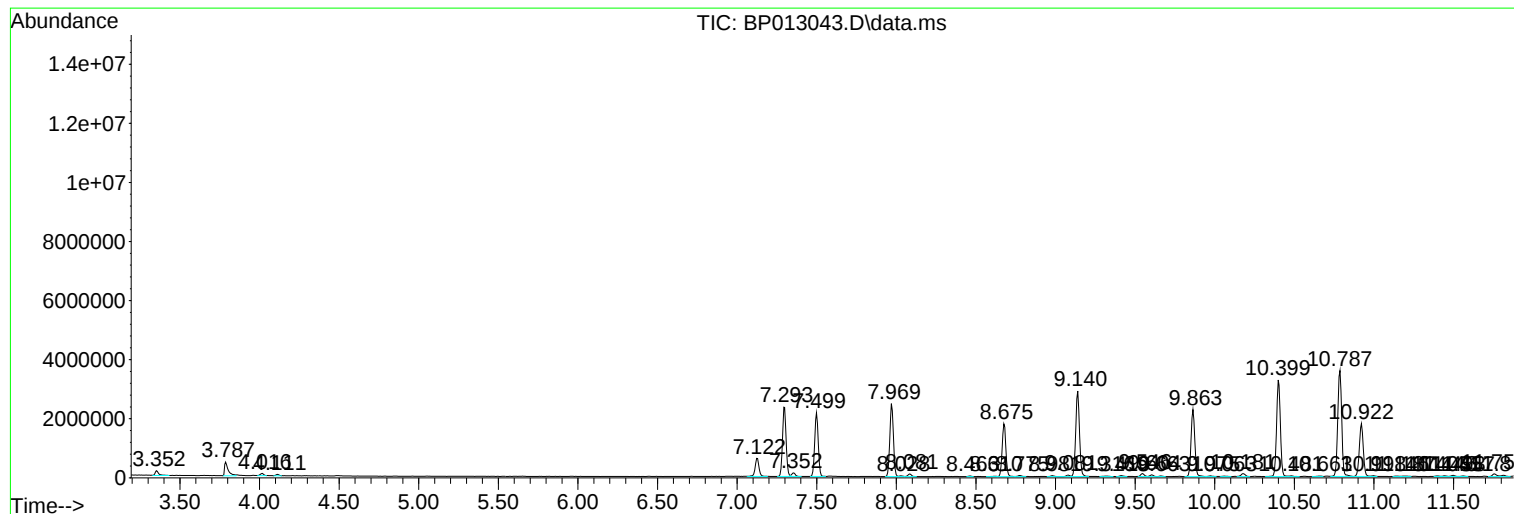

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\  
Data File : BP013043.D  
Acq On    : 10 Dec 2022  17:01  
Operator   : CG/JU  
Sample     : N5950-01  
Misc      :  
ALS Vial   : 13    Sample Multiplier: 1
```

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013043.D
Acq On : 10 Dec 2022 17:01
Operator : CG/JU
Sample : N5950-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF48










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Cyclic21.139 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.139	2.66 ng/ul	1259740	Chrysene-d12	21.451

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	96
2			n-Nonadecanol-1	284	C19H40O	001454-84-8	95
3			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
4			Pentacos-1-ene	350	C25H50	016980-85-1	94
5			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	94

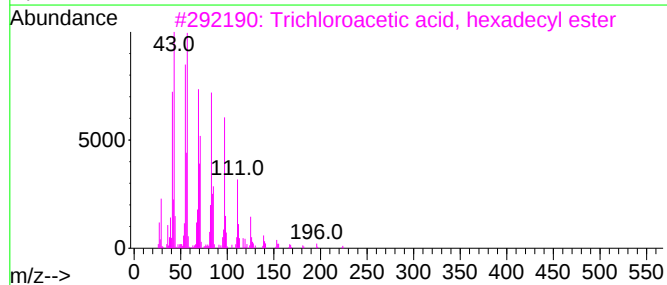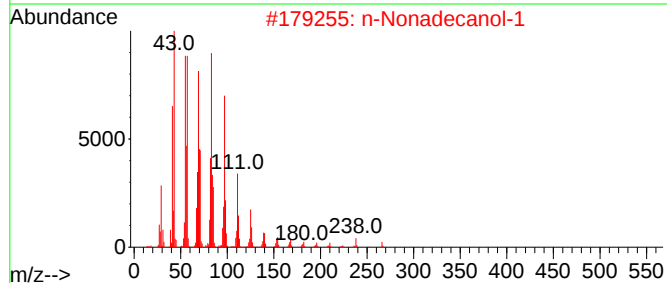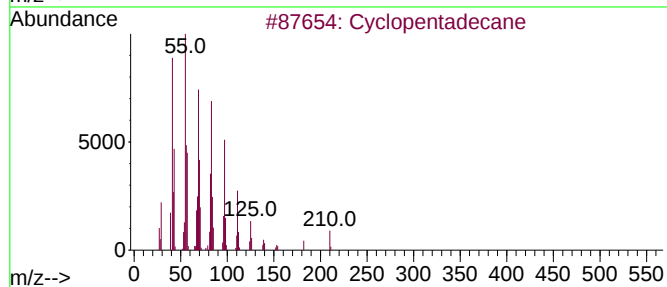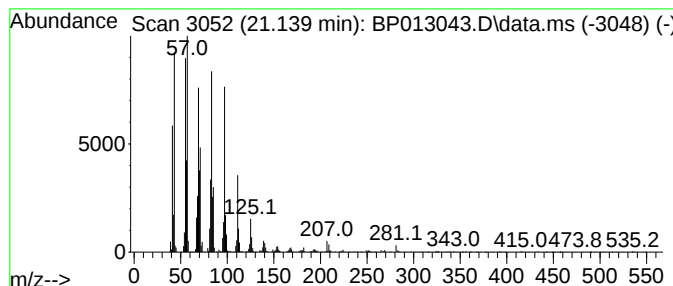

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013043.D
Acq On : 10 Dec 2022 17:01
Operator : CG/JU
Sample : N5950-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF48

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.969	2.9	ng/u1	1272740	3	14.610	8882230	20.0
(DEL) Alkane: C...	21.139	2.7	ng/u1	1259740	5	21.451	9485010	20.0