

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013051.D
 Acq On : 10 Dec 2022 21:34
 Operator : CG/JU
 Sample : N5950-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	18	22	26	rBV	386439	575574	2.35%	0.279%
2	3.352	26	28	44	rVB	202199	316823	1.29%	0.153%
3	3.793	100	103	117	rBV	190293	328561	1.34%	0.159%
4	4.016	136	141	148	rVB2	72825	126916	0.52%	0.061%
5	4.110	153	157	166	rVB	53081	87347	0.36%	0.042%
6	7.122	664	669	678	rVB	733909	1177697	4.81%	0.570%
7	7.292	692	698	711	rBV	2940500	4651780	19.00%	2.252%
8	7.498	725	733	741	rBV	2670527	4191750	17.12%	2.029%
9	7.969	804	813	820	rBV	2403319	3759304	15.35%	1.820%
10	8.034	820	824	828	rVB2	19413	29631	0.12%	0.014%
11	8.675	924	933	945	rBV	2109168	3349404	13.68%	1.621%
12	9.139	1004	1012	1022	rBV	3621706	5839935	23.85%	2.827%
13	9.239	1025	1029	1036	rVB2	24751	39246	0.16%	0.019%
14	9.545	1074	1081	1089	rVB	84614	134909	0.55%	0.065%
15	9.863	1125	1135	1149	rBV	2835904	4626960	18.89%	2.240%
16	10.398	1218	1226	1248	rBV	4027238	6683726	27.29%	3.235%
17	10.786	1284	1292	1299	rBV	3431771	5743308	23.45%	2.780%
18	10.922	1307	1315	1327	rBV	1591529	2724875	11.13%	1.319%
19	11.563	1418	1424	1430	rBV6	18145	40919	0.17%	0.020%
20	12.039	1497	1505	1511	rBV2	44401	71304	0.29%	0.035%
21	12.192	1525	1531	1536	rBV5	17358	32708	0.13%	0.016%
22	12.363	1555	1560	1569	rBV	81623	134194	0.55%	0.065%
23	13.427	1737	1741	1747	rVB	31596	46468	0.19%	0.022%
24	13.498	1747	1753	1758	rVV	52670	84019	0.34%	0.041%
25	13.575	1761	1766	1773	rVB6	22473	43916	0.18%	0.021%
26	14.016	1834	1841	1855	rBV	8753252	12191042	49.78%	5.902%
27	14.133	1856	1861	1866	rVB9	20252	33637	0.14%	0.016%
28	14.304	1883	1890	1905	rBV	10076926	14591771	59.59%	7.064%
29	14.610	1931	1942	1952	rBV	5848270	8319261	33.97%	4.027%
30	14.798	1967	1974	1988	rBV	578380	958010	3.91%	0.464%
31	15.021	2006	2012	2020	rVB6	56914	102621	0.42%	0.050%
32	15.604	2100	2111	2124	rBV	13109035	18712589	76.42%	9.058%
33	15.721	2124	2131	2144	rVV	4258802	5955170	24.32%	2.883%
34	15.839	2147	2151	2157	rVB	59657	102931	0.42%	0.050%
35	15.968	2167	2173	2183	rVB	918495	1231238	5.03%	0.596%
36	16.386	2239	2244	2251	rVB8	18016	30236	0.12%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013051.D
 Acq On : 10 Dec 2022 21:34
 Operator : CG/JU
 Sample : N5950-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF53

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	17.151	2370	2374	2381	rVB2	20813	43463	0.18%	0.021%
38	17.363	2403	2410	2417	rBV	7016561	10291432	42.03%	4.982%
39	17.468	2421	2428	2440	rVV	14051805	20428952	83.42%	9.889%
40	17.580	2445	2447	2454	rVV2	21822	30686	0.13%	0.015%
41	17.739	2470	2474	2479	rVB2	21674	32769	0.13%	0.016%
42	18.110	2534	2537	2547	rBV10	18891	37888	0.15%	0.018%
43	18.233	2553	2558	2567	rBV	259930	339367	1.39%	0.164%
44	18.645	2625	2628	2632	rVB3	42550	49819	0.20%	0.024%
45	18.715	2636	2640	2643	rVV6	25563	30301	0.12%	0.015%
46	19.268	2730	2734	2739	rBV2	192799	263310	1.08%	0.127%
47	19.339	2741	2746	2750	rBV	201060	299288	1.22%	0.145%
48	19.462	2763	2767	2772	rBV	95933	120785	0.49%	0.058%
49	19.609	2789	2792	2797	rVB3	58910	66447	0.27%	0.032%
50	19.698	2801	2807	2819	rVV	18382393	24487861	100.00%	11.854%
51	21.139	3048	3052	3061	rBV2	363251	591144	2.41%	0.286%
52	21.451	3099	3105	3111	rBV	8078947	10675458	43.59%	5.168%
53	22.727	3319	3322	3327	rVB	266040	336084	1.37%	0.163%
54	23.780	3493	3501	3512	rVB2	10566492	21651736	88.42%	10.481%
55	23.939	3521	3528	3544	rVB2	4569068	9728524	39.73%	4.709%




Sum of corrected areas: 206575094

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013051.D
Acq On : 10 Dec 2022 21:34
Operator : CG/JU
Sample : N5950-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF53

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

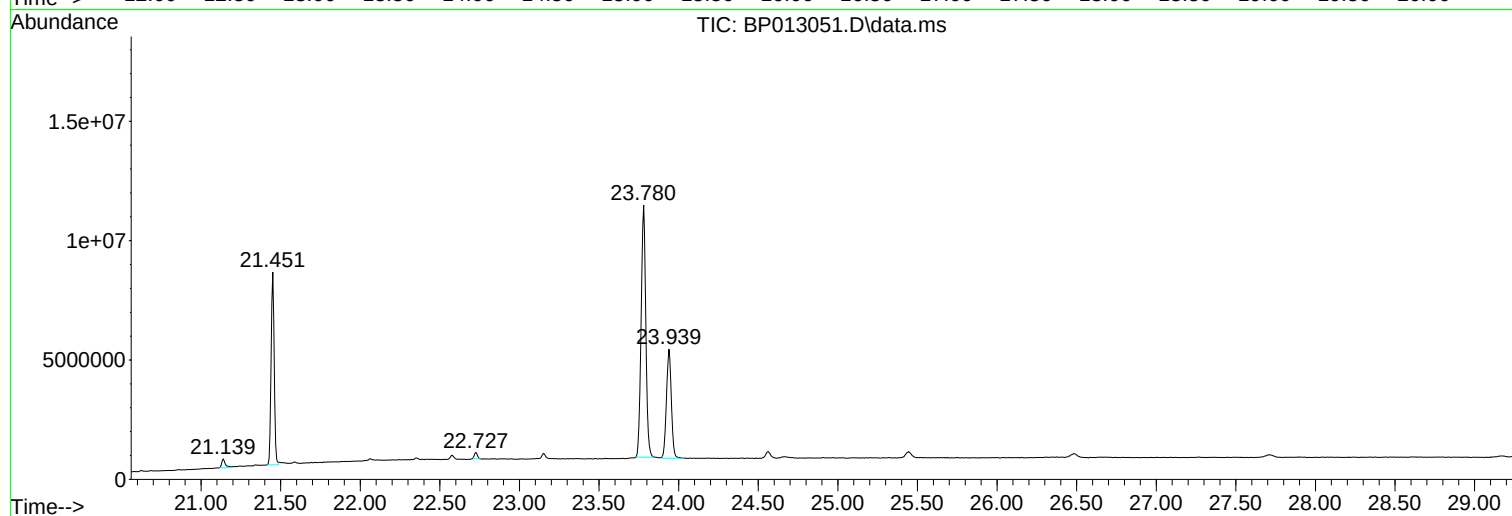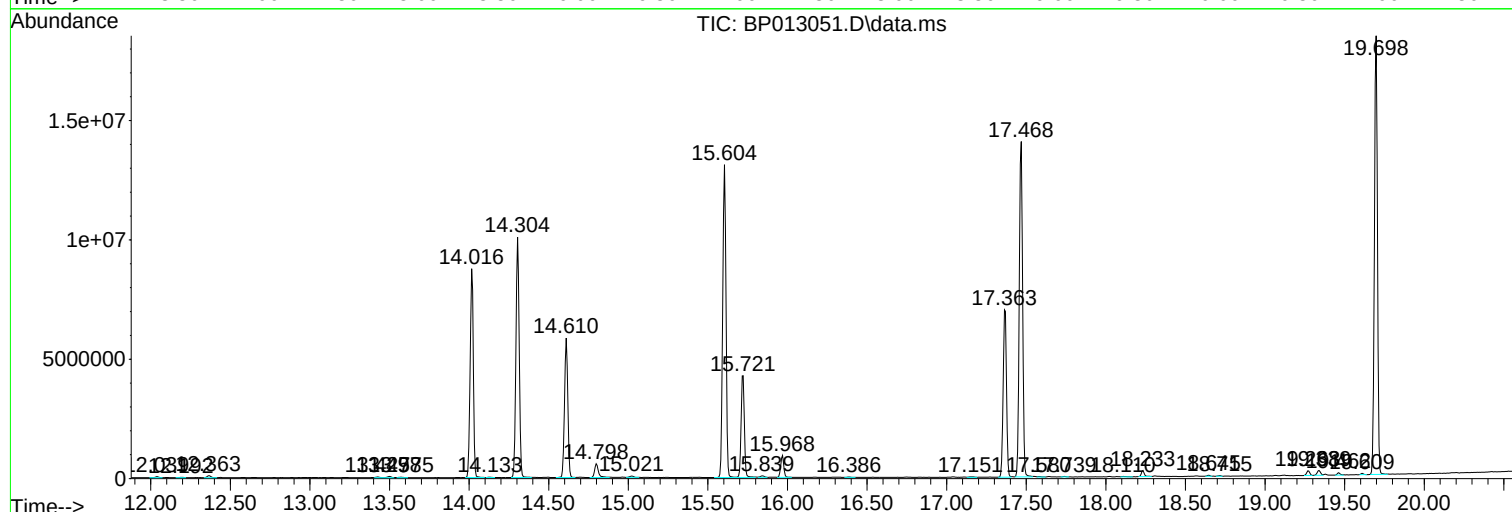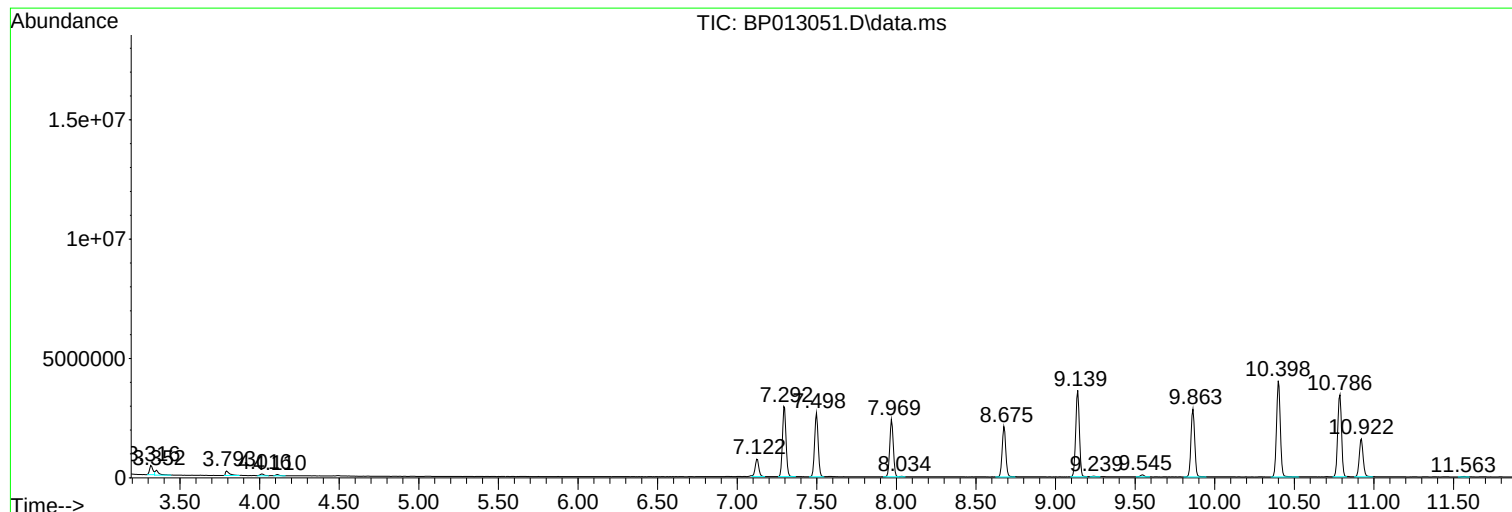

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013051.D
Acq On : 10 Dec 2022 21:34
Operator : CG/JU
Sample : N5950-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF53










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.969	2.96 ng/ul	1231240	Acenaphthene-d10	14.610

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzophenone	182	C13H10O	000119-61-9	95
3			Benzophenone	182	C13H10O	000119-61-9	94
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	91

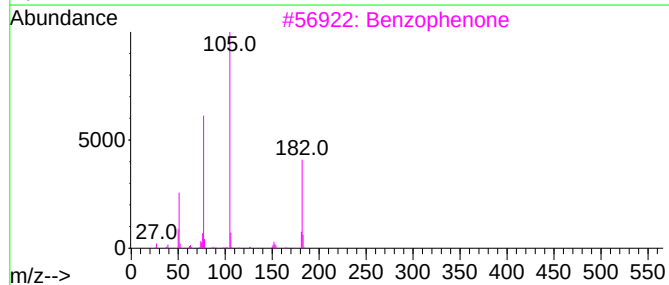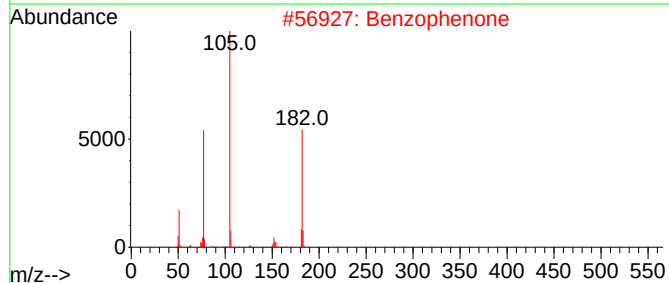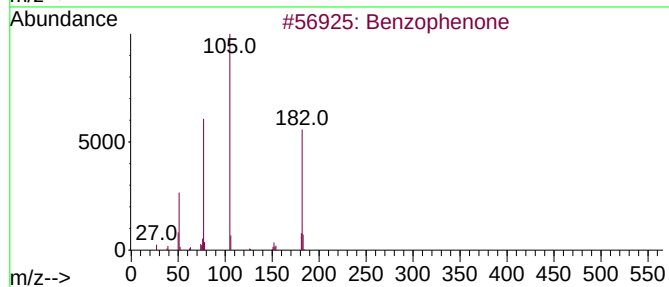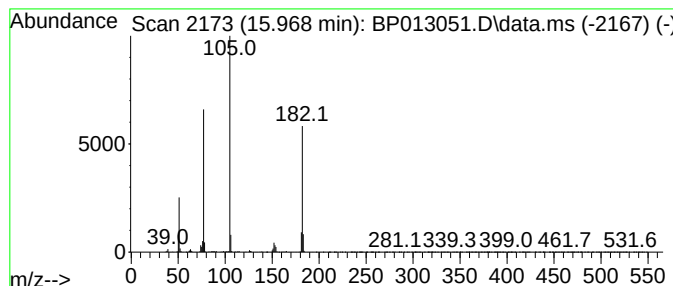

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013051.D
Acq On : 10 Dec 2022 21:34
Operator : CG/JU
Sample : N5950-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF53

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.969	3.0	ng/u1	1231240	3	14.610	8319260	20.0