

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013052.D
 Acq On : 10 Dec 2022 22:08
 Operator : CG/JU
 Sample : N5950-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013052.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	17	22	26	rBV	355303	531715	2.42%	0.302%
2	3.352	26	28	42	rVB	153648	223816	1.02%	0.127%
3	3.787	100	102	116	rBV	325098	563985	2.57%	0.321%
4	4.017	136	141	150	rVB	63071	110239	0.50%	0.063%
5	4.111	153	157	163	rVB	49417	71614	0.33%	0.041%
6	7.122	659	669	682	rVB	580541	941653	4.29%	0.535%
7	7.293	691	698	707	rBV	2351977	3701259	16.87%	2.105%
8	7.499	723	733	744	rBV	2026412	3249343	14.81%	1.848%
9	7.969	806	813	820	rBV	1948316	3031287	13.82%	1.724%
10	8.675	925	933	947	rBV	1673434	2648374	12.07%	1.506%
11	9.134	1004	1011	1023	rBV	2772738	4669203	21.28%	2.655%
12	9.540	1076	1080	1087	rVB2	31164	51798	0.24%	0.029%
13	9.863	1127	1135	1151	rBV	2215158	3649990	16.64%	2.075%
14	10.399	1219	1226	1240	rBV	3326378	5328183	24.29%	3.030%
15	10.569	1250	1255	1262	rBV9	10019	22101	0.10%	0.013%
16	10.781	1283	1291	1300	rBV	2791359	4665530	21.27%	2.653%
17	10.922	1307	1315	1332	rBV	1731608	3025273	13.79%	1.720%
18	12.040	1498	1505	1510	rBV2	19936	35632	0.16%	0.020%
19	12.363	1554	1560	1567	rVB2	69612	113558	0.52%	0.065%
20	13.499	1748	1753	1759	rBV	26400	40865	0.19%	0.023%
21	13.563	1761	1764	1772	rVB6	18060	36349	0.17%	0.021%
22	14.016	1833	1841	1856	rBV	7527905	10376992	47.30%	5.900%
23	14.128	1857	1860	1866	rVB8	12744	23081	0.11%	0.013%
24	14.251	1874	1881	1883	rBV8	20189	35810	0.16%	0.020%
25	14.304	1883	1890	1901	rVV	8584986	12329004	56.19%	7.010%
26	14.610	1935	1942	1949	rBV	4634847	6732919	30.69%	3.828%
27	14.798	1968	1974	1989	rBV	480459	799527	3.64%	0.455%
28	15.022	2006	2012	2017	rVB7	37176	65654	0.30%	0.037%
29	15.240	2044	2049	2055	rVB5	15944	26382	0.12%	0.015%
30	15.404	2071	2077	2079	rBV2	19102	29490	0.13%	0.017%
31	15.604	2103	2111	2122	rBV	11249521	16072998	73.26%	9.139%
32	15.716	2124	2130	2141	rBV	3653427	4931346	22.48%	2.804%
33	15.840	2147	2151	2157	rVB	56847	90131	0.41%	0.051%
34	15.963	2167	2172	2176	rBV2	35147	52066	0.24%	0.030%
35	16.316	2228	2232	2238	rVV8	18183	37688	0.17%	0.021%
36	16.387	2240	2244	2249	rVB7	19996	31980	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013052.D
 Acq On : 10 Dec 2022 22:08
 Operator : CG/JU
 Sample : N5950-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	17.034	2351	2354	2359	rVB4	14692	22915	0.10%	0.013%
38	17.110	2360	2367	2370	rVV6	19568	33489	0.15%	0.019%
39	17.157	2370	2375	2383	rVB3	24871	52254	0.24%	0.030%
40	17.269	2391	2394	2400	rVB6	30294	36308	0.17%	0.021%
41	17.363	2404	2410	2417	rBV	6018279	8498593	38.74%	4.832%
42	17.463	2420	2427	2438	rVV	12373685	17941801	81.78%	10.202%
43	17.551	2440	2442	2445	rVB4	32181	32963	0.15%	0.019%
44	17.645	2454	2458	2463	rBV	36036	50601	0.23%	0.029%
45	17.739	2471	2474	2481	rVB2	16316	22478	0.10%	0.013%
46	18.022	2518	2522	2526	rVB6	26435	35750	0.16%	0.020%
47	18.228	2553	2557	2563	rBV	155898	217903	0.99%	0.124%
48	18.310	2567	2571	2575	rVV	62708	80896	0.37%	0.046%
49	18.645	2625	2628	2634	rVB3	51540	59541	0.27%	0.034%
50	18.722	2637	2641	2645	rVV7	20795	33466	0.15%	0.019%
51	19.063	2695	2699	2702	rBV2	27560	38398	0.18%	0.022%
52	19.269	2730	2734	2739	rBV	183061	243671	1.11%	0.139%
53	19.339	2741	2746	2750	rBV	176892	254064	1.16%	0.144%
54	19.463	2763	2767	2771	rBV3	94545	127830	0.58%	0.073%
55	19.698	2800	2807	2818	rBV	16333913	21939743	100.00%	12.475%
56	21.139	3049	3052	3056	rBV3	131830	169371	0.77%	0.096%
57	21.451	3099	3105	3119	rBV	7108868	9220206	42.03%	5.243%
58	23.780	3493	3501	3516	rVB2	9632961	20112098	91.67%	11.436%
59	23.939	3521	3528	3541	rVB2	4011902	8298985	37.83%	4.719%




Sum of corrected areas: 175870159

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013052.D
Acq On : 10 Dec 2022 22:08
Operator : CG/JU
Sample : N5950-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

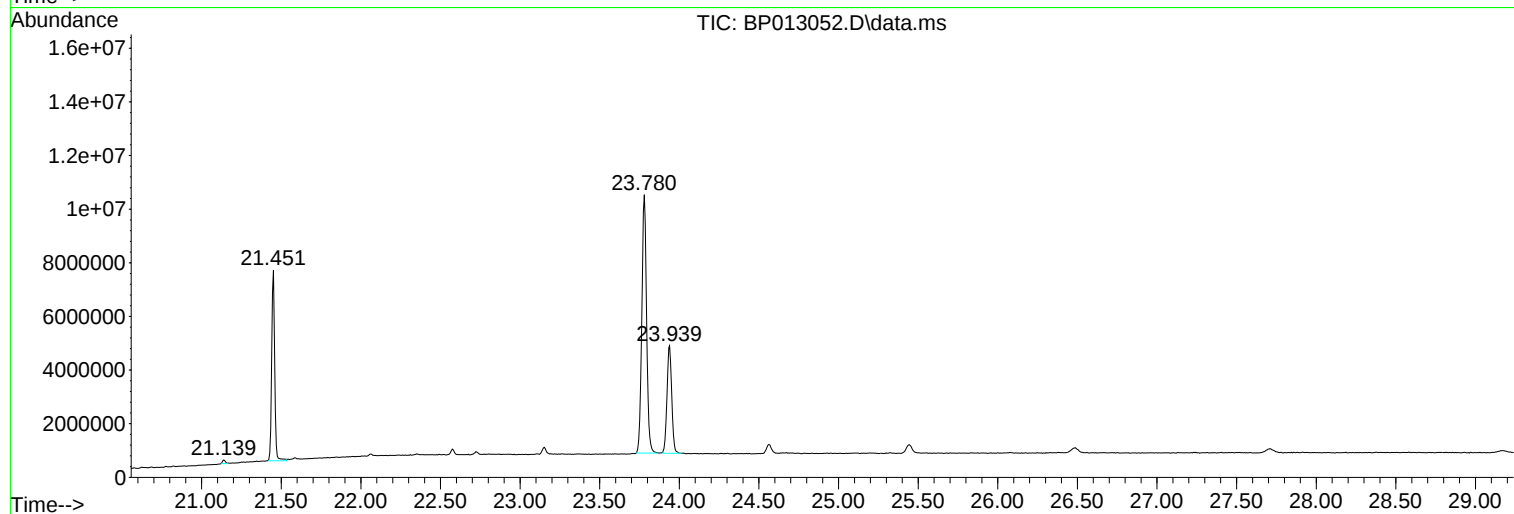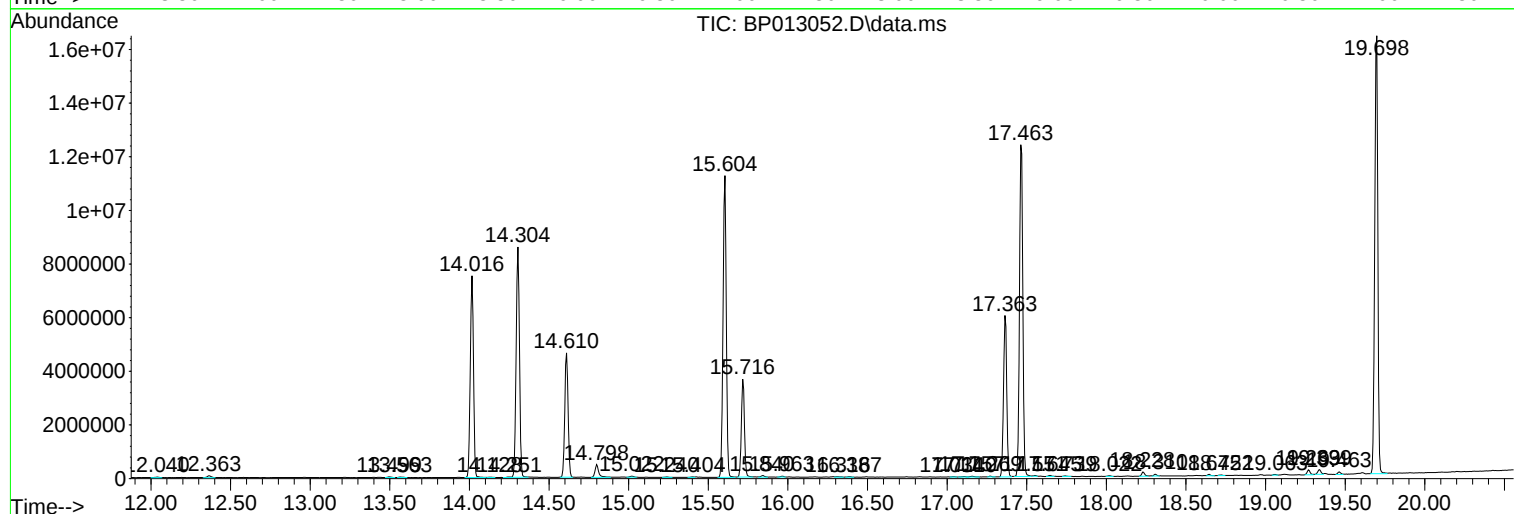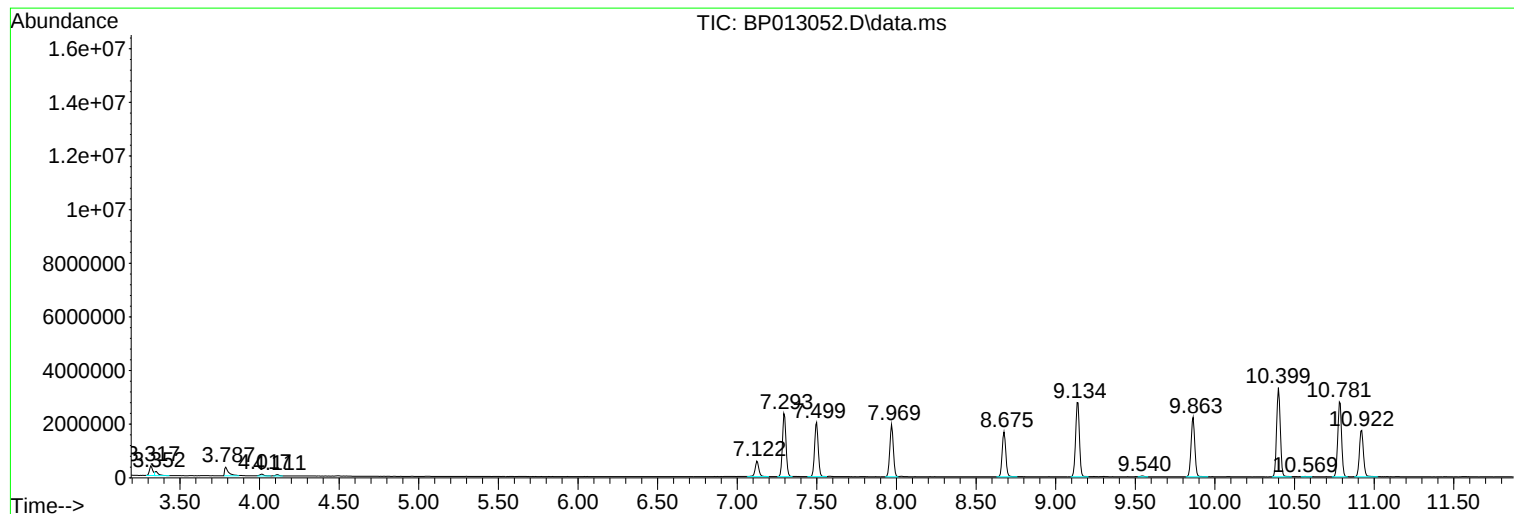

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013052.D
Acq On : 10 Dec 2022 22:08
Operator : CG/JU
Sample : N5950-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013052.D
Acq On : 10 Dec 2022 22:08
Operator : CG/JU
Sample : N5950-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc