

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013053.D
 Acq On : 10 Dec 2022 22:42
 Operator : CG/JU
 Sample : N5950-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	18	22	25	rBV	113451	160083	0.75%	0.090%
2	3.352	25	28	38	rVB	146797	220328	1.03%	0.125%
3	3.787	100	102	119	rBV	339863	586777	2.74%	0.332%
4	4.011	135	140	148	rVB	64623	108694	0.51%	0.061%
5	4.111	153	157	162	rVB	37372	50553	0.24%	0.029%
6	7.122	659	669	677	rBV	557035	922163	4.30%	0.521%
7	7.293	692	698	709	rVB	2425409	3730904	17.41%	2.109%
8	7.499	726	733	740	rBV	1942019	3068163	14.32%	1.734%
9	7.969	806	813	820	rBV	1973267	3064404	14.30%	1.732%
10	8.675	923	933	946	rBV	1602192	2490258	11.62%	1.407%
11	9.140	1003	1012	1024	rBV	2880414	4794544	22.37%	2.710%
12	9.540	1076	1080	1087	rVB2	48655	81147	0.38%	0.046%
13	9.863	1126	1135	1145	rBV	2197395	3611806	16.85%	2.041%
14	10.399	1218	1226	1238	rBV	3124547	5138154	23.98%	2.904%
15	10.787	1283	1292	1304	rVB	2842919	4767456	22.25%	2.694%
16	10.922	1307	1315	1331	rBV	1494313	2594822	12.11%	1.467%
17	11.451	1399	1405	1411	rVB9	10934	22073	0.10%	0.012%
18	12.034	1499	1504	1510	rVB2	20203	36212	0.17%	0.020%
19	12.363	1553	1560	1567	rVB	70624	127229	0.59%	0.072%
20	13.498	1746	1753	1757	rBV3	30164	52048	0.24%	0.029%
21	13.569	1759	1765	1773	rVB6	25308	51915	0.24%	0.029%
22	13.928	1822	1826	1830	rBV6	16175	21631	0.10%	0.012%
23	14.016	1834	1841	1852	rVV	7525415	10568032	49.32%	5.973%
24	14.128	1855	1860	1869	rVB	16378	36512	0.17%	0.021%
25	14.304	1883	1890	1899	rVV	8731895	12630398	58.94%	7.138%
26	14.610	1935	1942	1952	rVB	4854080	6973011	32.54%	3.941%
27	14.798	1968	1974	1989	rBV	437424	737246	3.44%	0.417%
28	15.022	2006	2012	2018	rVB6	46529	77506	0.36%	0.044%
29	15.604	2103	2111	2123	rBV	11497198	16334207	76.23%	9.232%
30	15.716	2123	2130	2143	rVV	3499478	4808431	22.44%	2.718%
31	15.839	2147	2151	2157	rVB2	52646	86247	0.40%	0.049%
32	15.957	2168	2171	2177	rBV6	12229	21929	0.10%	0.012%
33	16.386	2239	2244	2250	rVB8	15635	27400	0.13%	0.015%
34	17.045	2350	2356	2360	rBV8	16876	28426	0.13%	0.016%
35	17.151	2371	2374	2380	rVB4	19023	32503	0.15%	0.018%
36	17.363	2403	2410	2418	rBV	6260558	8753293	40.85%	4.947%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013053.D
 Acq On : 10 Dec 2022 22:42
 Operator : CG/JU
 Sample : N5950-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYF55

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	17.463	2420	2427	2438	rBV	12008897	17524957	81.78%	9.905%
38	17.551	2439	2442	2446	rVV3	44468	51098	0.24%	0.029%
39	17.639	2455	2457	2465	rVB3	15499	22597	0.11%	0.013%
40	17.745	2471	2475	2479	rVB4	15777	25137	0.12%	0.014%
41	18.016	2517	2521	2526	rVB7	32925	44542	0.21%	0.025%
42	18.228	2553	2557	2563	rBV3	85416	117901	0.55%	0.067%
43	18.310	2568	2571	2575	rVB	26811	33068	0.15%	0.019%
44	18.645	2624	2628	2632	rBV3	54456	64824	0.30%	0.037%
45	18.716	2637	2640	2646	rVB6	29528	39937	0.19%	0.023%
46	19.110	2703	2707	2712	rBV8	33616	64909	0.30%	0.037%
47	19.269	2729	2734	2739	rBV2	183247	253734	1.18%	0.143%
48	19.333	2741	2745	2750	rBV	176806	260571	1.22%	0.147%
49	19.463	2764	2767	2771	rVB6	38898	46395	0.22%	0.026%
50	19.610	2789	2792	2796	rVB2	54493	62577	0.29%	0.035%
51	19.692	2800	2806	2817	rBV	15884157	21428738	100.00%	12.111%
52	21.451	3099	3105	3113	rBV	6944451	9376327	43.76%	5.299%
53	22.574	3293	3296	3302	rVB2	249753	334585	1.56%	0.189%
54	23.151	3391	3394	3401	rVB	381253	554136	2.59%	0.313%
55	23.780	3493	3501	3514	rVB2	9510570	20246071	94.48%	11.443%
56	23.939	3521	3528	3538	rVB2	4287670	8638966	40.31%	4.883%
57	24.562	3630	3634	3641	rVB	495960	928891	4.33%	0.525%




Sum of corrected areas: 176936466

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013053.D
Acq On : 10 Dec 2022 22:42
Operator : CG/JU
Sample : N5950-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

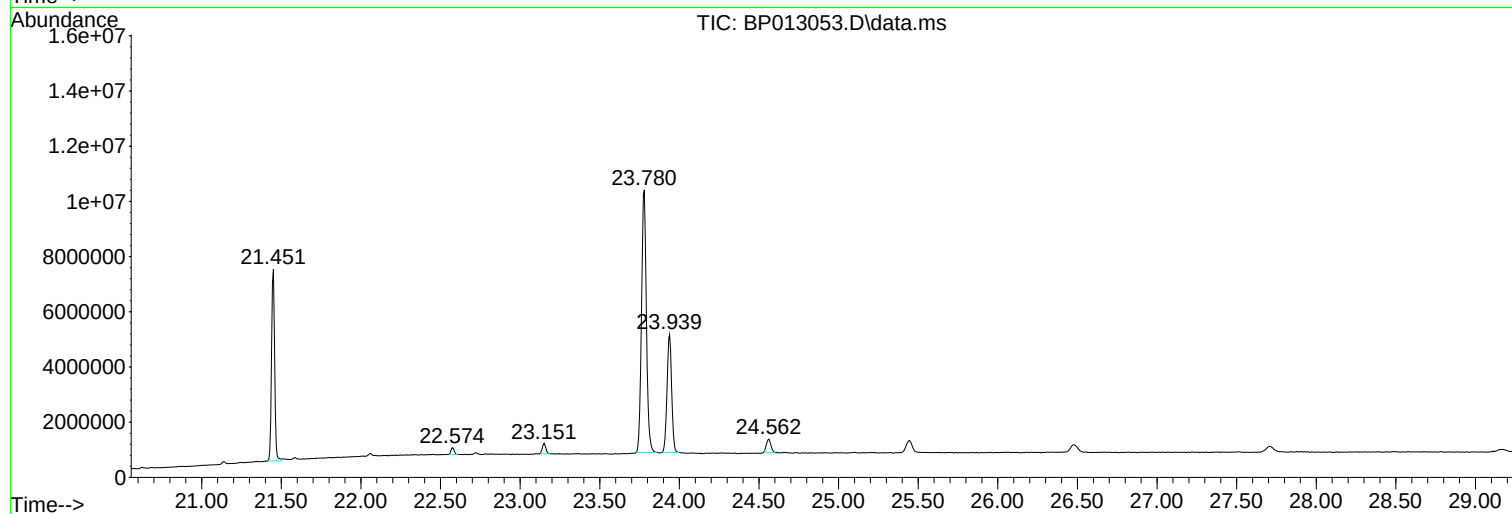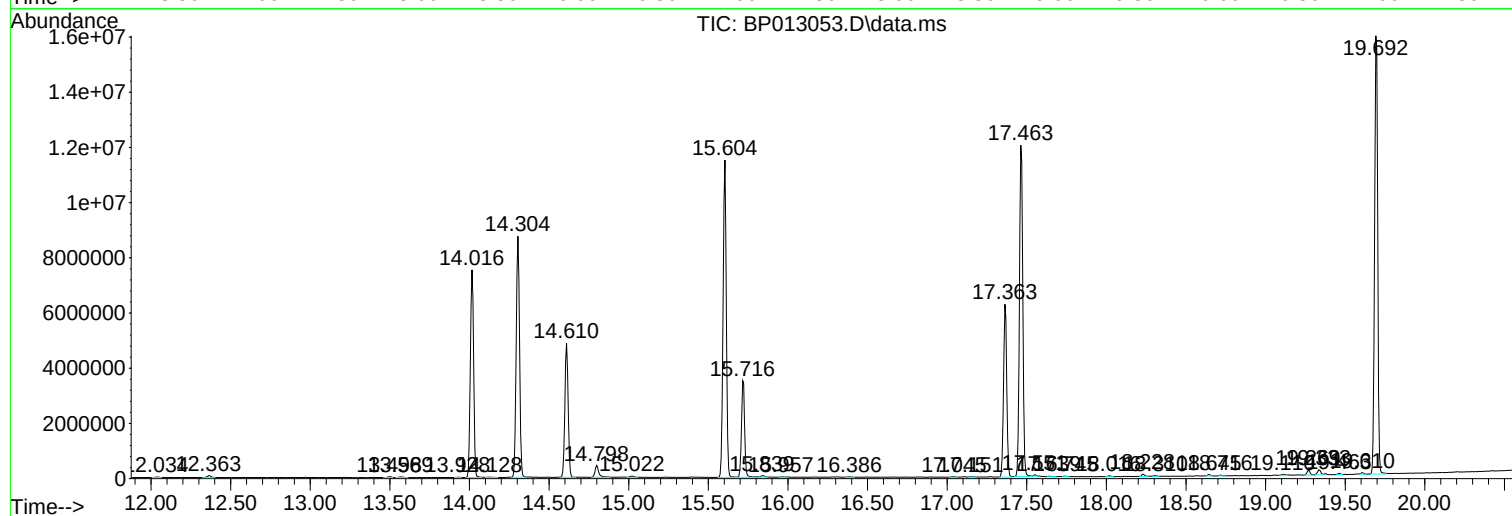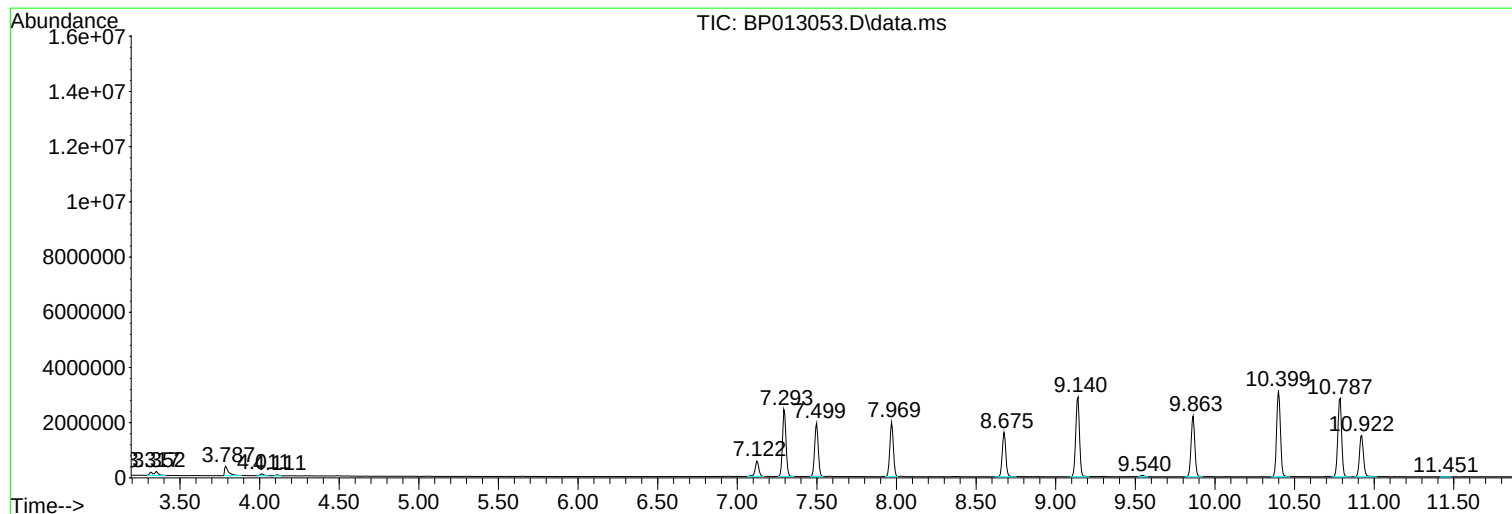

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013053.D
Acq On : 10 Dec 2022 22:42
Operator : CG/JU
Sample : N5950-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF55










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.563	2.15 ng/ul	928891	Perylene-d12	23.939

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Eicosane	282	C20H42	000112-95-8	96
2			Heptadecane	240	C17H36	000629-78-7	93
3			Eicosane	282	C20H42	000112-95-8	93
4			Heptadecane, 9-hexyl-	324	C23H48	055124-79-3	91
5			Heneicosane	296	C21H44	000629-94-7	87

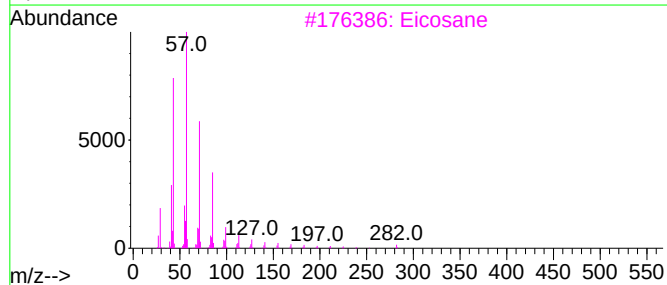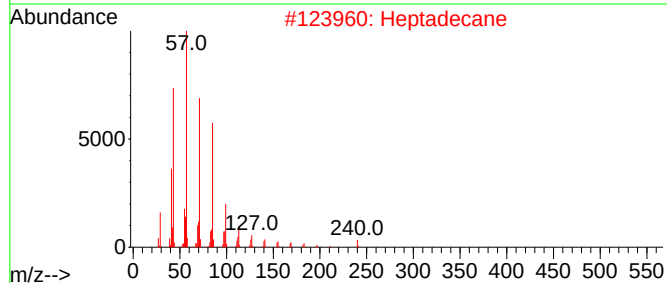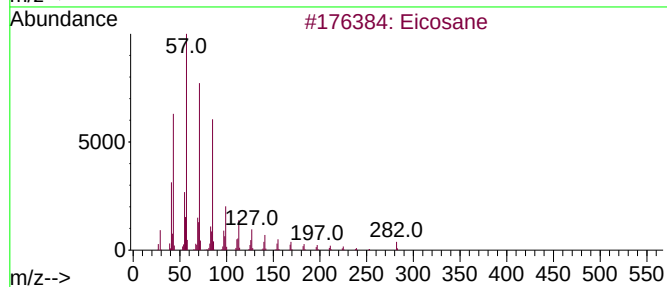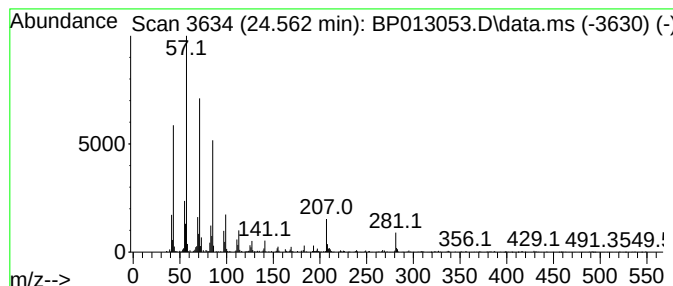

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013053.D
Acq On : 10 Dec 2022 22:42
Operator : CG/JU
Sample : N5950-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYF55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.563	2.1	ng/u1	928891	6	23.939	8638970	20.0