

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013056.D
 Acq On : 11 Dec 2022 00:24
 Operator : CG/JU
 Sample : N5927-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	20	22	25	rBV2	23140	24732	0.11%	0.012%
2	3.352	25	28	31	rVV	138593	168119	0.72%	0.082%
3	3.387	31	34	44	rVB	193465	289771	1.23%	0.141%
4	3.646	75	78	88	rVB	17190	33400	0.14%	0.016%
5	3.781	98	101	119	rBV	585431	1023470	4.36%	0.497%
6	4.011	136	140	151	rVB	71339	129454	0.55%	0.063%
7	4.111	153	157	162	rVB	39146	59172	0.25%	0.029%
8	4.652	244	249	256	rVB	54578	83996	0.36%	0.041%
9	7.122	659	669	683	rVB	617253	1055185	4.50%	0.512%
10	7.293	691	698	708	rBV	2694428	4197848	17.89%	2.038%
11	7.499	724	733	744	rBV	2420180	3834002	16.34%	1.861%
12	7.969	805	813	820	rBV	2350483	3674610	15.66%	1.784%
13	8.028	820	823	828	rVB2	22207	31190	0.13%	0.015%
14	8.675	925	933	945	rBV	1957504	3103751	13.23%	1.507%
15	9.140	1004	1012	1019	rBV	3208450	5264288	22.43%	2.556%
16	9.546	1074	1081	1089	rVB	134514	214157	0.91%	0.104%
17	9.863	1126	1135	1147	rBV	2561787	4183916	17.83%	2.031%
18	10.399	1217	1226	1238	rBV	3763798	6298756	26.84%	3.058%
19	10.563	1249	1254	1262	rVB3	26336	48814	0.21%	0.024%
20	10.781	1284	1291	1299	rBV	3354365	5670404	24.16%	2.753%
21	10.922	1305	1315	1333	rBV	2918033	5076102	21.63%	2.464%
22	11.563	1420	1424	1428	rBV7	17765	28958	0.12%	0.014%
23	12.040	1498	1505	1512	rVB2	81724	130413	0.56%	0.063%
24	12.363	1555	1560	1570	rVB	77275	132322	0.56%	0.064%
25	12.969	1659	1663	1667	rBV5	14673	23900	0.10%	0.012%
26	13.216	1700	1705	1711	rVB3	25637	40586	0.17%	0.020%
27	13.499	1748	1753	1761	rVB	53529	87369	0.37%	0.042%
28	13.928	1821	1826	1833	rBV10	11115	25069	0.11%	0.012%
29	14.016	1833	1841	1856	rBV	8621472	11759577	50.11%	5.709%
30	14.128	1856	1860	1865	rVB8	18393	29494	0.13%	0.014%
31	14.251	1876	1881	1884	rBV4	53216	98047	0.42%	0.048%
32	14.304	1884	1890	1901	rVB	9385001	13756598	58.62%	6.679%
33	14.610	1932	1942	1953	rBV	5688257	8279933	35.28%	4.020%
34	14.798	1965	1974	1992	rBV	562801	948963	4.04%	0.461%
35	15.010	2007	2010	2017	rVB8	31131	55026	0.23%	0.027%
36	15.240	2045	2049	2057	rVB2	42871	73569	0.31%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013056.D
 Acq On : 11 Dec 2022 00:24
 Operator : CG/JU
 Sample : N5927-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	15.398	2072	2076	2079	rBV	69261	98460	0.42%	0.048%
38	15.604	2103	2111	2123	rBV	12592204	17742356	75.60%	8.614%
39	15.716	2124	2130	2141	rVV	4151653	5705514	24.31%	2.770%
40	15.840	2147	2151	2158	rVB2	62330	102227	0.44%	0.050%
41	15.963	2168	2172	2176	rBV3	27991	39973	0.17%	0.019%
42	16.004	2176	2179	2185	rVB3	22252	30856	0.13%	0.015%
43	16.057	2185	2188	2193	rBV6	14036	23514	0.10%	0.011%
44	16.110	2193	2197	2201	rBV	59071	89219	0.38%	0.043%
45	16.240	2216	2219	2222	rBV4	19499	25863	0.11%	0.013%
46	16.281	2222	2226	2229	rVV	36989	56282	0.24%	0.027%
47	16.316	2229	2232	2240	rVV6	36771	76993	0.33%	0.037%
48	16.387	2240	2244	2248	rVB6	30720	46534	0.20%	0.023%
49	16.492	2258	2262	2267	rVB4	33625	41309	0.18%	0.020%
50	16.622	2281	2284	2287	rBV	36322	49984	0.21%	0.024%
51	16.745	2302	2305	2308	rVB3	21366	26053	0.11%	0.013%
52	16.834	2317	2320	2325	rVB7	28384	40685	0.17%	0.020%
53	17.104	2361	2366	2370	rBV7	36319	65267	0.28%	0.032%
54	17.157	2370	2375	2384	rVB6	43004	93881	0.40%	0.046%
55	17.269	2390	2394	2398	rVB2	72211	93905	0.40%	0.046%
56	17.363	2404	2410	2417	rBV	7231315	10233643	43.61%	4.969%
57	17.463	2421	2427	2439	rVB2	13417059	19775665	84.27%	9.601%
58	17.645	2454	2458	2470	rBV	82719	155572	0.66%	0.076%
59	17.739	2471	2474	2479	rVV3	32539	47773	0.20%	0.023%
60	18.016	2519	2521	2526	rVB	77747	94488	0.40%	0.046%
61	18.234	2553	2558	2564	rBV	583516	747145	3.18%	0.363%
62	18.310	2567	2571	2575	rVB	155900	191104	0.81%	0.093%
63	18.557	2610	2613	2619	rBV4	55391	72469	0.31%	0.035%
64	18.645	2625	2628	2635	rVB5	46626	62150	0.26%	0.030%
65	18.969	2681	2683	2687	rVB	57861	64501	0.27%	0.031%
66	19.057	2695	2698	2702	rBV	90750	108584	0.46%	0.053%
67	19.269	2730	2734	2738	rBV	209846	281093	1.20%	0.136%
68	19.339	2742	2746	2750	rVV	188137	258128	1.10%	0.125%
69	19.463	2763	2767	2771	rBV	220880	278587	1.19%	0.135%
70	19.698	2800	2807	2813	rBV	16979816	23468140	100.00%	11.394%
71	21.139	3048	3052	3060	rBV	908959	1371948	5.85%	0.666%
72	21.451	3099	3105	3121	rBV	8082540	10939248	46.61%	5.311%
73	23.151	3391	3394	3401	rVB	347266	514705	2.19%	0.250%
74	23.780	3493	3501	3519	rVB2	10368492	22069141	94.04%	10.715%
75	23.939	3521	3528	3539	rVB2	4804170	9973111	42.50%	4.842%
76	24.563	3630	3634	3642	rVB	442623	878492	3.74%	0.427%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013056.D
Acq On : 11 Dec 2022 00:24
Operator : CG/JU
Sample : N5927-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZA5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 205969523

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013056.D
Acq On : 11 Dec 2022 00:24
Operator : CG/JU
Sample : N5927-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

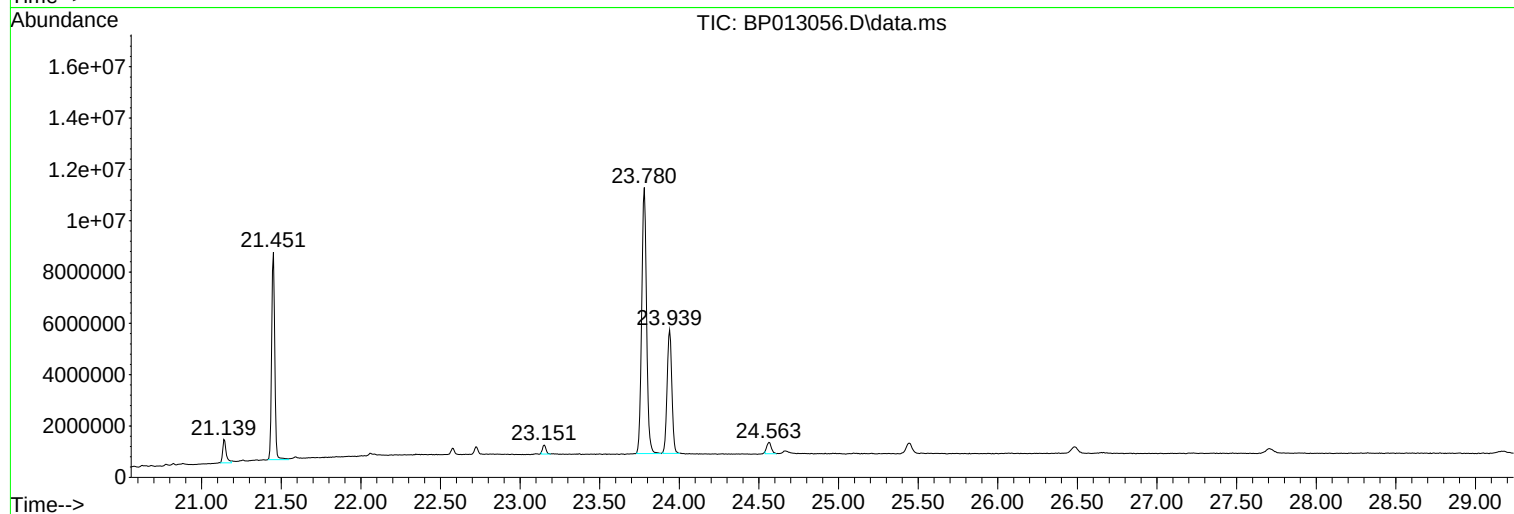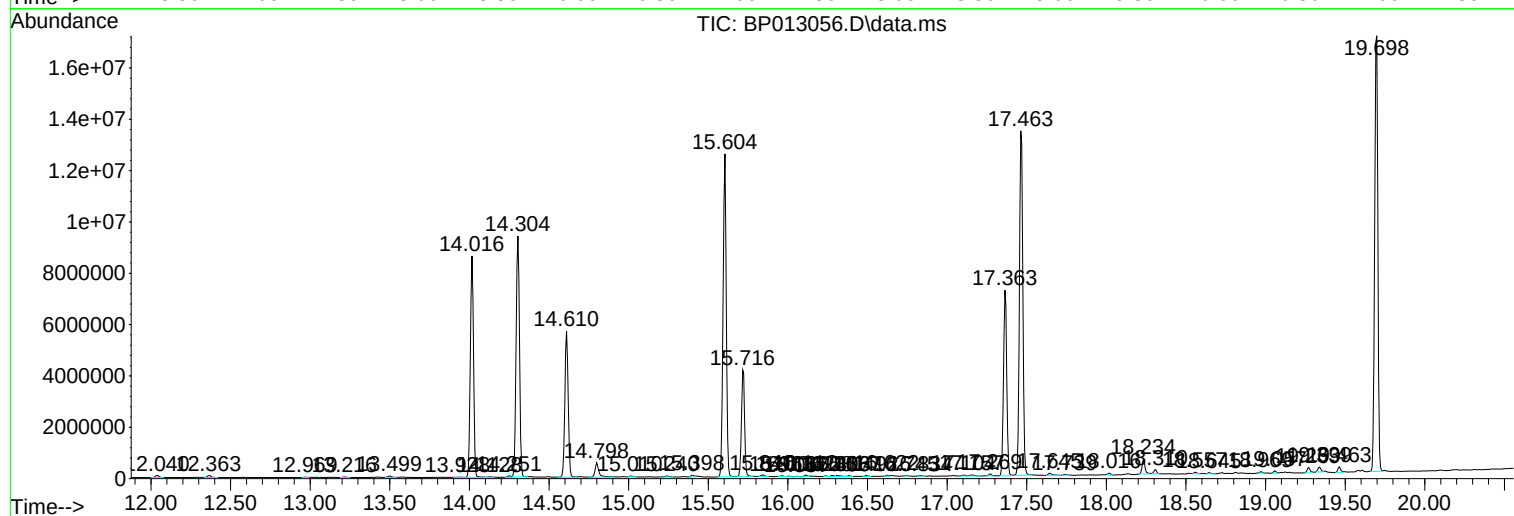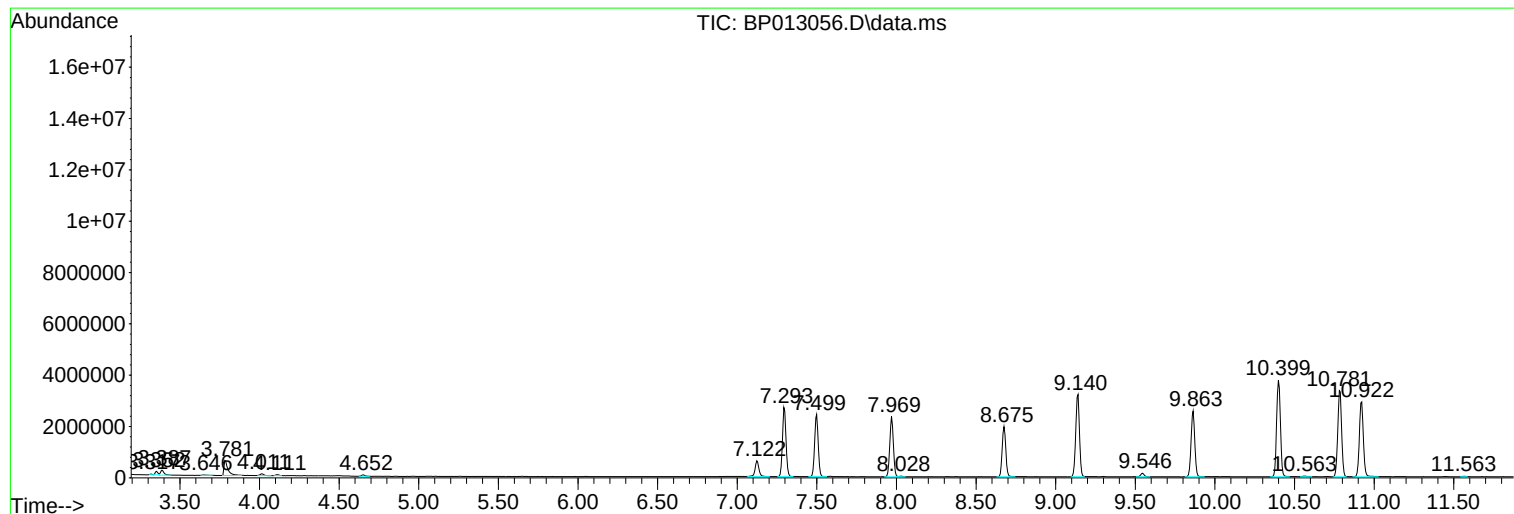

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013056.D
Acq On : 11 Dec 2022 00:24
Operator : CG/JU
Sample : N5927-20
Misc :
ALS Vial : 26 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
EXZA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
21.139	2.51 ng/ul	1371950	Chrysene-d12	21.451	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Tetracosene	336	C24H48	010192-32-2	99
2	Cyclotetracosane	336	C24H48	000297-03-0	98
3	Cyclopentadecane	210	C15H30	000295-48-7	97
4	1-Heneicosyl formate	340	C22H44O2	077899-03-7	96
5	9-Tricosene, (Z)-	322	C23H46	027519-02-4	96

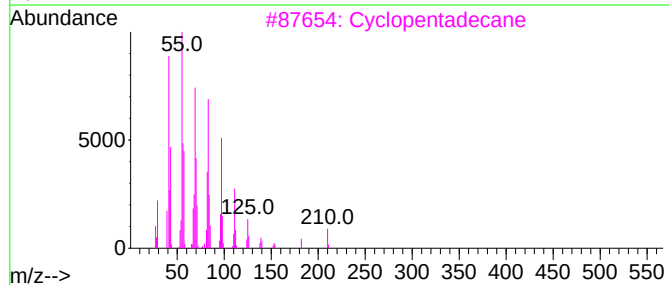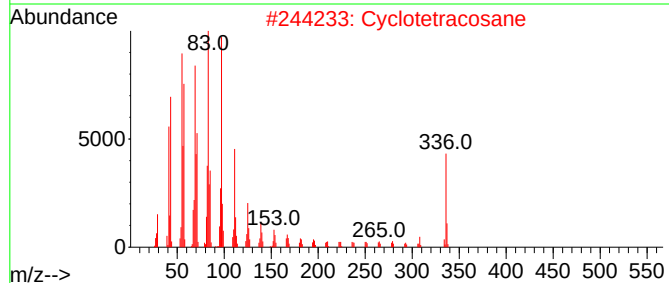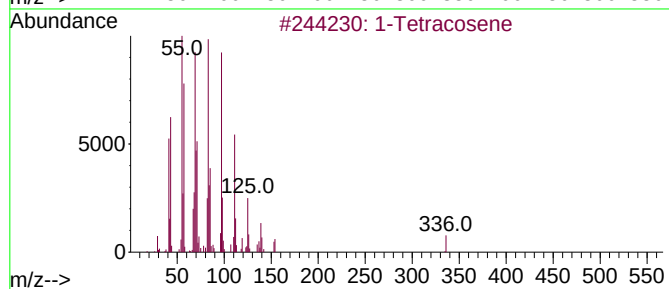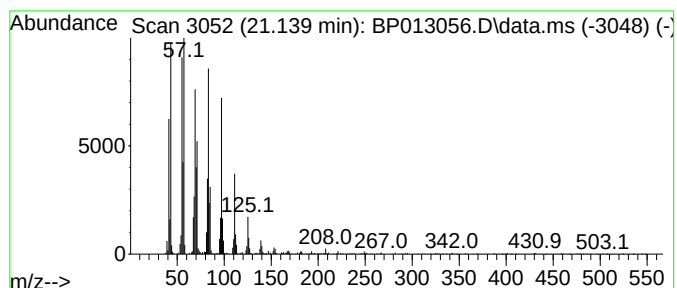

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013056.D
Acq On : 11 Dec 2022 00:24
Operator : CG/JU
Sample : N5927-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.139	2.5	ng/u1	1371950	5	21.451	10939200	20.0