

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013059.D
 Acq On : 11 Dec 2022 02:41
 Operator : CG/JU
 Sample : PB149488BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK488

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	36	rVB	179145	242045	1.19%	0.121%
2	3.775	97	100	127	rBV	2196446	3645577	17.87%	1.825%
3	4.110	153	157	165	rVB	45351	68835	0.34%	0.034%
4	7.122	662	669	682	rBV	2898926	4571685	22.41%	2.289%
5	7.293	691	698	708	rBV	2463840	3834155	18.80%	1.919%
6	7.498	725	733	747	rVB	2990712	4717029	23.13%	2.361%
7	7.969	805	813	823	rBV	2419420	3799457	18.63%	1.902%
8	8.675	925	933	946	rBV	3670533	5885251	28.85%	2.946%
9	9.140	1004	1012	1024	rBV	2885863	4706972	23.08%	2.356%
10	9.863	1125	1135	1147	rBV	2477505	4048024	19.85%	2.026%
11	10.398	1217	1226	1238	rBV	3879641	6293167	30.85%	3.150%
12	10.781	1284	1291	1300	rBV	3418225	5860139	28.73%	2.934%
13	10.922	1305	1315	1331	rBV	3501664	6178816	30.29%	3.093%
14	11.563	1421	1424	1430	rBV7	12420	21593	0.11%	0.011%
15	12.363	1554	1560	1568	rBV	68952	112483	0.55%	0.056%
16	13.498	1748	1753	1759	rBV2	28571	44980	0.22%	0.023%
17	14.016	1834	1841	1853	rBV	7381703	10153602	49.78%	5.083%
18	14.304	1882	1890	1901	rBV	8365250	12043320	59.05%	6.029%
19	14.610	1934	1942	1953	rBV	6002468	8594246	42.14%	4.302%
20	14.798	1967	1974	1998	rBV	3234785	4860376	23.83%	2.433%
21	15.010	2007	2010	2019	rVB9	17538	35598	0.17%	0.018%
22	15.604	2102	2111	2121	rBV	10551544	15279362	74.91%	7.649%
23	15.716	2124	2130	2147	rVV	3636117	5072503	24.87%	2.539%
24	15.839	2147	2151	2162	rVB2	51242	92499	0.45%	0.046%
25	16.380	2240	2243	2251	rBV8	13027	23787	0.12%	0.012%
26	17.039	2346	2355	2361	rBV9	17659	38744	0.19%	0.019%
27	17.151	2371	2374	2379	rVB3	14803	20459	0.10%	0.010%
28	17.363	2403	2410	2420	rBV	7400181	10720929	52.56%	5.367%
29	17.463	2420	2427	2448	rVV	11729993	16953675	83.12%	8.487%
30	17.739	2470	2474	2482	rBV4	13100	29222	0.14%	0.015%
31	19.268	2730	2734	2739	rBV2	140250	189616	0.93%	0.095%
32	19.339	2741	2746	2750	rBV	137121	203184	1.00%	0.102%
33	19.692	2800	2806	2817	rBV	15079776	20396270	100.00%	10.210%
34	21.451	3099	3105	3112	rBV	8453944	11463656	56.20%	5.739%
35	23.774	3493	3500	3513	rVB2	9019927	18771131	92.03%	9.397%
36	23.939	3520	3528	3541	rVB	5153771	10789490	52.90%	5.401%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013059.D
Acq On : 11 Dec 2022 02:41
Operator : CG/JU
Sample : PB149488BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK488

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 199761877

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013059.D
Acq On : 11 Dec 2022 02:41
Operator : CG/JU
Sample : PB149488BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

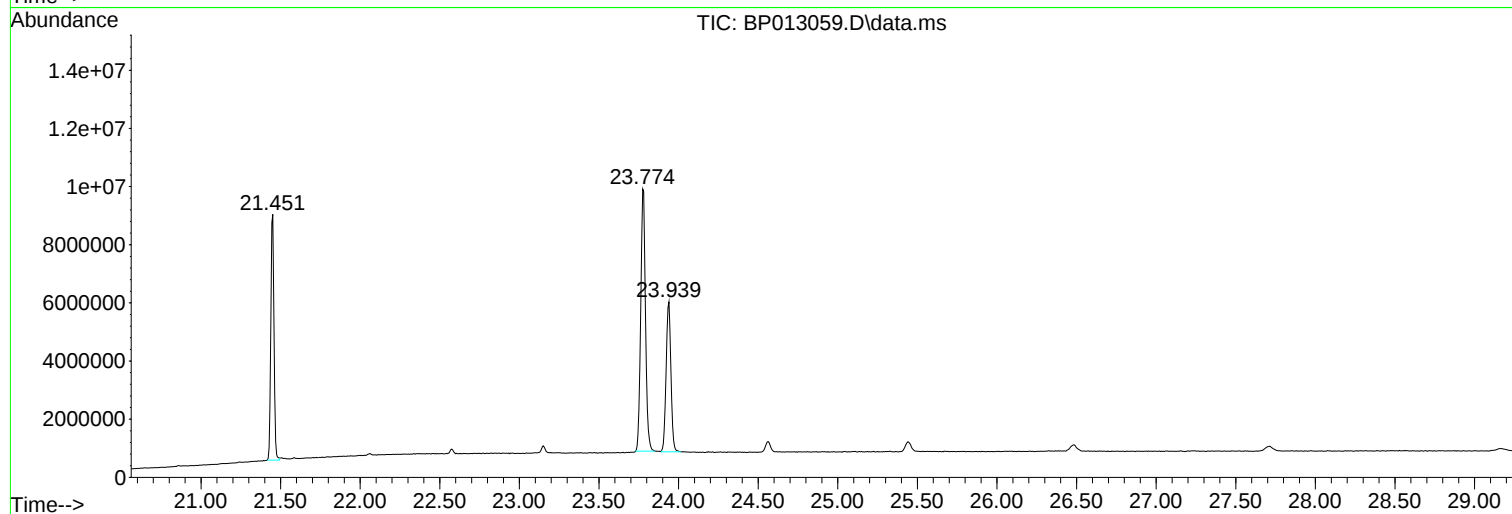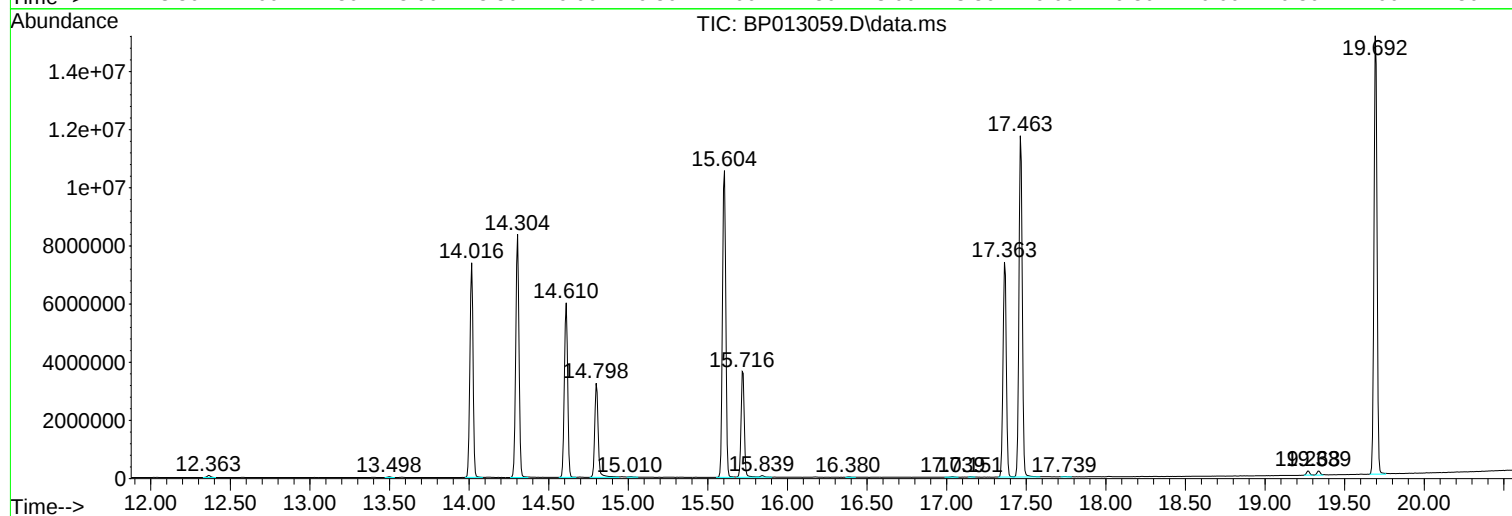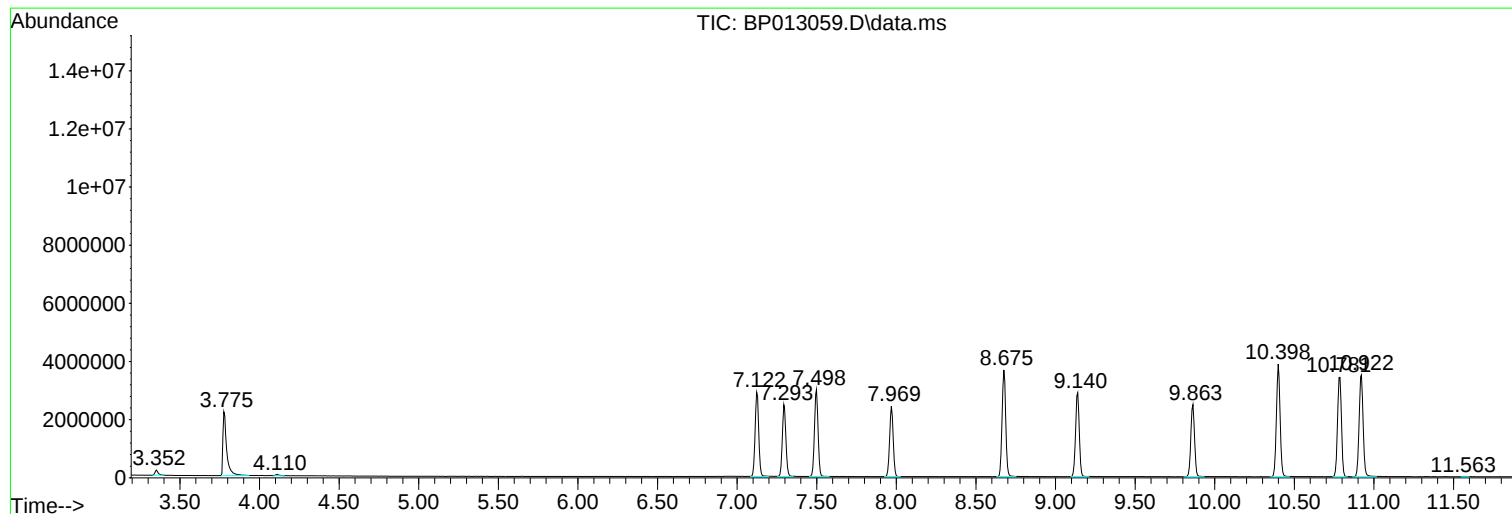

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013059.D
Acq On : 11 Dec 2022 02:41
Operator : CG/JU
Sample : PB149488BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013059.D
Acq On : 11 Dec 2022 02:41
Operator : CG/JU
Sample : PB149488BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc