

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013060.D
 Acq On : 11 Dec 2022 03:15
 Operator : CG/JU
 Sample : PB149498BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK498

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	38	rVB	153409	225686	1.24%	0.125%
2	3.775	97	100	118	rBV	1867122	3058265	16.79%	1.698%
3	4.111	153	157	163	rVB	39582	62525	0.34%	0.035%
4	7.122	662	669	680	rBV	2541861	3954023	21.71%	2.196%
5	7.293	692	698	711	rVB	2155352	3347714	18.38%	1.859%
6	7.499	725	733	745	rBV	2606181	4088485	22.45%	2.270%
7	7.969	805	813	823	rBV	2378394	3722883	20.44%	2.067%
8	8.675	925	933	950	rBV	3292682	5142798	28.24%	2.856%
9	9.134	1004	1011	1022	rBV	2459273	4065895	22.32%	2.258%
10	9.863	1123	1135	1147	rBV	2095652	3490008	19.16%	1.938%
11	10.399	1217	1226	1239	rBV	3314342	5469304	30.03%	3.037%
12	10.781	1283	1291	1301	rBV	3380420	5757913	31.62%	3.198%
13	10.922	1307	1315	1330	rBV	3131267	5517958	30.30%	3.064%
14	12.363	1554	1560	1569	rVB2	58541	99242	0.54%	0.055%
15	13.498	1748	1753	1757	rBV2	30391	47604	0.26%	0.026%
16	13.581	1763	1767	1774	rVB4	11342	19332	0.11%	0.011%
17	14.016	1834	1841	1853	rVB	6606143	9017223	49.51%	5.008%
18	14.304	1883	1890	1906	rBV	7303773	10508010	57.70%	5.835%
19	14.610	1933	1942	1953	rBV	5692807	8474579	46.53%	4.706%
20	14.798	1966	1974	1993	rBV	2773891	4127775	22.66%	2.292%
21	14.963	1999	2002	2007	rVB6	12231	19231	0.11%	0.011%
22	15.016	2007	2011	2016	rVB7	12657	22034	0.12%	0.012%
23	15.604	2104	2111	2123	rBV	9308336	13495660	74.10%	7.495%
24	15.716	2123	2130	2143	rVV	3323392	4482851	24.61%	2.489%
25	15.840	2147	2151	2157	rVB2	43825	66058	0.36%	0.037%
26	17.039	2350	2355	2360	rBV6	13783	19149	0.11%	0.011%
27	17.145	2370	2373	2378	rBV2	15811	25690	0.14%	0.014%
28	17.363	2403	2410	2420	rBV	7457093	10416153	57.19%	5.784%
29	17.463	2420	2427	2443	rVV2	10638595	15315782	84.09%	8.505%
30	19.269	2730	2734	2739	rBV	138173	180733	0.99%	0.100%
31	19.339	2742	2746	2750	rVV	119733	158899	0.87%	0.088%
32	19.692	2800	2806	2817	rBV	13884578	18212489	100.00%	10.114%
33	21.451	3099	3105	3119	rBV	7917216	11030937	60.57%	6.126%
34	23.774	3493	3500	3517	rVB2	7780965	16515057	90.68%	9.171%
35	23.939	3520	3528	3543	rVB2	4778737	9915189	54.44%	5.506%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013060.D
Acq On : 11 Dec 2022 03:15
Operator : CG/JU
Sample : PB149498BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK498

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 180073134

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013060.D
Acq On : 11 Dec 2022 03:15
Operator : CG/JU
Sample : PB149498BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK498

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

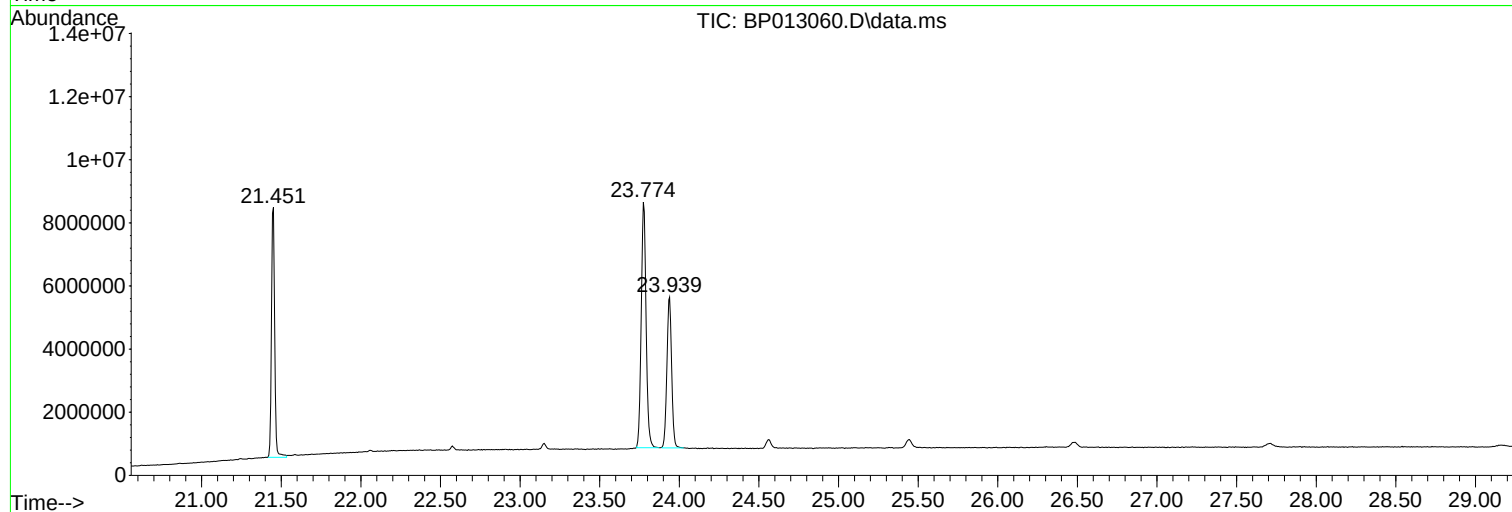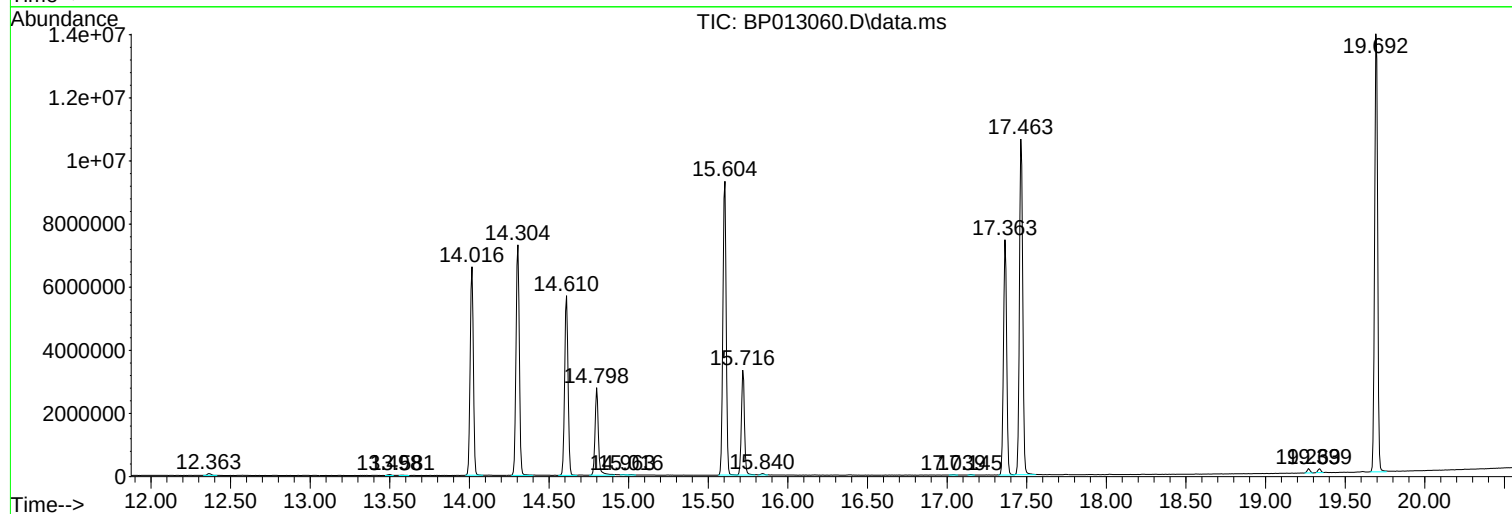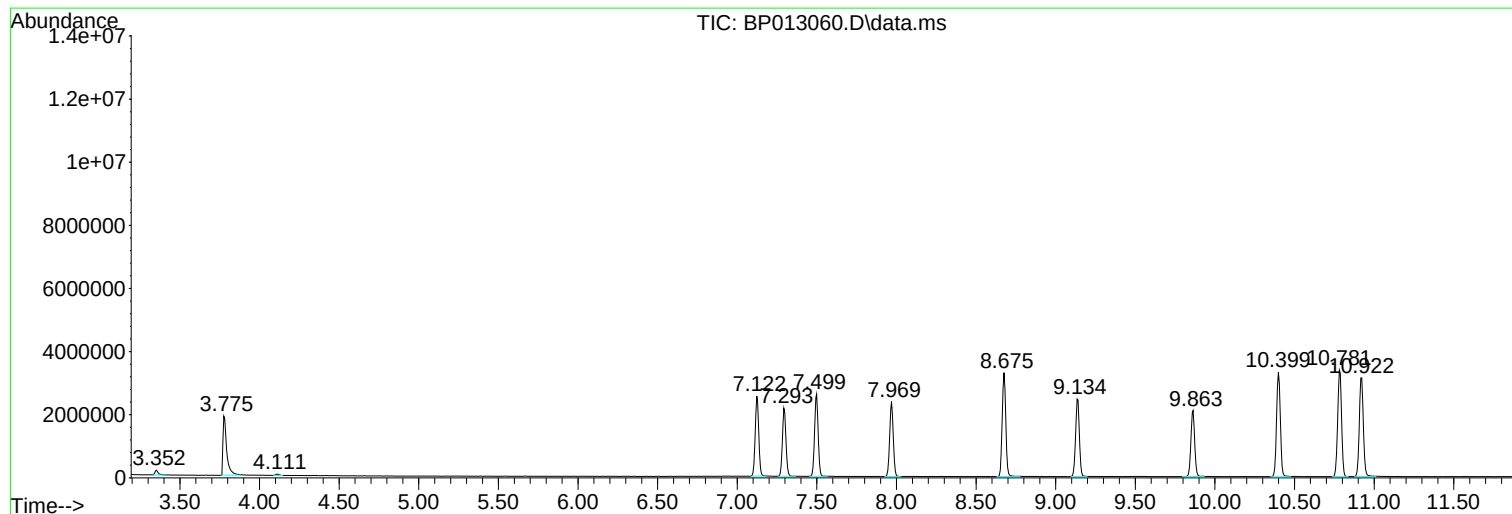

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013060.D
Acq On : 11 Dec 2022 03:15
Operator : CG/JU
Sample : PB149498BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK498

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013060.D
Acq On : 11 Dec 2022 03:15
Operator : CG/JU
Sample : PB149498BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK498

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
