

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013067.D
 Acq On : 11 Dec 2022 07:13
 Operator : CG/JU
 Sample : N5927-10
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.316	18	22	25	rBV	82491	113298	0.41%	0.050%
2	3.352	25	28	44	rVB	157296	285742	1.03%	0.125%
3	3.640	74	77	84	rVB	41405	56635	0.20%	0.025%
4	3.781	98	101	125	rBV2	666868	1272563	4.58%	0.558%
5	4.011	136	140	148	rVB	59084	98292	0.35%	0.043%
6	4.111	153	157	164	rVB	42273	67334	0.24%	0.030%
7	4.646	243	248	260	rVB	301007	489217	1.76%	0.215%
8	7.122	662	669	679	rVB	600390	966564	3.48%	0.424%
9	7.293	691	698	707	rBV	2497776	3859408	13.89%	1.692%
10	7.493	724	732	742	rBV	2255551	3618119	13.02%	1.587%
11	7.969	806	813	820	rBV	2657612	4178413	15.04%	1.832%
12	8.028	820	823	828	rVB2	26649	38746	0.14%	0.017%
13	8.675	924	933	943	rBV	1867656	2938308	10.58%	1.288%
14	9.134	1003	1011	1025	rBV	2956292	4822714	17.36%	2.115%
15	9.540	1076	1080	1091	rVB2	37243	65889	0.24%	0.029%
16	9.863	1127	1135	1148	rBV	2316279	3862399	13.90%	1.694%
17	10.398	1219	1226	1242	rBV	3651809	5926522	21.33%	2.599%
18	10.557	1249	1253	1260	rBV3	34757	64243	0.23%	0.028%
19	10.781	1280	1291	1299	rBV	3870260	6519007	23.47%	2.859%
20	10.916	1307	1314	1334	rBV	3145770	5500776	19.80%	2.412%
21	11.557	1417	1423	1428	rBV5	22569	39734	0.14%	0.017%
22	12.363	1555	1560	1566	rVB2	71596	106888	0.38%	0.047%
23	12.963	1654	1662	1666	rBV6	19407	35102	0.13%	0.015%
24	13.216	1699	1705	1713	rVB5	27761	46229	0.17%	0.020%
25	13.422	1737	1740	1747	rVB5	17623	30143	0.11%	0.013%
26	13.498	1747	1753	1758	rVV4	25870	45777	0.16%	0.020%
27	13.575	1762	1766	1775	rVB7	17295	32180	0.12%	0.014%
28	14.016	1834	1841	1856	rBV	8428872	11730642	42.22%	5.144%
29	14.134	1856	1861	1865	rVV6	24441	41555	0.15%	0.018%
30	14.245	1874	1880	1883	rBV3	88126	145485	0.52%	0.064%
31	14.304	1883	1890	1900	rVV	8818651	13118112	47.22%	5.752%
32	14.386	1901	1904	1909	rVB3	24472	36909	0.13%	0.016%
33	14.492	1919	1922	1927	rVB	30925	40183	0.14%	0.018%
34	14.610	1933	1942	1950	rBV	6399931	9408281	33.86%	4.126%
35	14.698	1954	1957	1965	rVB10	24907	42403	0.15%	0.019%
36	14.798	1965	1974	1989	rBV	622034	1098299	3.95%	0.482%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013067.D
 Acq On : 11 Dec 2022 07:13
 Operator : CG/JU
 Sample : N5927-10
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXZ98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	15.022	2005	2012	2019	rVB9	47297	103544	0.37%	0.045%
38	15.239	2044	2049	2056	rVB	53668	83871	0.30%	0.037%
39	15.345	2061	2067	2072	rBV	104584	146678	0.53%	0.064%
40	15.398	2072	2076	2078	rVV	77333	104922	0.38%	0.046%
41	15.445	2082	2084	2090	rVB	49451	52775	0.19%	0.023%
42	15.604	2103	2111	2123	rBV	11908605	18070415	65.04%	7.924%
43	15.716	2124	2130	2142	rVV	4698433	6263301	22.54%	2.746%
44	15.839	2146	2151	2158	rVB3	69809	121615	0.44%	0.053%
45	15.957	2167	2171	2176	rBV4	42010	55380	0.20%	0.024%
46	16.004	2176	2179	2184	rVB5	48437	65243	0.23%	0.029%
47	16.051	2184	2187	2194	rBV5	29689	48825	0.18%	0.021%
48	16.145	2198	2203	2206	rBV4	38405	64800	0.23%	0.028%
49	16.233	2215	2218	2222	rBV3	36089	47869	0.17%	0.021%
50	16.275	2222	2225	2228	rVV	63281	83947	0.30%	0.037%
51	16.310	2228	2231	2239	rVV5	71156	142161	0.51%	0.062%
52	16.386	2240	2244	2247	rVB4	39139	57072	0.21%	0.025%
53	16.492	2257	2262	2266	rBV3	65329	95551	0.34%	0.042%
54	16.657	2286	2290	2294	rBV7	20832	42443	0.15%	0.019%
55	16.716	2297	2300	2302	rBV3	23740	28374	0.10%	0.012%
56	16.745	2302	2305	2308	rVB2	30404	35428	0.13%	0.016%
57	16.828	2314	2319	2325	rVB8	46648	81829	0.29%	0.036%
58	17.110	2361	2367	2370	rBV3	70377	115573	0.42%	0.051%
59	17.157	2370	2375	2384	rVB3	66621	125181	0.45%	0.055%
60	17.269	2390	2394	2401	rVB	162336	197490	0.71%	0.087%
61	17.363	2403	2410	2417	rBV	8595466	12061807	43.42%	5.289%
62	17.463	2421	2427	2438	rVB2	14596881	21472040	77.29%	9.416%
63	17.645	2453	2458	2468	rBV	169338	337386	1.21%	0.148%
64	17.739	2471	2474	2486	rVB5	62326	138345	0.50%	0.061%
65	17.845	2490	2492	2497	rVB4	36981	40358	0.15%	0.018%
66	18.016	2518	2521	2526	rVB	192822	239633	0.86%	0.105%
67	18.186	2548	2550	2553	rBV2	29167	33897	0.12%	0.015%
68	18.233	2553	2558	2563	rVV	488558	666036	2.40%	0.292%
69	18.310	2567	2571	2574	rVB	285775	346849	1.25%	0.152%
70	18.516	2603	2606	2611	rBV3	65922	102509	0.37%	0.045%
71	18.645	2625	2628	2634	rVB4	91132	109892	0.40%	0.048%
72	18.969	2680	2683	2687	rVB	134673	162709	0.59%	0.071%
73	19.057	2694	2698	2703	rBV	184995	247104	0.89%	0.108%
74	19.122	2706	2709	2711	rBV2	97727	107052	0.39%	0.047%
75	19.269	2730	2734	2738	rBV2	243242	336864	1.21%	0.148%
76	19.339	2742	2746	2749	rBV	245428	337235	1.21%	0.148%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013067.D
Acq On : 11 Dec 2022 07:13
Operator : CG/JU
Sample : N5927-10
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ98

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION

77	19.463	2763	2767	2774	rBV	226776	363348	1.31%	0.159%
78	19.692	2800	2806	2813	rBV	18659931	26719575	96.18%	11.717%
79	21.139	3049	3052	3066	rVB	1142875	1637256	5.89%	0.718%
80	21.451	3099	3105	3120	rBV	10350189	13918227	50.10%	6.103%
81	23.780	3492	3501	3516	rVB2	13005585	27781800	100.00%	12.182%
82	23.939	3521	3528	3542	rVB2	6860036	13910668	50.07%	6.100%




Sum of corrected areas: 228046988

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013067.D
Acq On : 11 Dec 2022 07:13
Operator : CG/JU
Sample : N5927-10
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

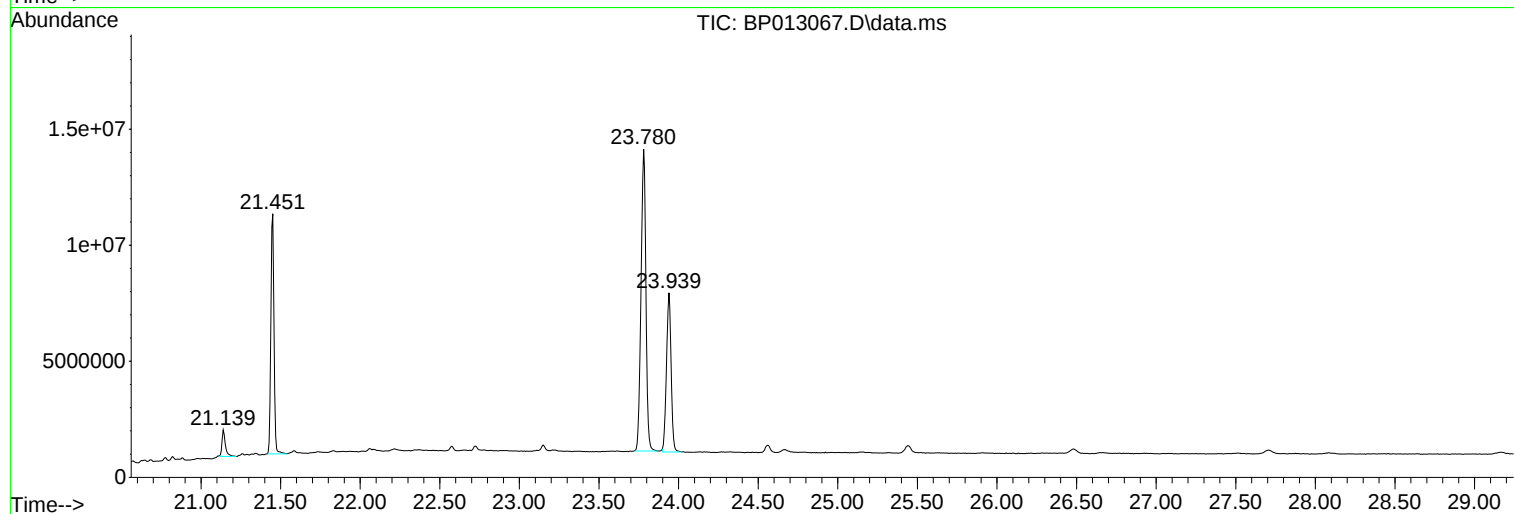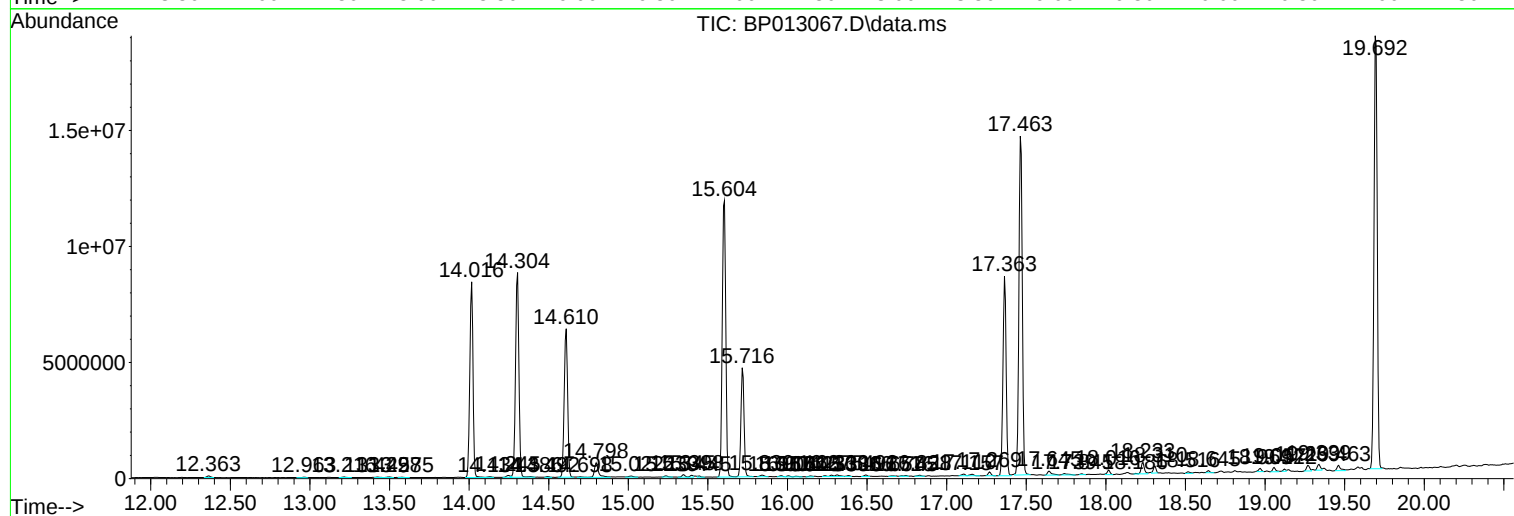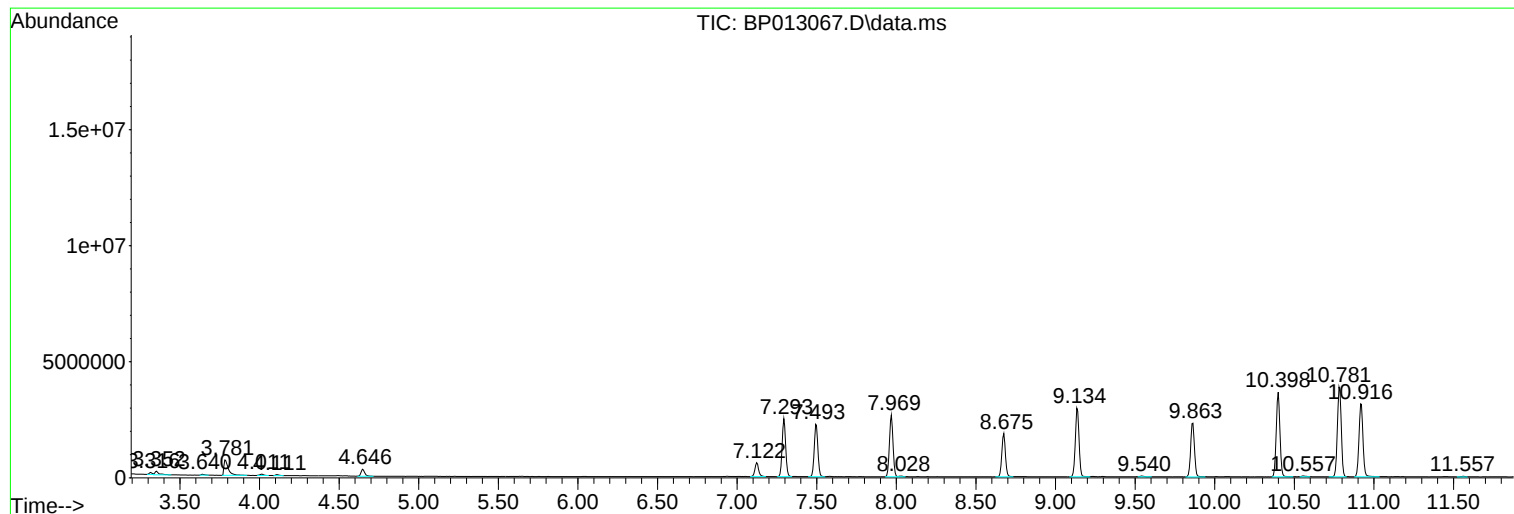

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013067.D
Acq On : 11 Dec 2022 07:13
Operator : CG/JU
Sample : N5927-10
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ98










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.646	2.34 ng/ul	489217	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	94
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	35

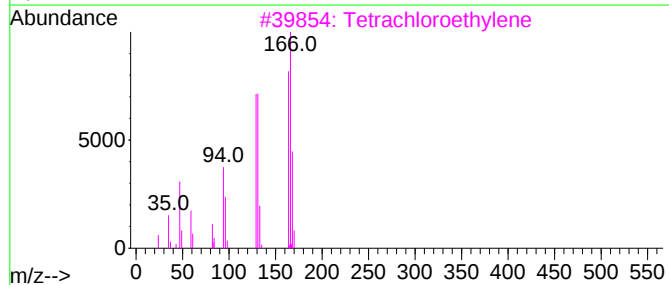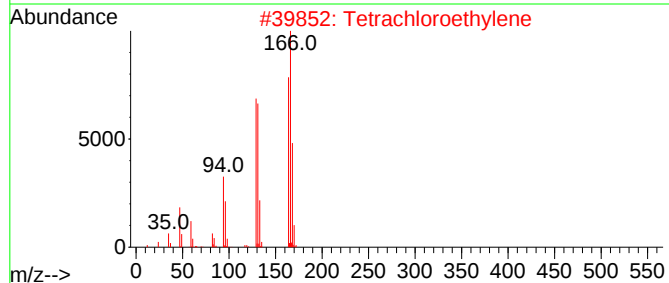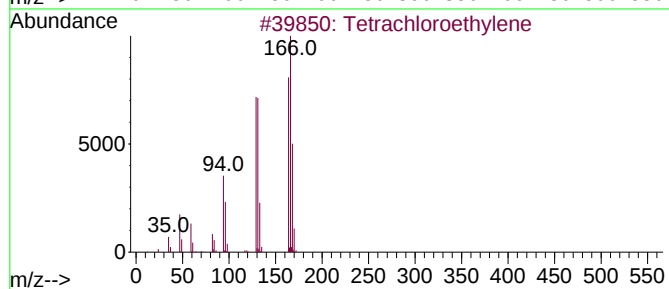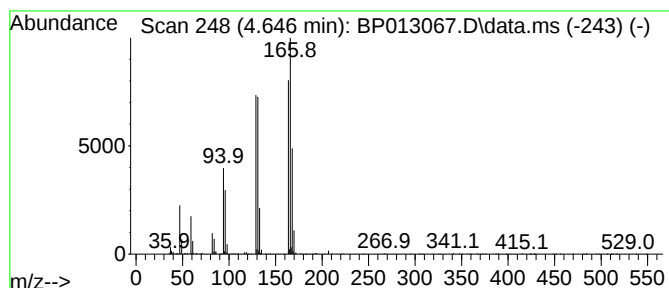

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013067.D
Acq On : 11 Dec 2022 07:13
Operator : CG/JU
Sample : N5927-10
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ98










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Fumaric acid, 2-chloropropyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.139	2.35 ng/ul	1637260	Chrysene-d12	21.451

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fumaric acid, 2-chloropropyl tri...	374	C20H35ClO4	1010348-57-1	98
2			1-Heneicosyl formate	340	C22H44O2	077899-03-7	97
3			1-Nonadecene	266	C19H38	018435-45-5	95
4			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
5			1-Hexacosene	364	C26H52	018835-33-1	94

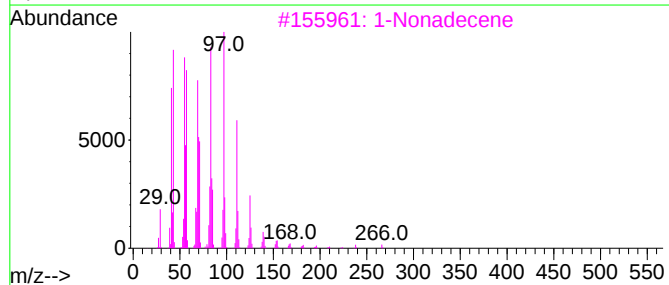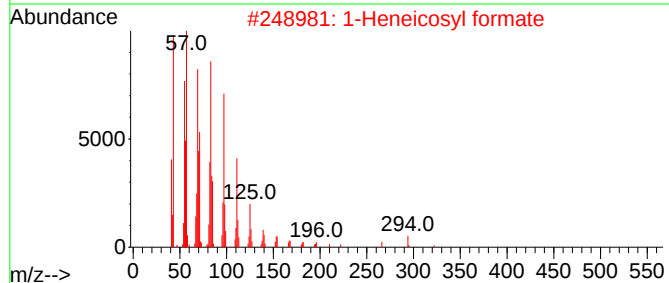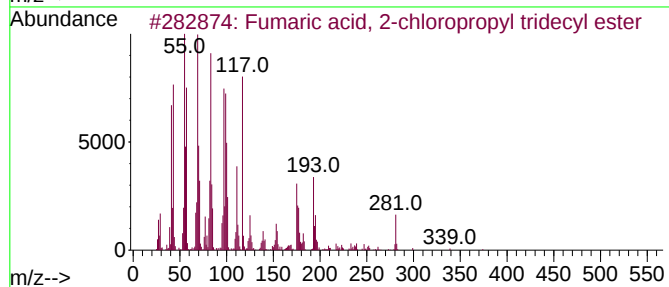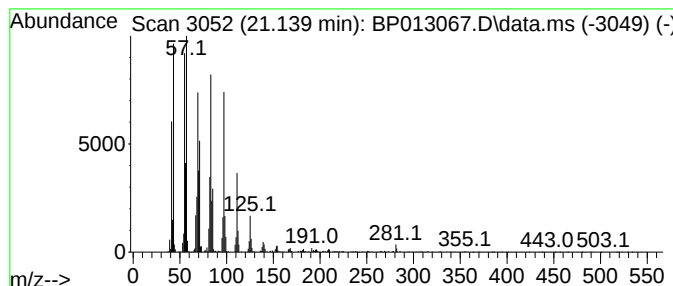

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013067.D
Acq On : 11 Dec 2022 07:13
Operator : CG/JU
Sample : N5927-10
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXZ98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.646	2.3	ng/ul	489217	1	7.969	4178410	20.0
Fumaric acid, 2...	21.139	2.4	ng/ul	1637260	5	21.451	13918200	20.0