

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
 Data File : BP013074.D
 Acq On : 11 Dec 2022 11:12
 Operator : CG/JU
 Sample : PB149495BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK495

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	24	28	39	rVB	164225	236478	1.41%	0.145%
2	3.775	97	100	117	rBV	2041201	3308278	19.77%	2.035%
3	4.111	153	157	164	rVB	33791	48027	0.29%	0.030%
4	7.122	662	669	682	rBV	2721346	4237415	25.33%	2.607%
5	7.293	691	698	711	rVB	2265413	3487483	20.84%	2.145%
6	7.493	725	732	747	rBV	2714430	4369680	26.12%	2.688%
7	7.969	806	813	821	rBV	1945866	3076200	18.39%	1.892%
8	8.675	924	933	948	rBV	3400044	5403773	32.30%	3.324%
9	9.134	998	1011	1027	rBV	2624034	4307705	25.75%	2.650%
10	9.857	1126	1134	1149	rBV	2217919	3638552	21.75%	2.238%
11	10.398	1218	1226	1237	rBV	3458051	5774563	34.51%	3.552%
12	10.781	1280	1291	1300	rBV	2821259	4662320	27.87%	2.868%
13	10.916	1307	1314	1335	rBV	3212996	5462056	32.65%	3.360%
14	11.569	1419	1425	1429	rBV9	9245	17962	0.11%	0.011%
15	12.363	1554	1560	1567	rVB2	62220	95568	0.57%	0.059%
16	13.498	1745	1753	1758	rBV2	20750	34115	0.20%	0.021%
17	13.575	1761	1766	1774	rVB7	10534	20756	0.12%	0.013%
18	14.016	1834	1841	1854	rVB	6138470	8651020	51.71%	5.322%
19	14.304	1882	1890	1901	rBV	6836388	10417672	62.27%	6.409%
20	14.610	1934	1942	1953	rBV	4324611	6533049	39.05%	4.019%
21	14.798	1967	1974	1989	rBV	2535474	3928972	23.48%	2.417%
22	15.010	2006	2010	2015	rVB7	12983	23232	0.14%	0.014%
23	15.604	2103	2111	2121	rBV	8989292	13060654	78.06%	8.034%
24	15.716	2124	2130	2142	rBV	2903035	3830686	22.90%	2.356%
25	15.839	2147	2151	2157	rVB2	45462	69770	0.42%	0.043%
26	16.386	2241	2244	2249	rVB5	11437	19578	0.12%	0.012%
27	17.039	2348	2355	2360	rVB9	12257	23229	0.14%	0.014%
28	17.363	2403	2410	2420	rBV	5788151	8001569	47.83%	4.922%
29	17.463	2420	2427	2440	rBV2	10146062	14398229	86.06%	8.857%
30	19.269	2729	2734	2741	rBV2	132491	196590	1.18%	0.121%
31	19.333	2741	2745	2750	rBV	120884	165169	0.99%	0.102%
32	19.692	2800	2806	2822	rBV	12825869	16730628	100.00%	10.292%
33	21.445	3099	3104	3112	rBV	5475381	7522420	44.96%	4.627%
34	23.774	3492	3500	3516	rBV	6542448	13922964	83.22%	8.565%
35	23.933	3520	3527	3542	rVB2	3351175	6882721	41.14%	4.234%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013074.D
Acq On : 11 Dec 2022 11:12
Operator : CG/JU
Sample : PB149495BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK495

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Title : SVOA CALIBRATION




Sum of corrected areas: 162559083

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013074.D
Acq On : 11 Dec 2022 11:12
Operator : CG/JU
Sample : PB149495BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

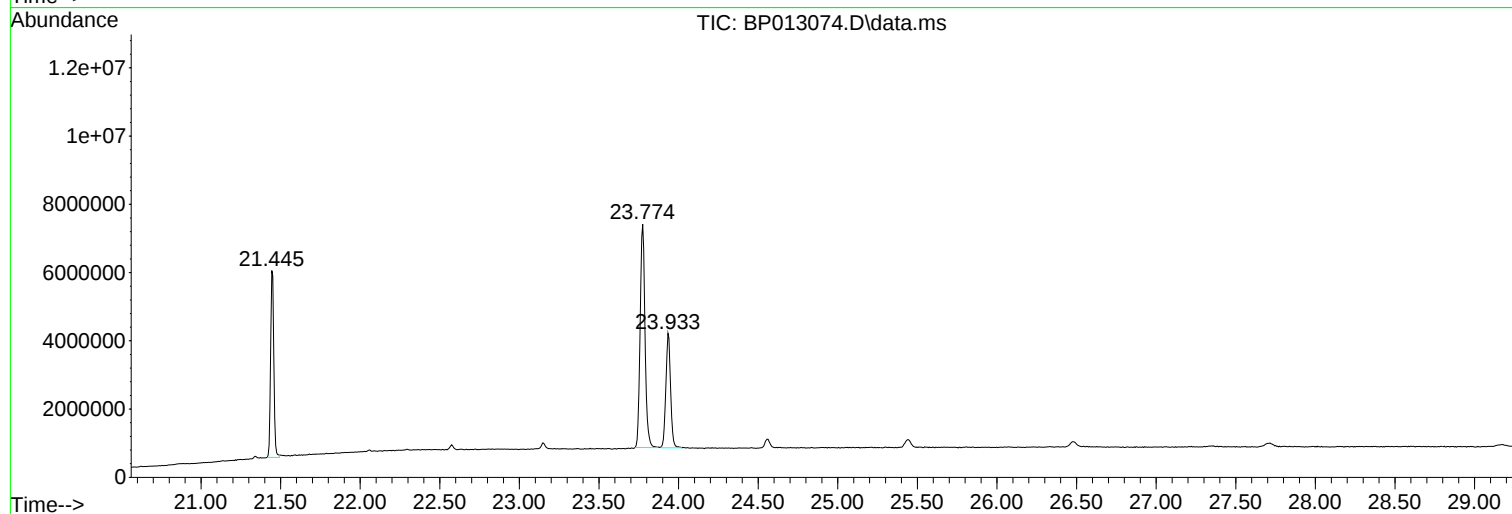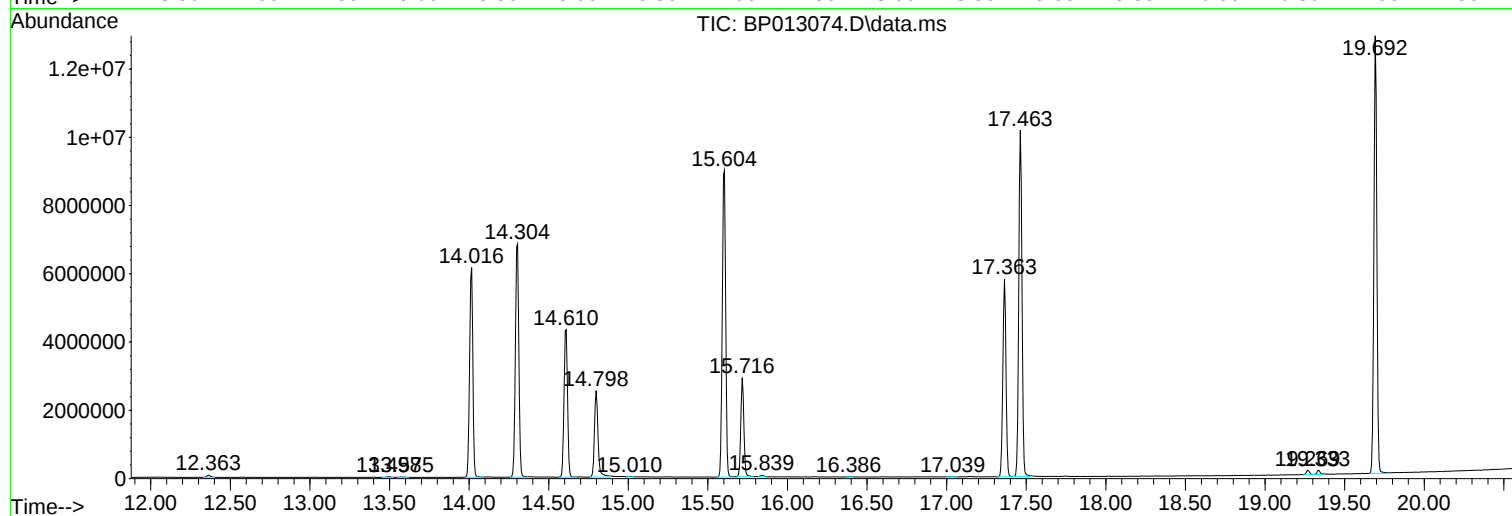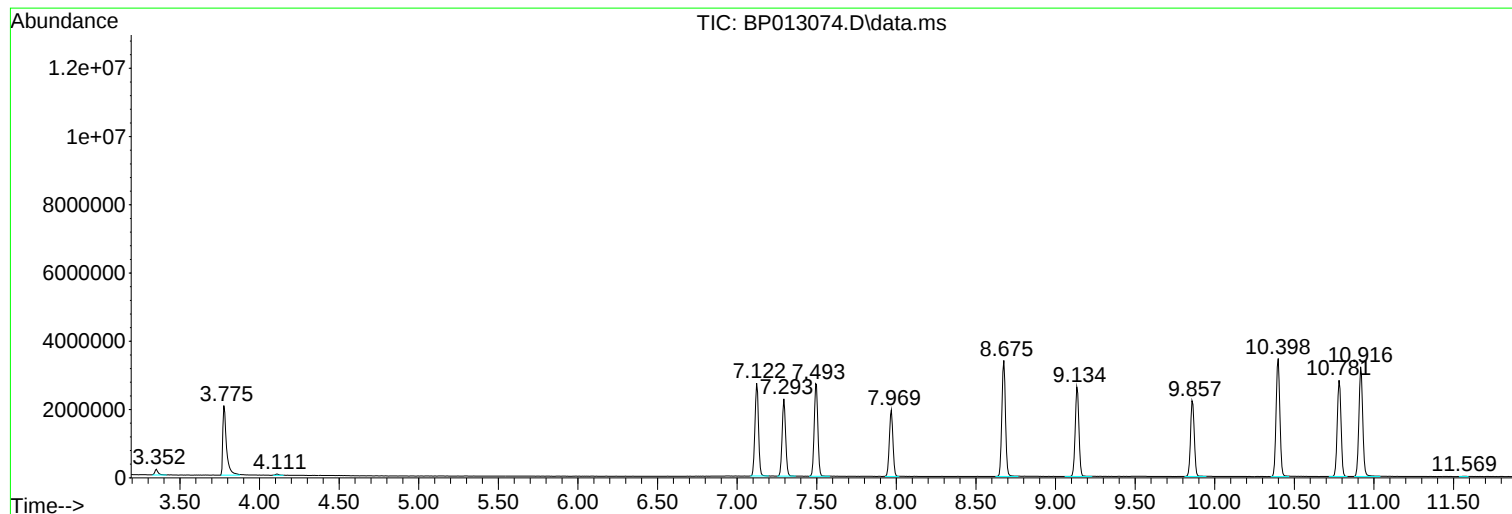

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013074.D
Acq On : 11 Dec 2022 11:12
Operator : CG/JU
Sample : PB149495BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121022\
Data File : BP013074.D
Acq On : 11 Dec 2022 11:12
Operator : CG/JU
Sample : PB149495BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK495

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc