

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121024\
 Data File : BP023360.D
 Acq On : 11 Dec 2024 00:39
 Operator : RC/JU
 Sample : P5111-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG450

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.069	10	14	18	rBV	51813	75986	3.03%	0.365%
2	3.105	18	20	24	rVB	21563	23025	0.92%	0.111%
3	3.534	90	93	109	rBV	36103	84558	3.37%	0.406%
4	3.828	139	143	147	rBV3	5528	8833	0.35%	0.042%
5	4.252	210	215	222	rVB2	10892	16831	0.67%	0.081%
6	4.334	222	229	239	rBV	132806	203880	8.13%	0.980%
7	4.728	292	296	299	rBV5	2107	3461	0.14%	0.017%
8	4.769	299	303	308	rVV8	2383	4843	0.19%	0.023%
9	6.681	623	628	634	rVB2	6163	9811	0.39%	0.047%
10	6.763	637	642	658	rBV	39026	118527	4.72%	0.569%
11	6.893	658	664	674	rVV	242544	384454	15.32%	1.847%
12	7.093	690	698	718	rBV	260419	471653	18.80%	2.266%
13	7.540	768	774	793	rBV	283326	498724	19.88%	2.396%
14	8.257	888	896	916	rBV	160731	366450	14.61%	1.761%
15	8.687	963	969	987	rBV	284561	540324	21.54%	2.596%
16	9.069	1028	1034	1038	rVB4	4359	7330	0.29%	0.035%
17	9.398	1083	1090	1110	rBV	219930	470518	18.75%	2.261%
18	9.940	1175	1182	1205	rBV	250203	647566	25.81%	3.111%
19	10.281	1233	1240	1252	rVB	357561	608039	24.23%	2.921%
20	10.451	1262	1269	1297	rBV	170127	475707	18.96%	2.286%
21	11.545	1448	1455	1459	rBV6	3024	4919	0.20%	0.024%
22	11.934	1513	1521	1524	rBV7	3861	6497	0.26%	0.031%
23	13.004	1698	1703	1714	rVB2	22392	37708	1.50%	0.181%
24	13.575	1791	1800	1816	rBV	609259	1087411	43.34%	5.225%
25	13.839	1835	1845	1864	rBV	628069	1063978	42.41%	5.112%
26	14.151	1891	1898	1908	rBV	552061	822938	32.80%	3.954%
27	14.516	1955	1960	1968	rBV6	12491	37570	1.50%	0.181%
28	14.975	2033	2038	2042	rBV7	1818	3017	0.12%	0.014%
29	15.033	2042	2048	2050	rVB6	1900	3524	0.14%	0.017%
30	15.163	2064	2070	2085	rBV	991288	1485847	59.22%	7.139%
31	15.339	2093	2100	2113	rBV	237569	500241	19.94%	2.403%
32	15.557	2131	2137	2148	rVV	33035	57350	2.29%	0.276%
33	15.804	2174	2179	2183	rBV4	3244	5066	0.20%	0.024%
34	16.133	2229	2235	2238	rBV7	2198	4676	0.19%	0.022%
35	16.433	2280	2286	2292	rVB10	1872	3135	0.12%	0.015%
36	16.757	2339	2341	2346	rVB6	2355	3483	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121024\
 Data File : BP023360.D
 Acq On : 11 Dec 2024 00:39
 Operator : RC/JU
 Sample : P5111-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BG450

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

37	16.833	2350	2354	2360	rVV8	1550	3450	0.14%	0.017%
38	16.963	2369	2376	2387	rBV	699222	1062820	42.36%	5.106%
39	17.069	2387	2394	2413	rVV	986803	1754549	69.93%	8.430%
40	17.498	2461	2467	2470	rBV7	1741	3671	0.15%	0.018%
41	17.651	2490	2493	2500	rVB9	2977	5166	0.21%	0.025%
42	17.904	2531	2536	2542	rBV2	35664	58631	2.34%	0.282%
43	18.204	2584	2587	2592	rVB7	2522	3453	0.14%	0.017%
44	18.351	2609	2612	2615	rVB4	3720	4379	0.17%	0.021%
45	18.774	2679	2684	2690	rVV10	4930	10849	0.43%	0.052%
46	19.004	2719	2723	2729	rBV3	16237	21523	0.86%	0.103%
47	19.080	2732	2736	2740	rBV	17570	24666	0.98%	0.119%
48	19.245	2760	2764	2768	rBV6	12818	20889	0.83%	0.100%
49	19.451	2794	2799	2814	rBV	1672080	2283943	91.03%	10.974%
50	21.398	3124	3130	3143	rBV2	732374	1352423	53.90%	6.498%
51	24.351	3623	3632	3649	rVB	955153	2508968	100.00%	12.055%
52	24.580	3662	3671	3689	rBV	514973	1545877	61.61%	7.427%




Sum of corrected areas: 20813137

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121024\
Data File : BP023360.D
Acq On : 11 Dec 2024 00:39
Operator : RC/JU
Sample : P5111-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG450

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

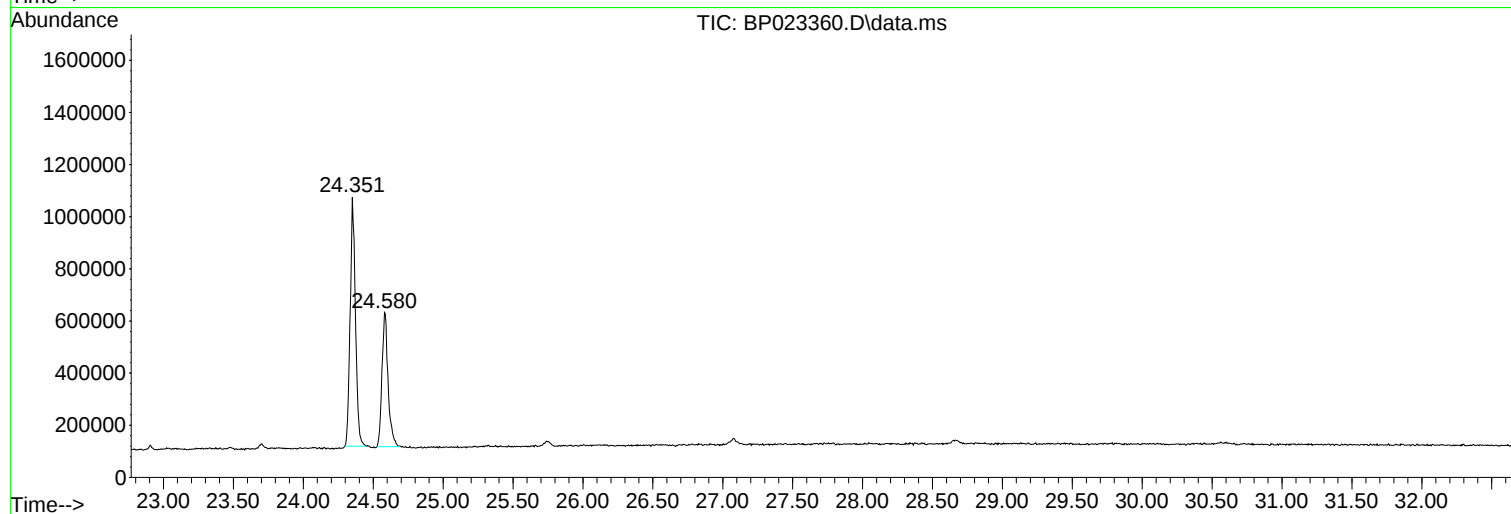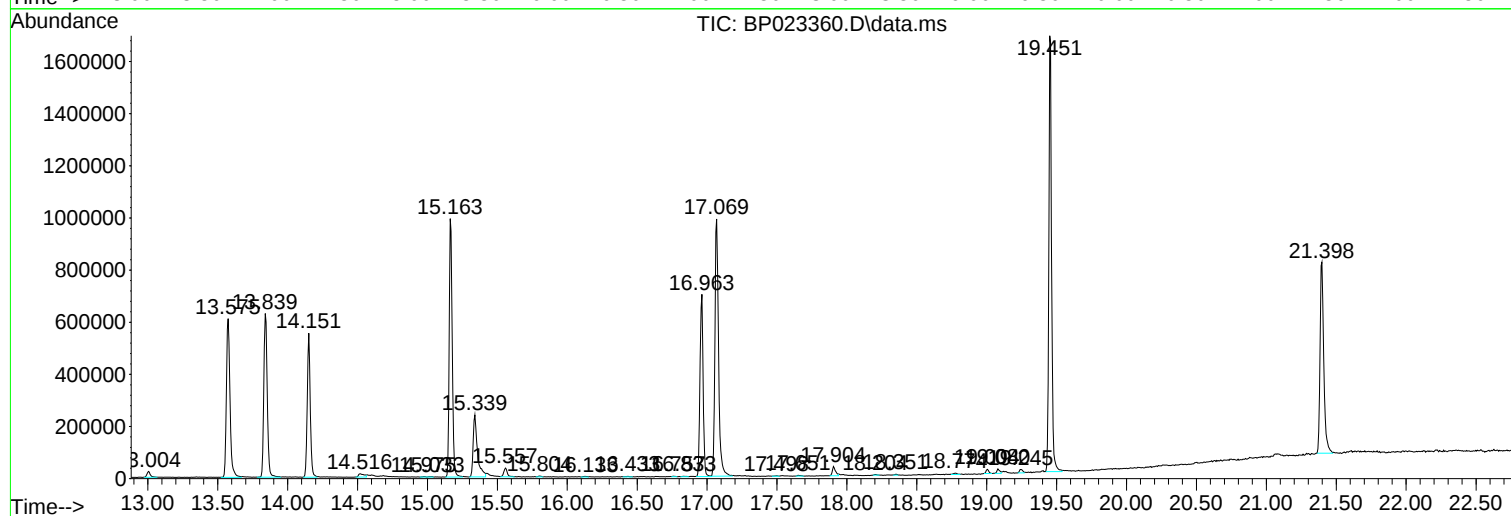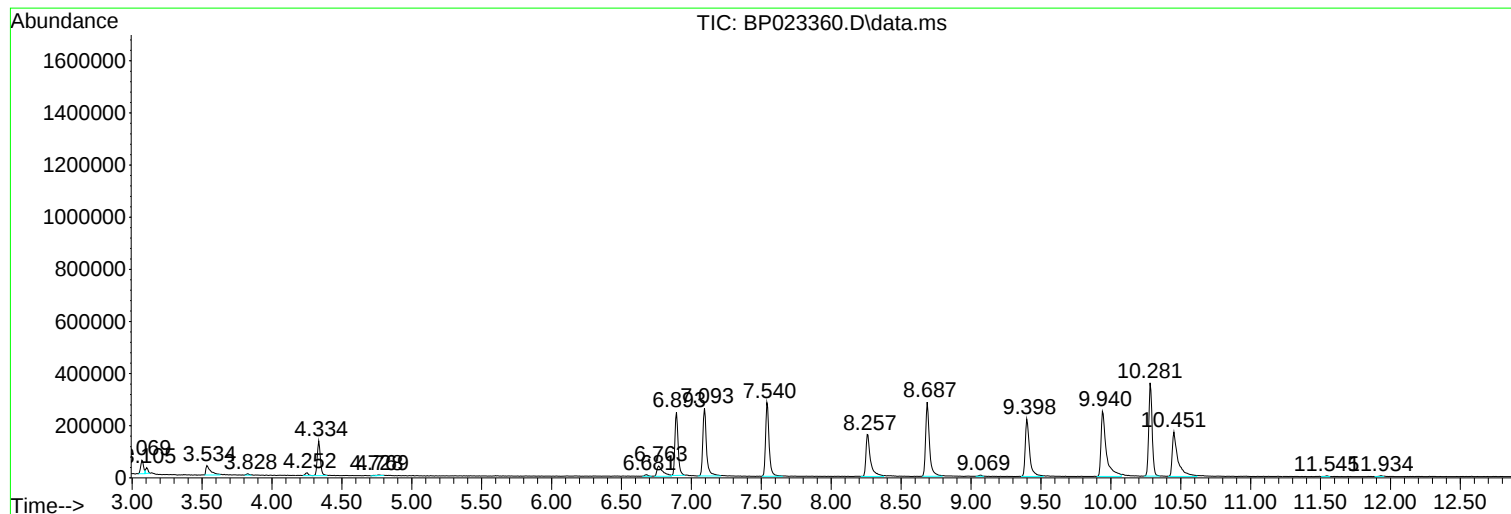

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121024\
Data File : BP023360.D
Acq On : 11 Dec 2024 00:39
Operator : RC/JU
Sample : P5111-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG450

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121024\
Data File : BP023360.D
Acq On : 11 Dec 2024 00:39
Operator : RC/JU
Sample : P5111-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BG450

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc