

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121119\
 Data File : BP001312.D
 Acq On : 11 Dec 2019 15:25
 Operator : JU
 Sample : K6204-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 K072-AB-WC-1

Quant Time: Dec 12 06:39:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 05 12:34:47 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.31	152	68085	20.00	ng	0.00
21) Naphthalene-d8	10.34	136	249224	20.00	ng	-0.01
39) Acenaphthene-d10	13.20	164	149088	20.00	ng	-0.01
64) Phenanthrene-d10	15.60	188	297479	20.00	ng	-0.01
76) Chrysene-d12	19.24	240	199798	20.00	ng	-0.02
87) Perylene-d12	21.01	264	172312	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.23	112	551984	134.51	ng	0.02
7) Phenol-d6	7.76	99	674314	123.34	ng	0.00
23) Nitrobenzene-d5	9.19	82	599763	104.41	ng	0.00
42) 2,4,6-Tribromophenol	14.50	330	262356	183.59	ng	0.00
45) 2-Fluorobiphenyl	12.12	172	1098635	107.85	ng	-0.01
79) Terphenyl-d14	17.89	244	1349596	124.97	ng	0.00
Target Compounds						
9) Benzaldehyde	7.62	77	320	Below Cal		Qvalue # 68
15) Benzyl Alcohol	8.55	79	12077	2.691 ng	#	58
19) n-Nitroso-di-n-propylamine	9.19	70	89345	22.647 ng	#	78
54) 2,4-Dinitrophenol	13.30	184	10	7.118 ng		99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121119\
Data File : BP001312.D
Acq On : 11 Dec 2019 15:25
Operator : JU
Sample : K6204-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
K072-AB-WC-1

Quant Time: Dec 12 06:39:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 05 12:34:47 2019
Response via : Initial Calibration

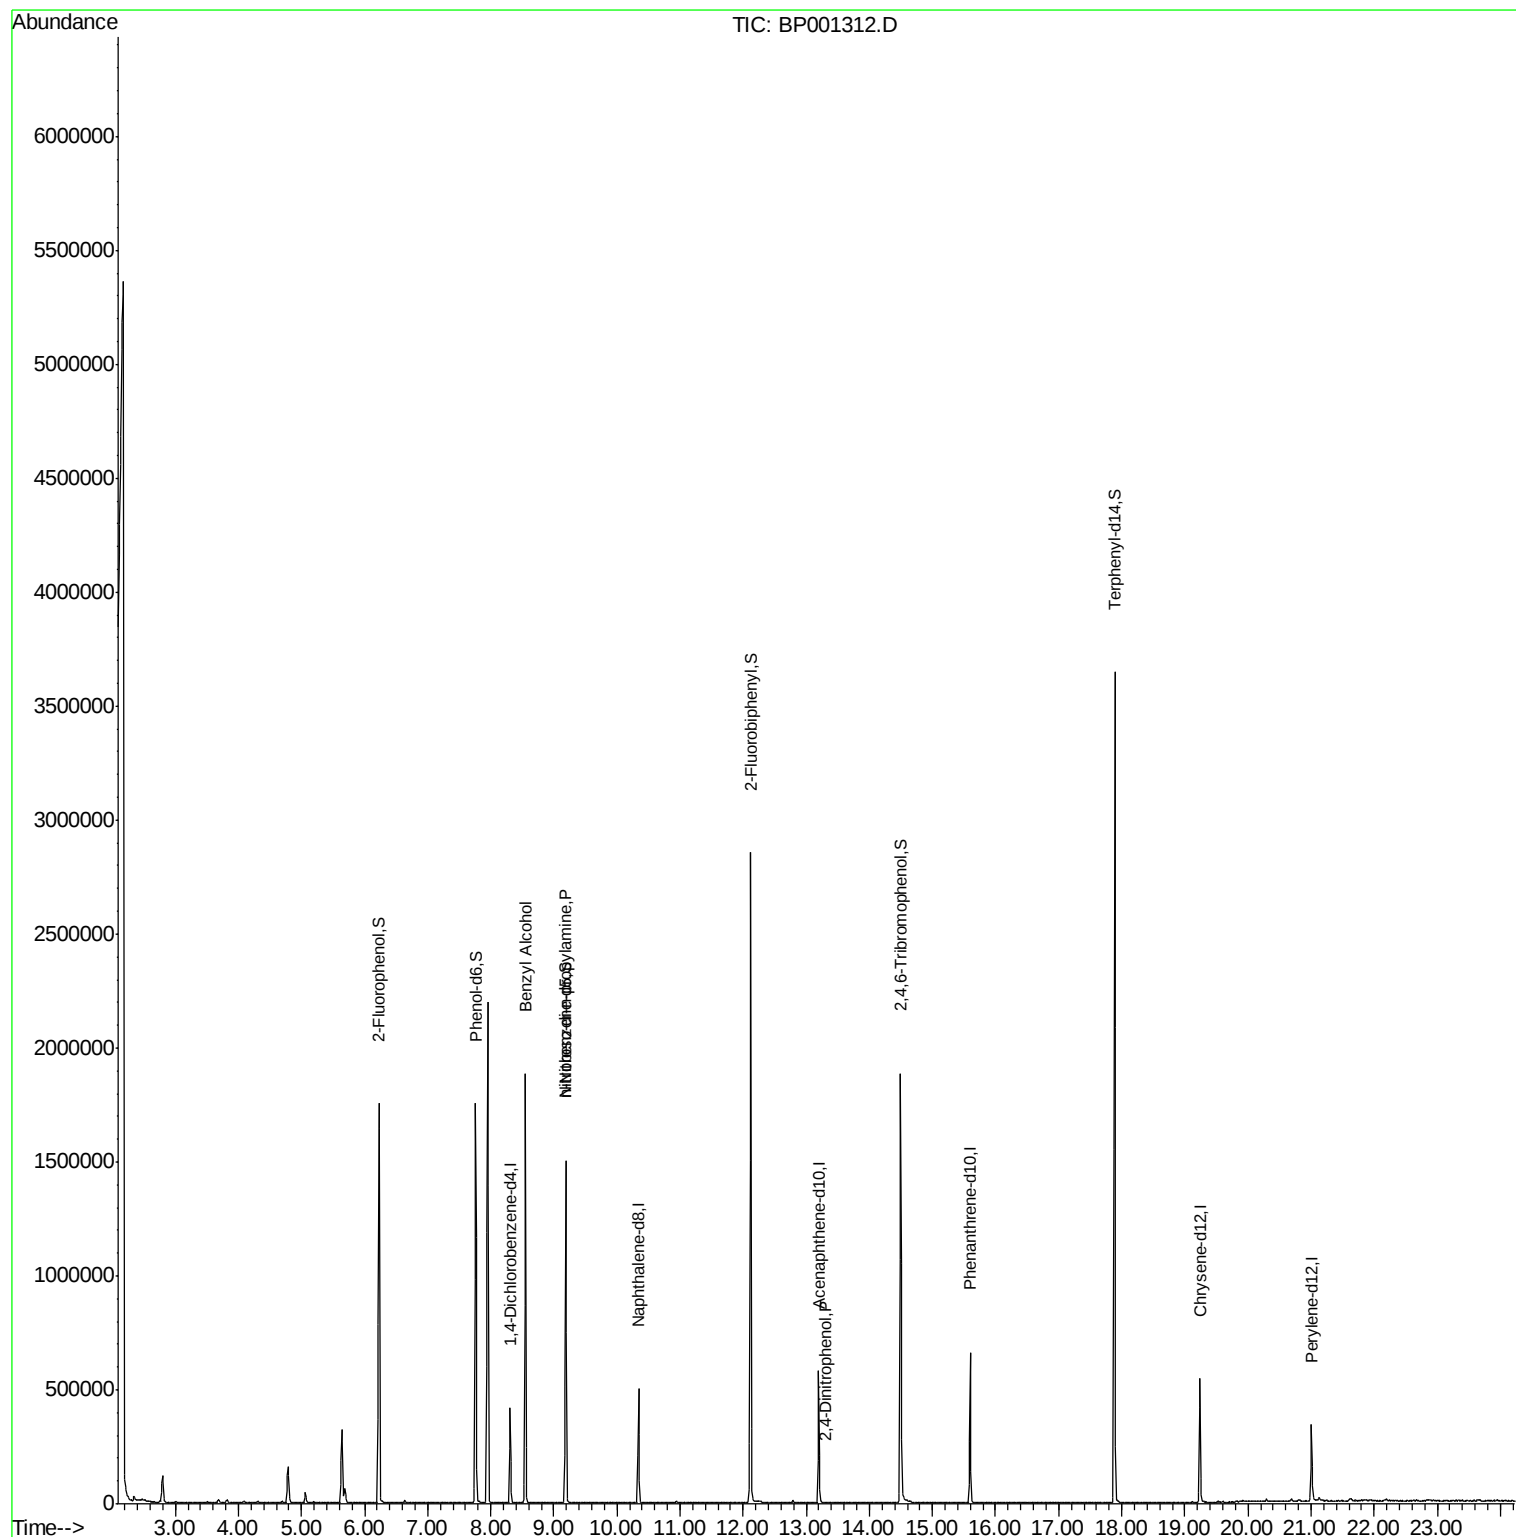

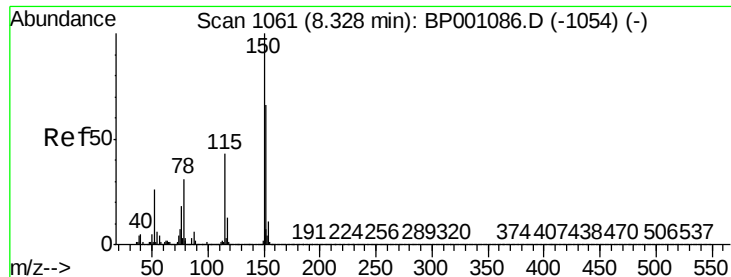

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.31 min Scan# 1058

Delta R.T. 0.00 min

Lab File: BP001312.D

Acq: 11 Dec 2019 15:25

Instrument :

BNA_P

ClientSampleId :

K072-AB-WC-1


Tot Ion:152 Resp: 68085

Ion Ratio Lower Upper

152 100

150 151.1 127.3 190.9




115 66.5 56.0 84.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

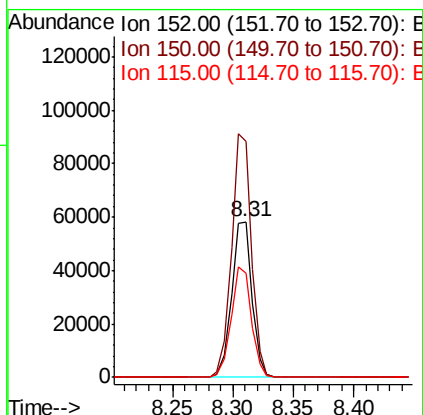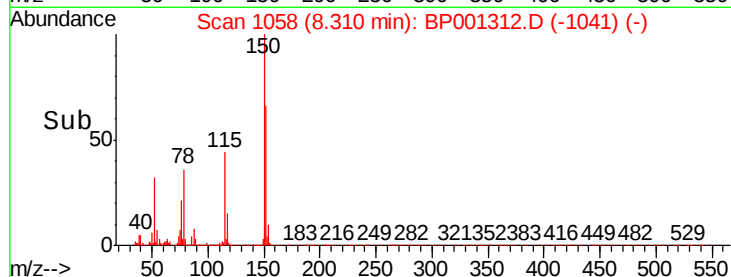

#5

2-Fluorophenol

Concen: 134.506 ng

RT: 6.23 min Scan# 704

Delta R.T. 0.02 min

Lab File: BP001312.D

Acq: 11 Dec 2019 15:25


Tgt Ion:112 Resp: 551984

Ion Ratio Lower Upper

112 100

64 71.3 56.8 85.2



63 43.3 32.2 48.2




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

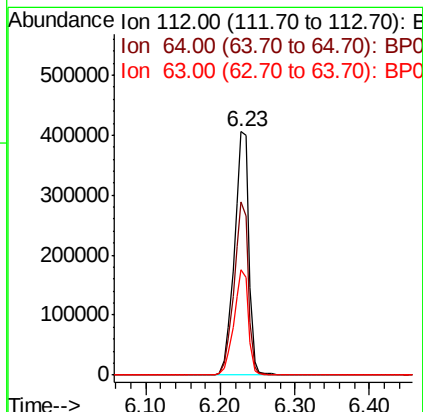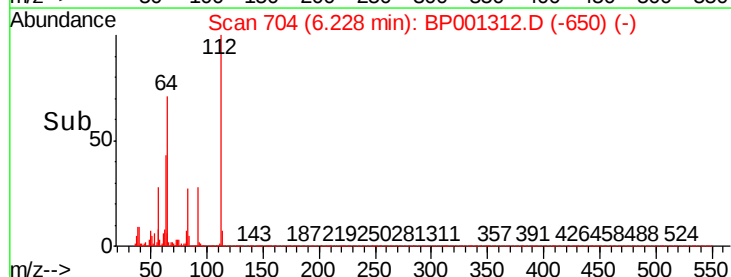

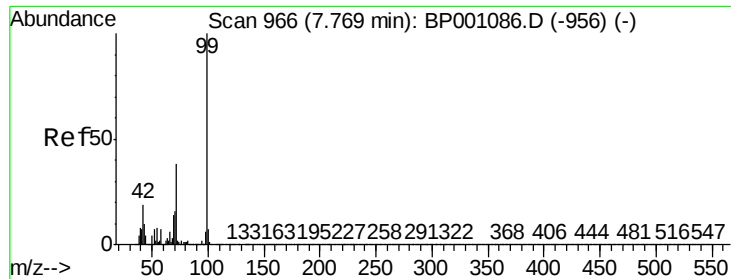

#7

Phenol-d6

Concen: 123.337 ng

RT: 7.76 min Scan# 965

Delta R.T. 0.00 min

Lab File: BP001312.D

Acq: 11 Dec 2019 15:25

Instrument :

BNA_P

ClientSampleId :

K072-AB-WC-1


Tot Ion: 99 Resp: 674314

Ion Ratio Lower Upper

99 100

42 24.3 17.6 26.4




71 48.0 33.8 50.8

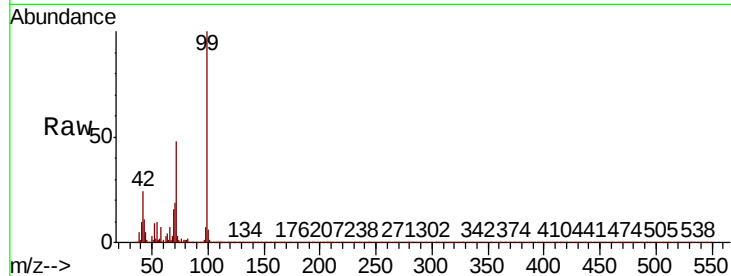

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

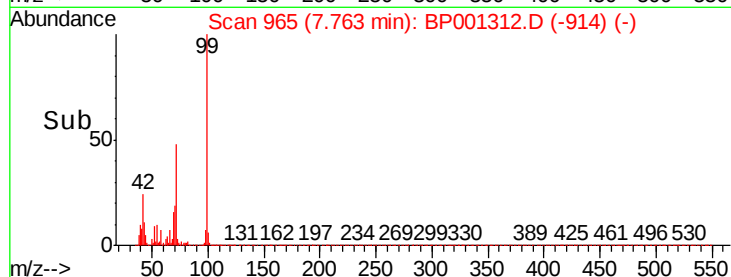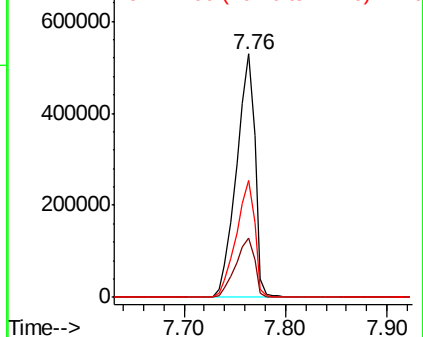

#9

Benzaldehyde

Concen: Below Cal

RT: 7.62 min Scan# 940

Delta R.T. 0.01 min

Lab File: BP001312.D

Acq: 11 Dec 2019 15:25


Tgt Ion: 77 Resp: 320

Ion Ratio Lower Upper

77 100

105 111.8 69.7 109.7#



106 125.1 67.1 107.1#




Abundance Ion 77.00 (76.70 to 77.70): BP0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E



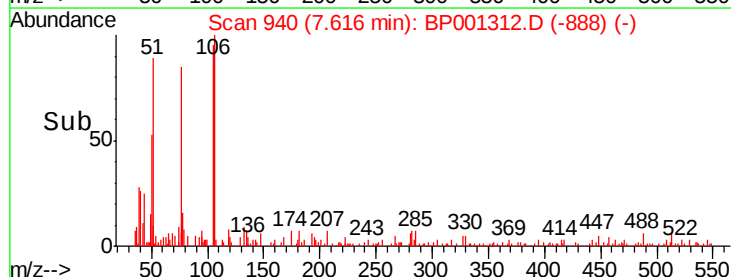
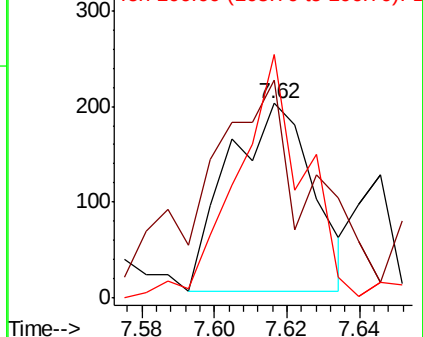


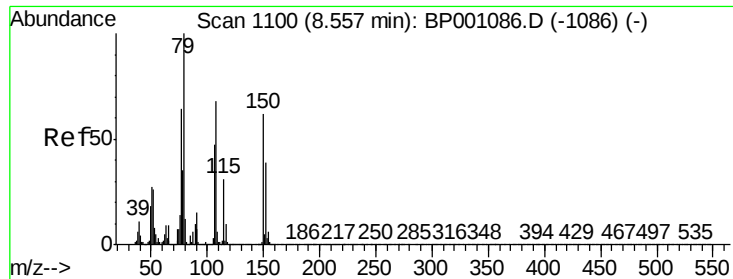

#15
Benzyl Alcohol
Concen: 2.691 ng
RT: 8.55 min Scan# 1099
Delta R.T. 0.01 min
Lab File: BP001312.D
Acq: 11 Dec 2019 15:25




Instrument :
BNA_P
ClientSampled :
K072-AB-WC-1


Tot Ion: 79 Resp: 12077
Ion Ratio Lower Upper
79 100
108 33.4 51.6 77.4#
77 102.8 53.5 80.3#

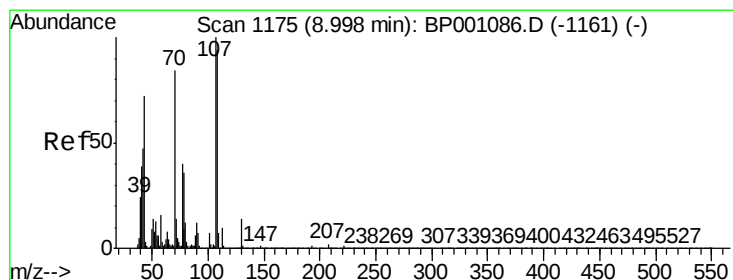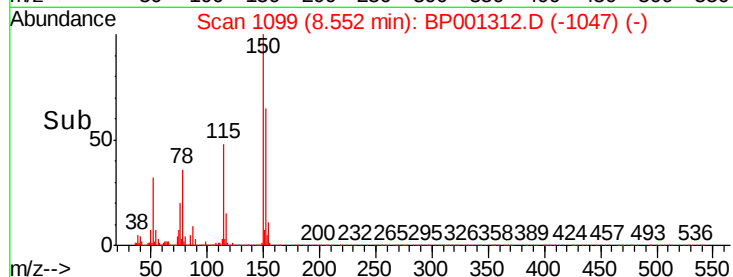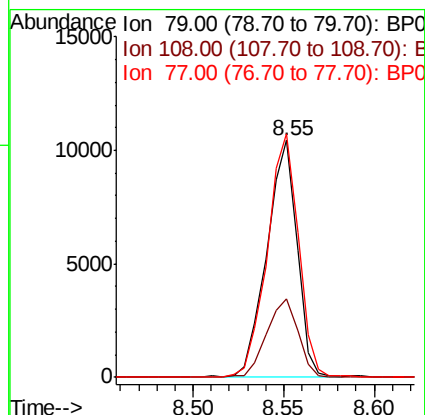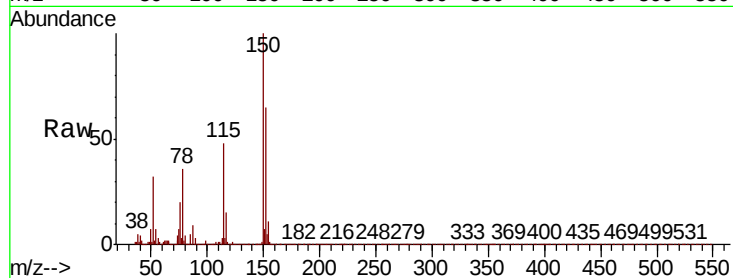

#19
n-Nitroso-di-n-propylamine
Concen: 22.647 ng
RT: 9.19 min Scan# 1208
Delta R.T. 0.21 min
Lab File: BP001312.D
Acq: 11 Dec 2019 15:25

Tgt Ion: 70 Resp: 89345
Ion Ratio Lower Upper
70 100
42 49.9 50.6 76.0#
101 0.0 7.1 10.7#
130 1.2 13.6 20.4#


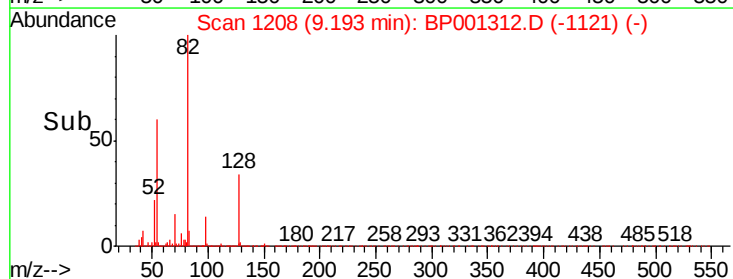
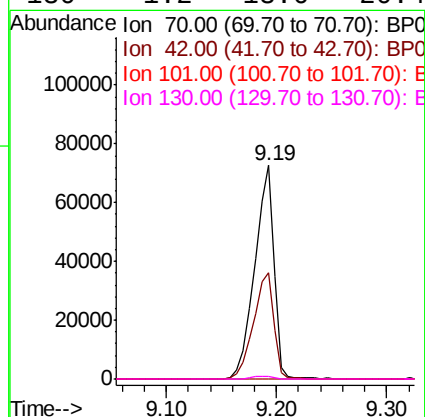
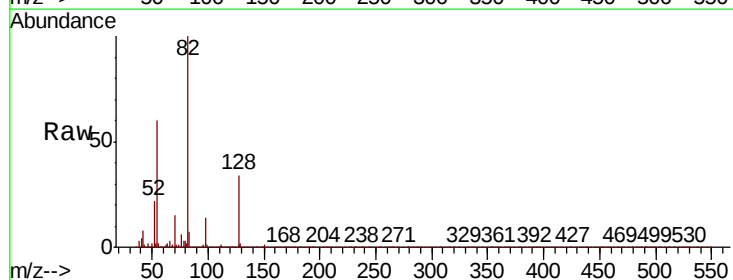


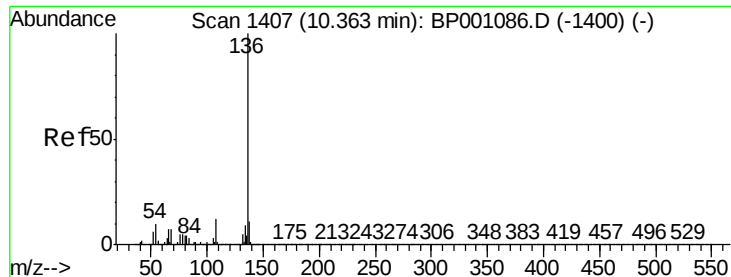

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.34 min Scan# 1403
Delta R.T. -0.01 min
Lab File: BP001312.D
Acq: 11 Dec 2019 15:25




Instrument :
BNA_P
ClientSampleId :
K072-AB-WC-1


Tot Ion:136	Resp:	249224
Ion Ratio	Lower	Upper
136 100		
137 10.7	8.4	12.6
54 9.6	7.4	11.0
68 5.2	4.6	7.0

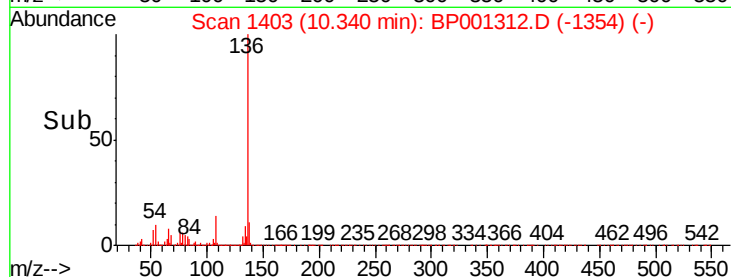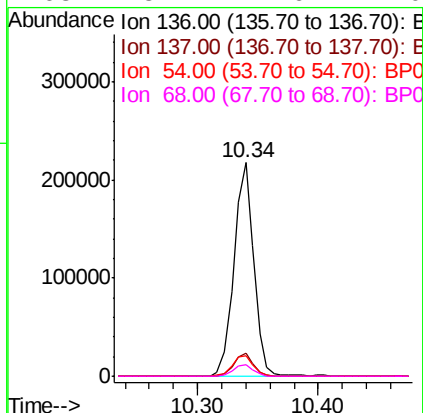

#23
Nitrobenzene-d5
Concen: 104.409 ng
RT: 9.19 min Scan# 1208
Delta R.T. -0.01 min
Lab File: BP001312.D
Acq: 11 Dec 2019 15:25

Tgt	Ion: 82	Resp:	599763
Ion	Ratio	Lower	Upper
82	100		
128	34.3	27.5	41.3
54	60.1	45.7	68.5

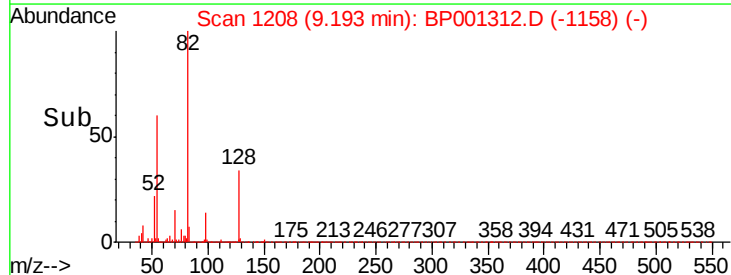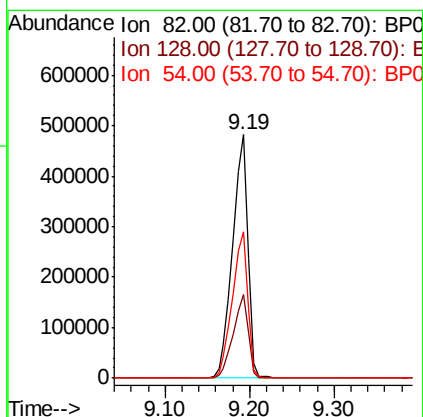

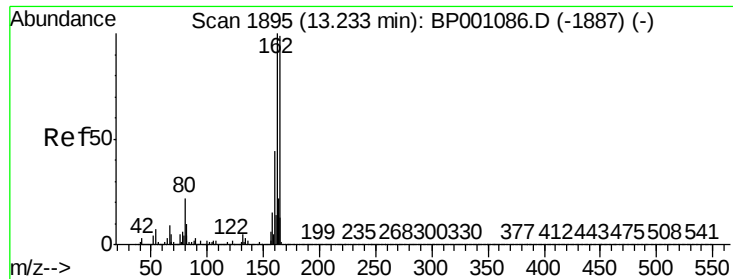

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 13.20 min Scan# 1889

Delta R.T. -0.01 min

Lab File: BP001312.D

Acq: 11 Dec 2019 15:25

Instrument :

BNA_P

ClientSampleId :

K072-AB-WC-1


Tot Ion:164 Resp: 149088

Ion Ratio Lower Upper

164 100

162 101.6 80.7 121.1




160 46.1 36.3 54.5

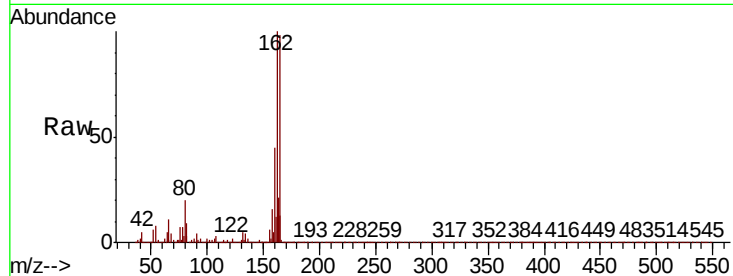

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

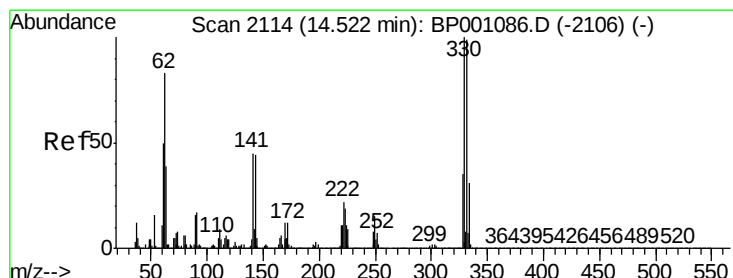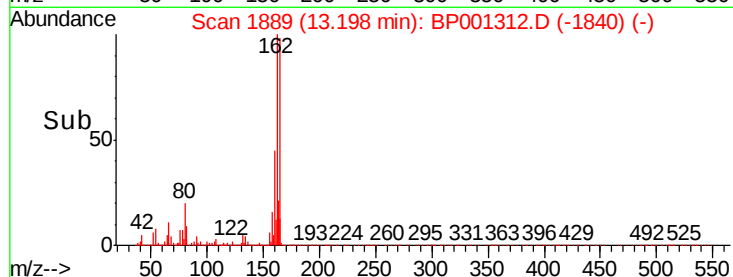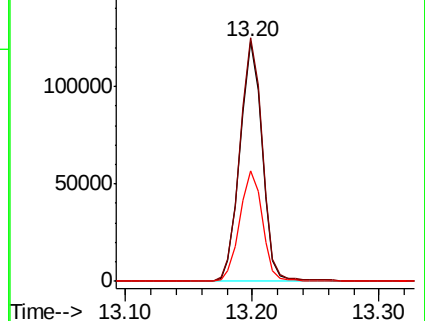

#42

2,4,6-Tribromophenol

Concen: 183.593 ng

RT: 14.50 min Scan# 2110

Delta R.T. -0.01 min

Lab File: BP001312.D

Acq: 11 Dec 2019 15:25


Tgt Ion:330 Resp: 262356

Ion Ratio Lower Upper

330 100

332 96.0 79.1 118.7



141 44.7 35.9 53.9

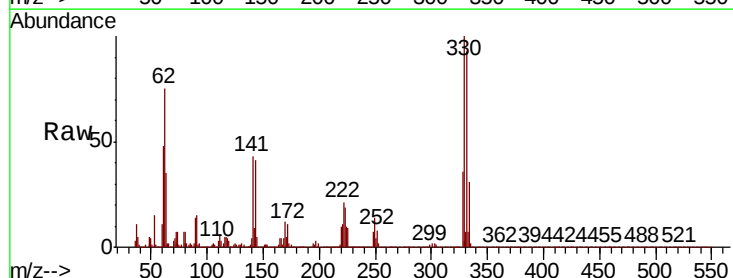


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



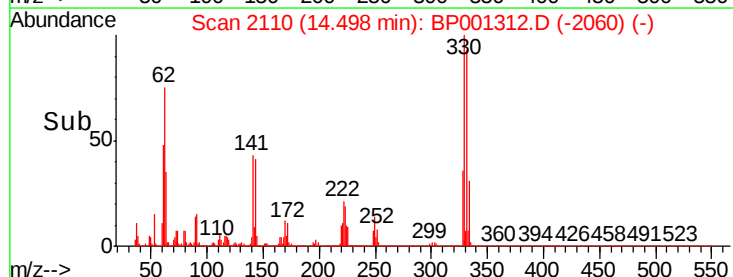
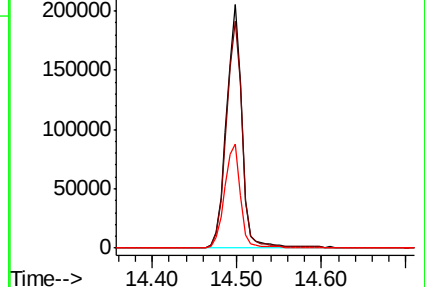


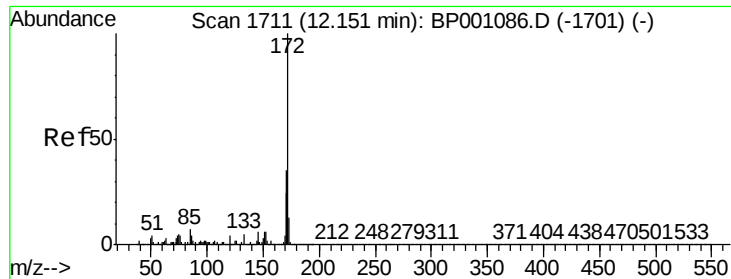

#45
2-Fluorobiphenyl
Concen: 107.851 ng
RT: 12.12 min Scan# 1706
Delta R.T. -0.01 min
Lab File: BP001312.D
Acq: 11 Dec 2019 15:25




Instrument :
BNA_P
ClientSampleId :
K072-AB-WC-1


Tot Ion:172 Resp: 1098635
Ion Ratio Lower Upper
172 100
171 35.0 28.7 43.1
170 23.4 19.2 28.8

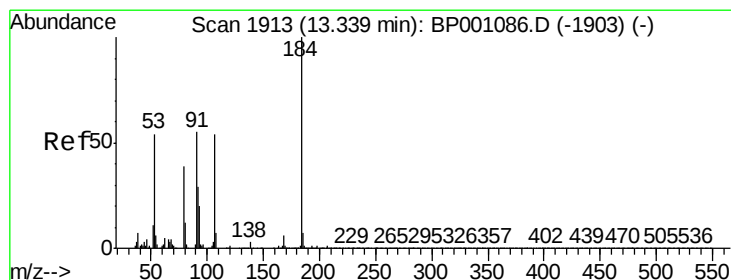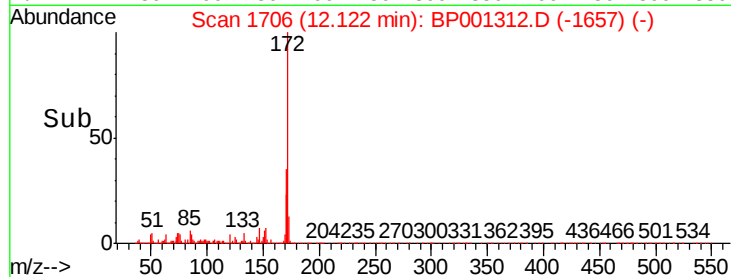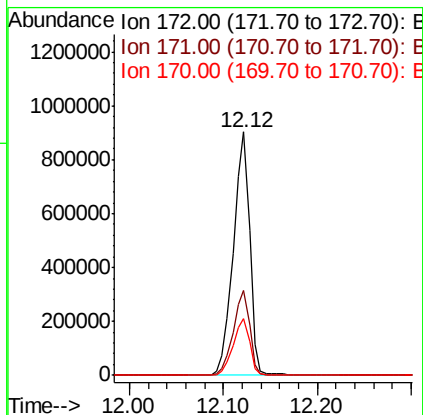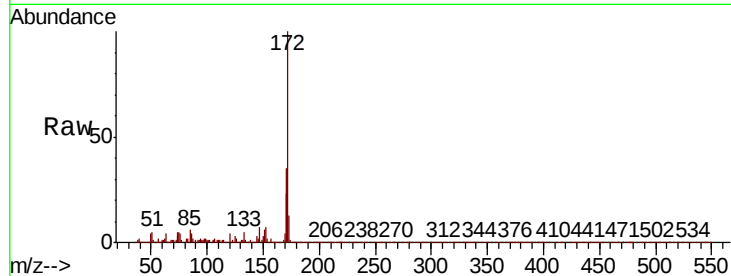

#54
2,4-Dinitrophenol
Concen: 7.118 ng
RT: 13.30 min Scan# 1907
Delta R.T. -0.02 min
Lab File: BP001312.D
Acq: 11 Dec 2019 15:25

Tgt Ion:184 Resp: 10
Ion Ratio Lower Upper
184 100
63 85.7 69.4 104.0
154 71.4 57.4 86.2


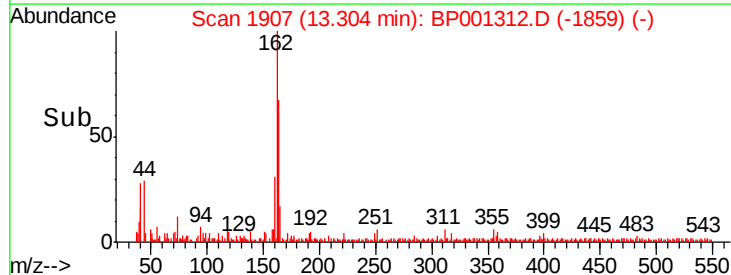
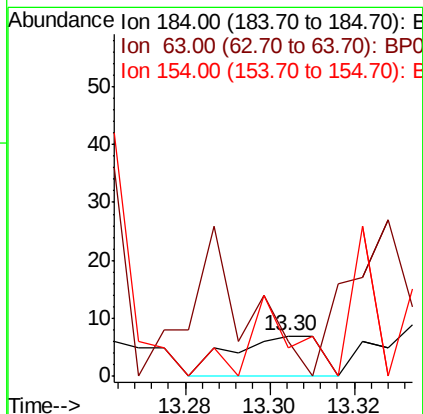



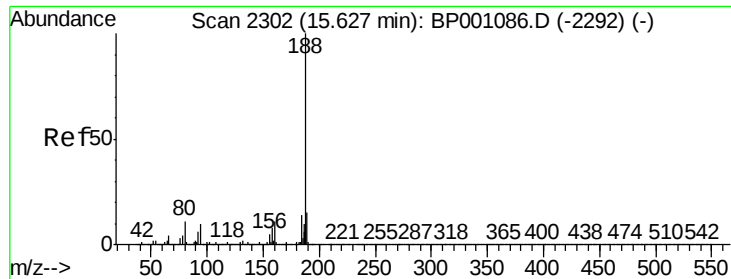

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 15.60 min Scan# 2297
Delta R.T. -0.01 min
Lab File: BP001312.D
Acq: 11 Dec 2019 15:25




Instrument :
BNA_P
ClientSampleId :
K072-AB-WC-1


Tot Ion	Ratio	Lower	Upper
188	100		
94	8.1	7.1	10.7
80	9.1	7.8	11.6

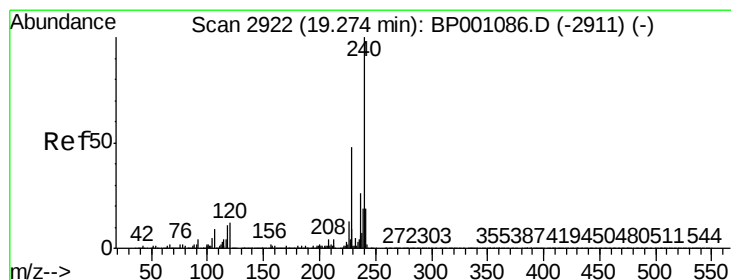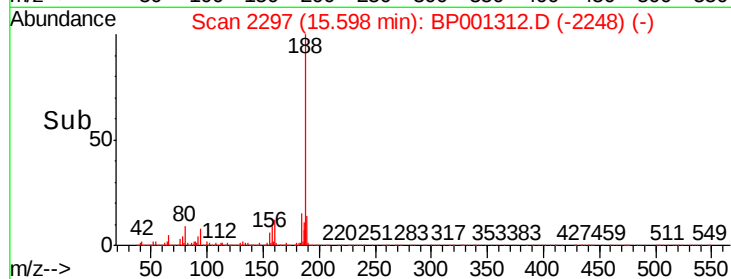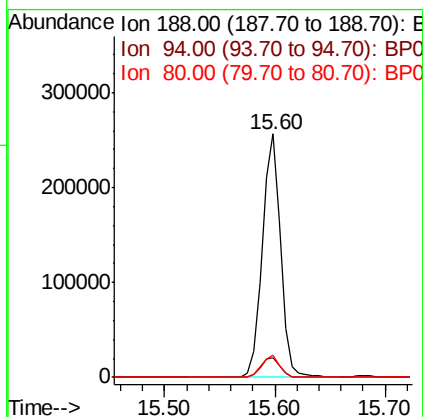

#76
Chrysene-d12
Concen: 20.000 ng
RT: 19.24 min Scan# 2916
Delta R.T. -0.02 min
Lab File: BP001312.D
Acq: 11 Dec 2019 15:25

Tgt Ion	Ratio	Lower	Upper
240	100		
120	8.0	7.0	10.6
236	26.9	21.7	32.5

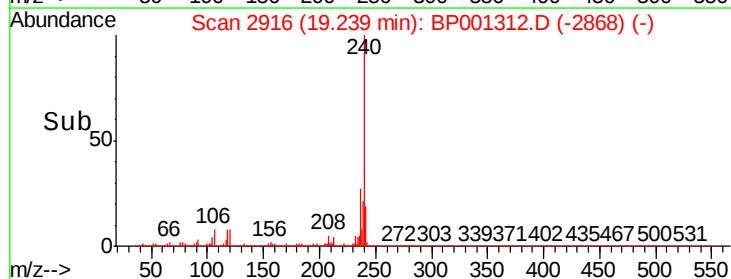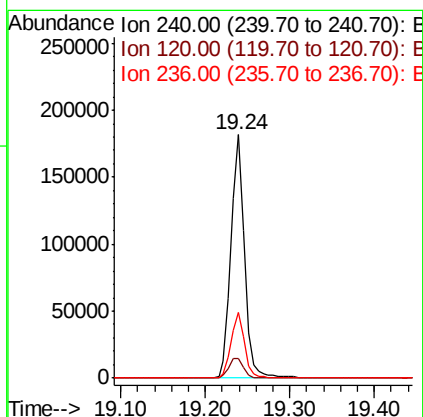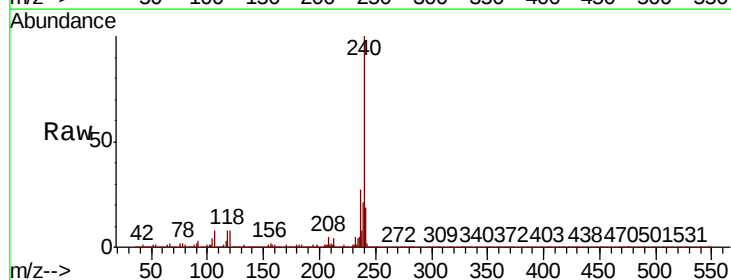

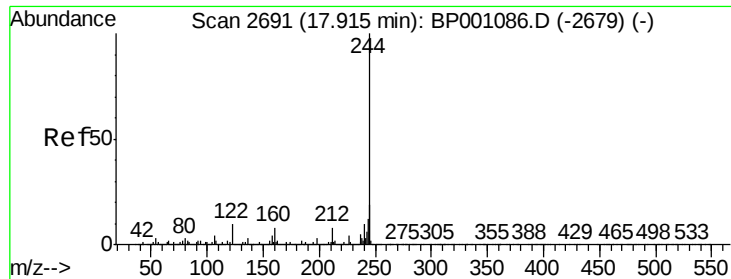

#79

Terphenyl-d14

Concen: 124.970 ng

RT: 17.89 min Scan# 2686

Delta R.T. -0.01 min

Lab File: BP001312.D

Acq: 11 Dec 2019 15:25

Instrument :

BNA_P

ClientSampleId :

K072-AB-WC-1


Tot Ion:244 Resp: 1349596

Ion Ratio Lower Upper

244 100

212 8.2 6.6 9.8




122 10.7 9.2 13.8



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

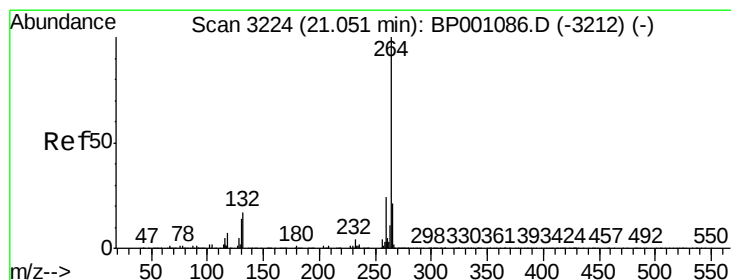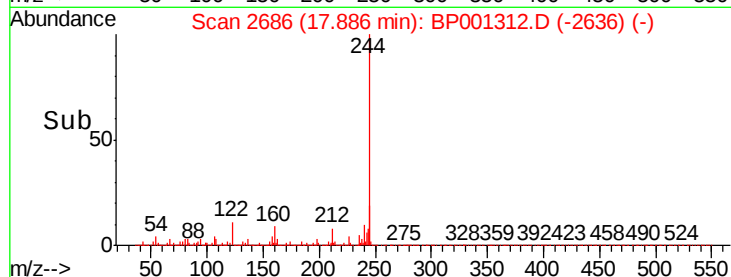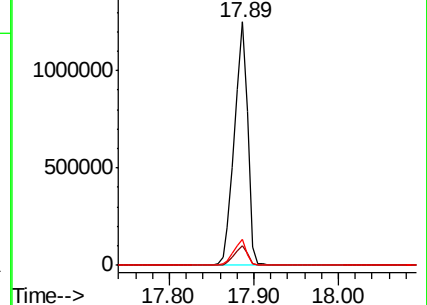

#87

Perylene-d12

Concen: 20.000 ng

RT: 21.01 min Scan# 3217

Delta R.T. -0.02 min

Lab File: BP001312.D

Acq: 11 Dec 2019 15:25


Tgt Ion:264 Resp: 172312

Ion Ratio Lower Upper

264 100

260 23.6 19.4 29.0

265 22.0 17.1 25.7

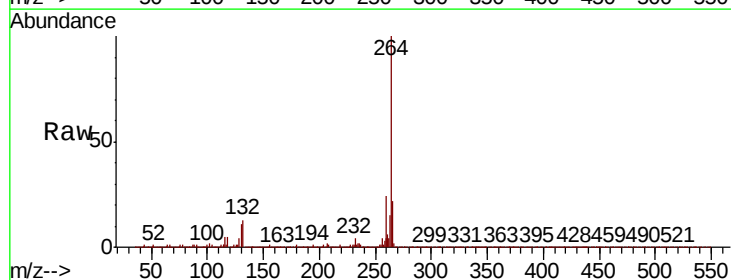

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

