
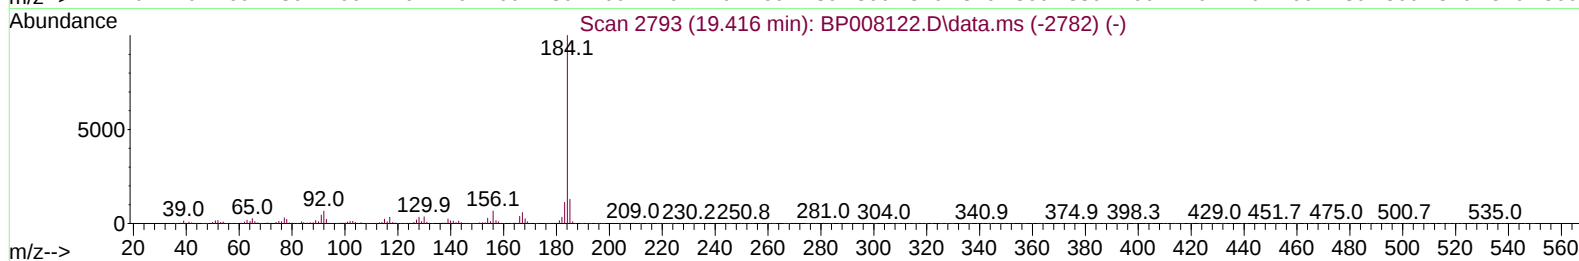
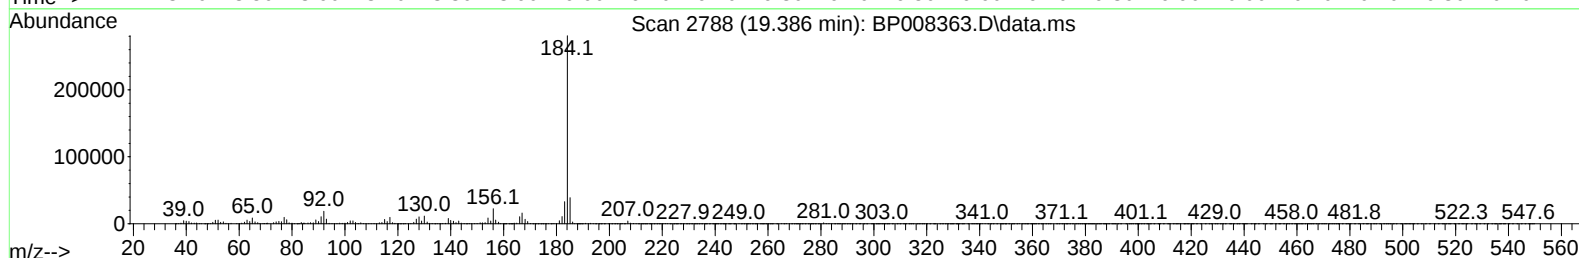


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
 Data File : BP008363.D
 Acq On : 11 Dec 2021 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 20:56:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 03:53:01 2021
 Response via : Initial Calibration

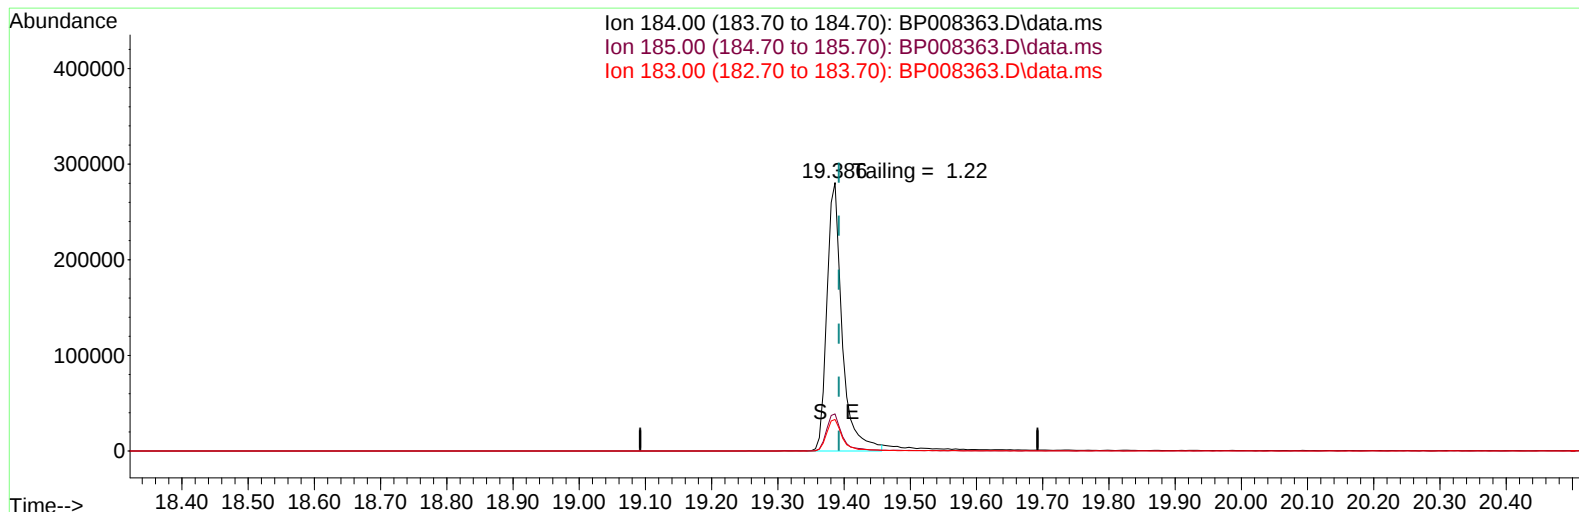




TIC: BP008363.D\data.ms

(77) Benzidine**19.386min (-0.006) 175958.75 ng****response 461010**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.85
183.00	11.40	11.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
Data File : BP008363.D
Acq On : 11 Dec 2021 12:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 20:56:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 03:53:01 2021
Response via : Initial Calibration

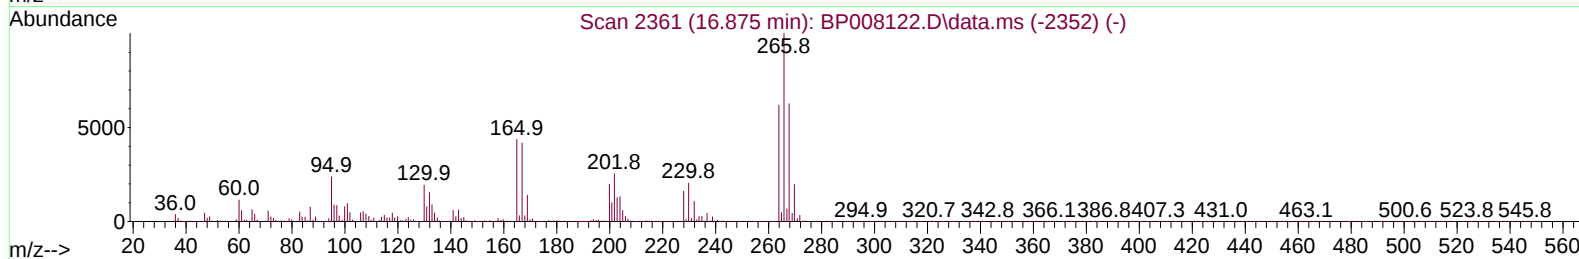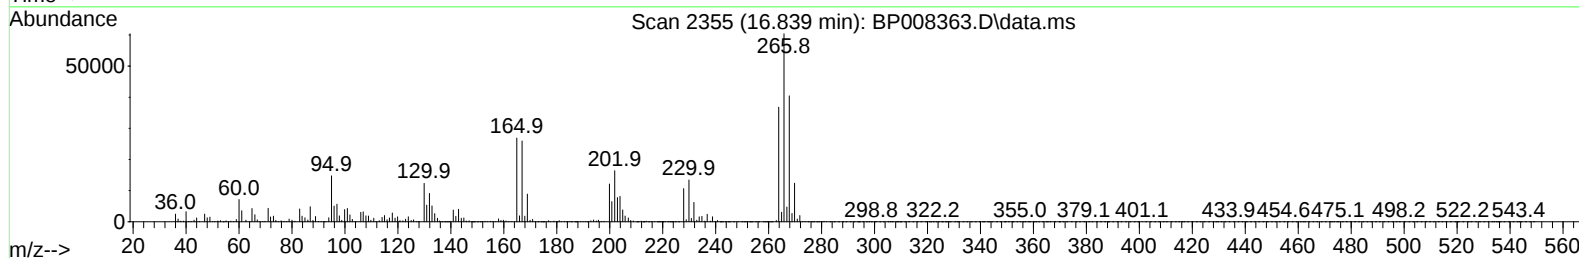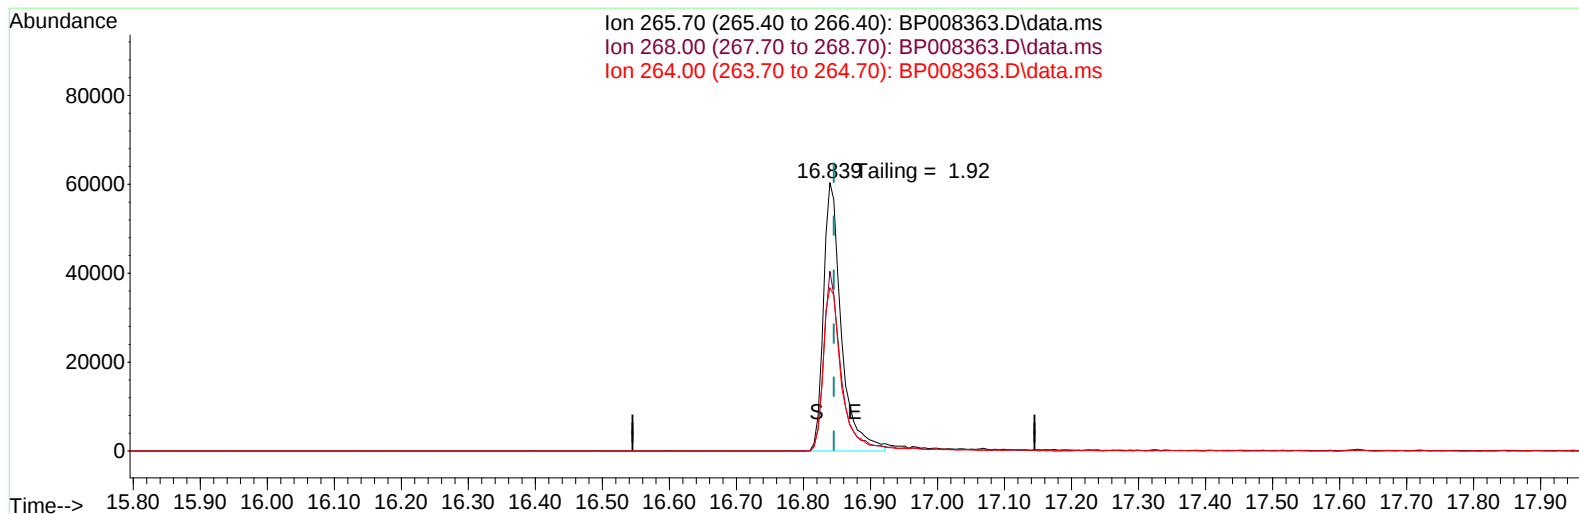

TIC: BP008363.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.006) 853154.63 ng

response 114573

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.98
264.00	61.90	60.90
0.00	0.00	0.00