

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
 Data File : BP008371.D
 Acq On : 11 Dec 2021 16:45
 Operator : CG/JU
 Sample : M5051-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP008371.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.881	317	322	333	rBV	330759	465147	11.25%	1.218%
2	5.352	396	402	423	rBV	1472126	2259810	54.65%	5.917%
3	5.952	498	504	511	rBV	26513	41386	1.00%	0.108%
4	6.946	667	673	694	rVB	1382035	2383174	57.64%	6.240%
5	7.399	742	750	760	rBV4	28069	71486	1.73%	0.187%
6	7.752	801	810	819	rBV	267579	426687	10.32%	1.117%
7	8.287	895	901	908	rBV2	30773	61527	1.49%	0.161%
8	8.916	1001	1008	1016	rBV	881491	1498550	36.24%	3.924%
9	10.546	1274	1285	1290	rBV	324676	563080	13.62%	1.474%
10	10.598	1290	1294	1305	rVB2	93520	181841	4.40%	0.476%
11	12.222	1563	1570	1575	rBV2	25333	45483	1.10%	0.119%
12	12.440	1603	1607	1619	rVB3	21799	46462	1.12%	0.122%
13	13.022	1699	1706	1717	rBV	1783977	2689617	65.05%	7.043%
14	14.128	1888	1894	1902	rBV	55986	89549	2.17%	0.234%
15	14.404	1935	1941	1948	rBV	477712	696088	16.84%	1.823%
16	14.469	1948	1952	1962	rVB2	40509	65519	1.58%	0.172%
17	14.810	2006	2010	2015	rBV	30518	41746	1.01%	0.109%
18	15.028	2040	2047	2054	rBV9	15057	45427	1.10%	0.119%
19	15.463	2116	2121	2129	rVB	46252	76114	1.84%	0.199%
20	15.675	2152	2157	2166	rBV3	41415	76012	1.84%	0.199%
21	15.910	2188	2197	2206	rBV	1786969	2704598	65.41%	7.082%
22	16.139	2232	2236	2243	rVB6	35819	78922	1.91%	0.207%
23	16.986	2376	2380	2388	rVB	46808	73976	1.79%	0.194%
24	17.169	2405	2411	2415	rBV	611937	872958	21.11%	2.286%
25	17.210	2415	2418	2426	rVV	545536	747307	18.07%	1.957%
26	17.304	2430	2434	2440	rVB	127817	184436	4.46%	0.483%
27	17.369	2440	2445	2450	rBV4	20724	44177	1.07%	0.116%
28	17.586	2478	2482	2487	rVB	42640	60490	1.46%	0.158%
29	17.680	2494	2498	2504	rBV3	21107	45171	1.09%	0.118%
30	18.045	2552	2560	2562	rBV	105372	176974	4.28%	0.463%
31	18.075	2562	2565	2573	rVB2	375421	620492	15.01%	1.625%
32	18.169	2578	2581	2586	rVV2	52533	74281	1.80%	0.194%
33	18.227	2586	2591	2595	rVV2	145003	253606	6.13%	0.664%
34	18.269	2595	2598	2604	rVB	80898	109716	2.65%	0.287%
35	18.357	2608	2613	2616	rBV3	53045	83568	2.02%	0.219%
36	18.527	2639	2642	2646	rVV	59900	71634	1.73%	0.188%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
 Data File : BP008371.D
 Acq On : 11 Dec 2021 16:45
 Operator : CG/JU
 Sample : M5051-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.580	2648	2651	2659	rVB	47739	66094	1.60%	0.173%
38	18.763	2677	2682	2686	rBV2	154040	197834	4.78%	0.518%
39	18.822	2689	2692	2695	rVB	48635	53128	1.28%	0.139%
40	18.904	2703	2706	2708	rBV	35519	46183	1.12%	0.121%
41	18.939	2708	2712	2715	rVB	90910	122265	2.96%	0.320%
42	19.080	2731	2736	2742	rBV4	65219	132858	3.21%	0.348%
43	19.192	2749	2755	2762	rBV	1150014	1569906	37.97%	4.111%
44	19.310	2769	2775	2785	rBV3	366405	624610	15.11%	1.635%
45	19.427	2792	2795	2799	rVB2	39050	43619	1.05%	0.114%
46	19.545	2806	2815	2824	rBV	1041908	1668121	40.34%	4.368%
47	19.622	2824	2828	2833	rVB2	89177	133674	3.23%	0.350%
48	19.745	2843	2849	2853	rBV	3531424	4134721	100.00%	10.826%
49	19.786	2853	2856	2863	rVB2	60483	106760	2.58%	0.280%
50	19.863	2865	2869	2877	rBV3	102824	236801	5.73%	0.620%
51	20.027	2888	2897	2905	rBV2	185085	507568	12.28%	1.329%
52	20.127	2911	2914	2917	rBV	87262	97114	2.35%	0.254%
53	20.186	2918	2924	2928	rVV2	166558	295195	7.14%	0.773%
54	20.322	2944	2947	2950	rBV	131599	167362	4.05%	0.438%
55	20.369	2951	2955	2959	rVB	151387	204852	4.95%	0.536%
56	20.533	2981	2983	2986	rVB2	55272	53689	1.30%	0.141%
57	20.769	3020	3023	3027	rBV	121974	146350	3.54%	0.383%
58	20.933	3048	3051	3053	rBV3	86290	120426	2.91%	0.315%
59	20.963	3053	3056	3059	rVV	283989	364669	8.82%	0.955%
60	20.998	3059	3062	3069	rVV3	415108	628909	15.21%	1.647%
61	21.063	3071	3073	3078	rVB	121794	157828	3.82%	0.413%
62	21.186	3092	3094	3097	rVB	71087	58756	1.42%	0.154%
63	21.274	3103	3109	3113	rBV2	1116574	2194646	53.08%	5.746%
64	21.316	3113	3116	3125	rVB	657890	857981	20.75%	2.247%
65	21.851	3204	3207	3210	rVB3	151826	179897	4.35%	0.471%
66	21.910	3214	3217	3223	rVB2	241307	337473	8.16%	0.884%
67	22.933	3385	3391	3396	rBV2	644367	1535590	37.14%	4.021%
68	23.445	3473	3478	3487	rVB	345595	666641	16.12%	1.746%
69	23.551	3490	3496	3504	rVB	497692	980377	23.71%	2.567%
70	23.657	3508	3514	3520	rBV2	502496	984464	23.81%	2.578%
71	24.262	3613	3617	3627	rVB3	224835	487779	11.80%	1.277%




Sum of corrected areas: 38191151

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
Data File : BP008371.D
Acq On : 11 Dec 2021 16:45
Operator : CG/JU
Sample : M5051-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

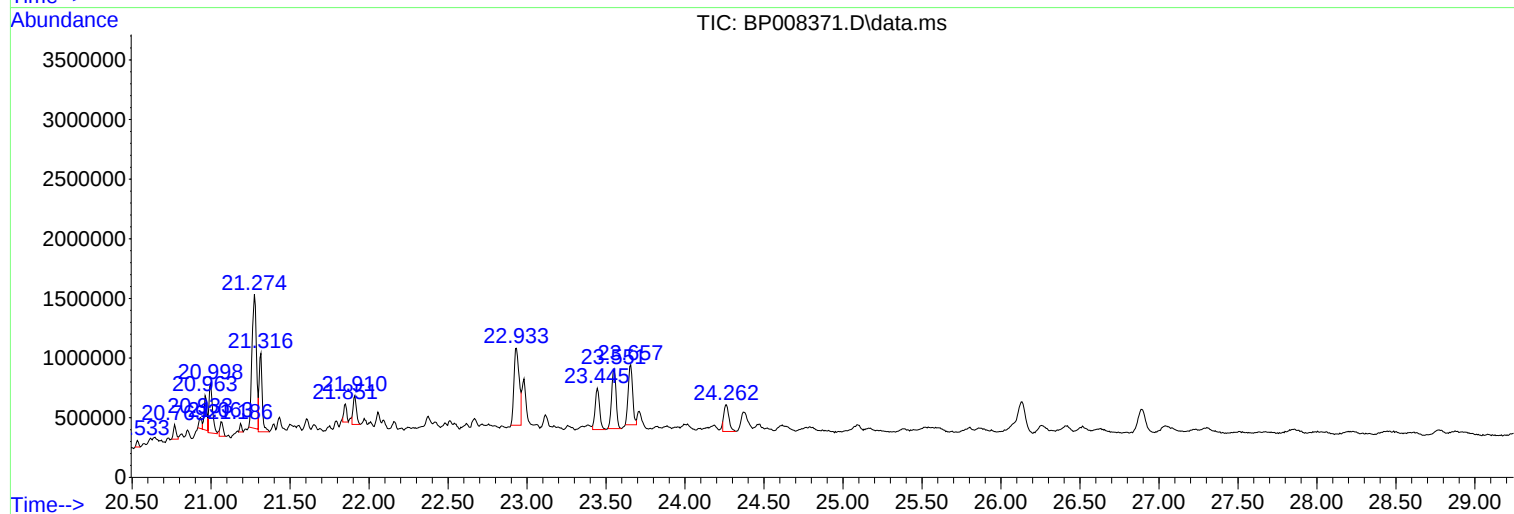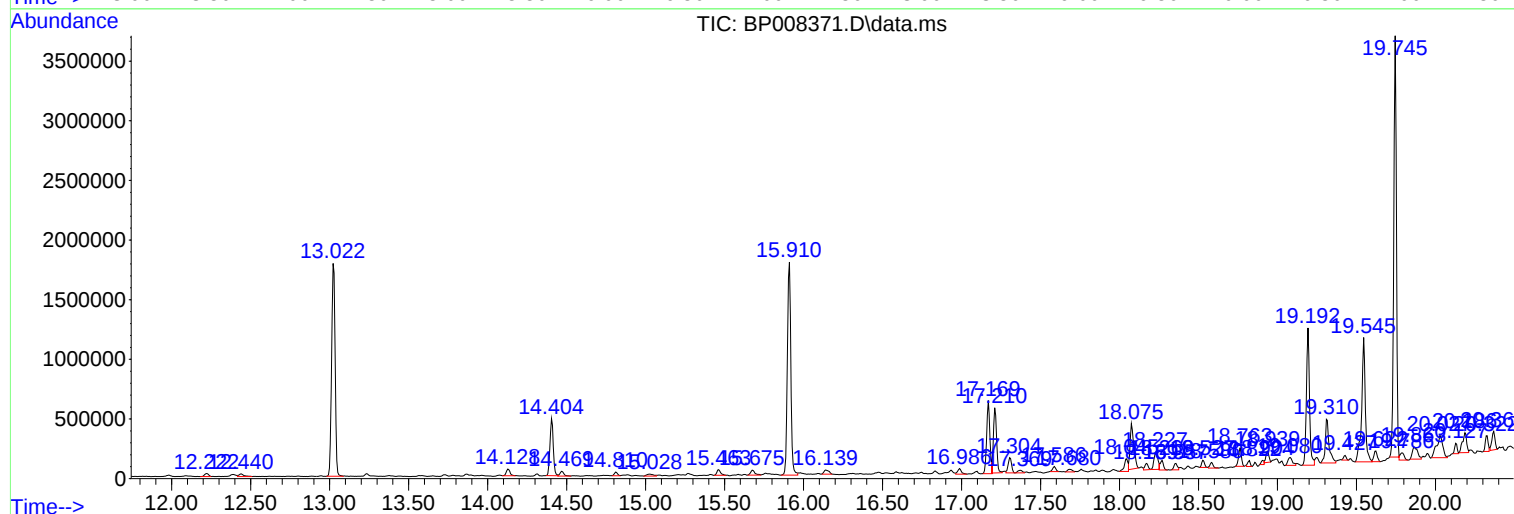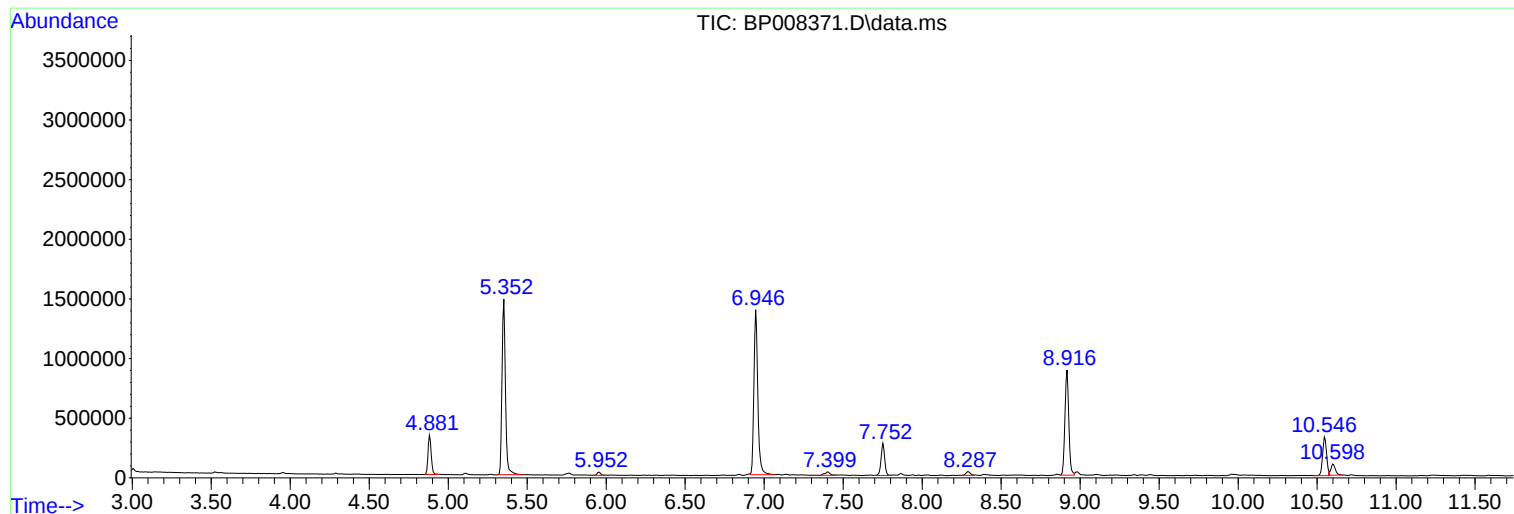

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
Data File : BP008371.D
Acq On : 11 Dec 2021 16:45
Operator : CG/JU
Sample : M5051-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
Data File : BP008371.D
Acq On : 11 Dec 2021 16:45
Operator : CG/JU
Sample : M5051-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc