
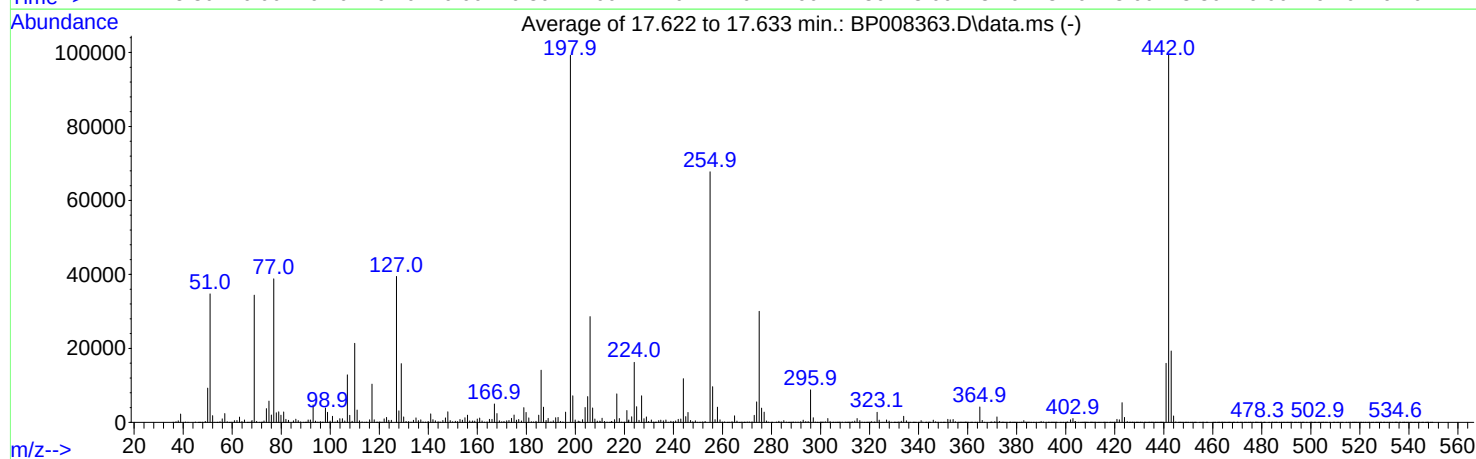


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
 Data File : BP008363.D
 Acq On : 11 Dec 2021 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 03:53:01 2021

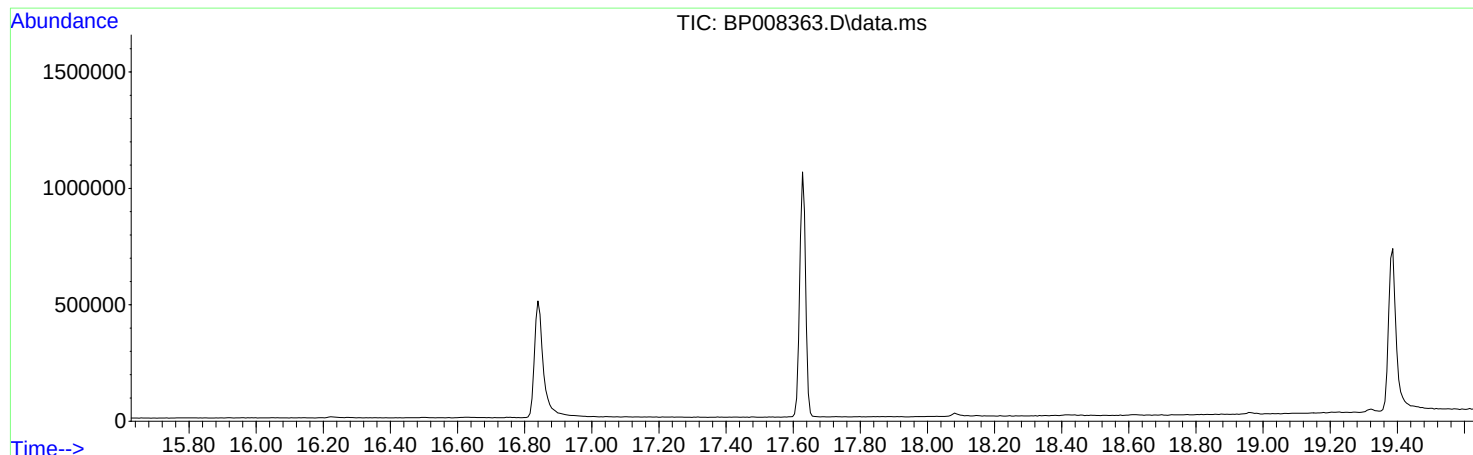

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	34733	PASS
68	69	0.00	2	1.6	539	PASS
69	198	0.00	100	34.7	34400	PASS
70	69	0.00	2	0.7	247	PASS
127	198	10	80	39.7	39440	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	99259	PASS
199	198	5	9	7.2	7175	PASS
275	198	10	60	30.2	30005	PASS
365	198	1	100	4.2	4171	PASS
441	198	0.01	100	16.1	15973	PASS
442	442	100	100	100.0	99451	PASS
443	442	15	24	19.4	19312	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/11/2021	BNA_P	<u>BP008363.D</u>
Compound Name	Response	Retention Time
DDT	351845	20.586
DDD	5471	20.198
DDE	1176	19.663
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6647	358492	1.85

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
 Data File : BP008363.D
 Acq On : 11 Dec 2021 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 11 20:56:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 03:53:01 2021
 Response via : Initial Calibration

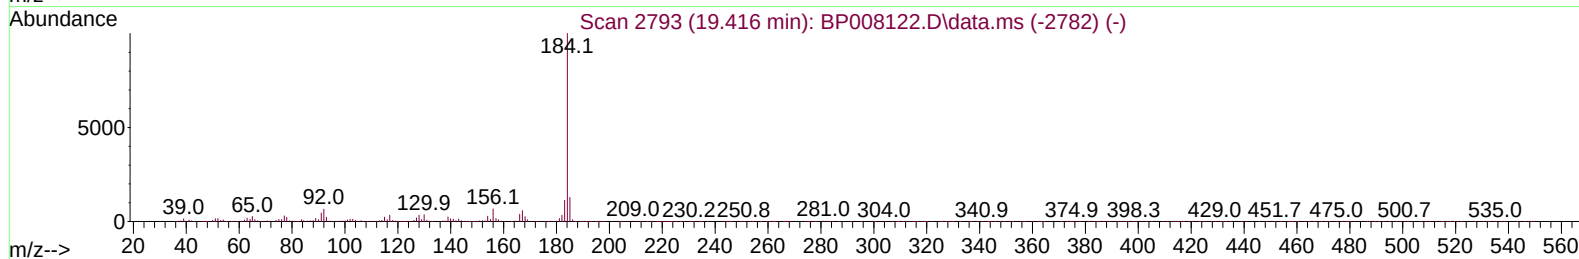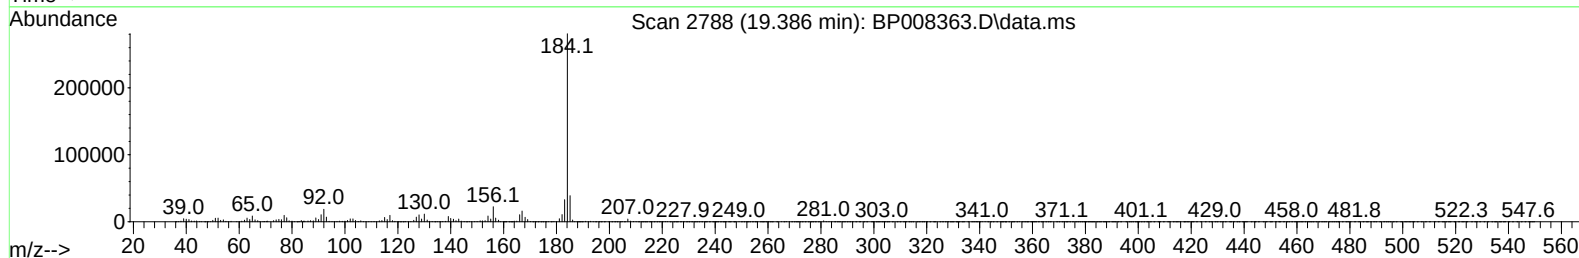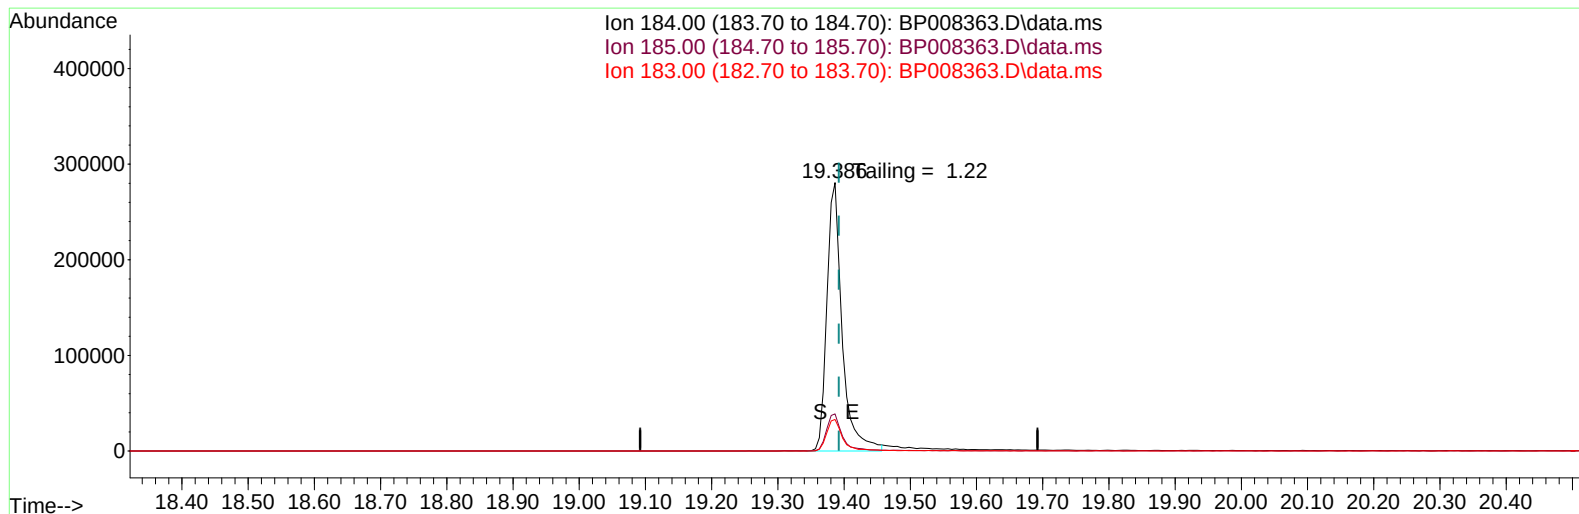

TIC: BP008363.D\data.ms

(77) Benzidine

19.386min (-0.006) 175958.75 ng




response 461010

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.85
183.00	11.40	11.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121121\
 Data File : BP008363.D
 Acq On : 11 Dec 2021 12:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 11 20:56:26 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 03:53:01 2021
 Response via : Initial Calibration

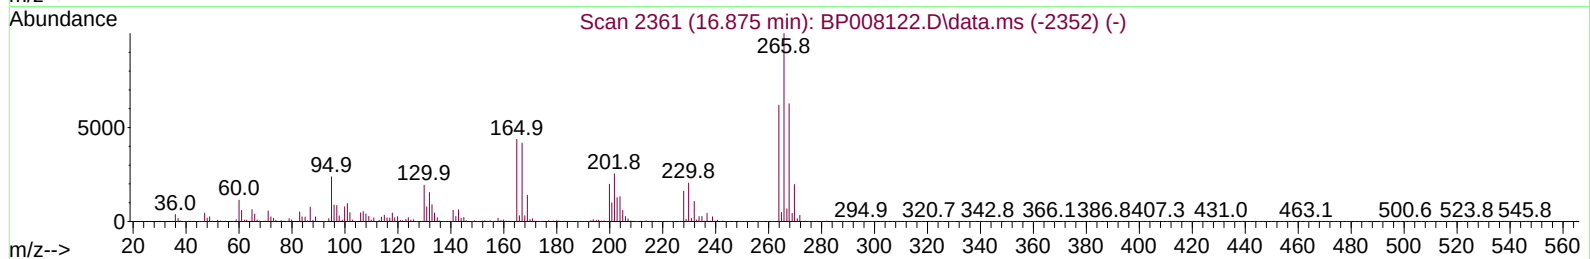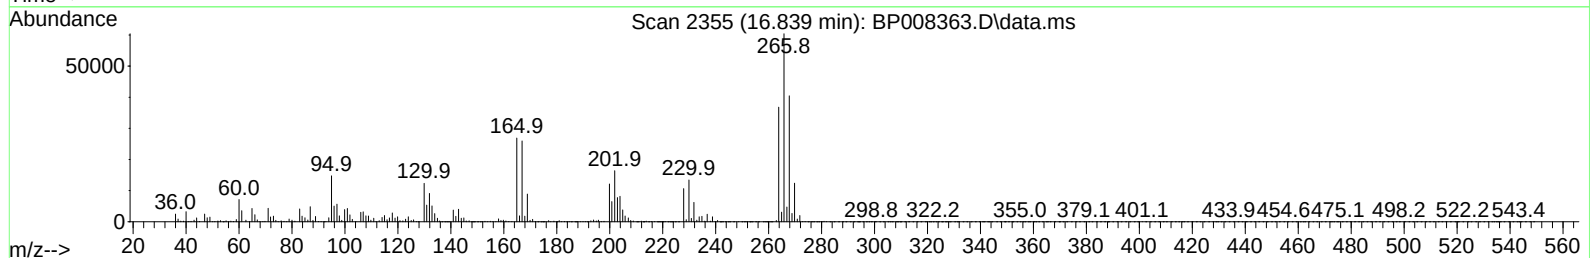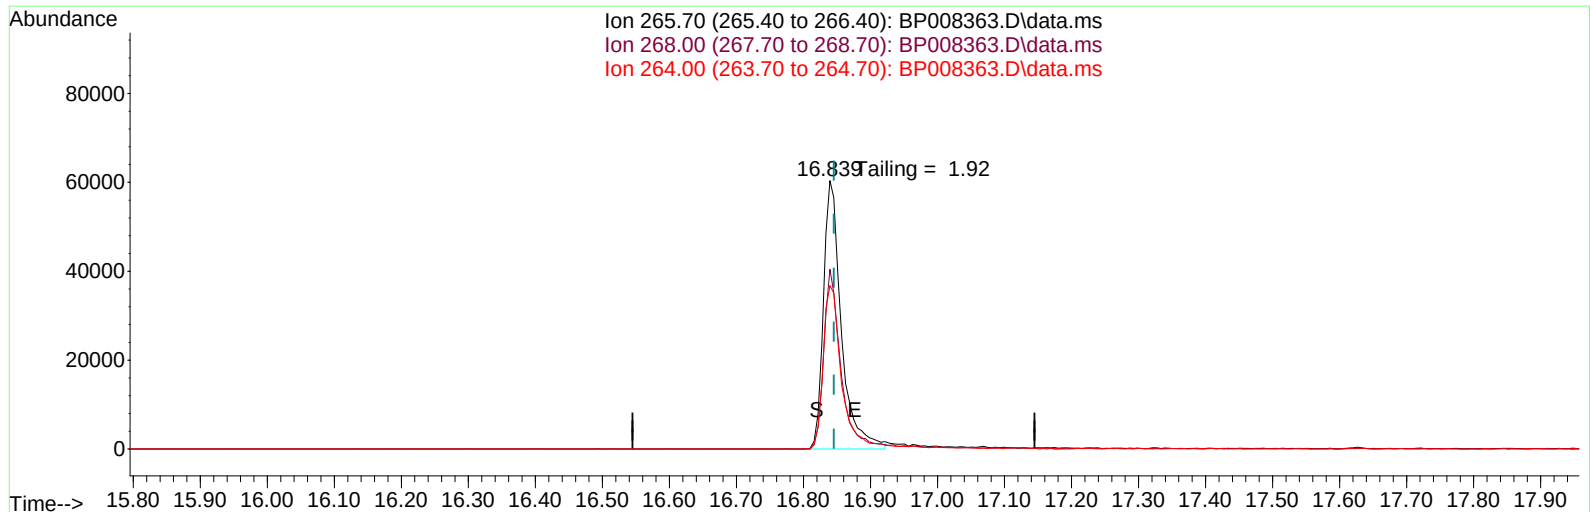

TIC: BP008363.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.006) 853154.63 ng

response 114573

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.98
264.00	61.90	60.90
0.00	0.00	0.00