

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121220\
 Data File : BP004231.D
 Acq On : 11 Dec 2020 16:55
 Operator : CG/JU
 Sample : PB133506BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK06

Quant Time: Dec 11 17:54:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 10 13:52:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	349138	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	1391646	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	826447	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	1795347	20.00	ng/ul	0.00
78) Chrysene-d12	21.32	240	1901604	20.00	ng/ul	0.00
86) Perylene-d12	23.67	264	2045838	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	43503	4.38	ng/uL	0.00
5) Phenol-d5	6.99	99	715515	24.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	457831	25.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	560310	25.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	538540	24.68	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	283637	24.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	254521	27.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	505742	24.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	747019	29.16	ng/ul	0.00
44) Dimethylphthalate-d6	13.88	166	1684466	26.67	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	2166879	26.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	213090	19.97	ng/ul	0.00
58) Fluorene-d10	15.47	176	1450186	25.35	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	150161	17.43	ng/ul	0.00
71) Anthracene-d10	17.33	188	2300543	26.29	ng/ul	0.00
79) Pyrene-d10	19.57	212	2727006	27.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.52	264	2932462	27.21	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.93	163	172980	2.689	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
Data File : BP004231.D
Acq On : 11 Dec 2020 16:55
Operator : CG/JU
Sample : PB133506BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK06

Quant Time: Dec 11 17:54:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 10 13:52:32 2020
Response via : Initial Calibration

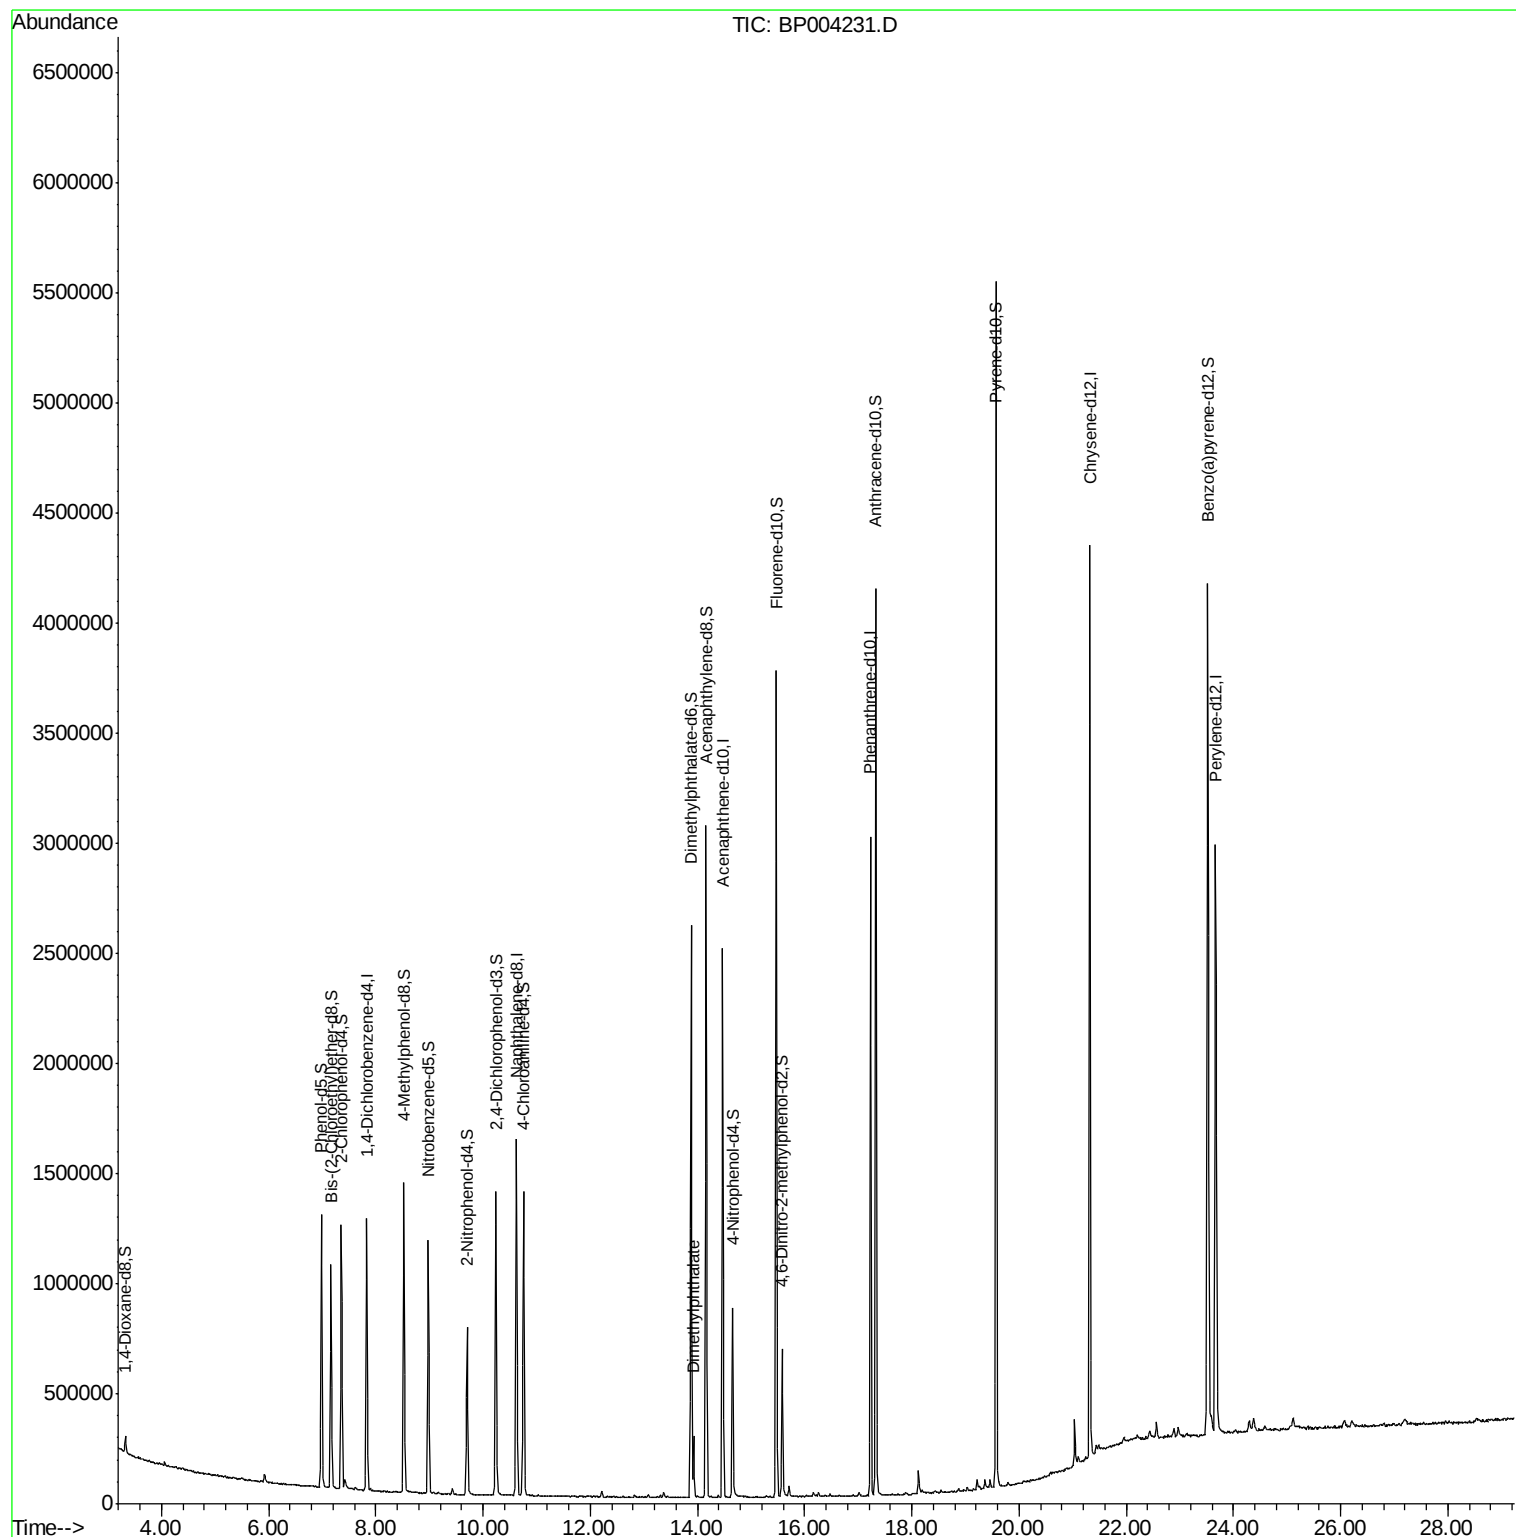

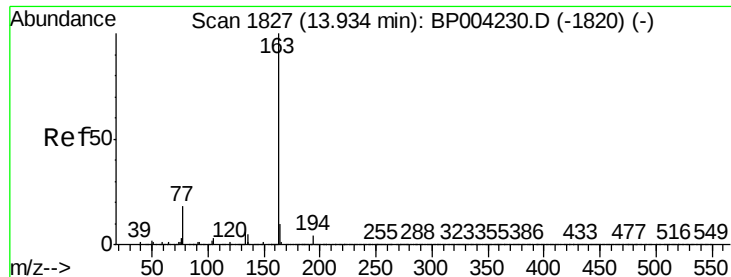

#45

Dimethylphthalate

Concen: 2.689 ng/ul

RT: 13.93 min Scan# 1826

Delta R.T. -0.00 min

Lab File: BP004231.D

Acq: 11 Dec 2020 16:55

Instrument :

BNA_P

ClientSampleId :

SBLK06


Tot Ion:163 Resp: 172980

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 10.1 8.4 12.6

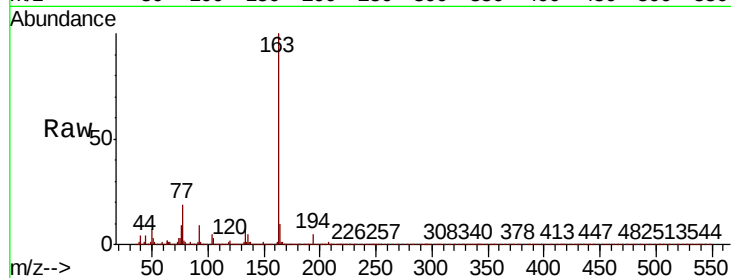

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

150000

100000

50000

0

13.93

13.85

13.90

13.95

14.00

Time-->

