

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
 Data File : BP004234.D
 Acq On : 11 Dec 2020 18:37
 Operator : CG/JU
 Sample : L5000-12
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54B1

Manual Integrations
 APPROVED

mohammad
 12/15/2020 12:18:27 PM

Quant Time: Dec 12 00:33:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 10 13:52:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	393336	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	1602422	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	947072	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	2030973	20.00	ng/ul	0.00
78) Chrysene-d12	21.32	240	2098931	20.00	ng/ul	0.00
86) Perylene-d12	23.67	264	2226827	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	25994	2.32	ng/uL	0.00
5) Phenol-d5	6.99	99	461026	14.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	323245	15.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	394049	15.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	279792	11.38	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	206601	15.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	175235	16.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	359666	15.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	397879	13.49	ng/ul	0.00
44) Dimethylphthalate-d6	13.88	166	1197437	16.54	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	1583082	17.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	78055	6.38	ng/ul	0.00
58) Fluorene-d10	15.47	176	1067121	16.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	83722	8.59	ng/ul	0.00
71) Anthracene-d10	17.33	188	1647227	16.64	ng/ul	0.00
79) Pyrene-d10	19.57	212	2021814	18.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.52	264	2104570	17.94	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	7.01	94	91918	2.706	ng/ul 92
45) Dimethylphthalate	13.93	163	206339	2.799	ng/ul 99
70) Phenanthrene	17.27	178	430749	3.595	ng/ul 99
77) Fluoranthene	19.25	202	1114449	8.711	ng/ul 98
80) Pyrene	19.60	202	1036856	7.323	ng/ul 99
83) Benzo(a)anthracene	21.30	228	542708	3.923	ng/ul 96
85) Chrysene	21.36	228	622693	4.588	ng/ul 97
88) Benzo(b)fluoranthene	22.96	252	867844	6.145	ng/ul 99
89) Benzo(k)fluoranthene	23.00	252	253592m	1.749	ng/ul
91) Benzo(a)pyrene	23.57	252	584203	4.433	ng/ul 98
92) Indeno(1,2,3-cd)pyrene	26.07	276	494808	2.994	ng/ul 97
94) Benzo(g,h,i)perylene	26.82	276	470951	3.397	ng/ul 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
Data File : BP004234.D
Acq On : 11 Dec 2020 18:37
Operator : CG/JU
Sample : L5000-12
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A54B1

Manual Integrations
APPROVED

mohammad
12/15/2020 12:18:27 PM

Quant Time: Dec 12 00:33:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 10 13:52:32 2020
Response via : Initial Calibration

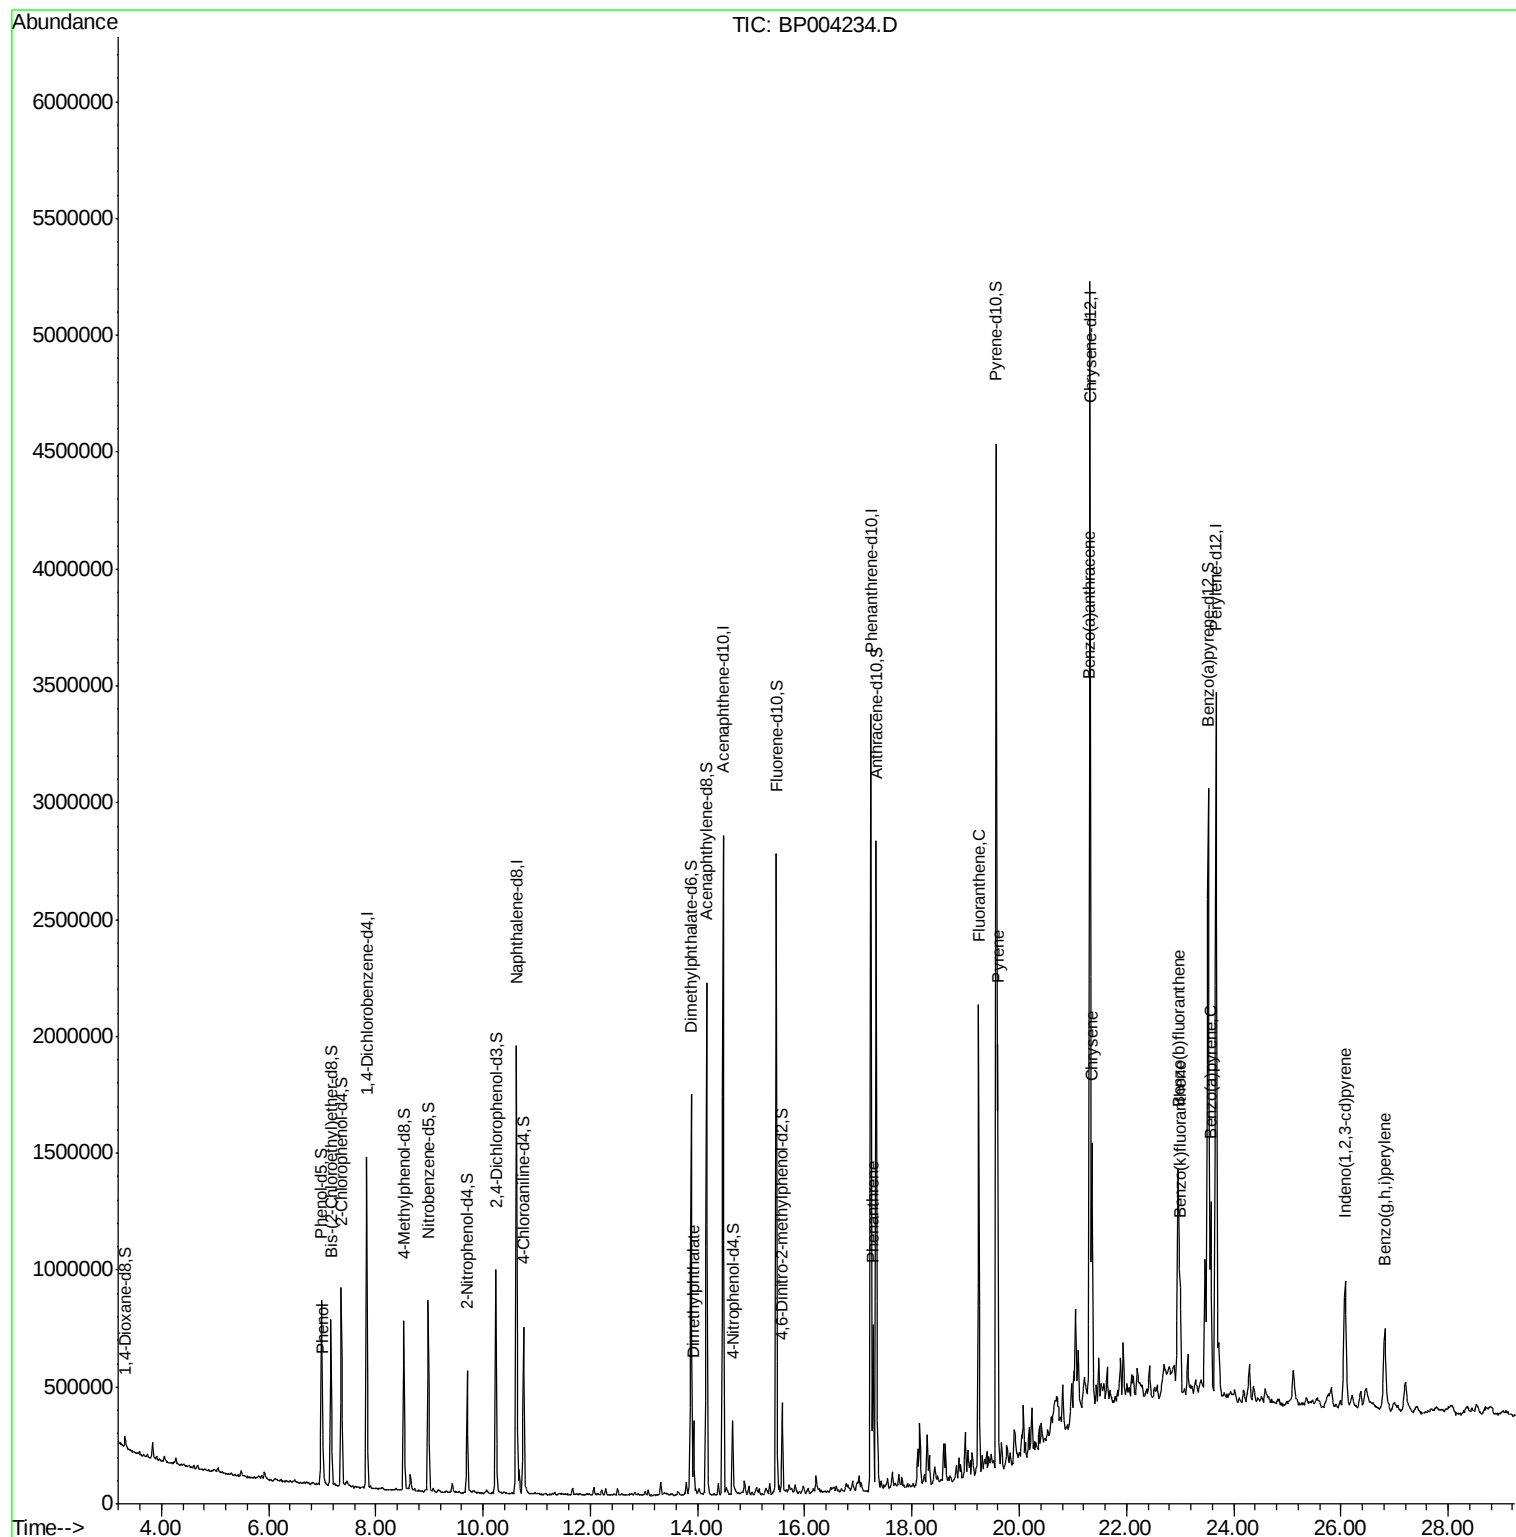

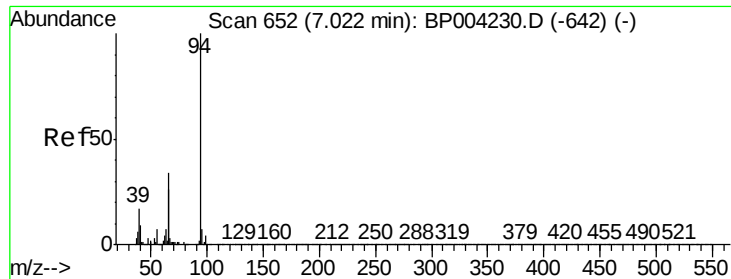

#6

Phenol





Concen: 2.706 ng/ul
 RT: 7.01 min Scan# 650
 Delta R.T. -0.01 min
 Lab File: BP004234.D
 Acq: 11 Dec 2020 18:37

Instrument :
 BNA_P
 ClientSampleId :
 A54B1

Tot Ion	Ratio	Lower	Upper
94	100		
65	29.2	20.8	31.2
66	38.1	26.5	39.7

Manual Integrations
 APPROVED

mohammad
 12/15/2020 12:18:27 PM

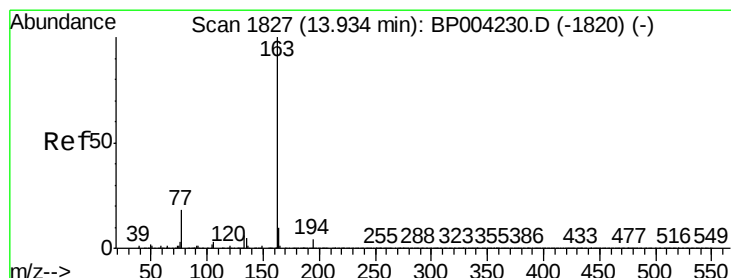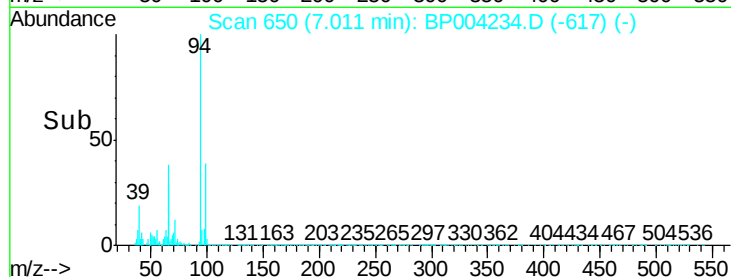
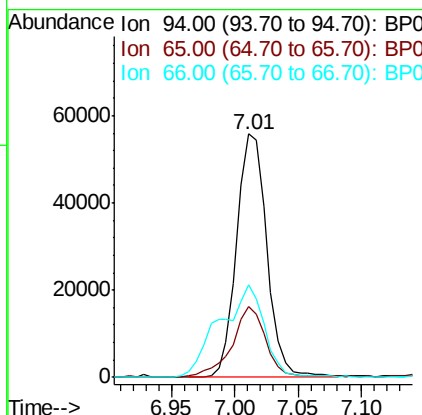
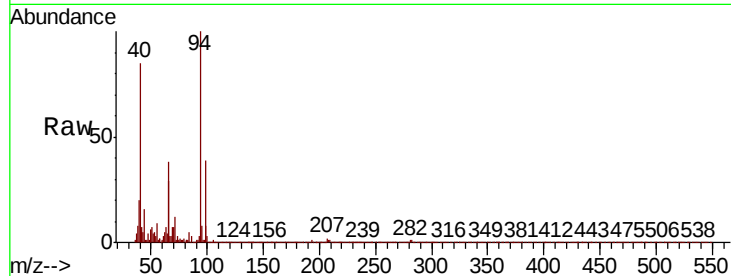



#45

Dimethylphthalate

Concen: 2.799 ng/ul
 RT: 13.93 min Scan# 1826
 Delta R.T. 0.00 min
 Lab File: BP004234.D
 Acq: 11 Dec 2020 18:37

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.2
164	9.8	8.4	12.6

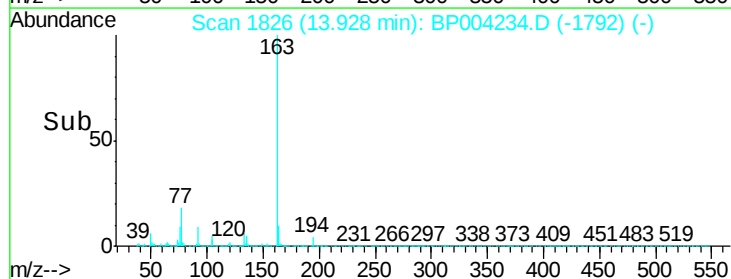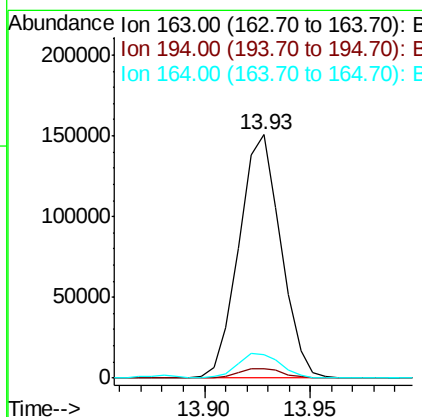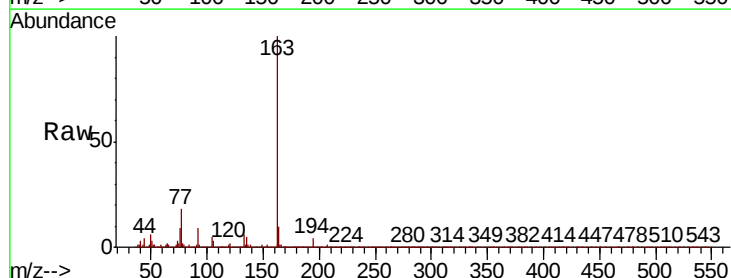

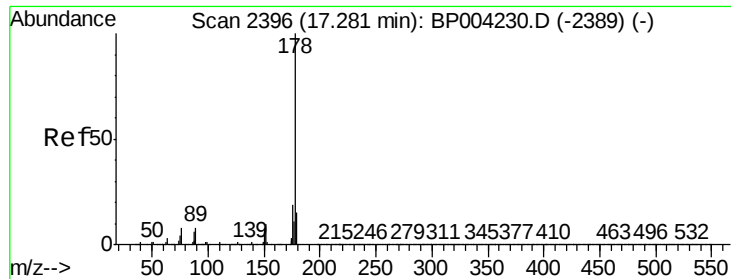





#70
Phenanthrene
Concen: 3.595 ng/ul
RT: 17.27 min Scan# 2395
Delta R.T. 0.00 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Instrument :
BNA_P
ClientSampleId :
A54B1

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.2	12.4	18.6
176	18.6	15.4	23.0




Manual Integrations
APPROVED


mohammad
12/15/2020 12:18:27 PM

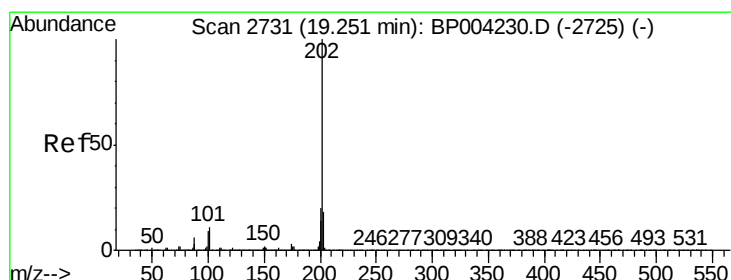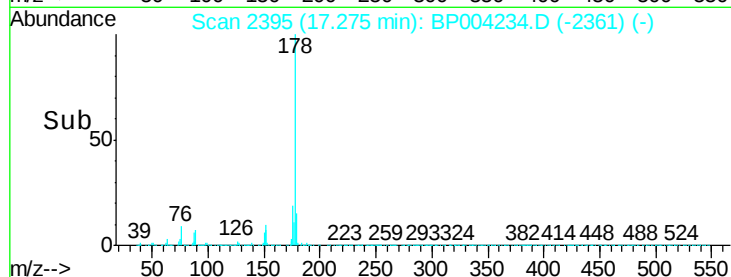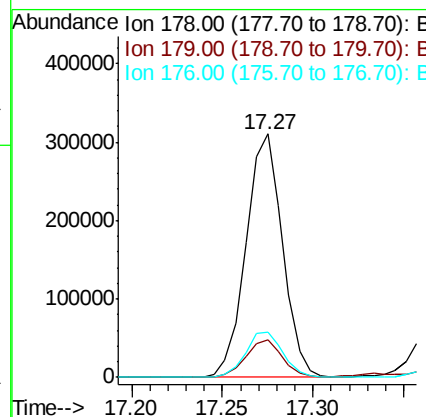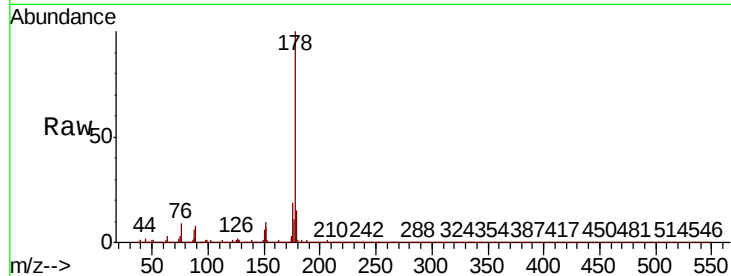

#77
Fluoranthene
Concen: 8.711 ng/ul
RT: 19.25 min Scan# 2730
Delta R.T. 0.00 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.7	9.1	13.7
100	8.3	7.1	10.7

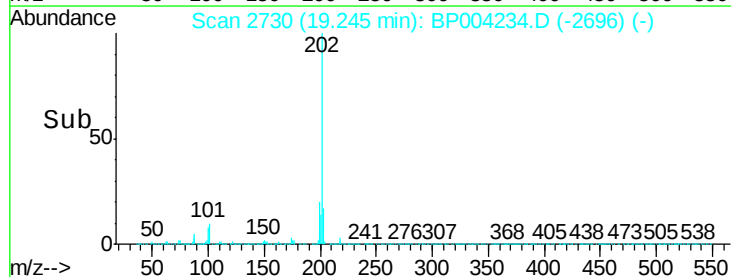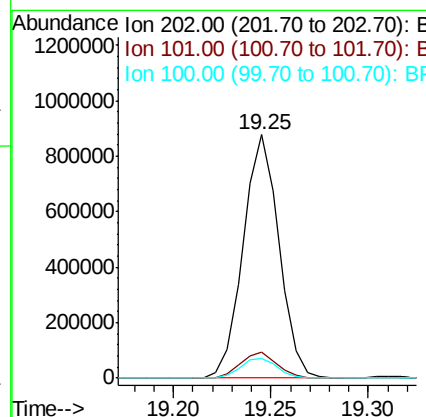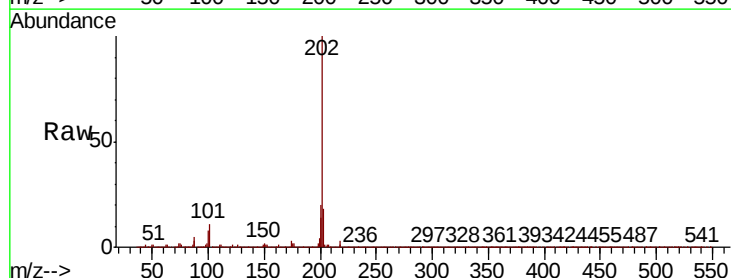

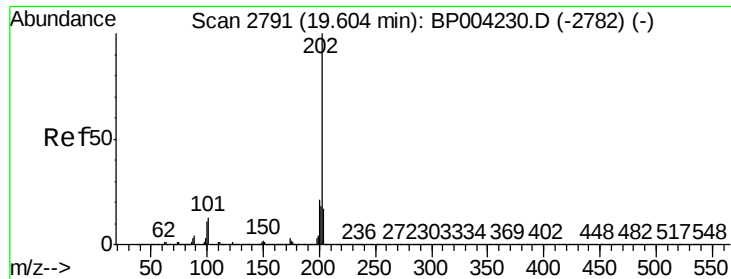





#80
Pvrene
Concen: 7.323 ng/ul
RT: 19.60 min Scan# 2790
Delta R.T. 0.00 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Instrument :
BNA_P
ClientSampled :
A54B1

Tot Ion	Ratio	Lower	Upper
202	100		
101	12.6	10.6	15.8
100	10.2	8.6	12.8




Manual Integrations
APPROVED


mohammad
12/15/2020 12:18:27 PM

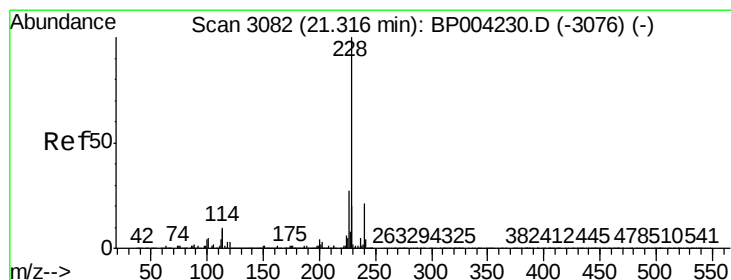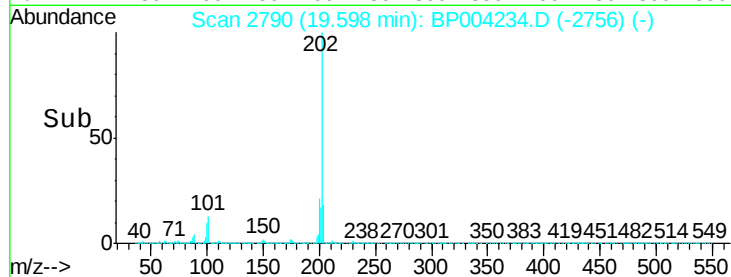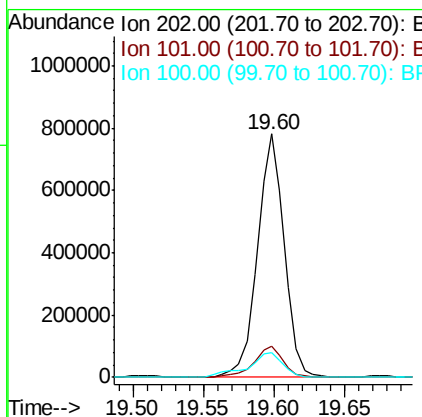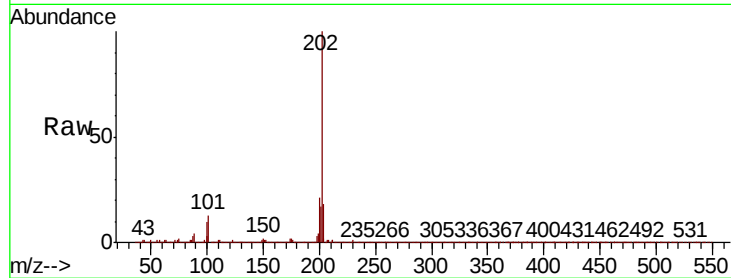

#83
Benzo(a)anthracene
Concen: 3.923 ng/ul
RT: 21.30 min Scan# 3080
Delta R.T. -0.01 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Tgt Ion	Ratio	Lower	Upper
228	100		
229	21.4	15.8	23.8
226	29.1	21.7	32.5

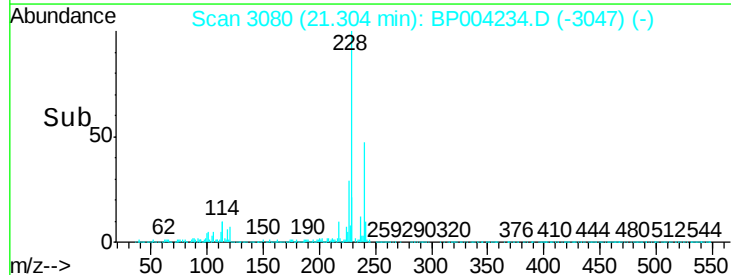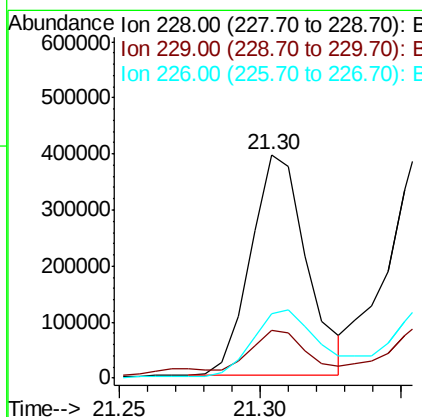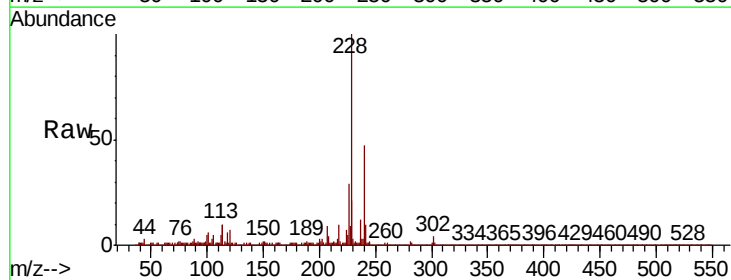

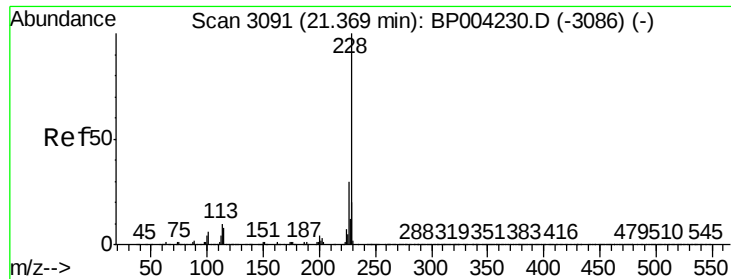





#85
Chrysene
Concen: 4.588 ng/ul
RT: 21.36 min Scan# 3089
Delta R.T. -0.01 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Instrument :
BNA_P
ClientSampleId :
A54B1

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.2	24.2	36.2
229	22.8	15.8	23.8




Manual Integrations
APPROVED


mohammad
12/15/2020 12:18:27 PM

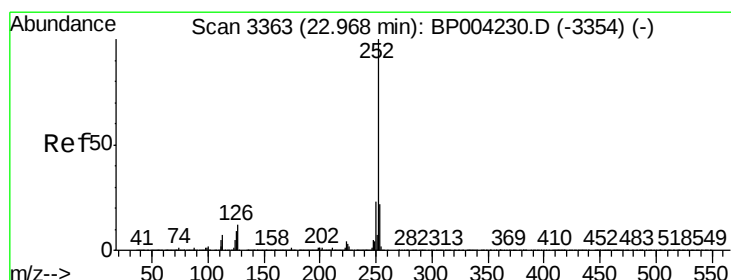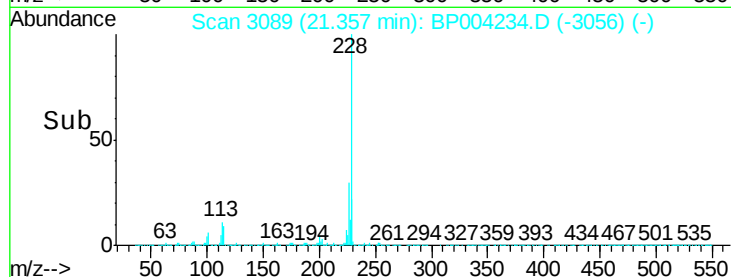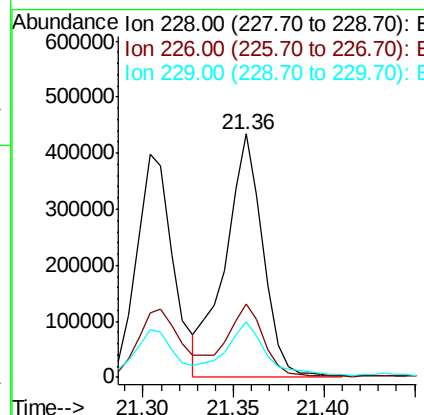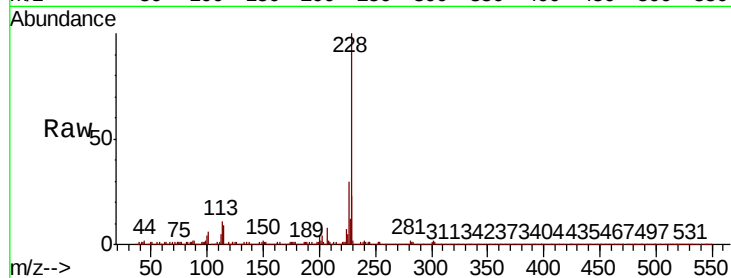

#88
Benzo(b)fluoranthene
Concen: 6.145 ng/ul
RT: 22.96 min Scan# 3361
Delta R.T. -0.01 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.6	26.4
125	10.1	7.7	11.5

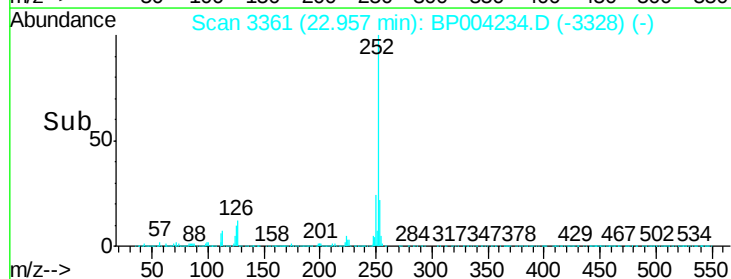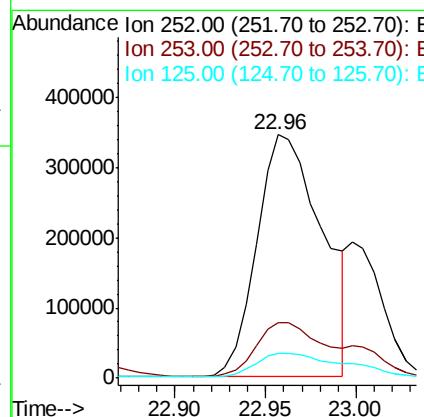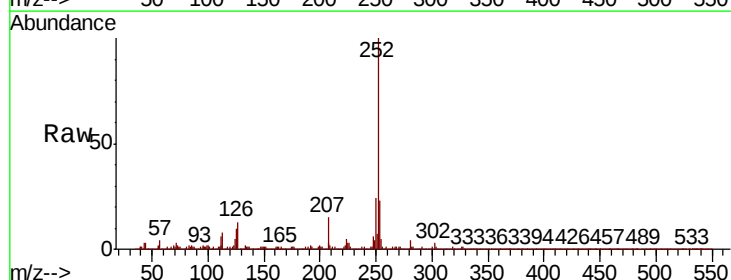

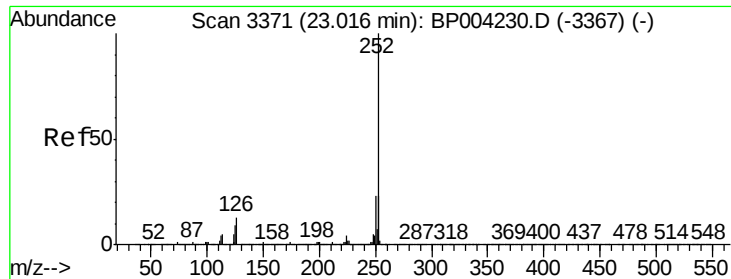





#89
Benzo(k)fluoranthene
Concen: 1.749 ng/ul
RT: 23.00 min Scan# 3368
Delta R.T. -0.01 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Instrument :
BNA_P
ClientSampleId :
A54B1

Tot Ion:	252	Resp:	253592
Ion Ratio	Lower	Upper	
252	100		
253	23.8	17.4	26.2
125	10.4	7.3	10.9




Manual Integrations
APPROVED


mohammad
12/15/2020 12:18:27 PM

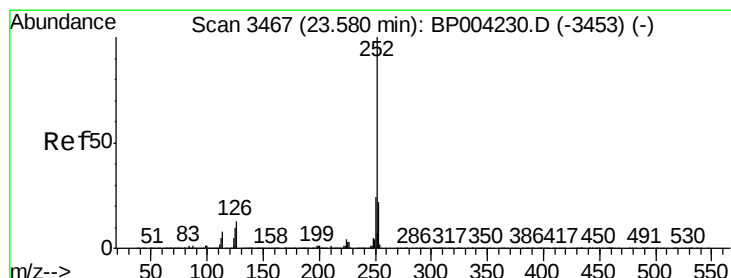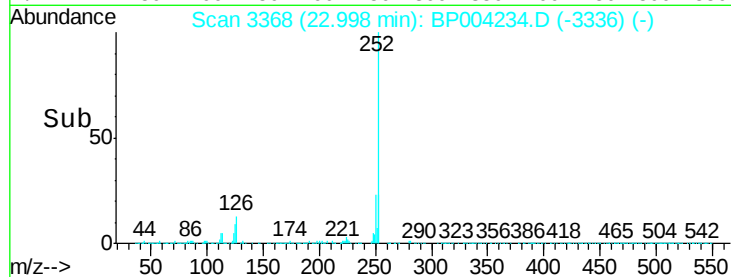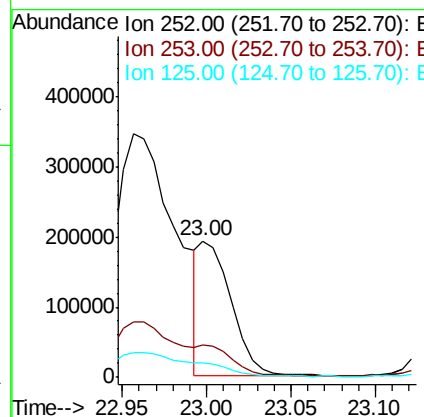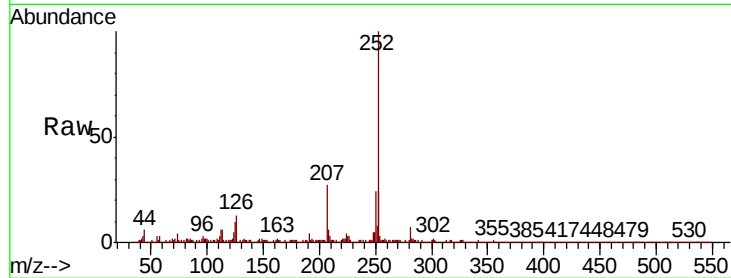

#91
Benzo(a)pyrene
Concen: 4.433 ng/ul
RT: 23.57 min Scan# 3465
Delta R.T. -0.01 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Tgt Ion:	252	Resp:	584203
Ion Ratio	Lower	Upper	
252	100		
253	22.6	17.3	25.9
125	10.9	7.8	11.6

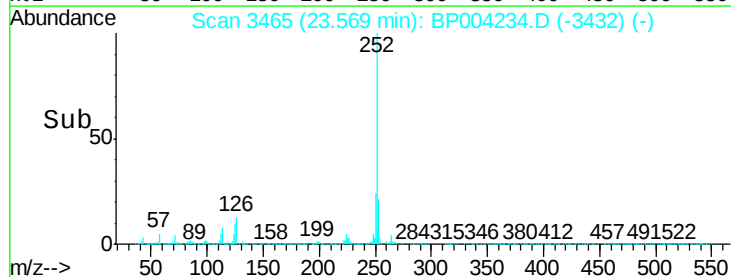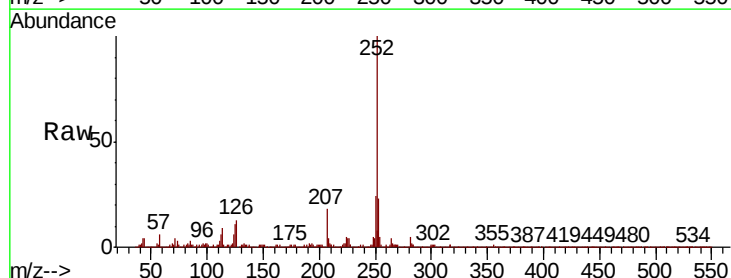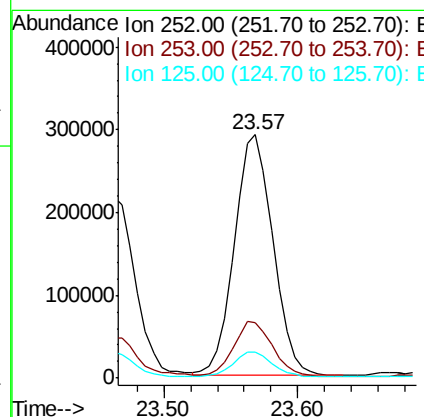

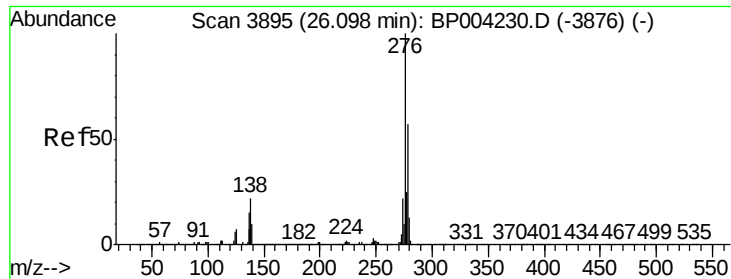





#92
Indeno(1,2,3-cd)pyrene
Concen: 2.994 ng/ul
RT: 26.07 min Scan# 3891
Delta R.T. -0.01 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Instrument :
BNA_P
ClientSampleId :
A54B1

Tot Ion	Ratio	Lower	Upper
276	100		
138	19.3	17.8	26.6
277	24.7	19.8	29.6

Manual Integrations
APPROVED

mohammad
12/15/2020 12:18:27 PM

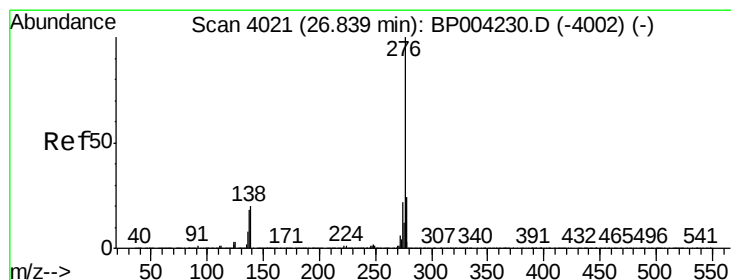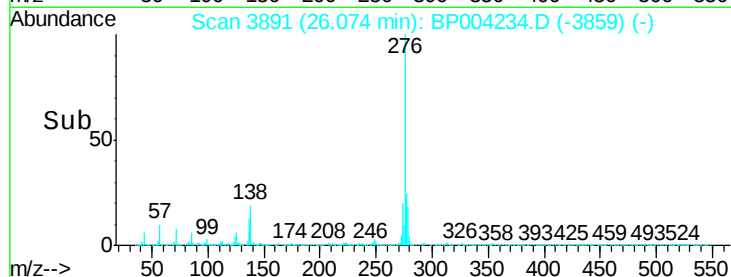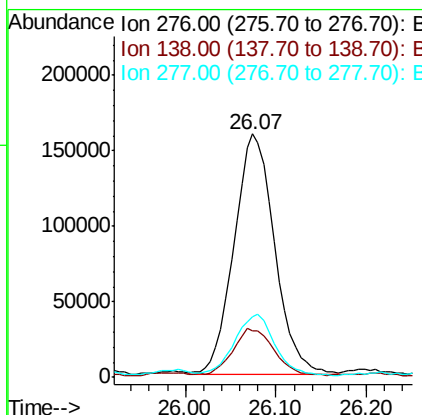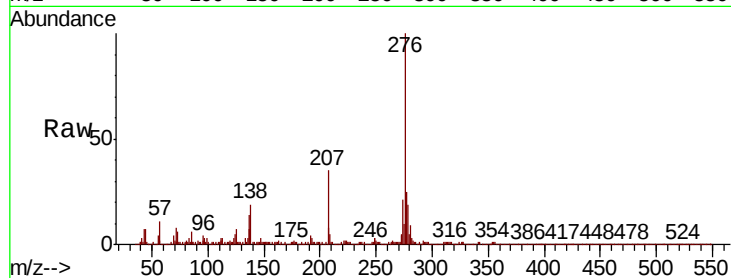

#94
Benzo(g,h,i)perylene
Concen: 3.397 ng/ul
RT: 26.82 min Scan# 4017
Delta R.T. -0.01 min
Lab File: BP004234.D
Acq: 11 Dec 2020 18:37

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.6	16.6	25.0
277	24.8	18.5	27.7

