

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121220\
 Data File : BP004244.D
 Acq On : 12 Dec 2020 00:17
 Operator : CG/JU
 Sample : L5000-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54B0

Quant Time: Dec 12 01:48:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 10 13:52:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	375433	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	1539107	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	919788	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	1977031	20.00	ng/ul	0.00
78) Chrysene-d12	21.32	240	2046945	20.00	ng/ul	0.00
86) Perylene-d12	23.67	264	2161969	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	53082	4.97	ng/uL	0.00
5) Phenol-d5	6.99	99	1011280	32.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	593268	30.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	790012	33.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	785683	33.48	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	395139	31.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	393465	37.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	764227	33.43	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	1053336	37.17	ng/ul	0.00
44) Dimethylphthalate-d6	13.88	166	2252130	32.04	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	2965632	33.05	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	351275	29.58	ng/ul	0.00
58) Fluorene-d10	15.47	176	1962395	30.82	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	222285	23.43	ng/ul	0.00
71) Anthracene-d10	17.33	188	3050088	31.66	ng/ul	0.00
79) Pyrene-d10	19.57	212	3532934	33.13	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.52	264	3737466	32.82	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	7.02	94	61504	1.897	ng/ul 97
45) Dimethylphthalate	13.93	163	635727	8.878	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
Data File : BP004244.D
Acq On : 12 Dec 2020 00:17
Operator : CG/JU
Sample : L5000-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54B0

Quant Time: Dec 12 01:48:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 10 13:52:32 2020
Response via : Initial Calibration




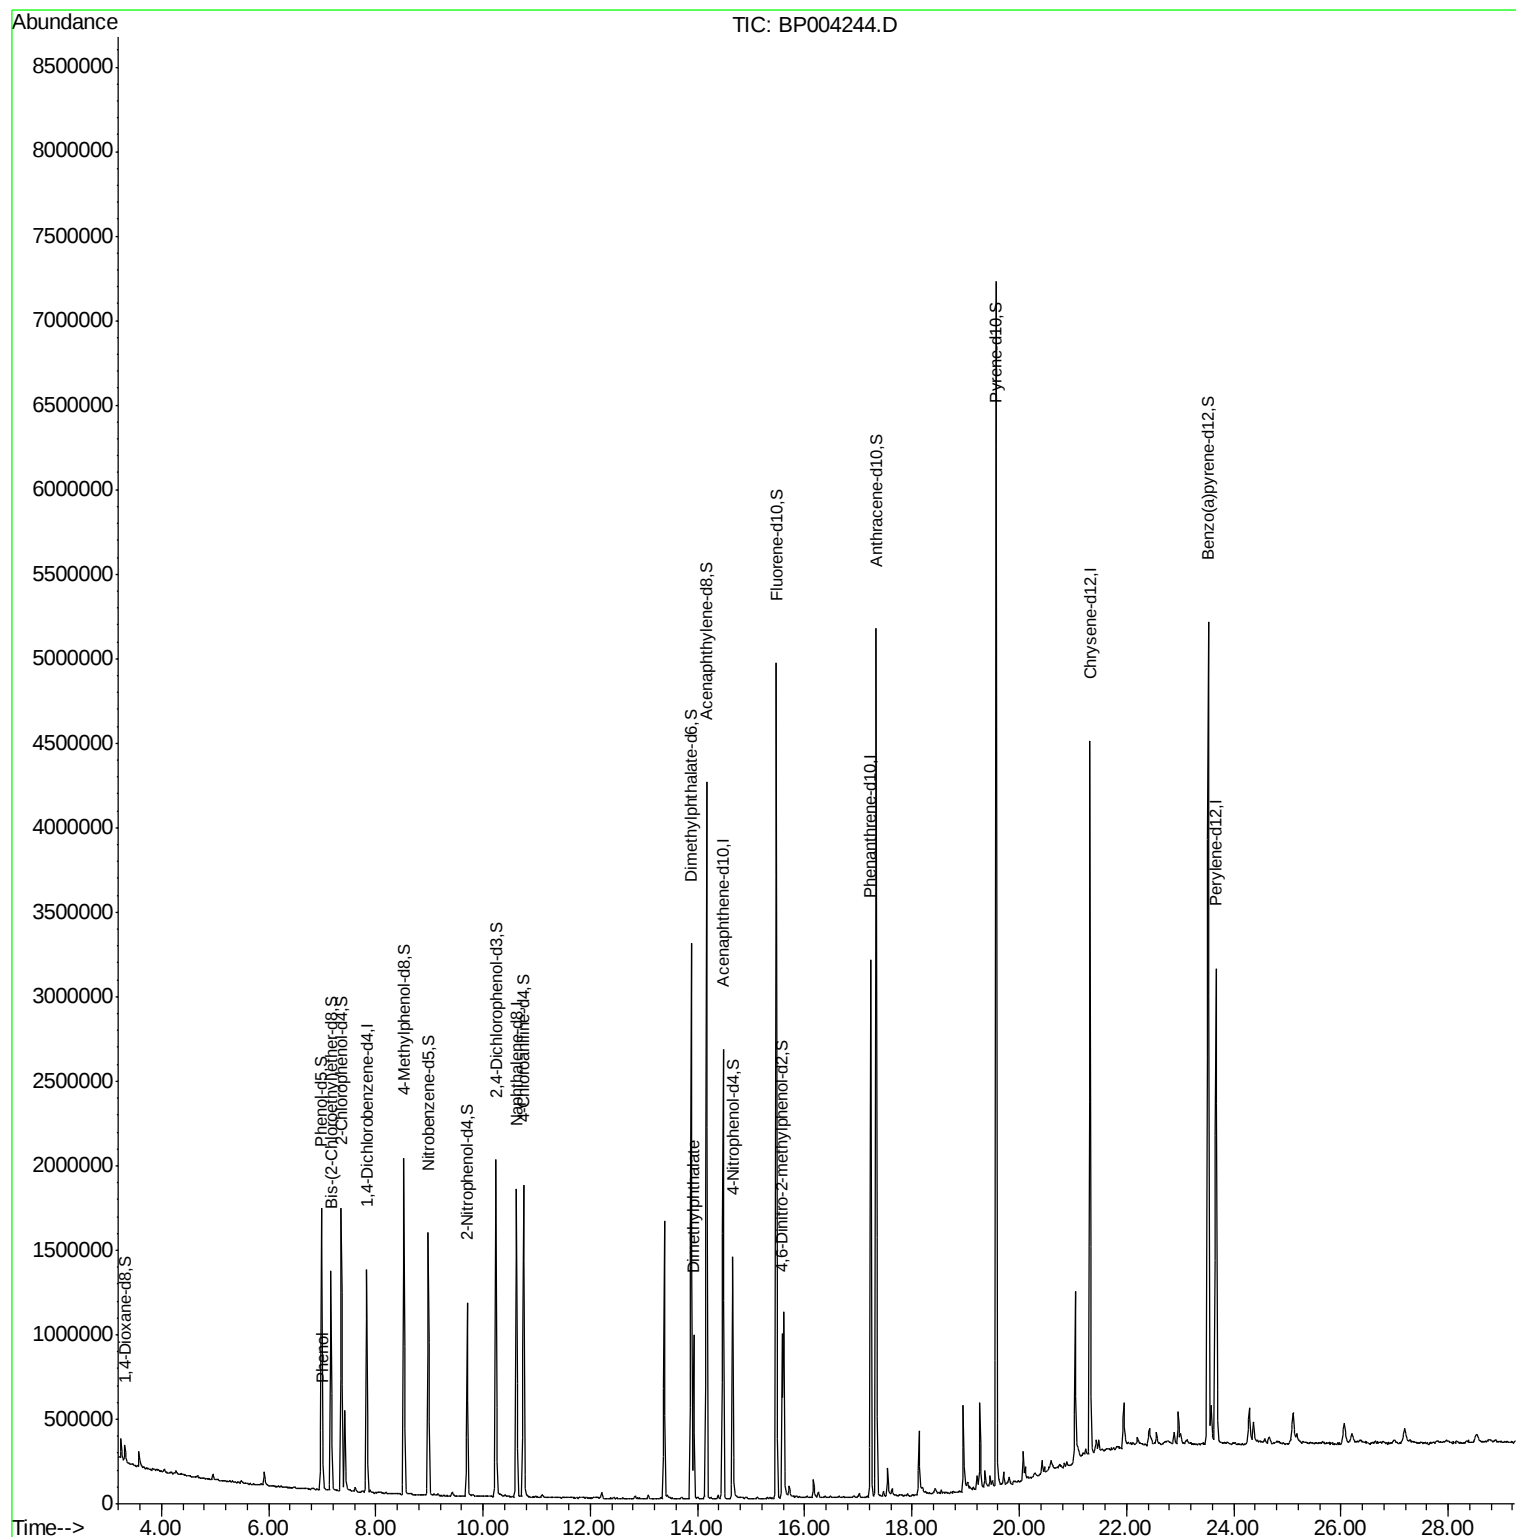


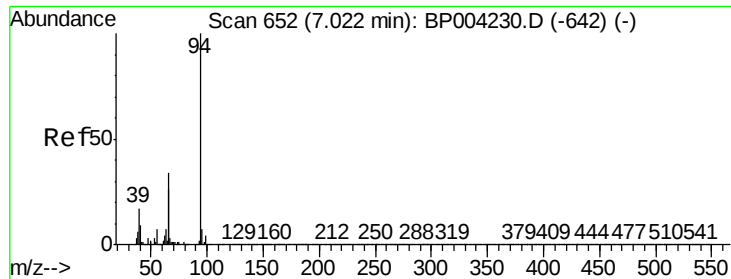

#6
Phenol
Concen: 1.897 ng/ul
RT: 7.02 min Scan# 651
Delta R.T. 0.00 min
Lab File: BP004244.D
Acq: 12 Dec 2020 00:17

Instrument :
BNA_P
ClientSampleId :
A54B0

Tot Ion	Ion	Ratio	Lower	Upper
94	100			
65	26.8	20.8	31.2	
66	35.0	26.5	39.7	

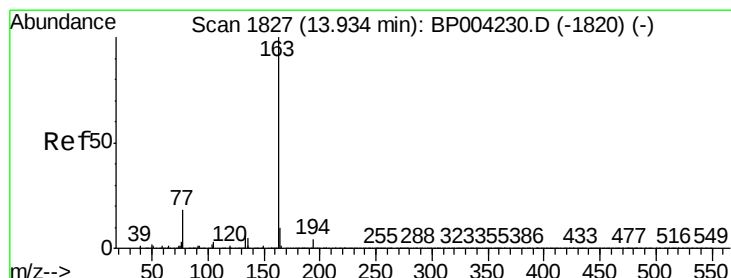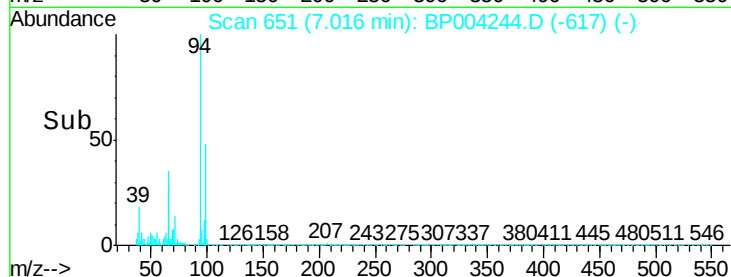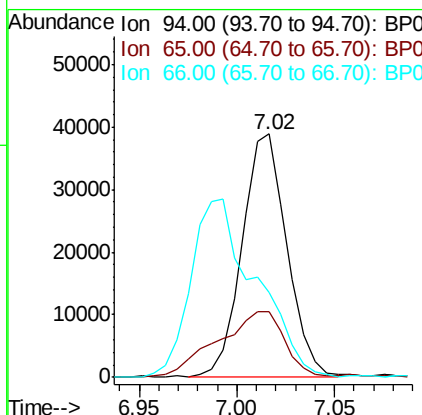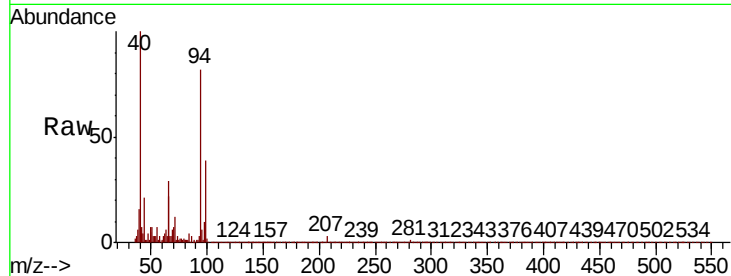

#45
Dimethylphthalate
Concen: 8.878 ng/ul
RT: 13.93 min Scan# 1826
Delta R.T. 0.00 min
Lab File: BP004244.D
Acq: 12 Dec 2020 00:17

Tgt Ion	Ion	Ratio	Lower	Upper
163	100			
194	4.4	3.4	5.2	
164	10.1	8.4	12.6	

