

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
 Data File : BP004231.D
 Acq On : 11 Dec 2020 16:55
 Operator : CG/JU
 Sample : PB133506BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	21	24	37	rVB2	88471	157382	2.13%	0.205%
2	5.922	461	465	475	rVB2	37507	72384	0.98%	0.094%
3	6.987	639	646	656	rBV	1234762	1885015	25.46%	2.457%
4	7.163	669	676	689	rVB	1011550	1632721	22.06%	2.128%
5	7.357	703	709	717	rBV	1196586	1954586	26.40%	2.548%
6	7.428	718	721	735	rVB2	42605	82391	1.11%	0.107%
7	7.828	782	789	797	rBV	1234134	1999224	27.01%	2.606%
8	8.522	900	907	918	rBV	1406279	2259982	30.53%	2.946%
9	8.981	978	985	997	rBV	1152978	1887923	25.50%	2.461%
10	9.434	1057	1062	1067	rVB2	27574	44231	0.60%	0.058%
11	9.704	1101	1108	1124	rBV	758894	1254076	16.94%	1.635%
12	10.240	1192	1199	1212	rBV	1376869	2229183	30.11%	2.906%
13	10.622	1256	1264	1275	rBV	1619523	2789301	37.68%	3.636%
14	10.751	1278	1286	1300	rVV	1379613	2362820	31.92%	3.080%
15	12.063	1504	1509	1514	rVB9	4895	9015	0.12%	0.012%
16	12.216	1527	1535	1543	rVB2	27313	49241	0.67%	0.064%
17	12.828	1635	1639	1645	rBV6	9342	14276	0.19%	0.019%
18	13.087	1677	1683	1686	rVB4	14250	20637	0.28%	0.027%
19	13.310	1717	1721	1724	rBV4	10622	13008	0.18%	0.017%
20	13.375	1727	1732	1738	rVV2	24763	42461	0.57%	0.055%
21	13.440	1738	1743	1749	rVB8	6431	11801	0.16%	0.015%
22	13.881	1811	1818	1823	rBV	2599442	3481413	47.03%	4.538%
23	13.928	1823	1826	1832	rVB	277670	352359	4.76%	0.459%
24	14.163	1856	1866	1878	rBV	3051345	4487977	60.63%	5.850%
25	14.387	1899	1904	1908	rVB6	9381	11787	0.16%	0.015%
26	14.475	1912	1919	1929	rBV	2492739	3656186	49.39%	4.766%
27	14.657	1943	1950	1962	rBV	862352	1313715	17.75%	1.712%
28	15.010	2004	2010	2016	rVB	3623	7823	0.11%	0.010%
29	15.286	2053	2057	2062	rBV6	8825	17682	0.24%	0.023%
30	15.339	2062	2066	2070	rVB5	7721	9238	0.12%	0.012%
31	15.469	2080	2088	2097	rBV	3753947	5373396	72.59%	7.004%
32	15.581	2100	2107	2118	rBV	670953	973216	13.15%	1.269%
33	15.710	2124	2129	2135	rBV	42777	60207	0.81%	0.078%
34	15.839	2146	2151	2157	rVB9	5893	11457	0.15%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
 Data File : BP004231.D
 Acq On : 11 Dec 2020 16:55
 Operator : CG/JU
 Sample : PB133506BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

35	15.898	2157	2161	2168	rVB9	5499	9479	0.13%	0.012%
36	16.033	2180	2184	2189	rBV8	7464	11730	0.16%	0.015%
37	16.163	2201	2206	2212	rBV4	14117	21527	0.29%	0.028%
38	16.257	2218	2222	2226	rVB5	16202	25576	0.35%	0.033%
39	16.381	2239	2243	2247	rVB6	5880	9763	0.13%	0.013%
40	16.481	2254	2260	2266	rVB3	16755	22102	0.30%	0.029%
41	16.910	2328	2333	2339	rVB9	8665	12549	0.17%	0.016%
42	17.010	2347	2350	2357	rVB3	13800	21536	0.29%	0.028%
43	17.233	2381	2388	2397	rVV	2993913	4299425	58.08%	5.604%
44	17.328	2398	2404	2419	rVV	4116286	5825324	78.69%	7.593%
45	17.880	2495	2498	2502	rBV6	8496	12090	0.16%	0.016%
46	18.128	2535	2540	2547	rBV3	105022	165310	2.23%	0.215%
47	18.439	2586	2593	2599	rBV3	9216	28856	0.39%	0.038%
48	18.545	2609	2611	2617	rVB6	9470	10750	0.15%	0.014%
49	18.875	2664	2667	2671	rVB4	13380	17225	0.23%	0.022%
50	19.033	2692	2694	2699	rVB6	13623	17749	0.24%	0.023%
51	19.145	2710	2713	2716	rBV5	7842	10801	0.15%	0.014%
52	19.216	2720	2725	2728	rBV	46740	67267	0.91%	0.088%
53	19.363	2746	2750	2754	rBV4	41140	58297	0.79%	0.076%
54	19.463	2762	2767	2771	rBV	38192	54811	0.74%	0.071%
55	19.569	2779	2785	2794	rBV	5475831	7297243	98.57%	9.512%
56	21.039	3031	3035	3043	rBV2	210886	289800	3.91%	0.378%
57	21.321	3078	3083	3094	rBV	4139153	5157536	69.67%	6.723%
58	23.521	3449	3457	3466	rBV	3860020	7402774	100.00%	9.649%
59	23.668	3475	3482	3500	rVB	2663829	5341414	72.15%	6.962%


Sum of corrected areas: 76719048

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
Data File : BP004231.D
Acq On : 11 Dec 2020 16:55
Operator : CG/JU
Sample : PB133506BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

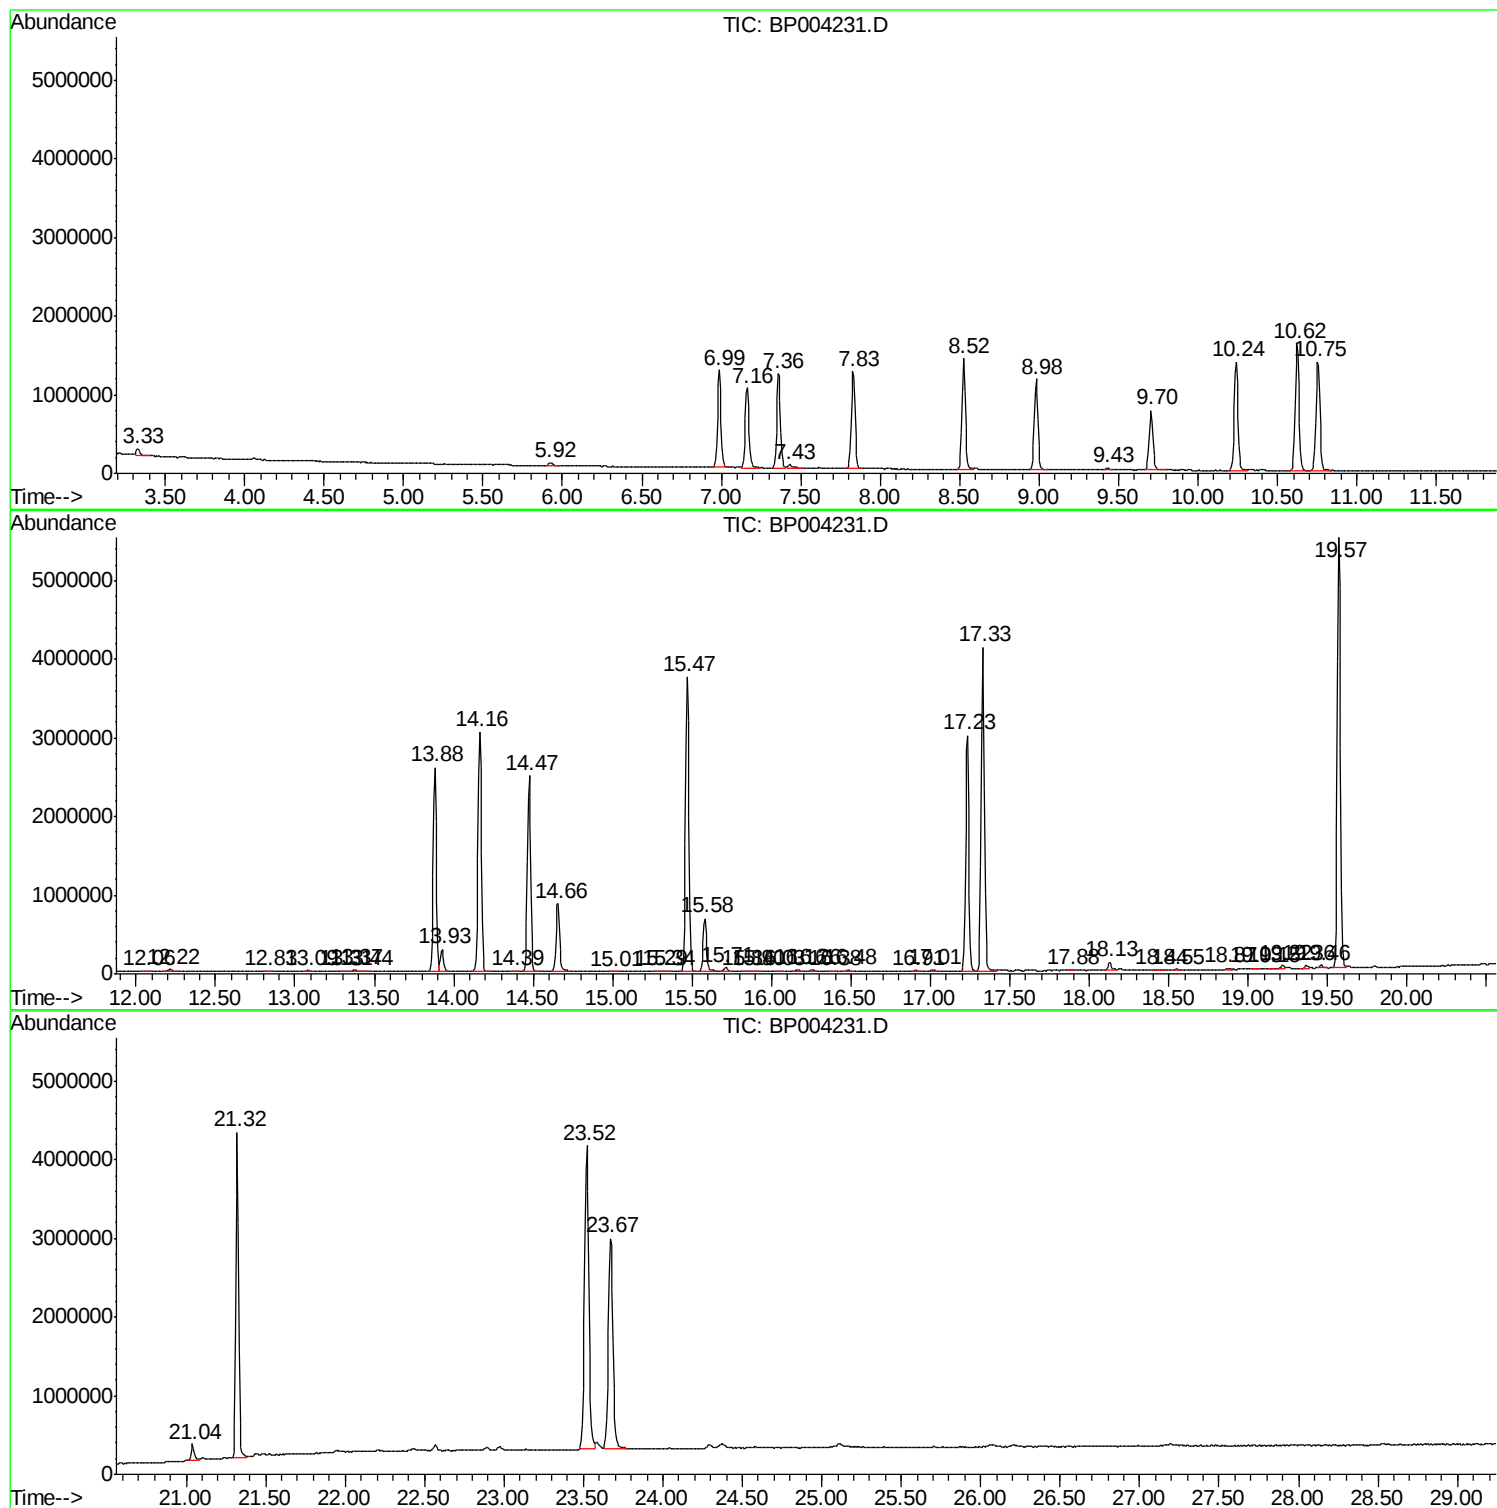

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121220\
Data File : BP004231.D
Acq On : 11 Dec 2020 16:55
Operator : CG/JU
Sample : PB133506BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121220\
Data File : BP004231.D
Acq On : 11 Dec 2020 16:55
Operator : CG/JU
Sample : PB133506BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc