

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
 Data File : BP004239.D
 Acq On : 11 Dec 2020 21:27
 Operator : CG/JU
 Sample : L5000-22
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54C1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.987	639	646	660	rBV2	924296	1753897	27.18%	2.391%
2	7.164	670	676	689	rVB	742064	1190702	18.45%	1.623%
3	7.358	703	709	717	rBV	931299	1517291	23.51%	2.068%
4	7.422	717	720	734	rVB	83609	165505	2.56%	0.226%
5	7.828	782	789	796	rBV	1456318	2319616	35.95%	3.162%
6	8.522	901	907	916	rBV	1001410	1636881	25.37%	2.231%
7	8.981	978	985	993	rVB	871343	1425449	22.09%	1.943%
8	9.152	1011	1014	1022	rVB7	10775	16632	0.26%	0.023%
9	9.428	1056	1061	1073	rVB	54403	89803	1.39%	0.122%
10	9.705	1100	1108	1119	rBV	598710	999787	15.49%	1.363%
11	10.240	1191	1199	1211	rBV	1099301	1799914	27.89%	2.453%
12	10.405	1223	1227	1232	rVB8	4370	9046	0.14%	0.012%
13	10.622	1256	1264	1272	rBV	1959184	3298511	51.12%	4.496%
14	10.752	1279	1286	1298	rBV	984034	1735180	26.89%	2.365%
15	10.975	1320	1324	1329	rBV2	16244	28353	0.44%	0.039%
16	11.163	1352	1356	1362	rVB	16591	24380	0.38%	0.033%
17	11.228	1362	1367	1370	rVV	18842	26738	0.41%	0.036%
18	11.410	1393	1398	1402	rBV7	3628	7156	0.11%	0.010%
19	11.652	1437	1439	1446	rBV8	3670	8214	0.13%	0.011%
20	12.057	1504	1508	1513	rVB4	10127	15584	0.24%	0.021%
21	12.216	1528	1535	1541	rVB3	21140	39234	0.61%	0.053%
22	12.834	1633	1640	1645	rBV5	9015	15229	0.24%	0.021%
23	13.028	1670	1673	1677	rVB5	5828	8597	0.13%	0.012%
24	13.081	1677	1682	1689	rBV3	18164	30496	0.47%	0.042%
25	13.310	1715	1721	1726	rBV3	27937	39906	0.62%	0.054%
26	13.375	1726	1732	1738	rVV5	17322	30028	0.47%	0.041%
27	13.440	1738	1743	1748	rVB8	7044	11092	0.17%	0.015%
28	13.710	1784	1789	1791	rBV5	4260	8679	0.13%	0.012%
29	13.881	1810	1818	1822	rVV	1845614	2561870	39.70%	3.492%
30	13.928	1822	1826	1837	rVV	496475	691153	10.71%	0.942%
31	14.010	1837	1840	1846	rVB8	7267	13124	0.20%	0.018%
32	14.163	1856	1866	1879	rBV	2296241	3450911	53.48%	4.704%
33	14.387	1899	1904	1909	rVB3	21186	28805	0.45%	0.039%
34	14.475	1909	1919	1926	rBV	2953447	4326205	67.04%	5.897%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
 Data File : BP004239.D
 Acq On : 11 Dec 2020 21:27
 Operator : CG/JU
 Sample : L5000-22
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54C1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

35	14.534	1926	1929	1939	rVB5	12778	24985	0.39%	0.034%
36	14.657	1939	1950	1959	rBV	600160	909815	14.10%	1.240%
37	14.822	1974	1978	1979	rBV4	5980	6863	0.11%	0.009%
38	14.881	1986	1988	1995	rVB8	11158	17739	0.27%	0.024%
39	15.016	2006	2011	2016	rVB8	4814	9915	0.15%	0.014%
40	15.116	2024	2028	2038	rVB6	10794	20036	0.31%	0.027%
41	15.293	2053	2058	2063	rBV4	9594	19148	0.30%	0.026%
42	15.340	2063	2066	2070	rVB	17616	21078	0.33%	0.029%
43	15.469	2080	2088	2095	rBV	2841953	4093512	63.44%	5.580%
44	15.522	2095	2097	2101	rVV4	10970	13988	0.22%	0.019%
45	15.581	2101	2107	2117	rVV	425913	621348	9.63%	0.847%
46	15.710	2123	2129	2134	rBV3	31777	51189	0.79%	0.070%
47	15.845	2146	2152	2154	rBV7	5341	7916	0.12%	0.011%
48	15.898	2158	2161	2165	rVB6	6858	8919	0.14%	0.012%
49	15.969	2169	2173	2176	rBV5	7650	11269	0.17%	0.015%
50	16.157	2200	2205	2210	rBV6	10570	22094	0.34%	0.030%
51	16.210	2210	2214	2217	rVV4	16095	26257	0.41%	0.036%
52	16.257	2219	2222	2230	rVB7	17267	33966	0.53%	0.046%
53	16.381	2239	2243	2246	rBV6	6085	8448	0.13%	0.012%
54	16.481	2255	2260	2264	rVB	30383	42653	0.66%	0.058%
55	16.528	2264	2268	2269	rBV4	5215	6720	0.10%	0.009%
56	16.628	2282	2285	2291	rVB8	7291	12227	0.19%	0.017%
57	16.775	2307	2310	2315	rVB6	7890	10596	0.16%	0.014%
58	16.957	2337	2341	2342	rBV4	6937	7406	0.11%	0.010%
59	17.010	2343	2350	2354	rVV3	28404	58180	0.90%	0.079%
60	17.051	2355	2357	2361	rVB5	11837	16758	0.26%	0.023%
61	17.234	2381	2388	2393	rBV	3526255	5071099	78.58%	6.912%
62	17.275	2393	2395	2399	rVV	138962	161038	2.50%	0.220%
63	17.328	2399	2404	2417	rVV	2925843	4451052	68.98%	6.067%
64	17.416	2417	2419	2425	rVV6	8021	13341	0.21%	0.018%
65	17.469	2426	2428	2432	rVB5	5513	7101	0.11%	0.010%
66	17.634	2453	2456	2460	rVB	17108	20976	0.33%	0.029%
67	17.751	2472	2476	2481	rBV4	16393	23610	0.37%	0.032%
68	18.128	2531	2540	2548	rBV3	93433	205857	3.19%	0.281%
69	18.287	2563	2567	2572	rBV5	32749	57049	0.88%	0.078%
70	18.428	2587	2591	2597	rBV5	34562	69317	1.07%	0.094%
71	18.587	2614	2618	2621	rBV	21835	30830	0.48%	0.042%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121220\
 Data File : BP004239.D
 Acq On : 11 Dec 2020 21:27
 Operator : CG/JU
 Sample : L5000-22
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54C1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

72	18.622	2621	2624	2630	rVB3	27559	42133	0.65%	0.057%
73	18.875	2663	2667	2670	rBV	39590	47283	0.73%	0.064%
74	18.986	2682	2686	2690	rBV2	32524	48411	0.75%	0.066%
75	19.034	2691	2694	2700	rVB2	49021	66392	1.03%	0.090%
76	19.245	2726	2730	2736	rVB	535459	684193	10.60%	0.933%
77	19.363	2747	2750	2753	rBV4	41006	48973	0.76%	0.067%
78	19.569	2779	2785	2795	rBV2	4263853	6453070	100.00%	8.796%
79	20.081	2869	2872	2875	rBV2	41694	46721	0.72%	0.064%
80	20.110	2875	2877	2881	rVB	75414	69276	1.07%	0.094%
81	20.592	2957	2959	2962	rBV	91148	99376	1.54%	0.135%
82	21.045	3032	3036	3041	rBV4	254319	397463	6.16%	0.542%
83	21.322	3077	3083	3087	rBV	4619603	6312512	97.82%	8.605%
84	21.357	3087	3089	3096	rVB	321276	397210	6.16%	0.541%
85	21.480	3107	3110	3115	rVB2	176749	210649	3.26%	0.287%
86	21.939	3185	3188	3195	rVB3	195650	270972	4.20%	0.369%
87	22.969	3358	3363	3378	rVB2	487264	1298388	20.12%	1.770%
88	23.522	3450	3457	3463	rBV	2733823	5184606	80.34%	7.067%
89	23.674	3476	3483	3500	rVB	3011799	6166823	95.56%	8.406%


Sum of corrected areas: 73362714

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121220\
Data File : BP004239.D
Acq On : 11 Dec 2020 21:27
Operator : CG/JU
Sample : L5000-22
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
A54C1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

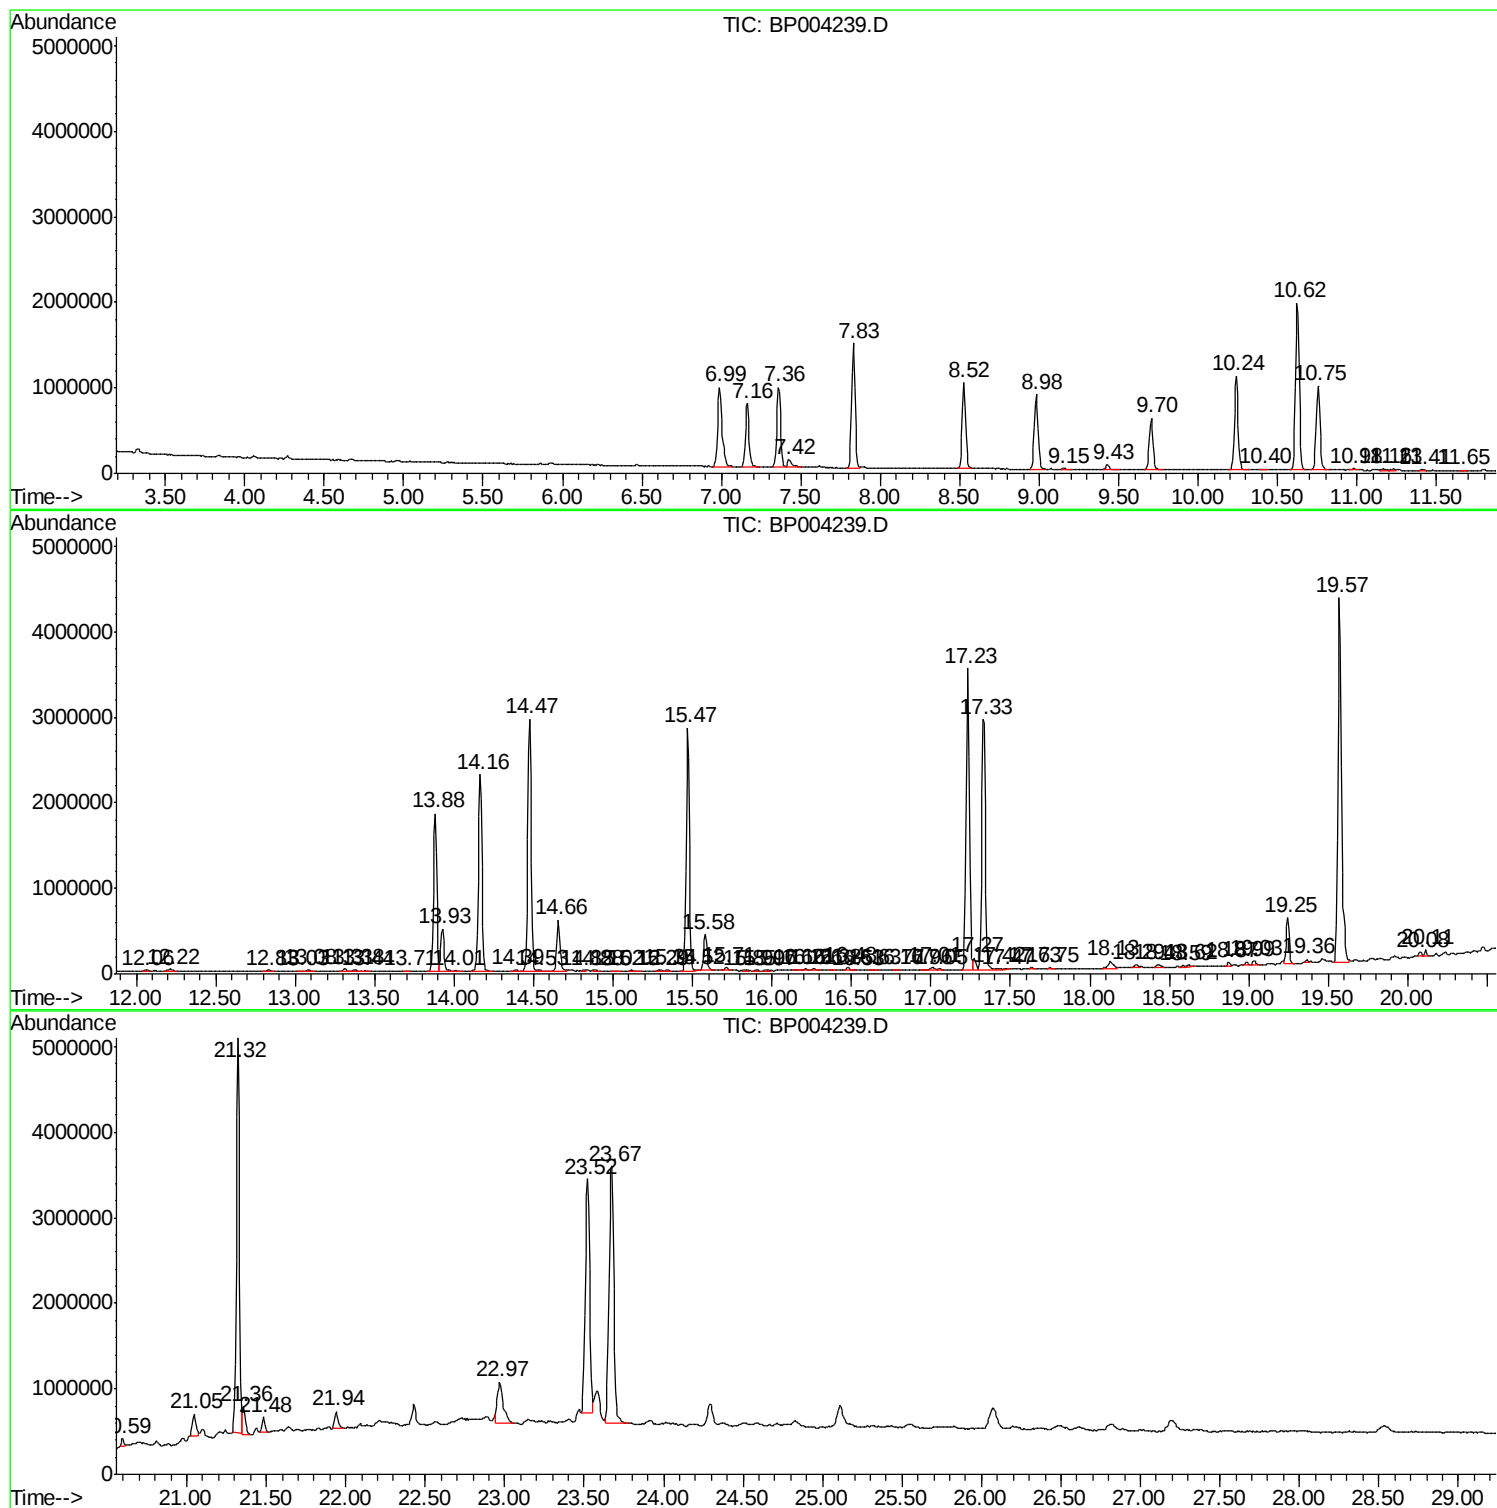

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121220\
Data File : BP004239.D
Acq On : 11 Dec 2020 21:27
Operator : CG/JU
Sample : L5000-22
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54C1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121220\
Data File : BP004239.D
Acq On : 11 Dec 2020 21:27
Operator : CG/JU
Sample : L5000-22
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54C1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc