

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121222\
 Data File : BP013080.D
 Acq On : 12 Dec 2022 10:00
 Operator : CG/JU
 Sample : N5832-09MEDL2 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXK6MEDL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013080.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.110	153	157	163	rVB	39316	51594	0.43%	0.058%
2	5.063	316	319	322	rVB4	11080	12019	0.10%	0.014%
3	7.128	664	670	677	rVB	91346	151237	1.27%	0.171%
4	7.298	694	699	709	rVB	87598	146325	1.23%	0.166%
5	7.498	727	733	740	rBV	91472	146408	1.23%	0.166%
6	7.969	806	813	822	rBV	2356657	3769422	31.64%	4.266%
7	8.510	901	905	909	rBV4	11212	19739	0.17%	0.022%
8	8.681	928	934	942	rBV	109279	184551	1.55%	0.209%
9	9.139	1005	1012	1019	rBV	89582	156067	1.31%	0.177%
10	9.863	1127	1135	1142	rBV	61544	112811	0.95%	0.128%
11	10.404	1220	1227	1239	rBV	115515	212478	1.78%	0.240%
12	10.786	1282	1292	1299	rBV	3416390	5706098	47.90%	6.458%
13	10.928	1309	1316	1331	rVB	66066	140576	1.18%	0.159%
14	12.445	1569	1574	1579	rBV8	7655	13459	0.11%	0.015%
15	13.427	1737	1741	1749	rBV9	10218	18508	0.16%	0.021%
16	13.780	1797	1801	1809	rVB9	6789	14122	0.12%	0.016%
17	13.939	1821	1828	1831	rBV6	12461	24404	0.20%	0.028%
18	14.016	1834	1841	1850	rVV	329509	477882	4.01%	0.541%
19	14.151	1857	1864	1865	rBV5	7560	13825	0.12%	0.016%
20	14.310	1885	1891	1905	rBV2	285193	514051	4.31%	0.582%
21	14.498	1917	1923	1927	rBV2	31239	41612	0.35%	0.047%
22	14.616	1932	1943	1949	rBV	5479586	8164939	68.54%	9.241%
23	14.674	1949	1953	1960	rVB	118374	186436	1.56%	0.211%
24	14.810	1971	1976	1983	rBV6	29426	68373	0.57%	0.077%
25	14.922	1988	1995	2000	rVV9	11345	22562	0.19%	0.026%
26	15.010	2005	2010	2017	rVV	97055	151408	1.27%	0.171%
27	15.086	2019	2023	2025	rVB4	11384	13584	0.11%	0.015%
28	15.233	2043	2048	2053	rVB9	11733	20930	0.18%	0.024%
29	15.280	2053	2056	2059	rBV3	11083	13471	0.11%	0.015%
30	15.398	2070	2076	2078	rBV7	9560	17826	0.15%	0.020%
31	15.451	2081	2085	2090	rVB	41920	50900	0.43%	0.058%
32	15.604	2104	2111	2116	rBV	516715	738837	6.20%	0.836%
33	15.663	2116	2121	2126	rVB	234056	327310	2.75%	0.370%
34	15.721	2127	2131	2135	rBV2	56192	83551	0.70%	0.095%
35	15.786	2139	2142	2145	rVB2	22991	24954	0.21%	0.028%
36	15.827	2145	2149	2151	rBV5	16250	17509	0.15%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121222\
 Data File : BP013080.D
 Acq On : 12 Dec 2022 10:00
 Operator : CG/JU
 Sample : N5832-09MEDL2 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXK6MEDL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

37	15.916	2160	2164	2167	rVB4	13787	16776	0.14%	0.019%
38	15.957	2167	2171	2177	rVB	58084	89139	0.75%	0.101%
39	16.010	2177	2180	2185	rBV6	8296	15080	0.13%	0.017%
40	16.104	2187	2196	2203	rBV2	60205	145139	1.22%	0.164%
41	16.316	2227	2232	2235	rBV2	101146	150011	1.26%	0.170%
42	16.633	2282	2286	2287	rBV4	9710	13161	0.11%	0.015%
43	16.668	2287	2292	2297	rVV4	44858	82084	0.69%	0.093%
44	16.721	2298	2301	2306	rVB6	28541	39852	0.33%	0.045%
45	16.768	2306	2309	2311	rBV4	10051	14310	0.12%	0.016%
46	16.898	2327	2331	2334	rBV2	28802	38524	0.32%	0.044%
47	16.939	2334	2338	2341	rVV3	28403	37164	0.31%	0.042%
48	17.021	2347	2352	2358	rBV3	67366	105882	0.89%	0.120%
49	17.116	2361	2368	2372	rVV4	94312	182646	1.53%	0.207%
50	17.186	2372	2380	2388	rVB3	110834	250755	2.10%	0.284%
51	17.368	2405	2411	2415	rBV	6838551	10051163	84.37%	11.376%
52	17.410	2415	2418	2423	rVV	1677115	2264067	19.00%	2.563%
53	17.468	2423	2428	2430	rVV2	535976	767882	6.45%	0.869%
54	17.504	2430	2434	2440	rVB	4431204	5997723	50.35%	6.788%
55	17.651	2455	2459	2466	rVB	38713	68776	0.58%	0.078%
56	17.774	2475	2480	2490	rBV	323843	508763	4.27%	0.576%
57	17.851	2490	2493	2496	rVV	68183	85271	0.72%	0.097%
58	17.886	2496	2499	2505	rVB	74342	95404	0.80%	0.108%
59	17.951	2506	2510	2512	rBV2	31103	45262	0.38%	0.051%
60	18.233	2554	2558	2562	rBV2	167174	214339	1.80%	0.243%
61	18.280	2562	2566	2572	rVB	220908	310305	2.60%	0.351%
62	18.357	2575	2579	2584	rBV	141213	184687	1.55%	0.209%
63	18.427	2585	2591	2594	rBV	620760	954948	8.02%	1.081%
64	18.521	2604	2607	2611	rBV2	80645	103980	0.87%	0.118%
65	18.715	2636	2640	2643	rBV	119640	146201	1.23%	0.165%
66	18.757	2643	2647	2653	rVB2	79884	115701	0.97%	0.131%
67	18.951	2677	2680	2685	rVB2	49158	63804	0.54%	0.072%
68	19.004	2686	2689	2691	rVV2	40078	45285	0.38%	0.051%
69	19.039	2692	2695	2698	rVB	46605	55177	0.46%	0.062%
70	19.121	2704	2709	2713	rBV2	112543	220830	1.85%	0.250%
71	19.257	2727	2732	2740	rBV	250818	439632	3.69%	0.498%
72	19.374	2746	2752	2758	rBV	5081724	6450381	54.14%	7.301%
73	19.468	2765	2768	2772	rVB	72749	93158	0.78%	0.105%
74	19.610	2789	2792	2797	rVB	169452	216728	1.82%	0.245%
75	19.698	2801	2807	2809	rBV2	1430858	2213874	18.58%	2.506%
76	19.727	2809	2812	2819	rVV	4209106	5176310	43.45%	5.859%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121222\
 Data File : BP013080.D
 Acq On : 12 Dec 2022 10:00
 Operator : CG/JU
 Sample : N5832-09MEDL2 20X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBXK6MEDL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
 Title : SVOA CALIBRATION

77	19.792	2820	2823	2829	rVB2	136263	203591	1.71%	0.230%
78	19.898	2837	2841	2847	rBV	206668	282529	2.37%	0.320%
79	19.962	2849	2852	2857	rVB	118817	156604	1.31%	0.177%
80	20.045	2860	2866	2872	rBV3	196526	494816	4.15%	0.560%
81	20.204	2883	2893	2899	rBV2	356500	878611	7.38%	0.994%
82	20.304	2907	2910	2913	rBV	158220	183271	1.54%	0.207%
83	20.362	2914	2920	2924	rVV2	242925	427218	3.59%	0.484%
84	20.498	2940	2943	2946	rBV	159117	204724	1.72%	0.232%
85	20.545	2948	2951	2954	rVB2	135043	164386	1.38%	0.186%
86	20.939	3015	3018	3023	rBV	159217	202235	1.70%	0.229%
87	21.104	3043	3046	3049	rBV	200306	229641	1.93%	0.260%
88	21.139	3049	3052	3055	rVV2	236169	282513	2.37%	0.320%
89	21.180	3056	3059	3063	rVB2	272941	340335	2.86%	0.385%
90	21.456	3099	3106	3110	rBV2	7640207	11913164	100.00%	13.484%
91	21.492	3110	3112	3123	rVB	1196738	1590806	13.35%	1.800%
92	23.180	3393	3399	3405	rBV2	642287	1613149	13.54%	1.826%
93	23.945	3522	3529	3538	rBV2	4645953	9286049	77.95%	10.510%




Sum of corrected areas: 88353594

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121222\
Data File : BP013080.D
Acq On : 12 Dec 2022 10:00
Operator : CG/JU
Sample : N5832-09MEDL2 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXK6MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

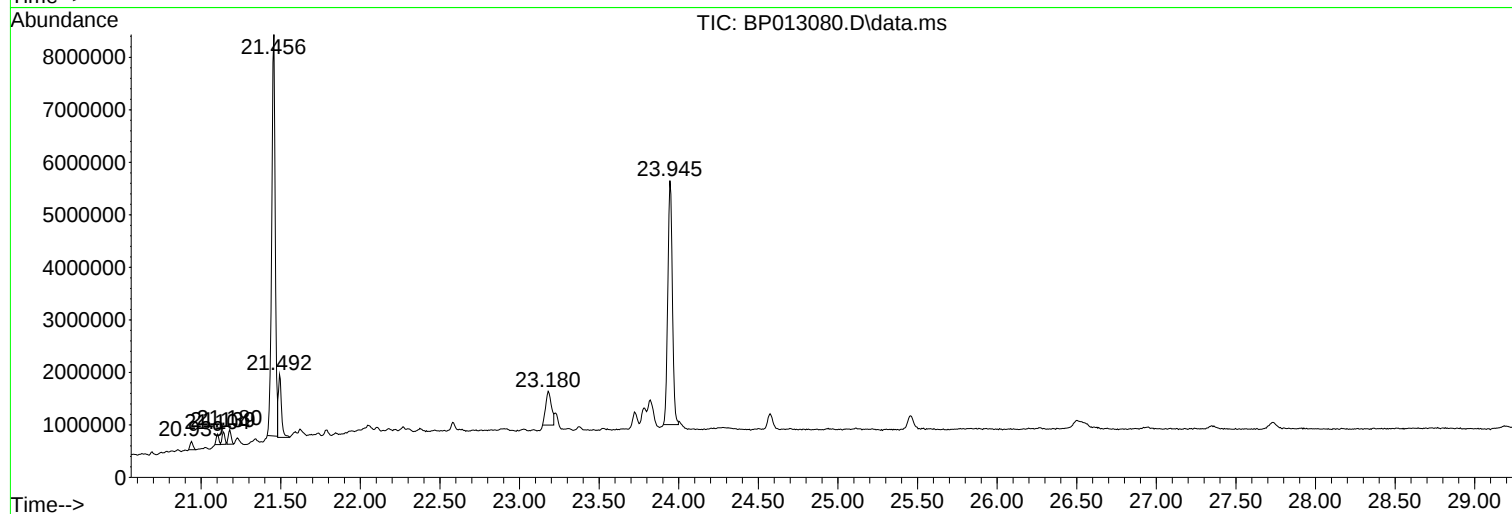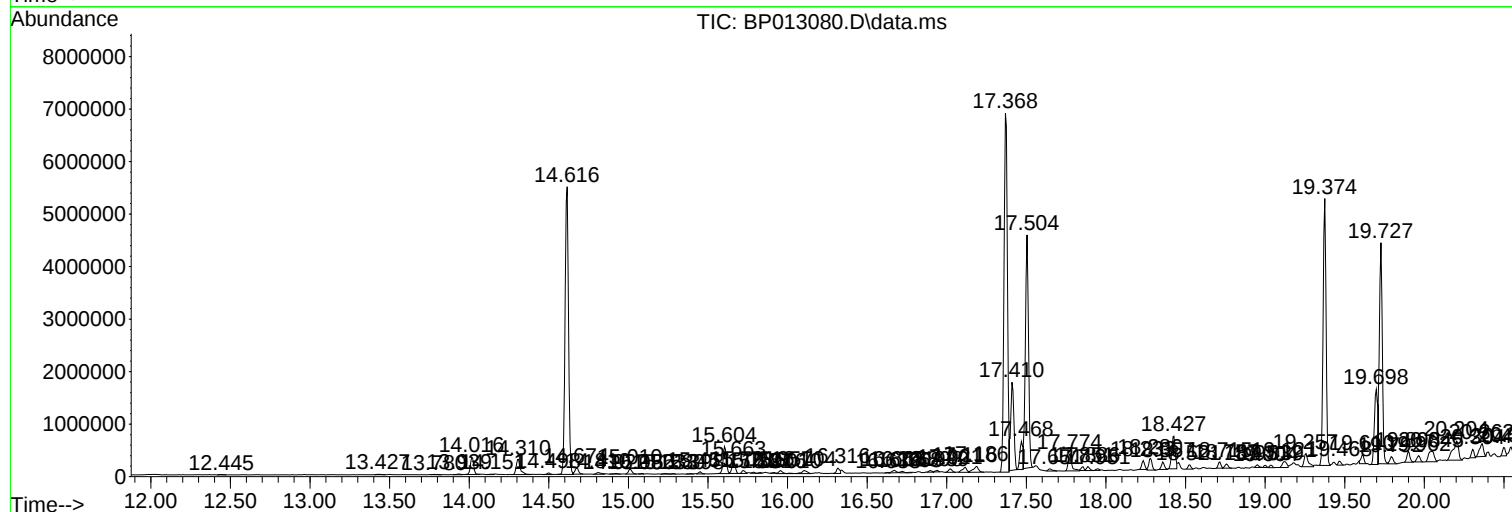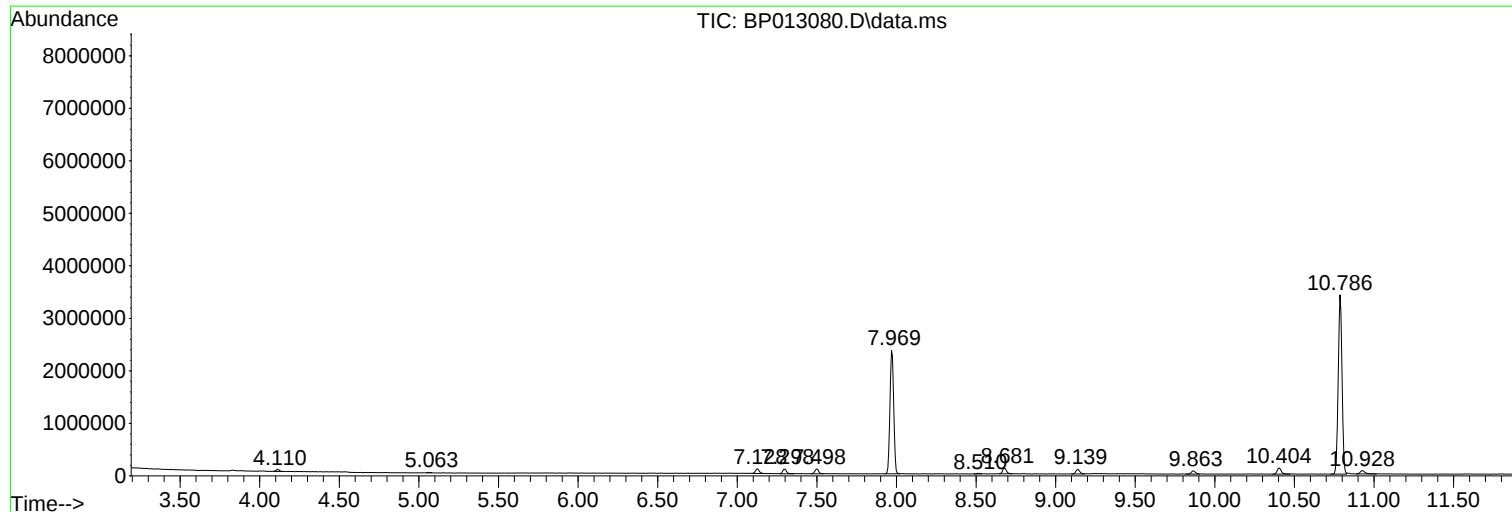

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121222\
Data File : BP013080.D
Acq On : 12 Dec 2022 10:00
Operator : CG/JU
Sample : N5832-09MEDL2 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXK6MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121222\
Data File : BP013080.D
Acq On : 12 Dec 2022 10:00
Operator : CG/JU
Sample : N5832-09MEDL2 20X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBXK6MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc