
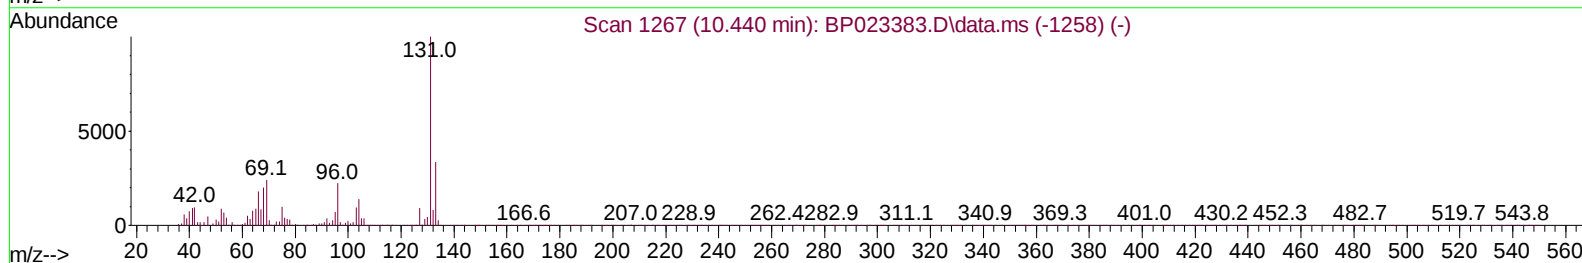
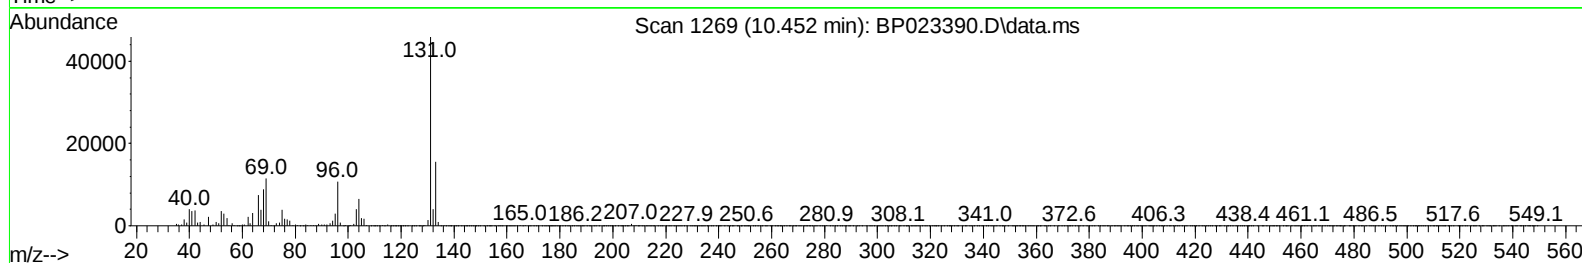


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023390.D
Acq On : 12 Dec 2024 10:27
Operator : RC/JU
Sample : PB165481BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 13 00:23:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

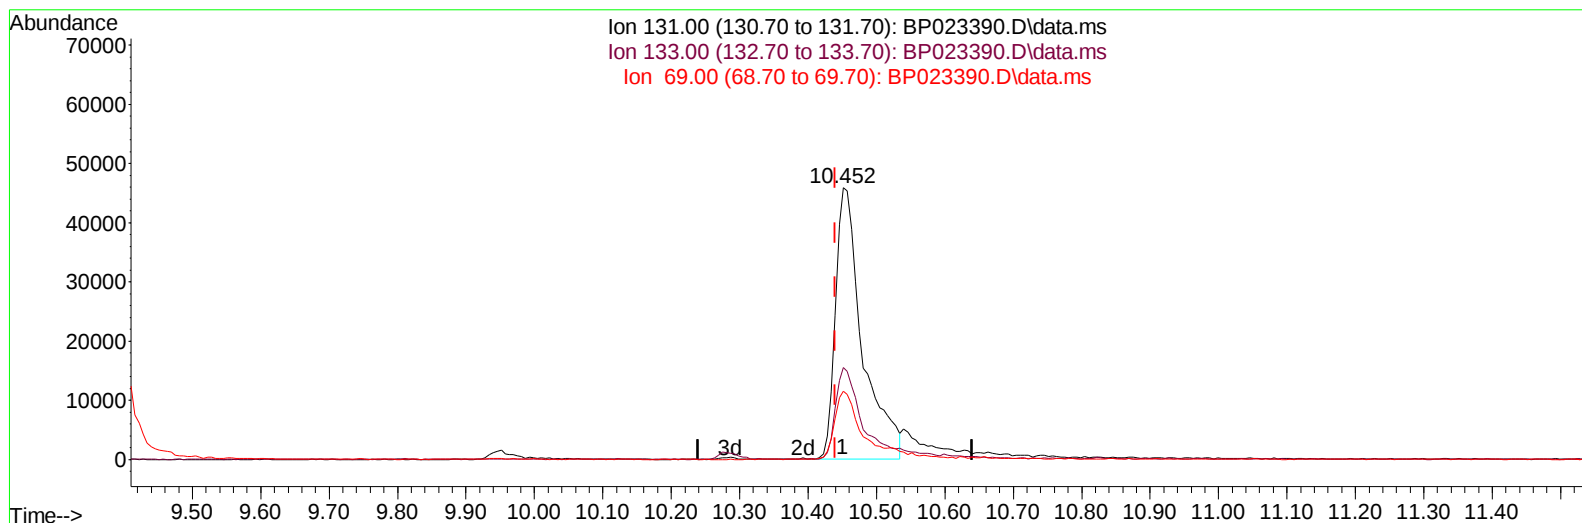

TIC: BP023390.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.452min (+ 0.012) 22.11 ng/u1

response 125187

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	33.90
69.00	24.30	25.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023390.D
Acq On : 12 Dec 2024 10:27
Operator : RC/JU
Sample : PB165481BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 13 00:23:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

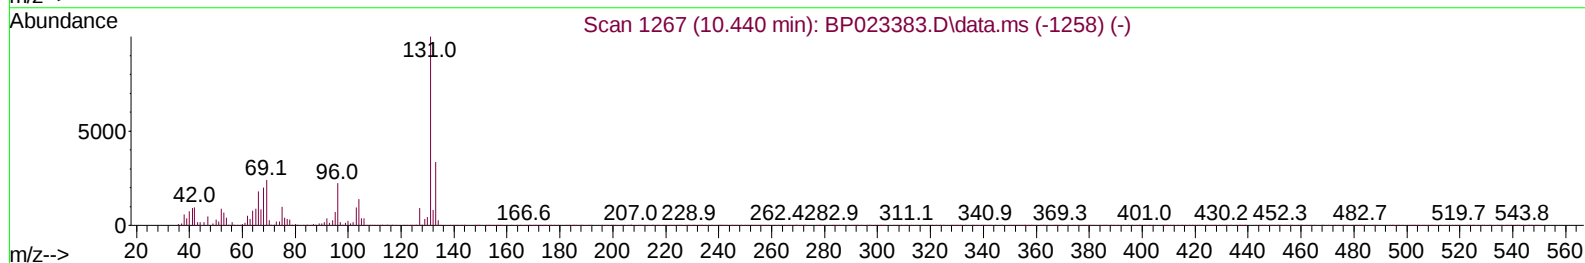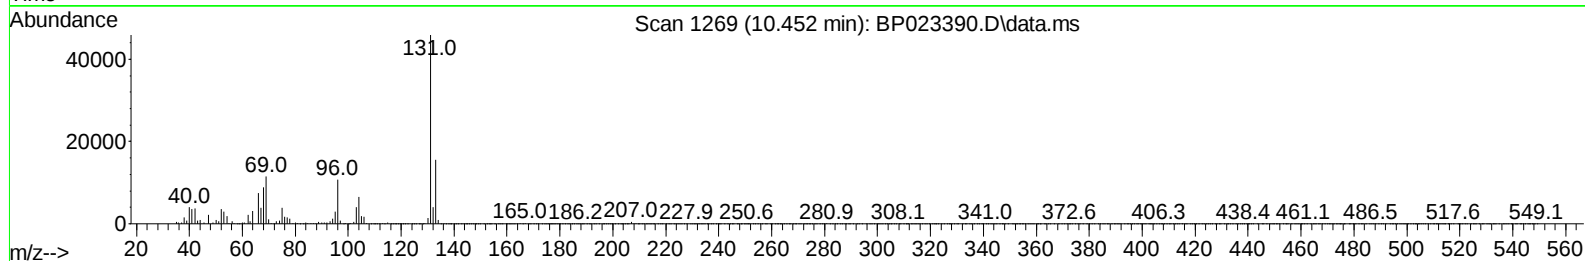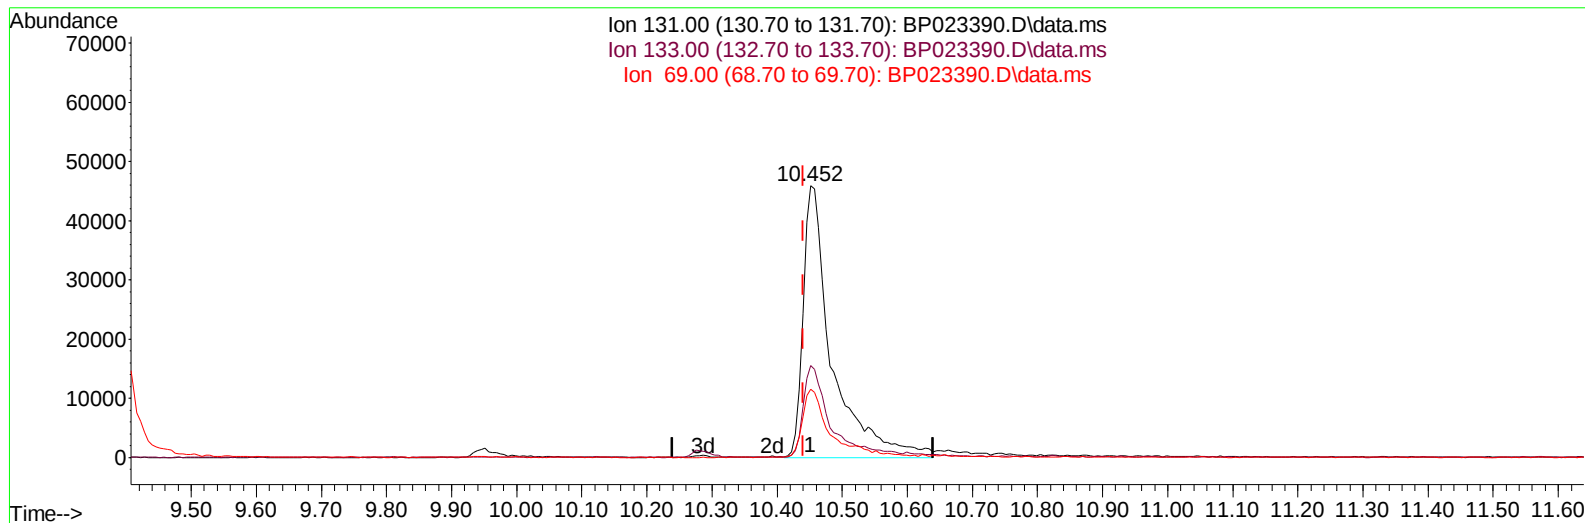

TIC: BP023390.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.452min (+ 0.012) 24.85 ng/ul m

response 140723

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	33.90
69.00	24.30	25.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023390.D
Acq On : 12 Dec 2024 10:27
Operator : RC/JU
Sample : PB165481BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 13 00:23:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

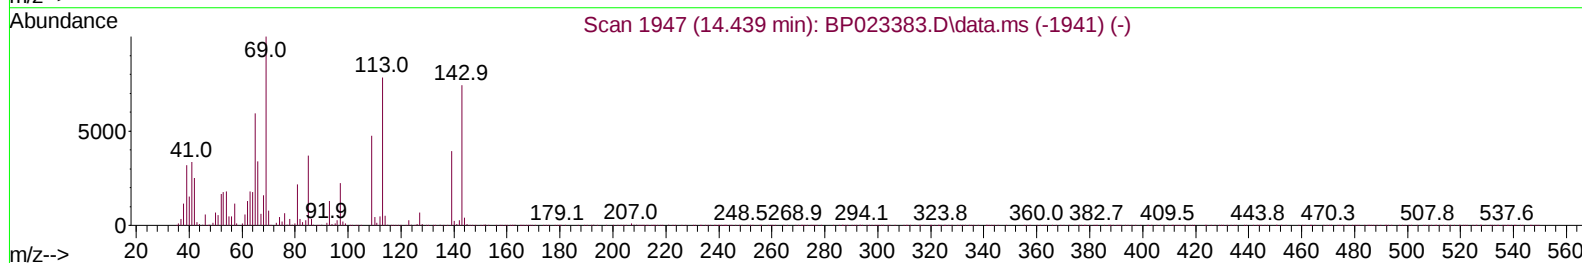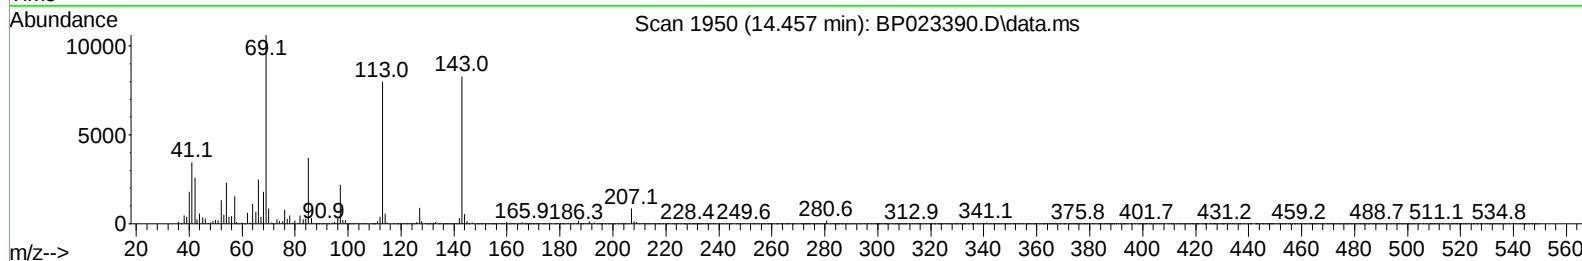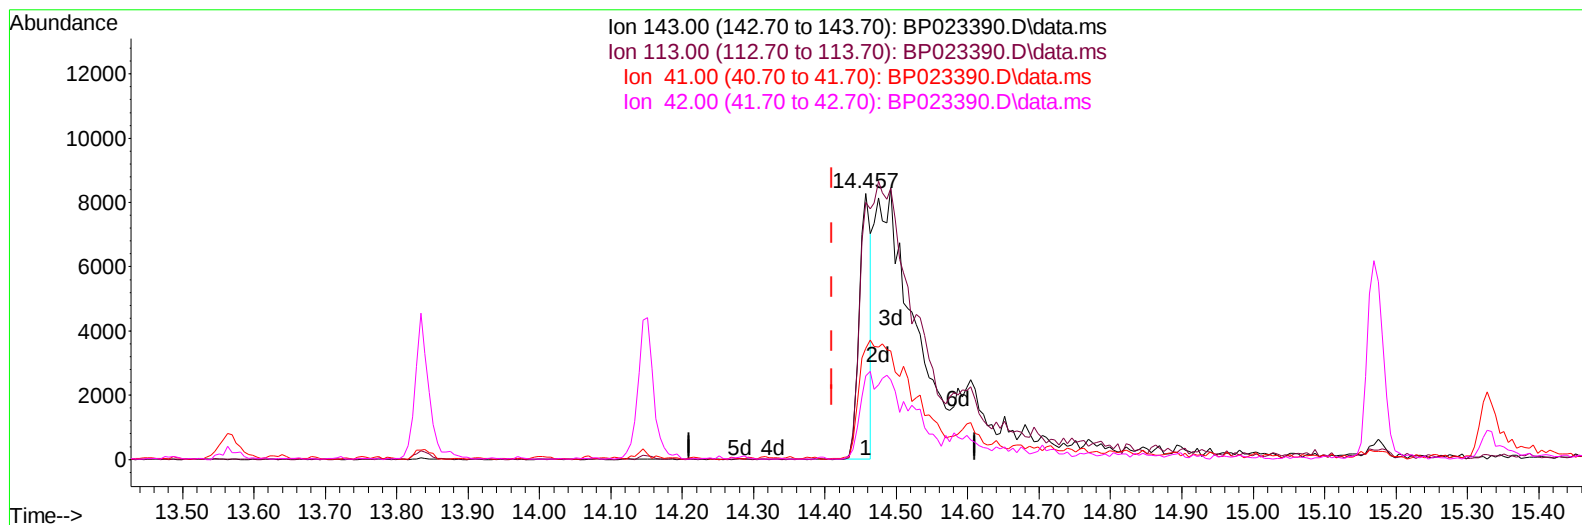

TIC: BP023390.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.457min (+ 0.047) 4.88 ng/ul

response 9252

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	96.62
41.00	45.60	41.84
42.00	31.70	31.47

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023390.D
Acq On : 12 Dec 2024 10:27
Operator : RC/JU
Sample : PB165481BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 13 00:23:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

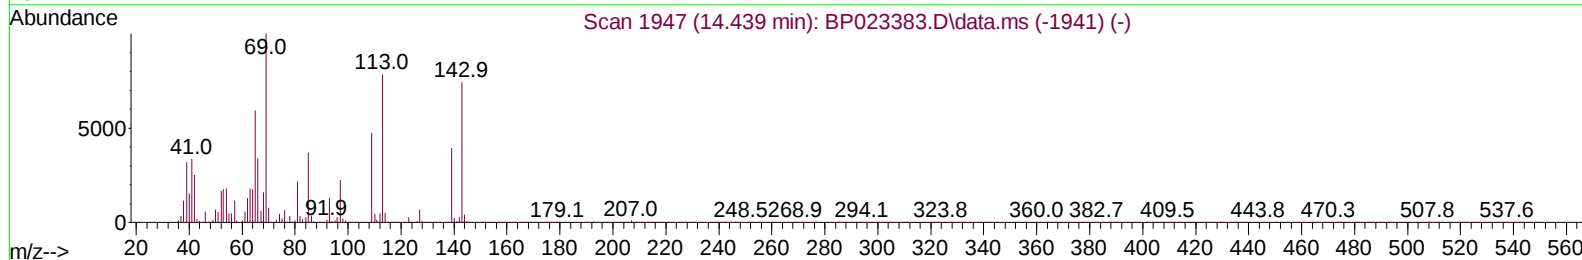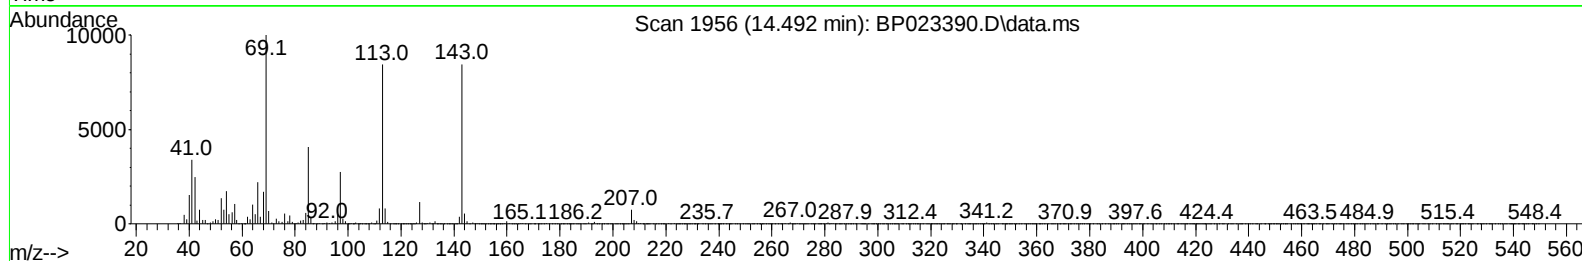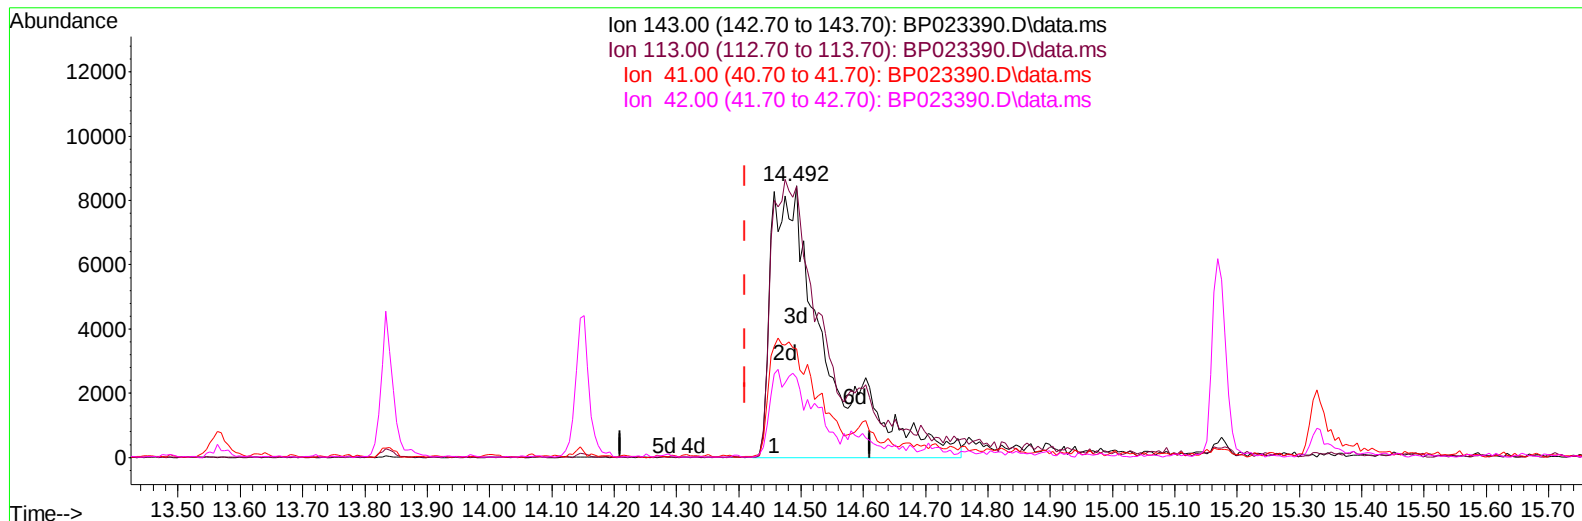

TIC: BP023390.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.492min (+ 0.082) 27.43 ng/ul m

response 51993

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	99.93
41.00	45.60	40.03
42.00	31.70	29.44

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023390.D
Acq On : 12 Dec 2024 10:27
Operator : RC/JU
Sample : PB165481BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 13 00:23:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

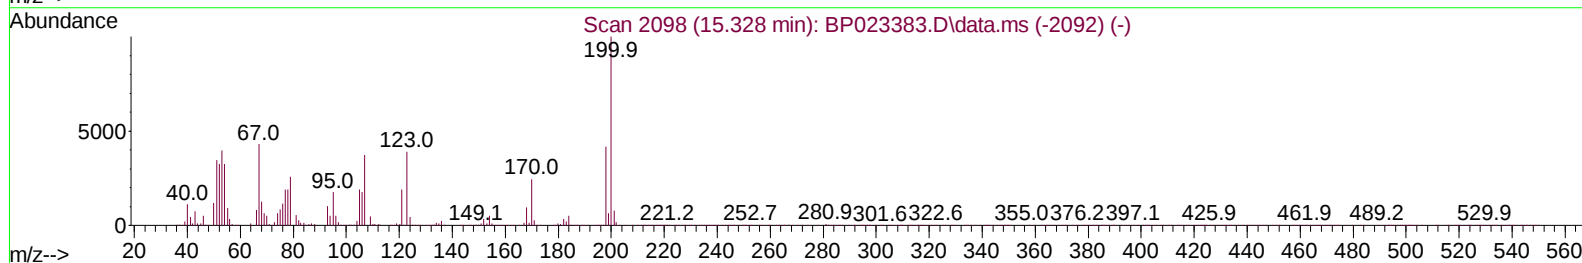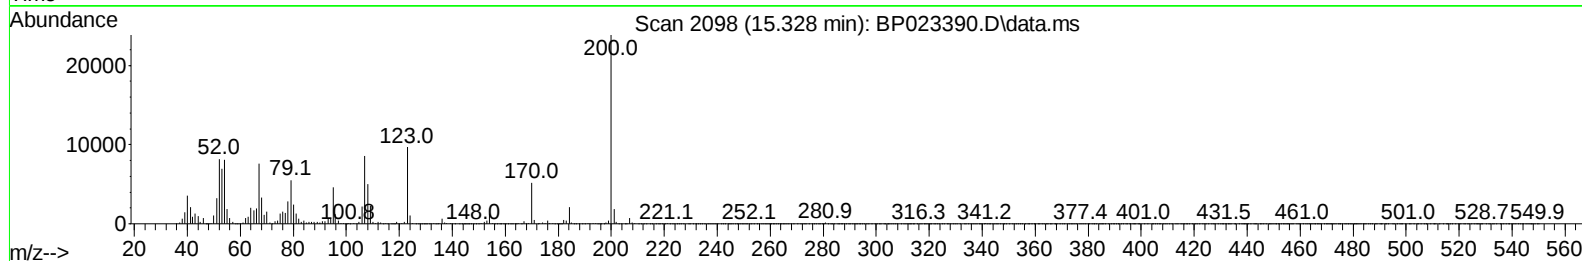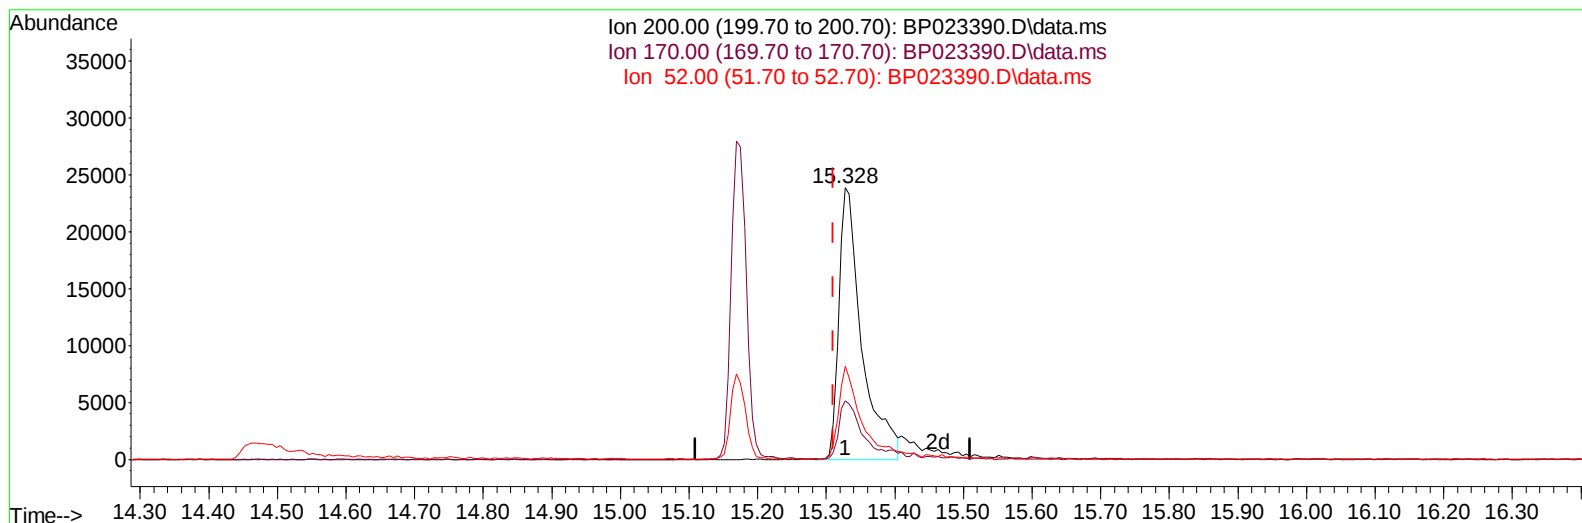

TIC: BP023390.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)




15.328min (+ 0.018) 18.66 ng/u1

response 55602

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	21.64
52.00	37.90	34.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023390.D
Acq On : 12 Dec 2024 10:27
Operator : RC/JU
Sample : PB165481BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 13 00:23:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

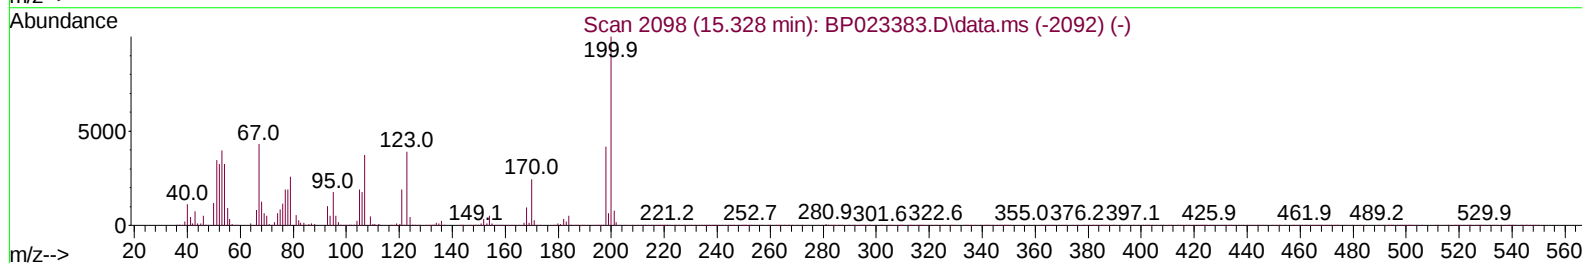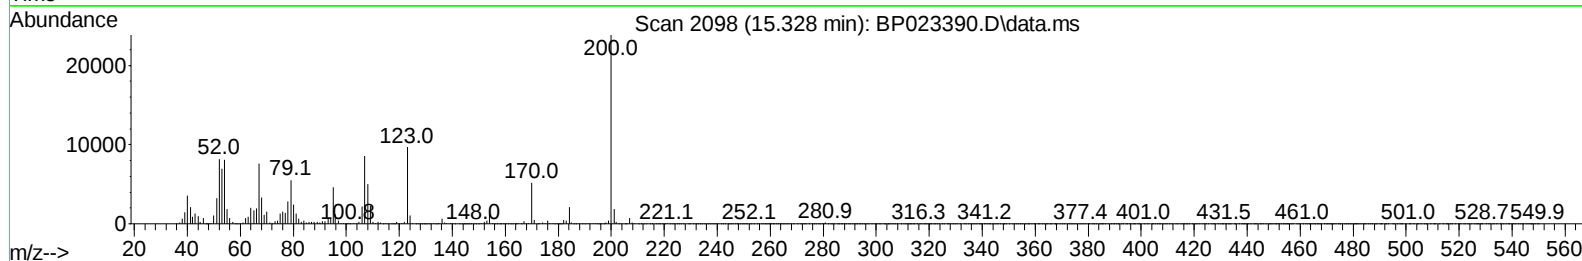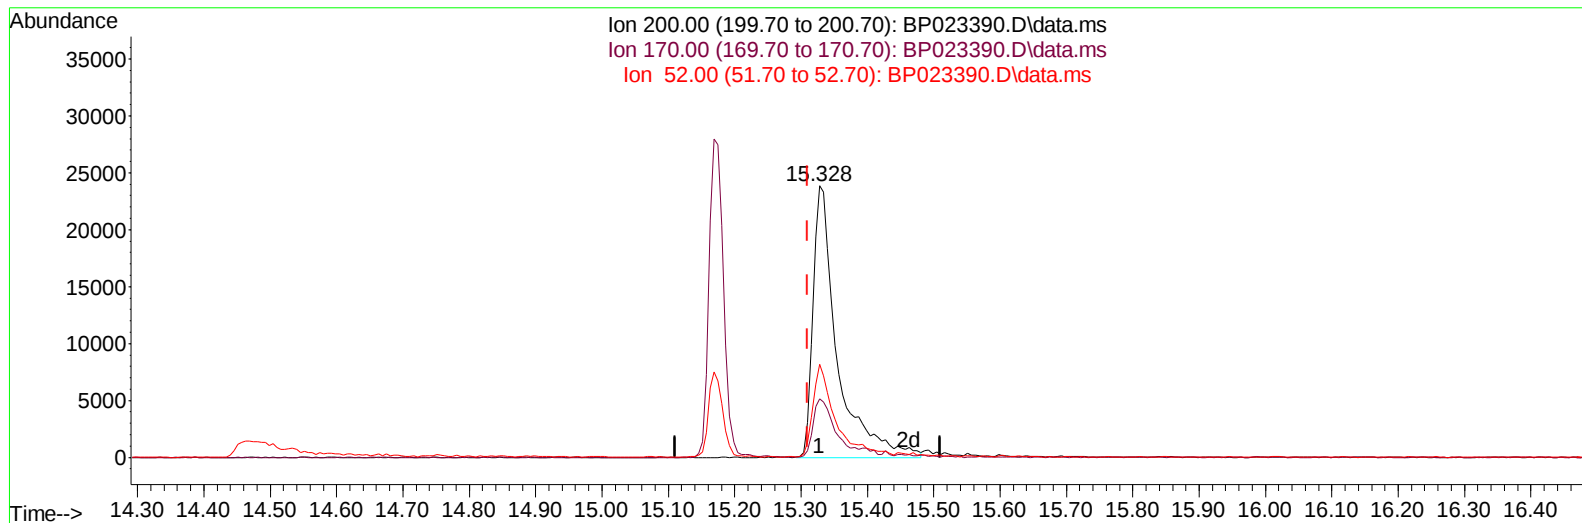

TIC: BP023390.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)**15.328min (+ 0.018) 20.29 ng/ul m****response 60463**

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	21.64
52.00	37.90	34.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
 Data File : BP023390.D
 Acq On : 12 Dec 2024 10:27
 Operator : RC/JU
 Sample : PB165481BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 13 00:25:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.534	152	77696	20.000	ng/ul	0.00
20) Naphthalene-d8	10.281	136	278309	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	199217	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.963	188	493040	20.000	ng/ul	0.00
79) Chrysene-d12	21.386	240	567293	20.000	ng/ul	0.00
88) Perylene-d12	24.557	264	646354	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	12381	5.867	ng/uL	0.00
4) Pyridine-d5	3.517	84	141842	26.138	ng/ul	0.00
7) Phenol-d5	6.752	99	160040	26.252	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.887	67	103911	27.017	ng/ul	0.00
11) 2-Chlorophenol-d4	7.087	132	121490	27.002	ng/ul	0.00
15) 4-Methylphenol-d8	8.252	113	123944	25.191	ng/ul	0.00
21) Nitrobenzene-d5	8.681	128	52642	25.330	ng/ul	0.00
24) 2-Nitrophenol-d4	9.399	143	61596	25.717	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.946	165	120995	23.935	ng/ul	0.01
31) 4-Chloroaniline-d4	10.452	131	140723m	24.849	ng/ul	0.01
46) Dimethylphthalate-d6	13.569	166	412508	26.673	ng/ul	0.01
49) Acenaphthylene-d8	13.834	160	424229	26.006	ng/ul	0.00
54) 4-Nitrophenol-d4	14.492	143	51993m	27.435	ng/ul	0.08
60) Fluorene-d10	15.169	176	358934	26.387	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.328	200	60463m	20.291	ng/ul	0.02
73) Anthracene-d10	17.063	188	592163	26.316	ng/ul	0.01
81) Pyrene-d10	19.451	212	778973	26.282	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.333	264	917104	26.505	ng/ul	-0.01

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023390.D
Acq On : 12 Dec 2024 10:27
Operator : RC/JU
Sample : PB165481BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Dec 13 00:25:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

