
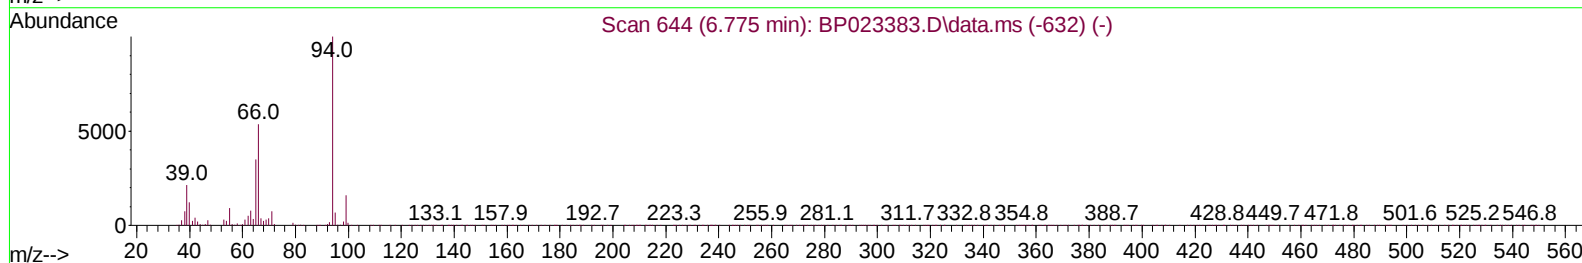
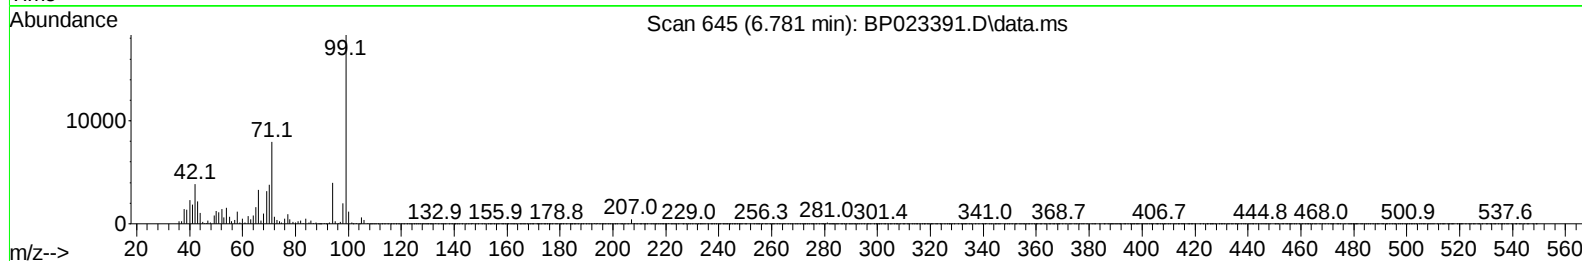


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023391.D
Acq On : 12 Dec 2024 11:47
Operator : RC/JU
Sample : P5153-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 13 00:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

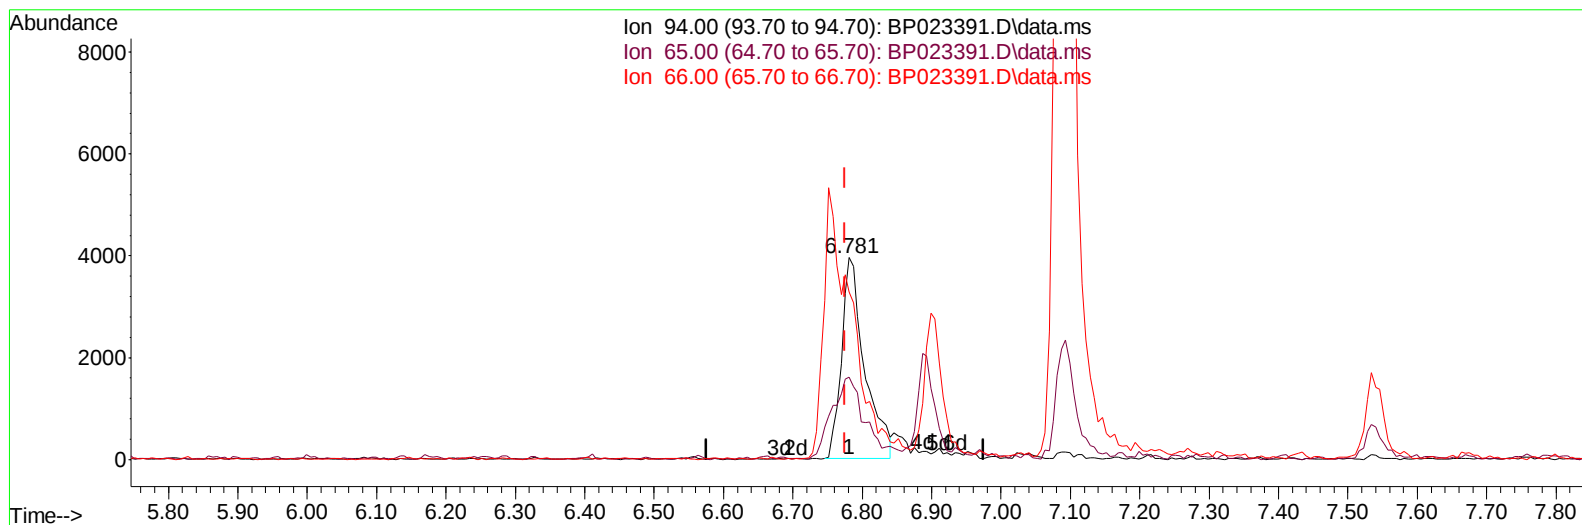

TIC: BP023391.D\data.ms

(8) Phenol




6.781min (+ 0.006) 1.12 ng/u1

response 9131

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	35.00	40.89
66.00	52.50	82.91#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023391.D
Acq On : 12 Dec 2024 11:47
Operator : RC/JU
Sample : P5153-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 13 00:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

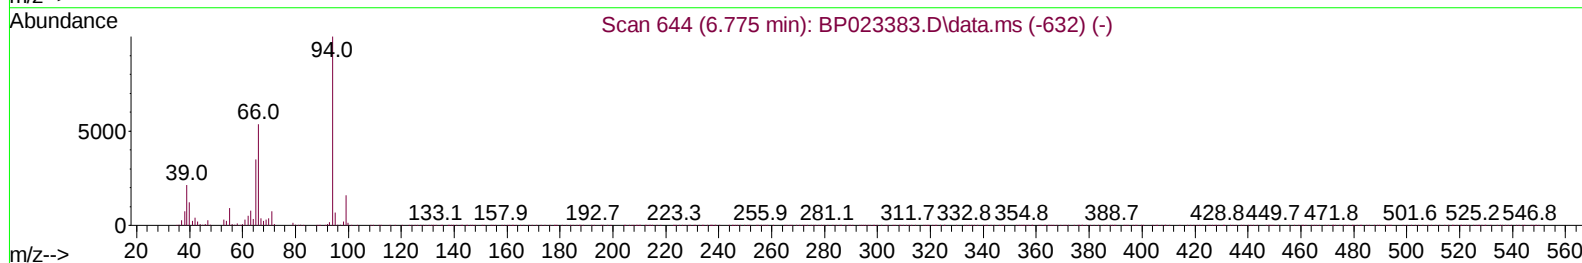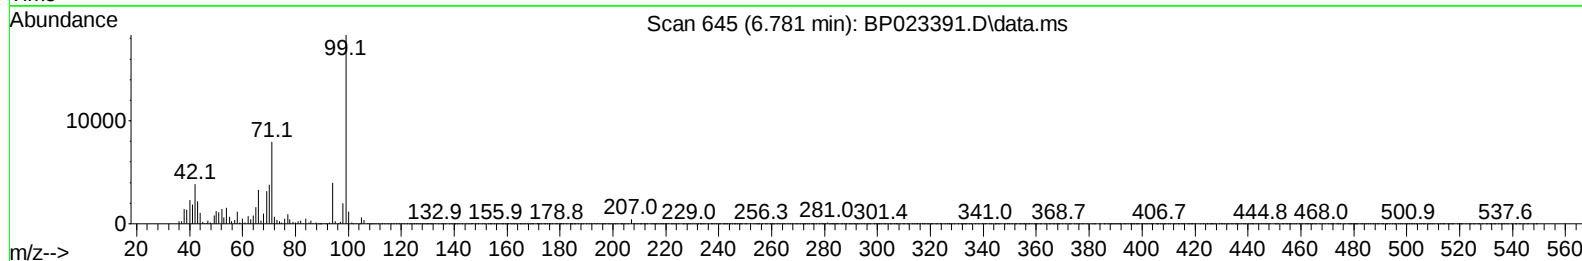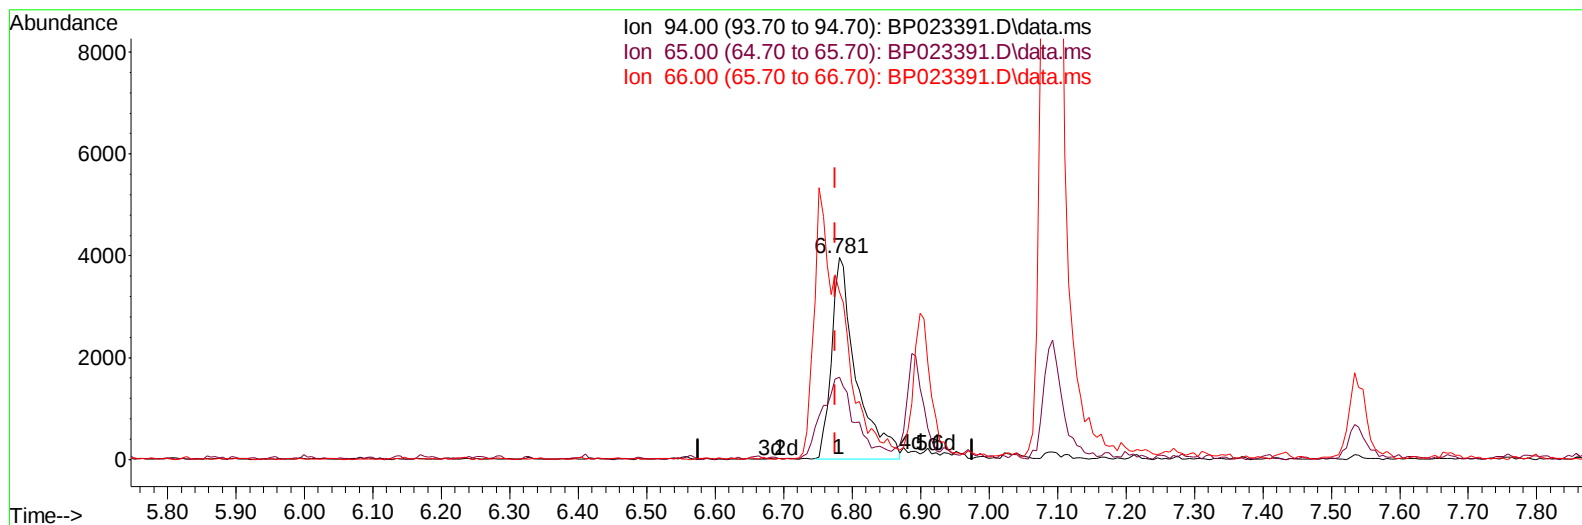

TIC: BP023391.D\data.ms

(8) Phenol




6.781min (+ 0.006) 1.21 ng/ul m

response 9813

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	35.00	40.89
66.00	52.50	82.91#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023391.D
Acq On : 12 Dec 2024 11:47
Operator : RC/JU
Sample : P5153-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 13 00:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

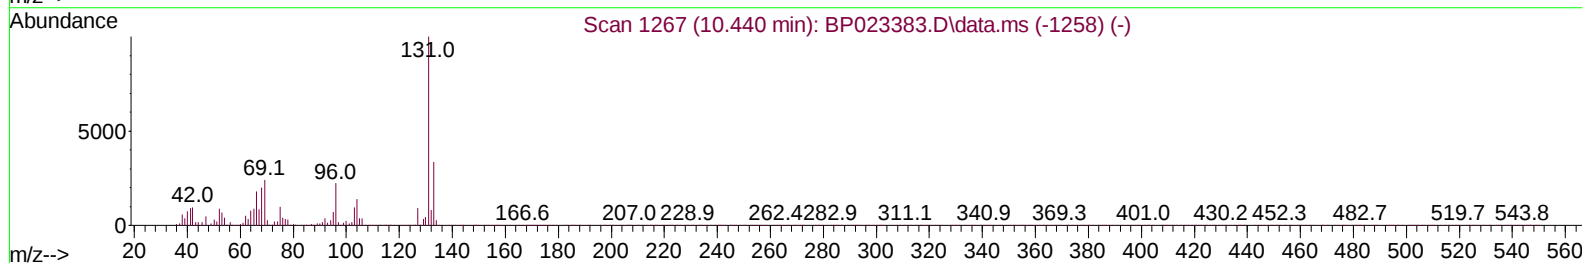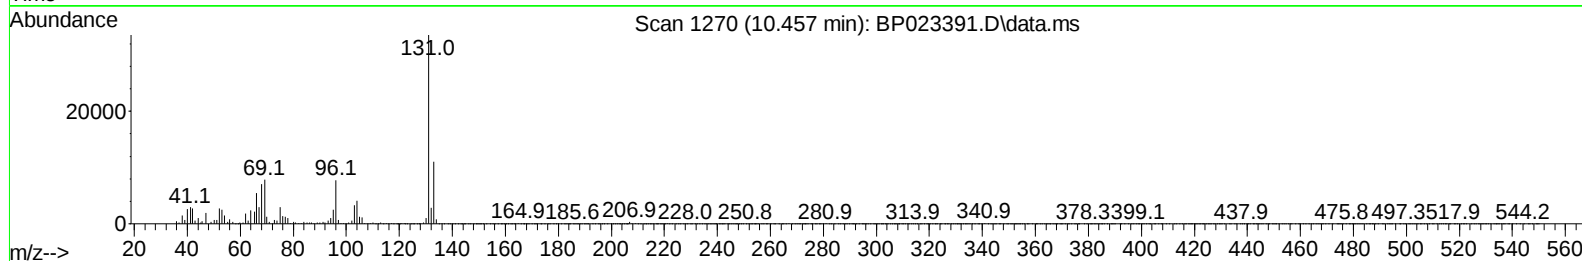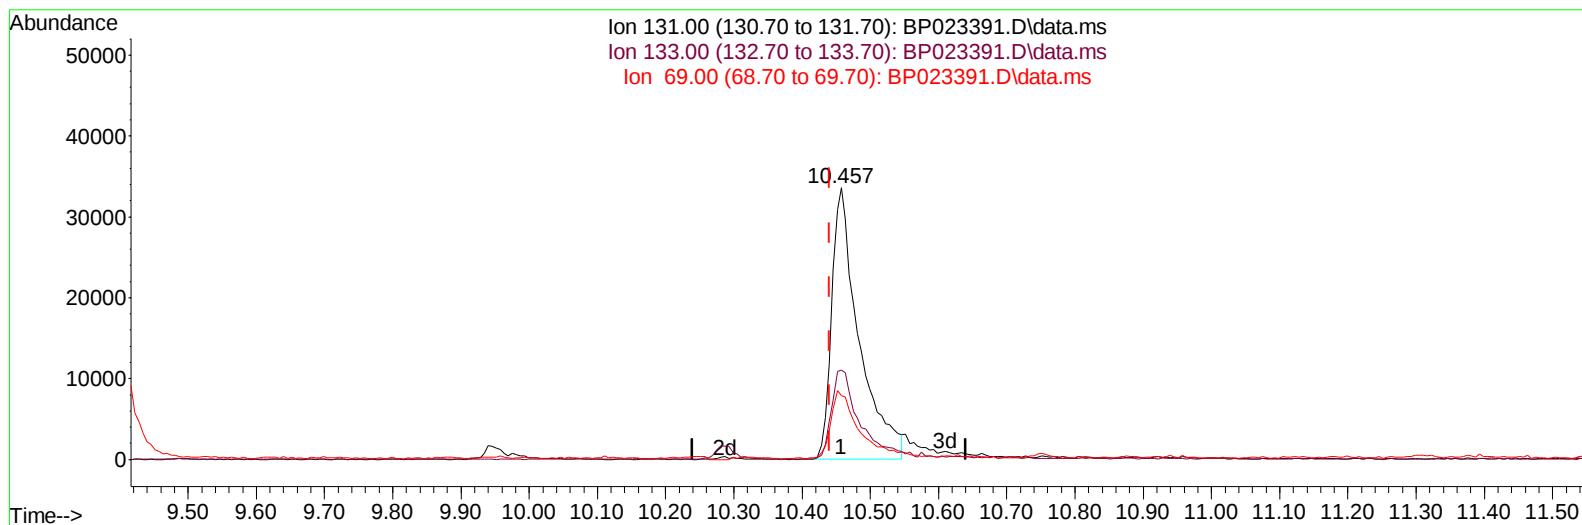




TIC: BP023391.D\data.ms

(31) 4-Chloroaniline-d4 (S)**10.457min (+ 0.018) 12.38 ng/ul****response 92746**

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	32.91
69.00	24.30	23.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023391.D
Acq On : 12 Dec 2024 11:47
Operator : RC/JU
Sample : P5153-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 13 00:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

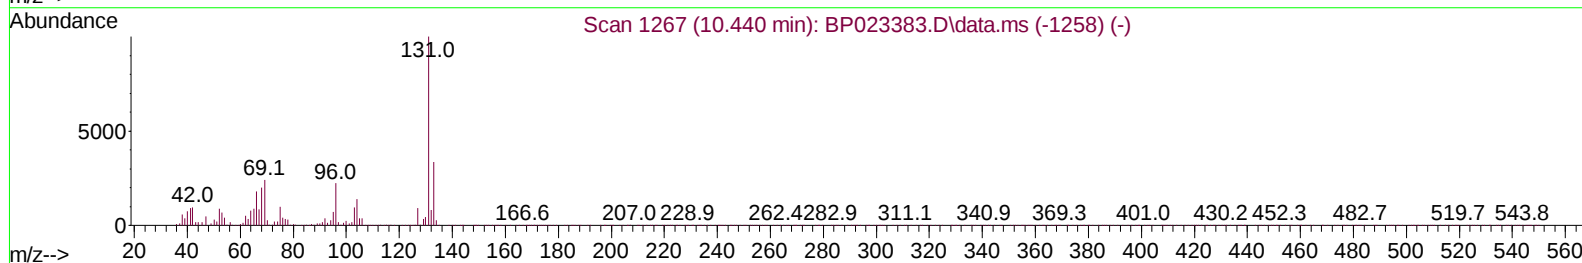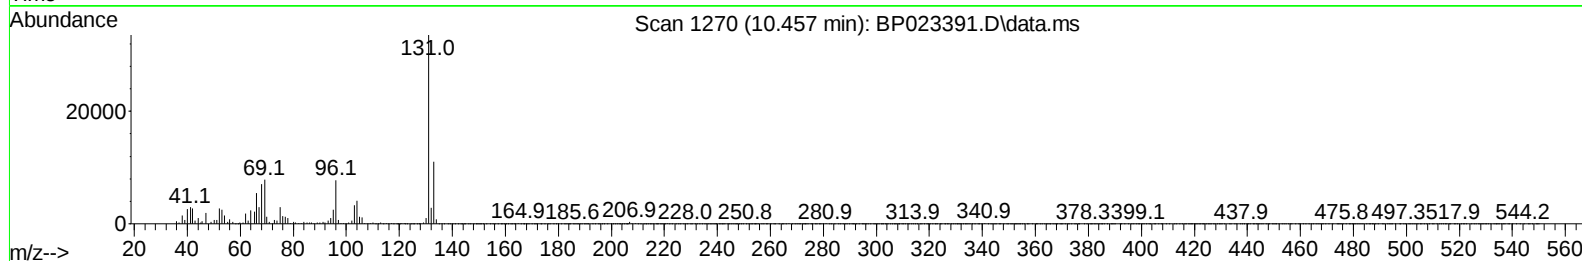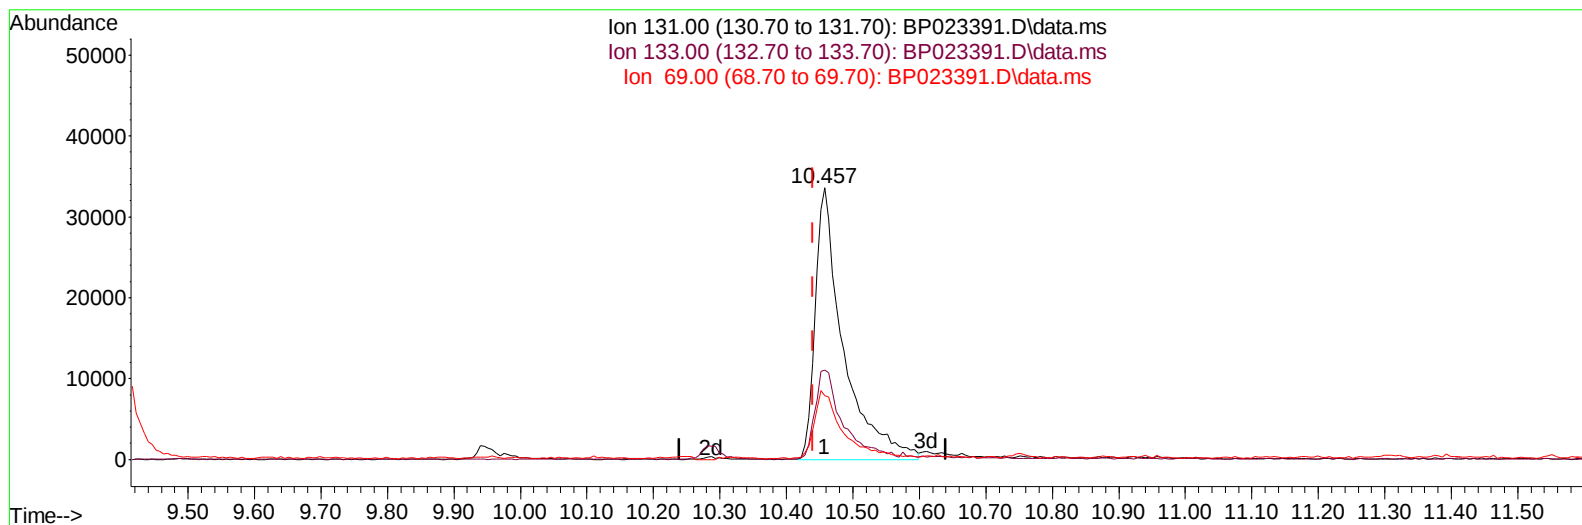

TIC: BP023391.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.457min (+ 0.018) 13.16 ng/ul m

response 98541

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	32.91
69.00	24.30	23.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023391.D
Acq On : 12 Dec 2024 11:47
Operator : RC/JU
Sample : P5153-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 13 00:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

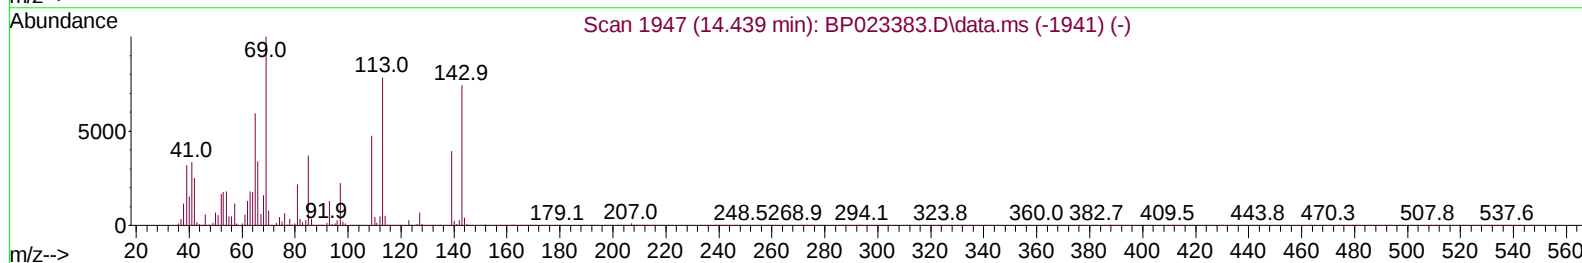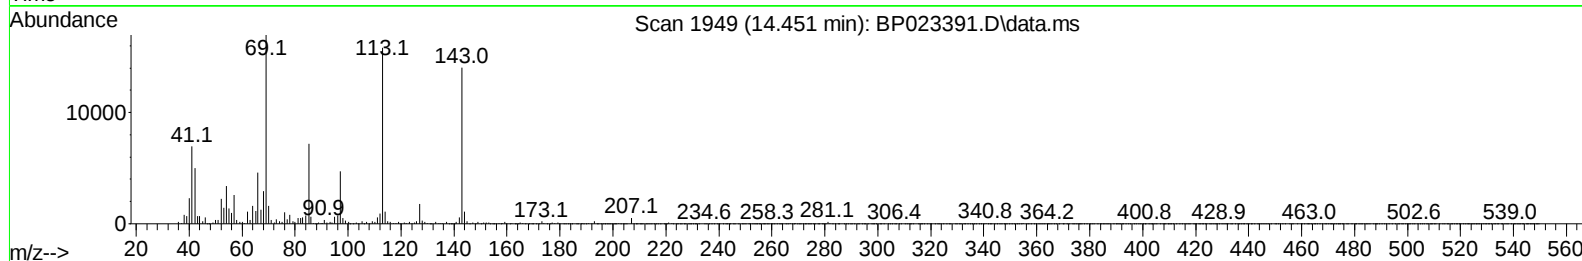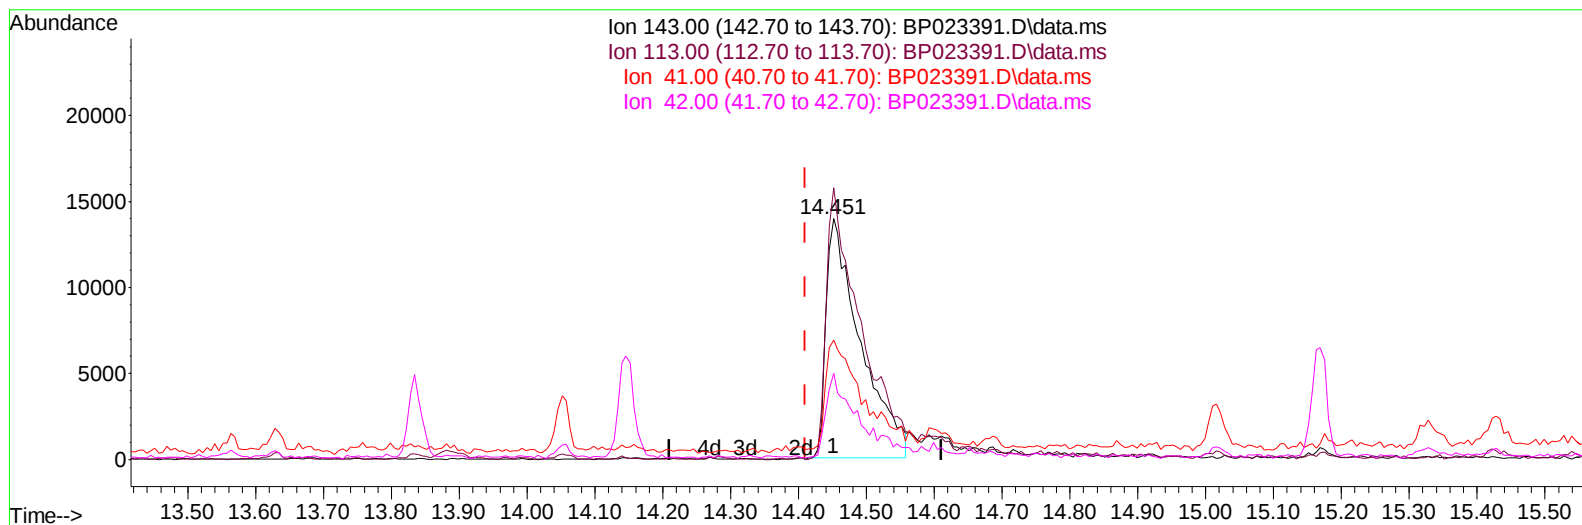

TIC: BP023391.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.451min (+ 0.041) 19.35 ng/ul

response 48796

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	112.67
41.00	45.60	49.49
42.00	31.70	35.80

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023391.D
Acq On : 12 Dec 2024 11:47
Operator : RC/JU
Sample : P5153-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 13 00:26:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

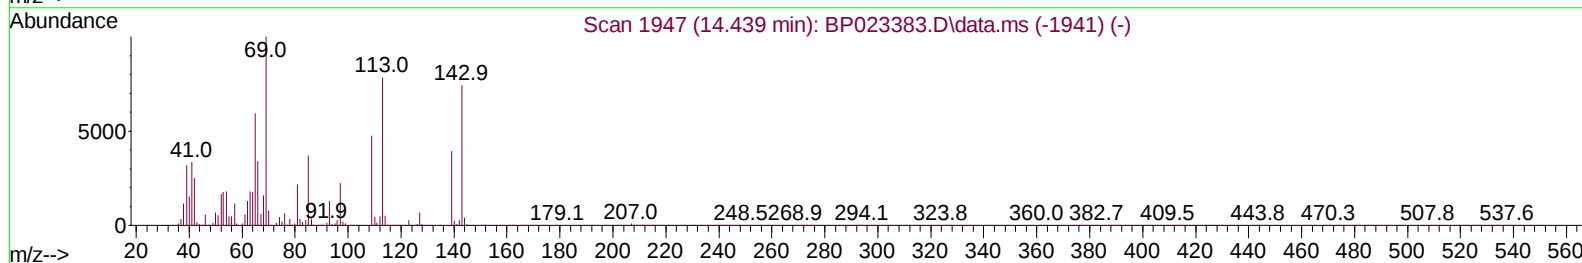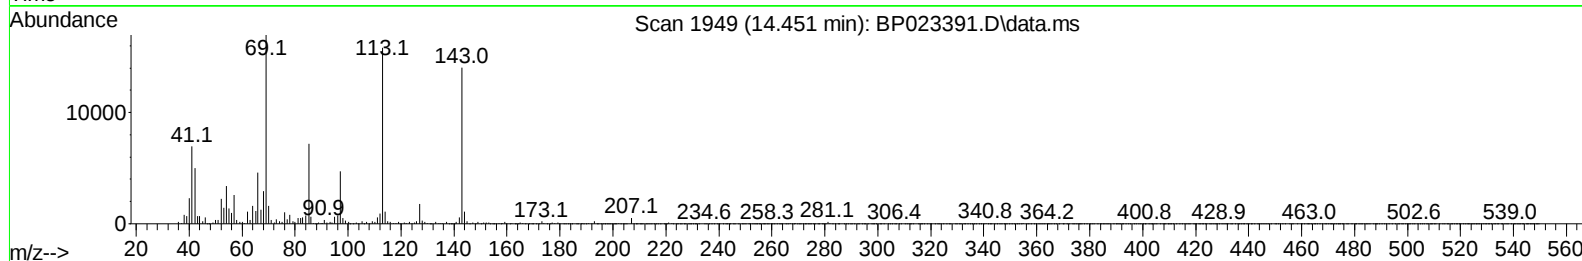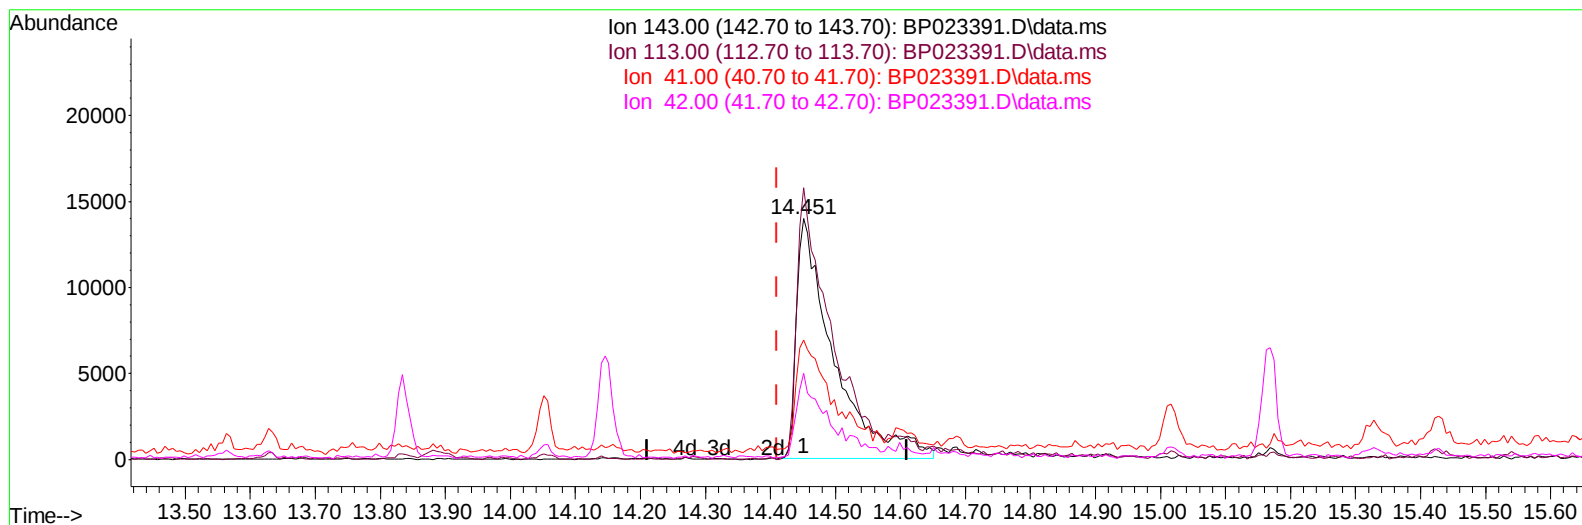

TIC: BP023391.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.451min (+ 0.041) 21.74 ng/ul m

response 54819

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	112.67
41.00	45.60	49.49
42.00	31.70	35.80

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
 Data File : BP023391.D
 Acq On : 12 Dec 2024 11:47
 Operator : RC/JU
 Sample : P5153-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 13 00:29:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	99552	20.000	ng/ul	0.00
20) Naphthalene-d8	10.281	136	368124	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.146	164	265024	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.957	188	617783	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240	743780	20.000	ng/ul	0.00
88) Perylene-d12	24.568	264	841561	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.105	96	9094	3.363	ng/uL	0.00
4) Pyridine-d5	3.523	84	92680	13.329	ng/ul	0.00
7) Phenol-d5	6.752	99	150751	19.300	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.893	67	99566	20.204	ng/ul	0.00
11) 2-Chlorophenol-d4	7.093	132	109008	18.908	ng/ul	0.00
15) 4-Methylphenol-d8	8.258	113	110057	17.458	ng/ul	0.00
21) Nitrobenzene-d5	8.687	128	51379	18.691	ng/ul	0.00
24) 2-Nitrophenol-d4	9.399	143	61913	19.542	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.946	165	131281	19.633	ng/ul	0.01
31) 4-Chloroaniline-d4	10.457	131	98541m	13.155	ng/ul	0.02
46) Dimethylphthalate-d6	13.563	166	429681	20.885	ng/ul	0.00
49) Acenaphthylene-d8	13.834	160	445556	20.532	ng/ul	0.00
54) 4-Nitrophenol-d4	14.451	143	54819m	21.743	ng/ul	0.04
60) Fluorene-d10	15.169	176	368245	20.349	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.328	200	45793	12.265	ng/ul	0.02
73) Anthracene-d10	17.057	188	579685	20.560	ng/ul	0.00
81) Pyrene-d10	19.451	212	749790	19.295	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.351	264	716958	15.915	ng/ul	0.00
Target Compounds						
8) Phenol	6.781	94	9813m	1.207	ng/ul	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023391.D
Acq On : 12 Dec 2024 11:47
Operator : RC/JU
Sample : P5153-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Dec 13 00:29:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

