
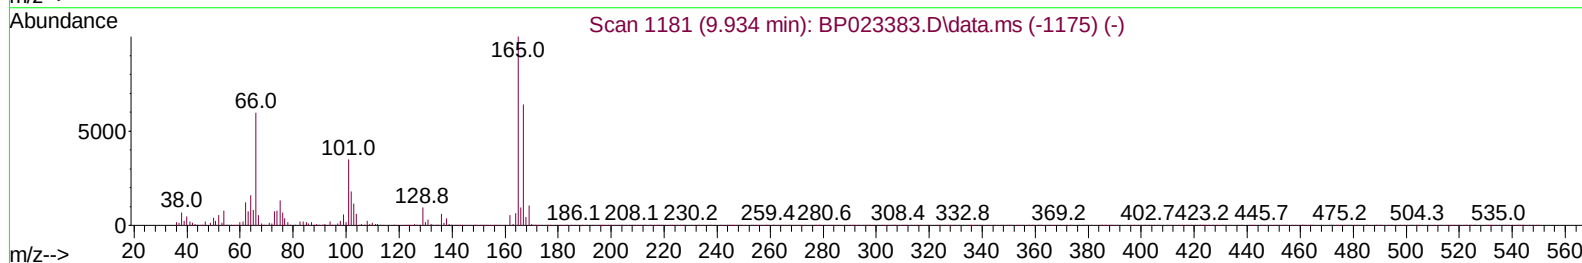
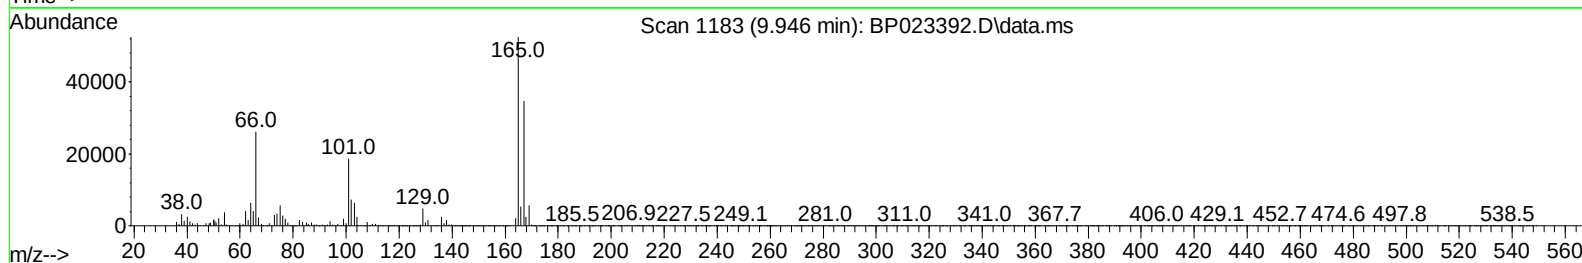


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023392.D
Acq On : 12 Dec 2024 12:28
Operator : RC/JU
Sample : P5153-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 13 00:33:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

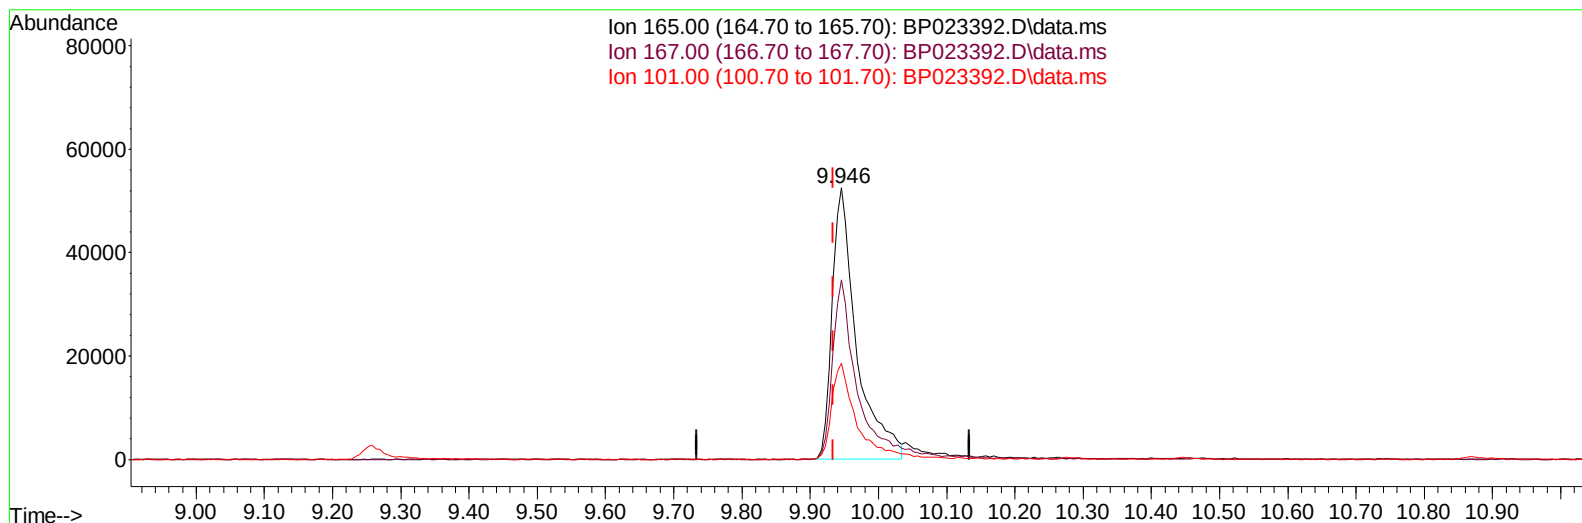

TIC: BP023392.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)




9.946min (+ 0.012) 15.90 ng/ul

response 130929

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.00	66.06
101.00	34.30	35.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023392.D
Acq On : 12 Dec 2024 12:28
Operator : RC/JU
Sample : P5153-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 13 00:33:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

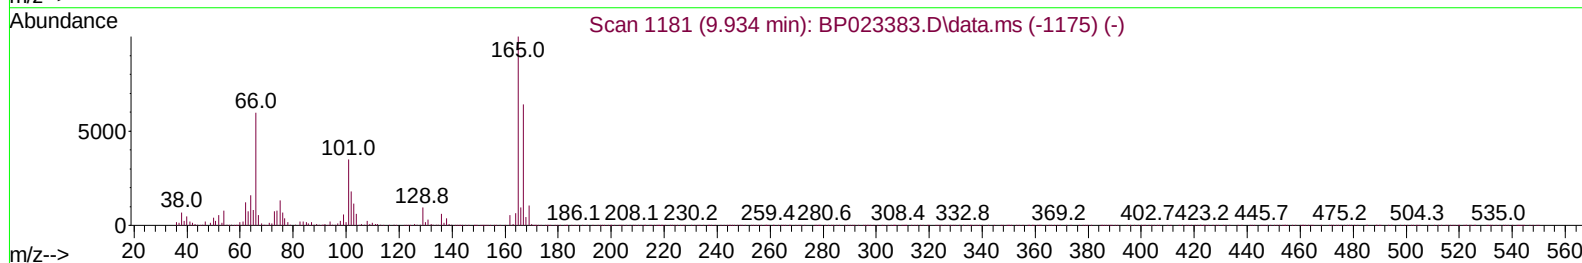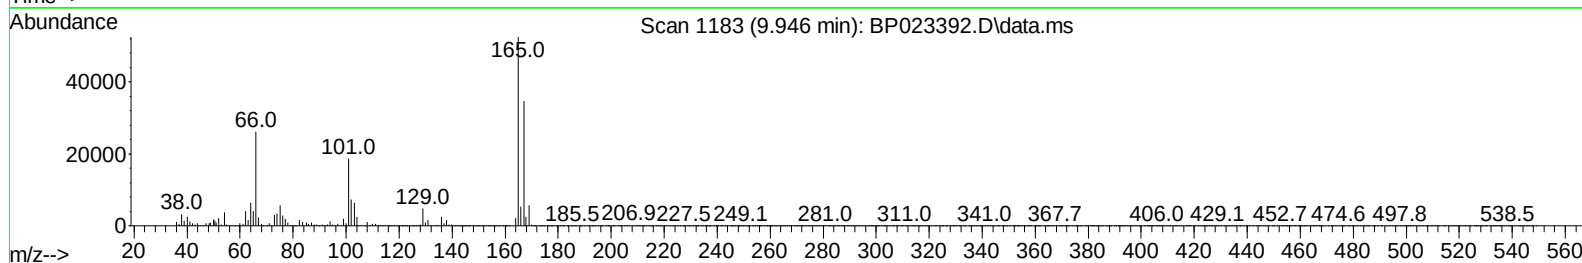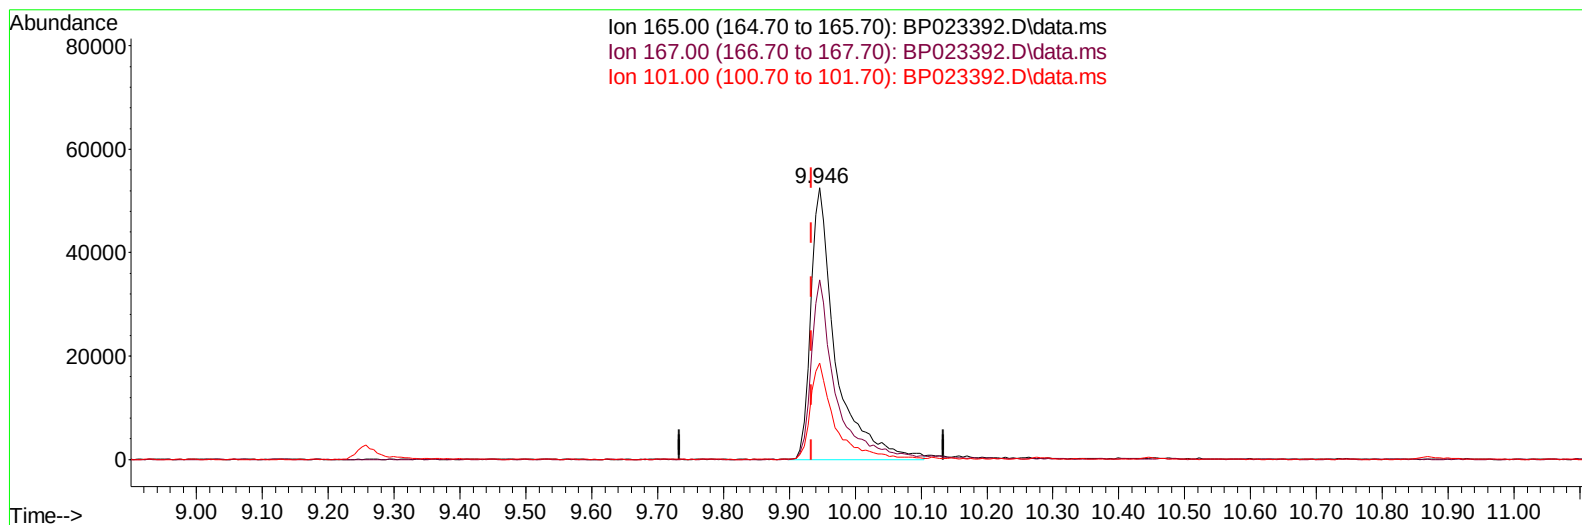

TIC: BP023392.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)




9.946min (+ 0.012) 16.80 ng/ul m

response 138331

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.00	66.06
101.00	34.30	35.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023392.D
Acq On : 12 Dec 2024 12:28
Operator : RC/JU
Sample : P5153-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 13 00:33:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

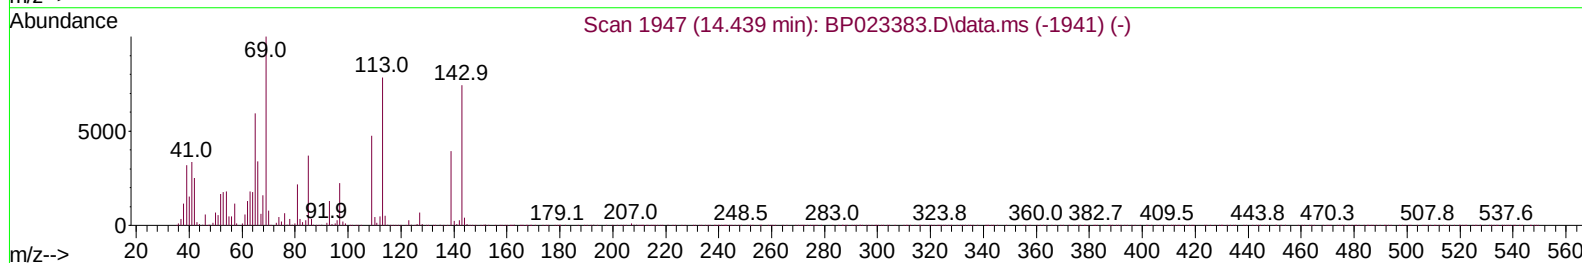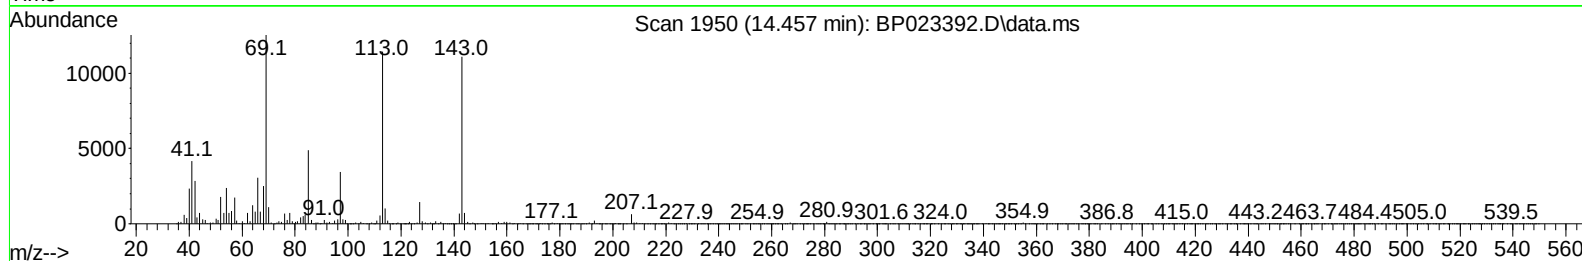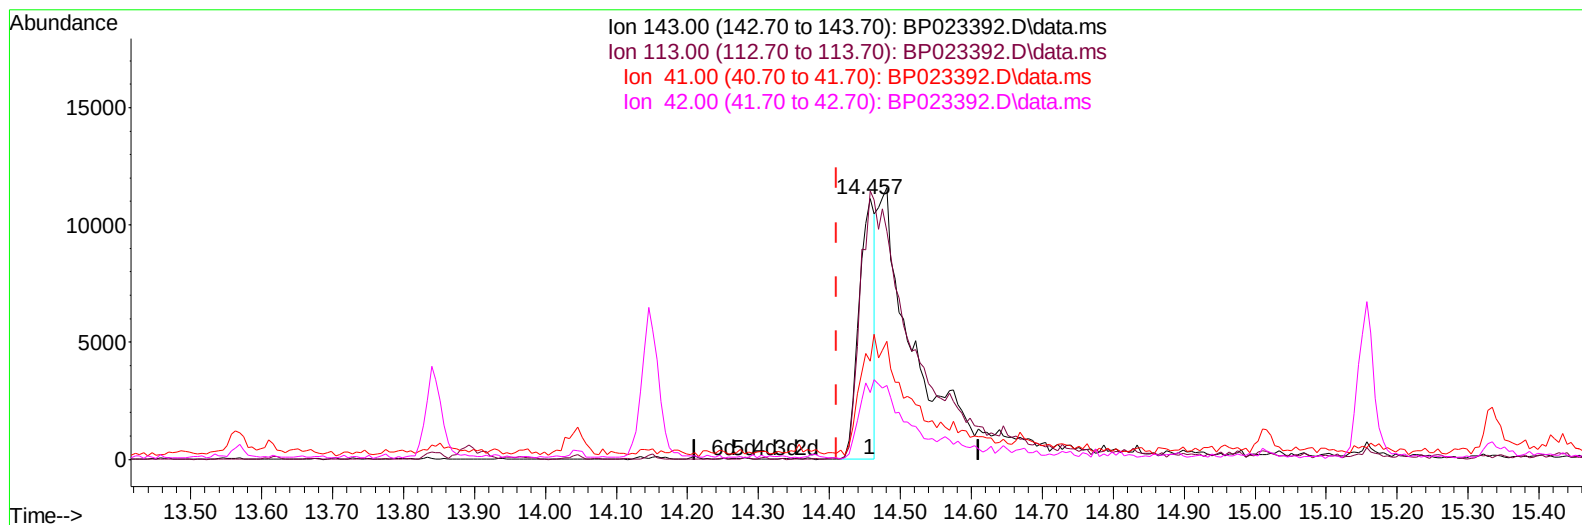

TIC: BP023392.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.457min (+ 0.047) 5.22 ng/ul

response 17282

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	102.87
41.00	45.60	37.58
42.00	31.70	25.65

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023392.D
Acq On : 12 Dec 2024 12:28
Operator : RC/JU
Sample : P5153-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 13 00:33:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

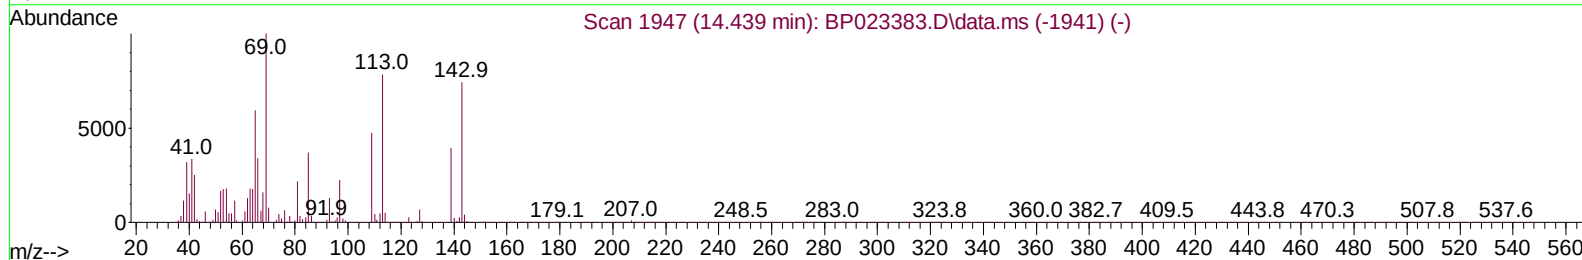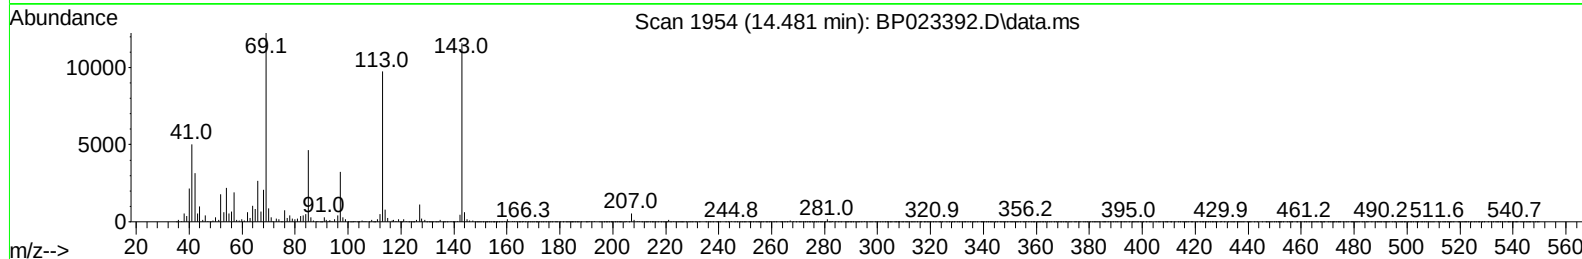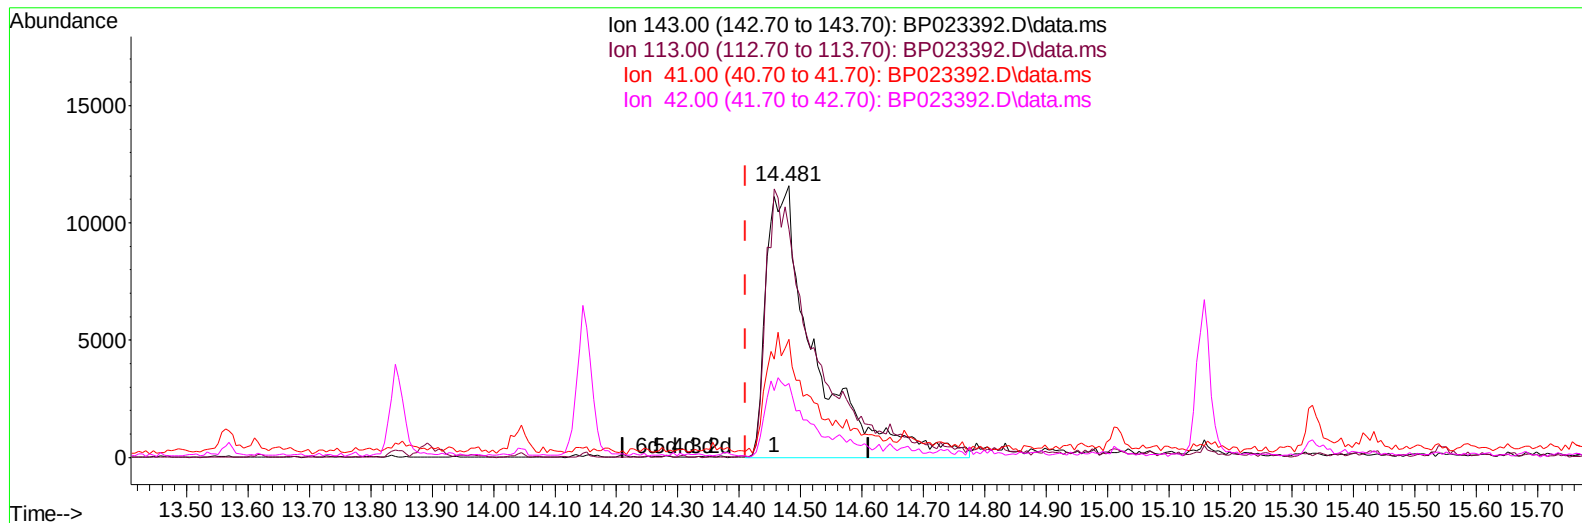

TIC: BP023392.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.481min (+ 0.070) 19.42 ng/ul m

response 64344

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	84.12#
41.00	45.60	43.51
42.00	31.70	27.35

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
 Data File : BP023392.D
 Acq On : 12 Dec 2024 12:28
 Operator : RC/JU
 Sample : P5153-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 13 00:35:58 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	115552	20.000	ng/ul	0.00
20) Naphthalene-d8	10.281	136	453262	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	348223	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.957	188	820049	20.000	ng/ul	0.00
79) Chrysene-d12	21.386	240	860024	20.000	ng/ul	0.00
88) Perylene-d12	24.568	264	924309	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	8295	2.643	ng/uL	0.00
4) Pyridine-d5	3.517	84	94161	11.667	ng/ul	0.00
7) Phenol-d5	6.752	99	147755	16.297	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.893	67	95354	16.670	ng/ul	0.00
11) 2-Chlorophenol-d4	7.087	132	109982	16.436	ng/ul	0.00
15) 4-Methylphenol-d8	8.257	113	125083	17.094	ng/ul	0.00
21) Nitrobenzene-d5	8.687	128	54784	16.186	ng/ul	0.00
24) 2-Nitrophenol-d4	9.399	143	62398	15.996	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.946	165	138331m	16.802	ng/ul	0.01
31) 4-Chloroaniline-d4	10.446	131	144956	15.717	ng/ul	0.00
46) Dimethylphthalate-d6	13.563	166	499783	18.488	ng/ul	0.00
49) Acenaphthylene-d8	13.845	160	508188	17.823	ng/ul	0.01
54) 4-Nitrophenol-d4	14.481	143	64344m	19.424	ng/ul	0.07
60) Fluorene-d10	15.157	176	428321	18.014	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.334	200	46328	9.348	ng/ul	0.02
73) Anthracene-d10	17.069	188	703780	18.805	ng/ul	0.02
81) Pyrene-d10	19.445	212	868767	19.335	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.351	264	840130	16.979	ng/ul	0.00
Target Compounds						
80) Fluoranthene	19.098	202	53628	1.042	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023392.D
Acq On : 12 Dec 2024 12:28
Operator : RC/JU
Sample : P5153-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 13 00:35:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

