
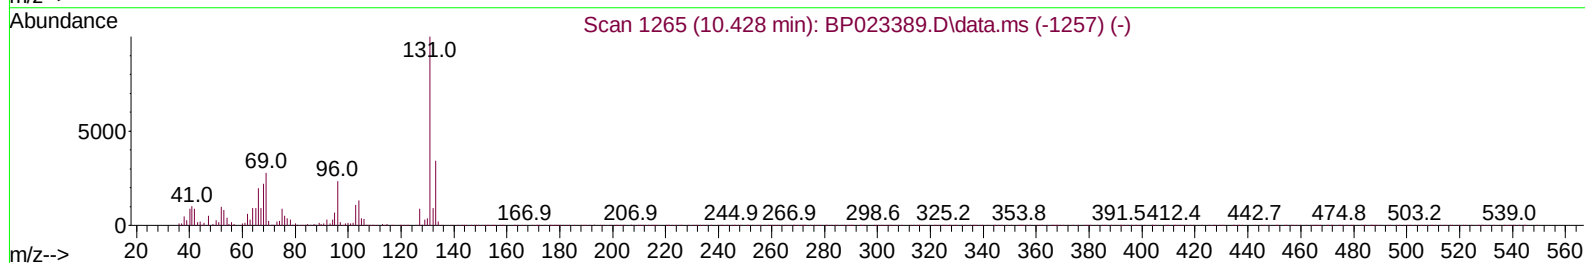
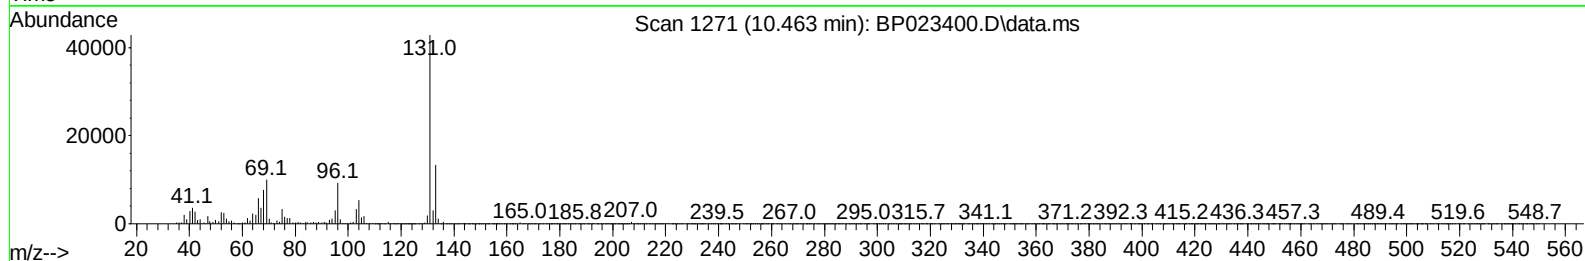


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023400.D
Acq On : 12 Dec 2024 17:51
Operator : RC/JU
Sample : P5153-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 13 01:59:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

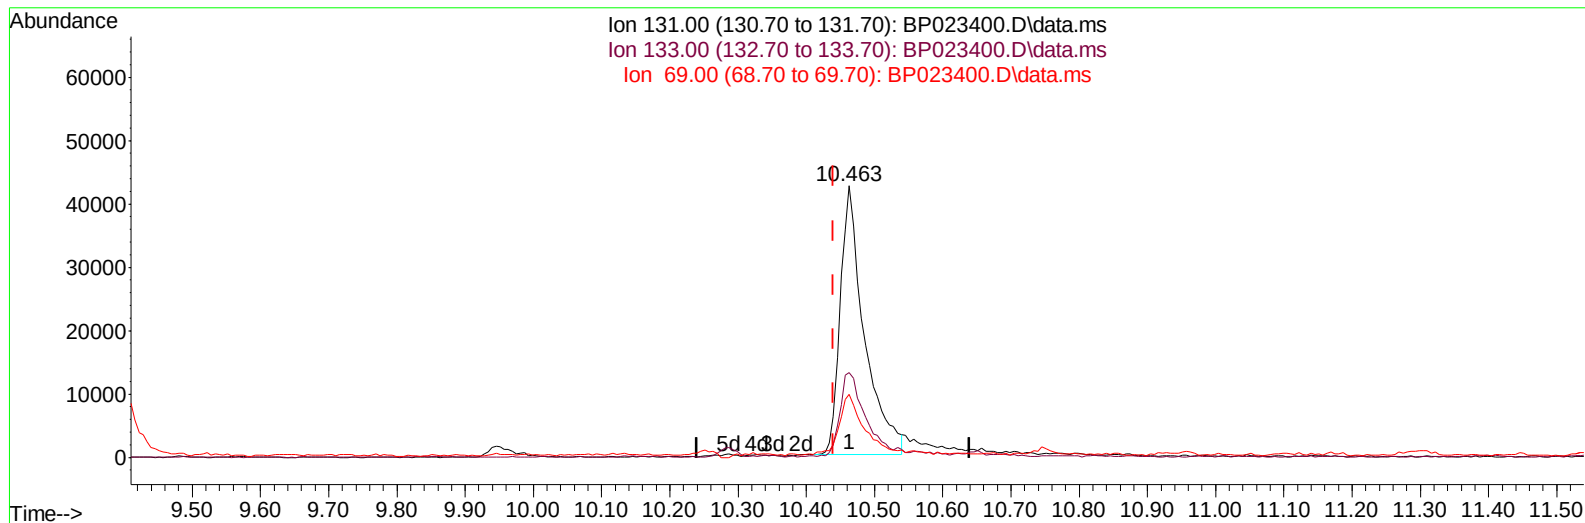

TIC: BP023400.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.463min (+ 0.023) 14.02 ng/ul

response 103465

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	31.26
69.00	24.30	23.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023400.D
Acq On : 12 Dec 2024 17:51
Operator : RC/JU
Sample : P5153-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 13 01:59:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

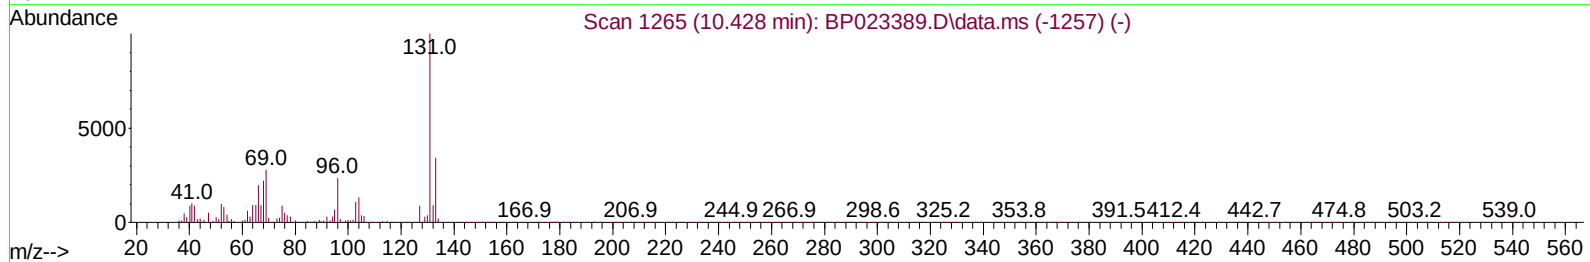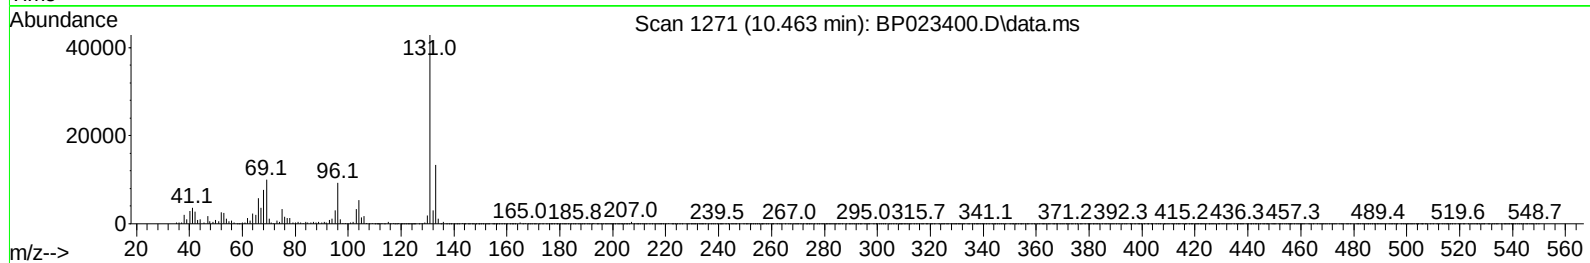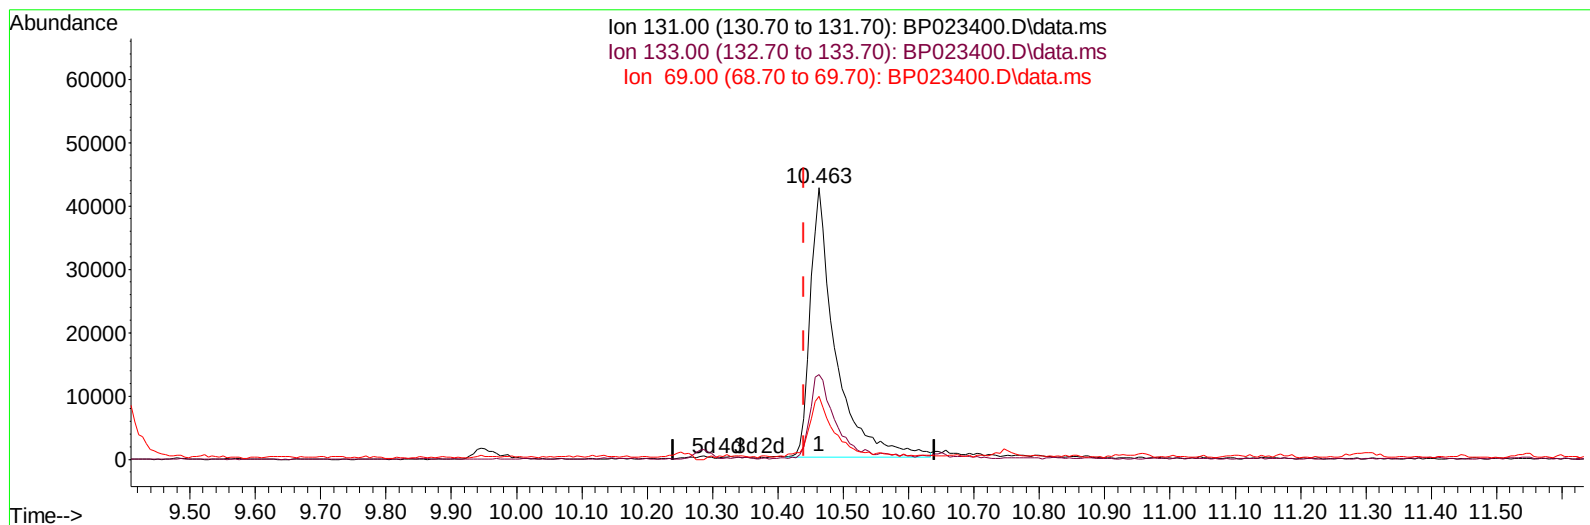

TIC: BP023400.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.463min (+ 0.023) 15.38 ng/ul m

response 113526

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	31.26
69.00	24.30	23.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023400.D
Acq On : 12 Dec 2024 17:51
Operator : RC/JU
Sample : P5153-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 13 01:59:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

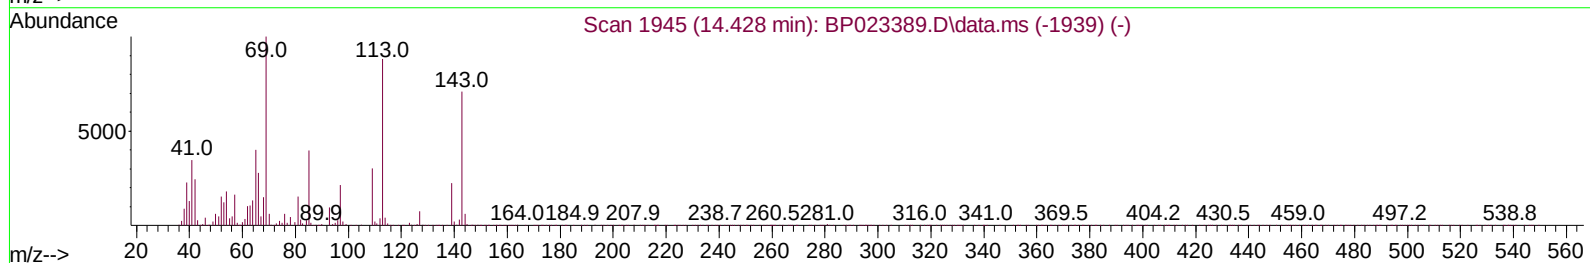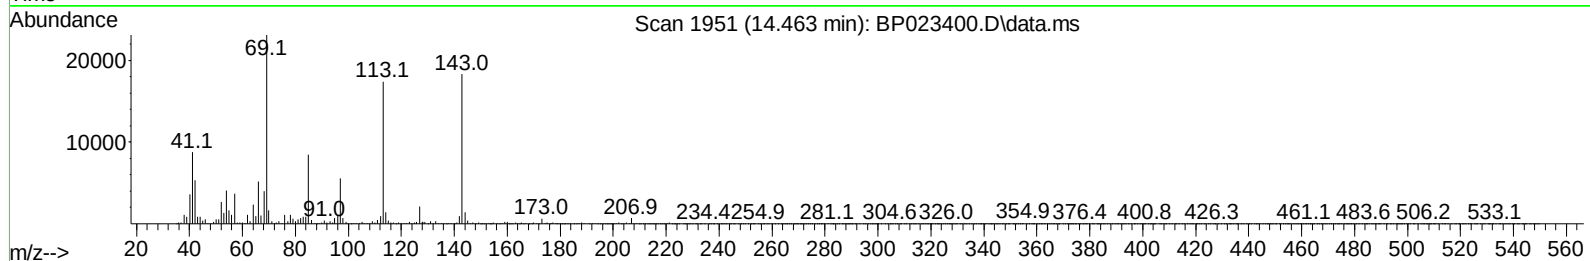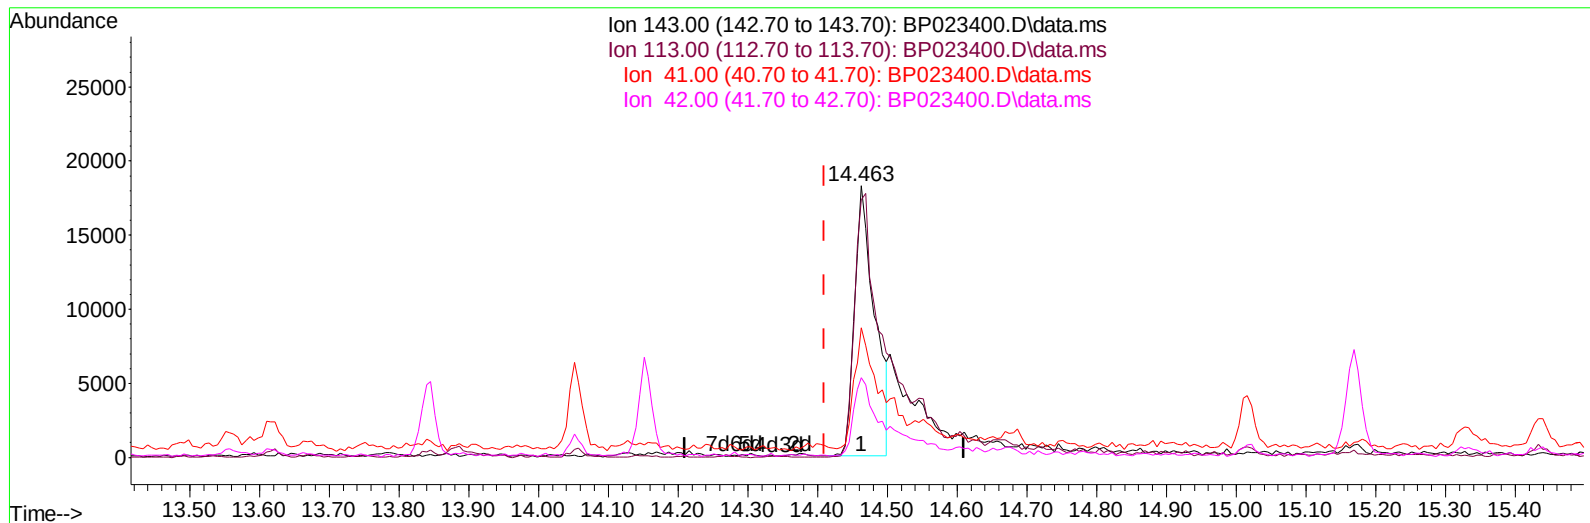

TIC: BP023400.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.463min (+ 0.053) 13.73 ng/ul

response 36582

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	94.80
41.00	45.60	47.70
42.00	31.70	29.28

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023400.D
Acq On : 12 Dec 2024 17:51
Operator : RC/JU
Sample : P5153-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 13 01:59:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

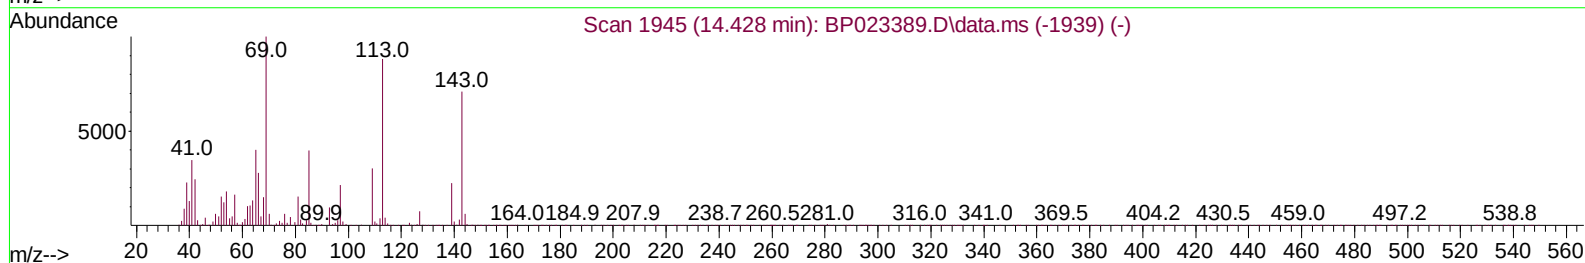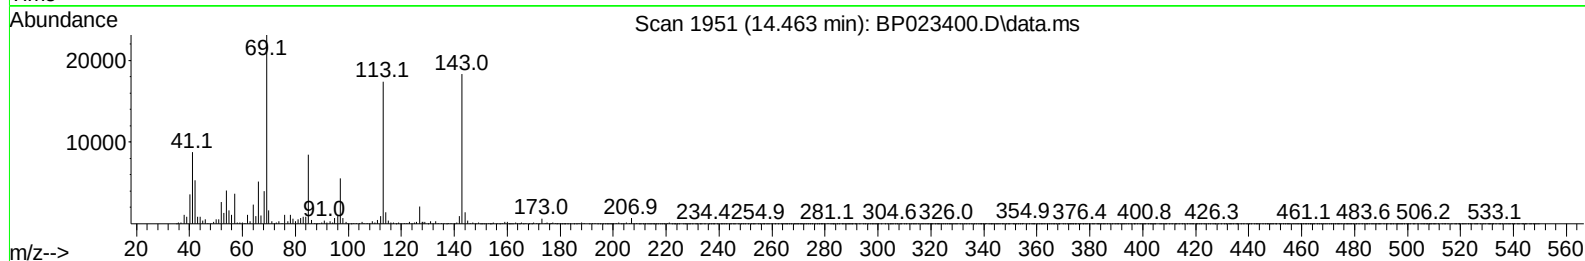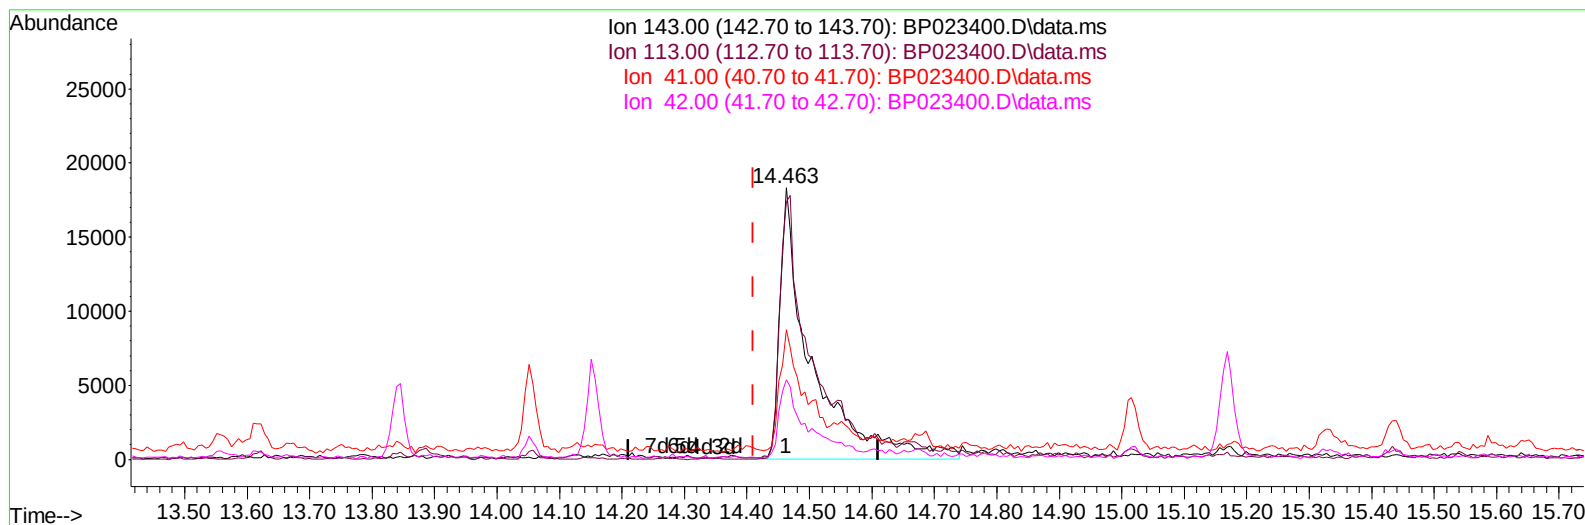

TIC: BP023400.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.463min (+ 0.053) 24.11 ng/ul m

response 64250

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	94.80
41.00	45.60	47.70
42.00	31.70	29.28

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023400.D
Acq On : 12 Dec 2024 17:51
Operator : RC/JU
Sample : P5153-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 13 01:59:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

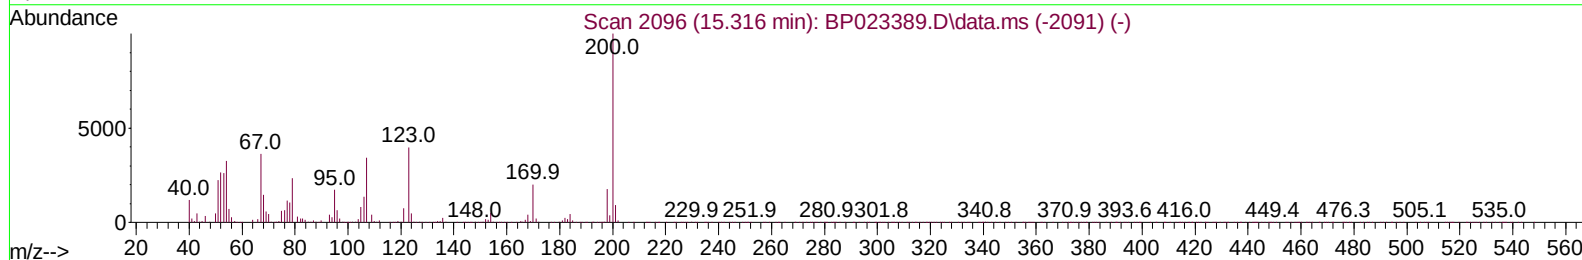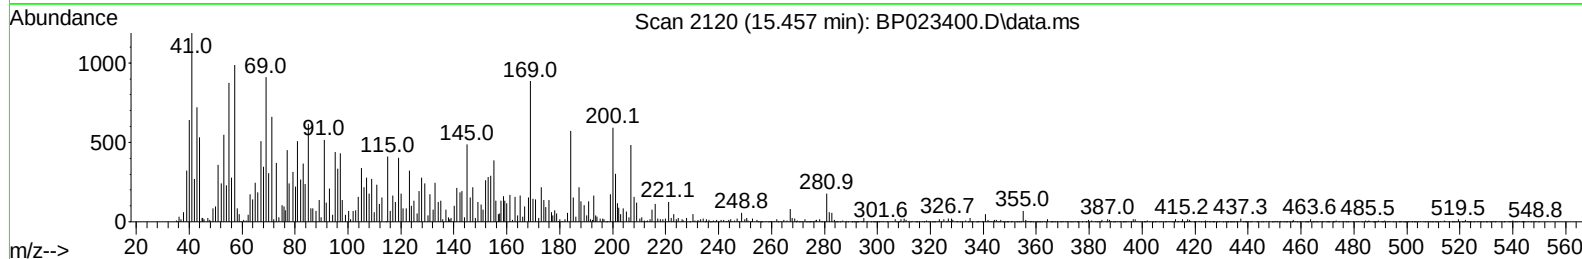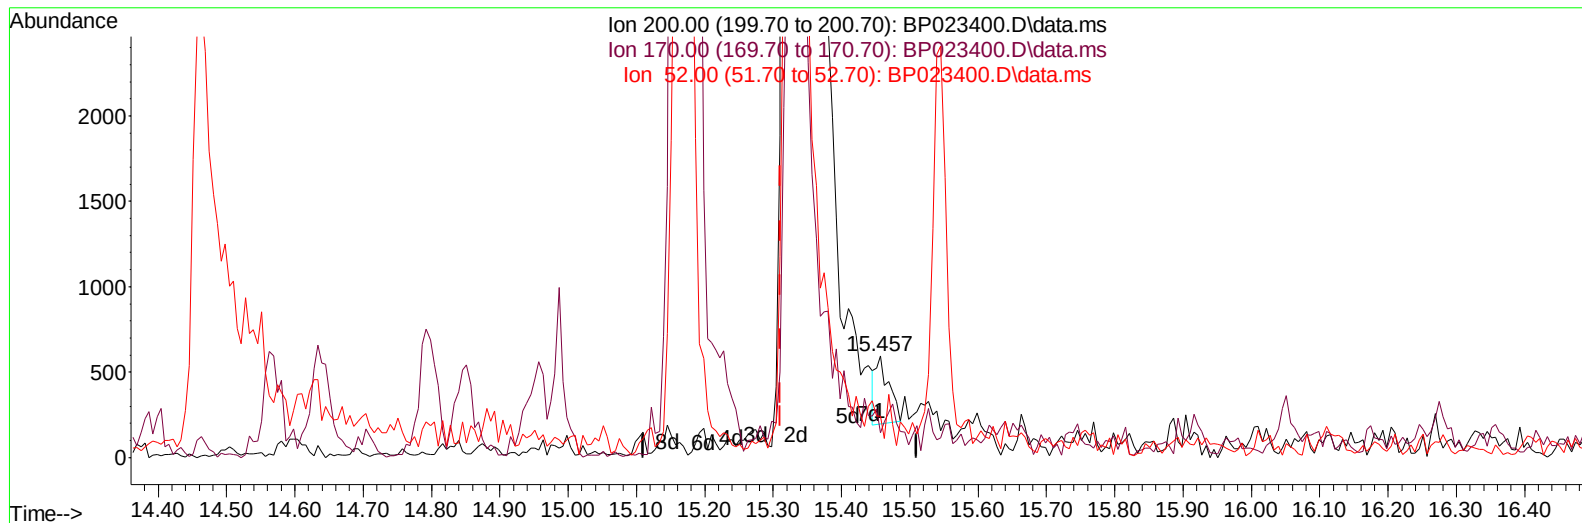




TIC: BP023400.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)**15.457min (+ 0.147) 0.13 ng/ul****response 529**

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	24.62
52.00	37.90	40.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023400.D
Acq On : 12 Dec 2024 17:51
Operator : RC/JU
Sample : P5153-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 13 01:59:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

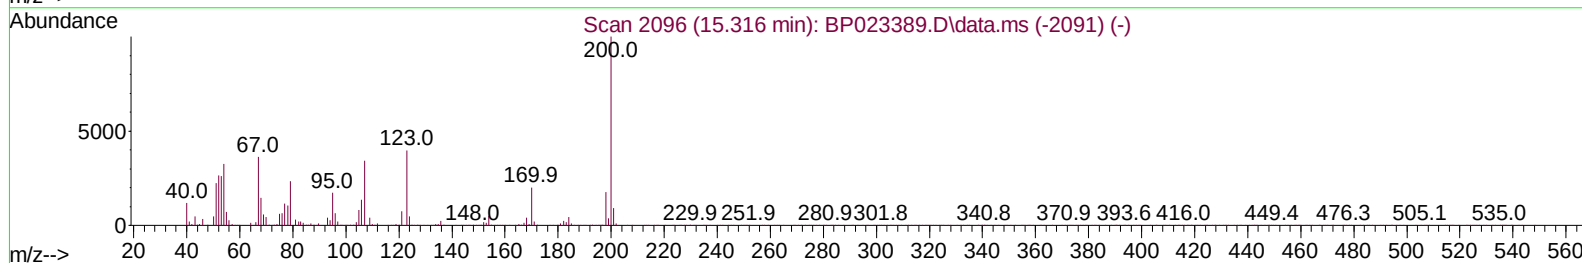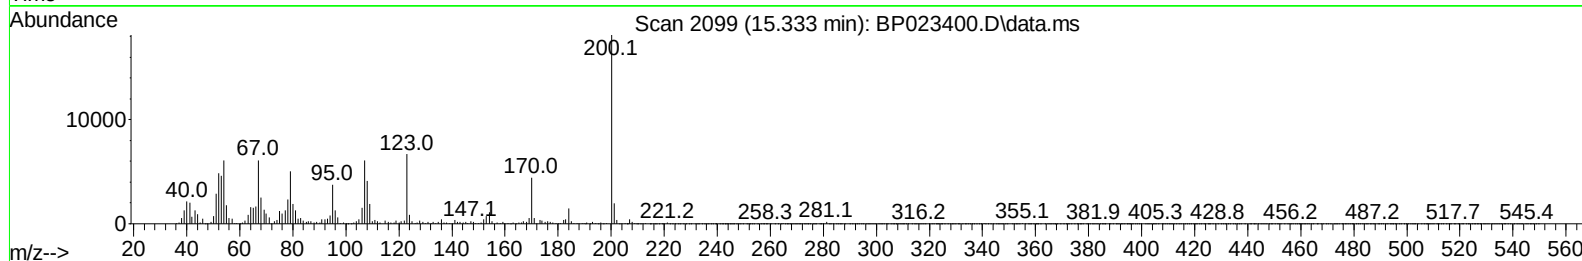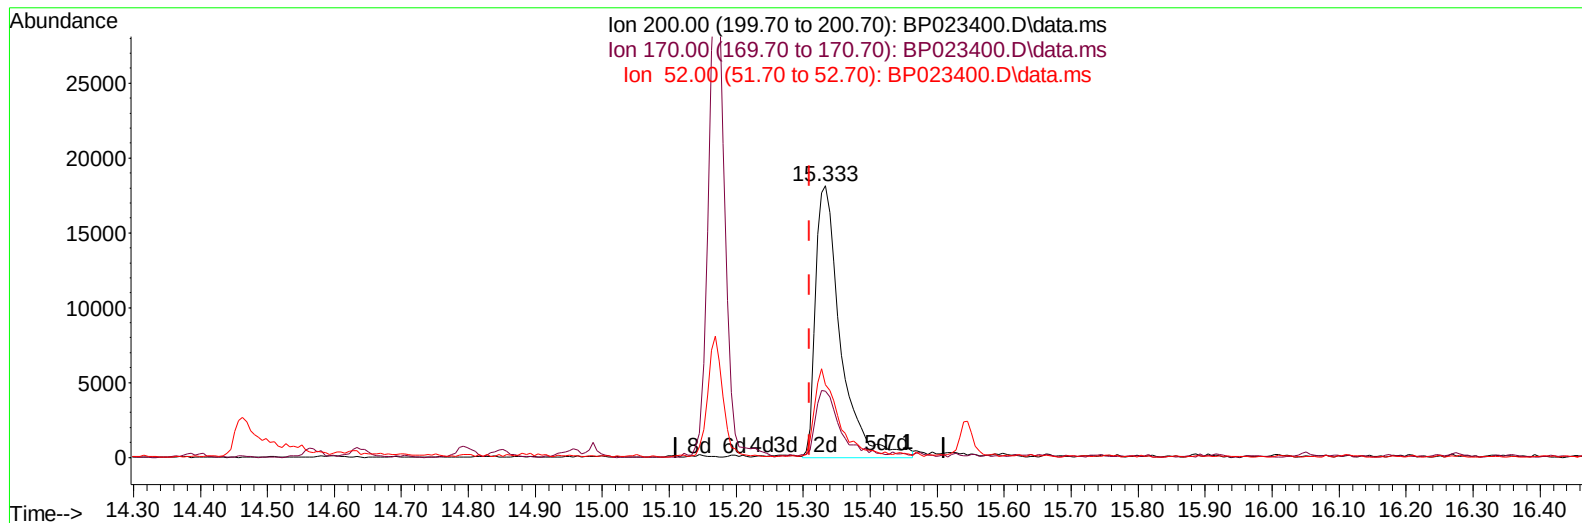

TIC: BP023400.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)**15.333min (+ 0.023) 11.66 ng/ul m****response 46947**

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	24.42
52.00	37.90	26.78#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
 Data File : BP023400.D
 Acq On : 12 Dec 2024 17:51
 Operator : RC/JU
 Sample : P5153-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 13 02:03:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	96515	20.000	ng/ul	0.00
20) Naphthalene-d8	10.281	136	362788	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.157	164	280146	20.000	ng/ul	0.01
64) Phenanthrene-d10	16.957	188	666155	20.000	ng/ul	0.00
79) Chrysene-d12	21.380	240	839181	20.000	ng/ul	0.00
88) Perylene-d12	24.545	264	868955	20.000	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	9592	3.659	ng/uL	0.00
4) Pyridine-d5	3.516	84	123040	18.252	ng/ul	0.00
7) Phenol-d5	6.752	99	162021	21.395	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.887	67	106262	22.241	ng/ul	0.00
11) 2-Chlorophenol-d4	7.087	132	120285	21.521	ng/ul	0.00
15) 4-Methylphenol-d8	8.257	113	134660	22.032	ng/ul	0.00
21) Nitrobenzene-d5	8.681	128	59112	21.820	ng/ul	0.00
24) 2-Nitrophenol-d4	9.393	143	81976	26.256	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.946	165	140649	21.344	ng/ul	0.01
31) 4-Chloroaniline-d4	10.463	131	113526m	15.378	ng/ul	0.02
46) Dimethylphthalate-d6	13.557	166	512164	23.550	ng/ul	0.00
49) Acenaphthylene-d8	13.845	160	545193	23.767	ng/ul	0.01
54) 4-Nitrophenol-d4	14.463	143	64250m	24.108	ng/ul	0.05
60) Fluorene-d10	15.169	176	455823	23.829	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.333	200	46947m	11.661	ng/ul	0.02
73) Anthracene-d10	17.057	188	760698	25.021	ng/ul	0.00
81) Pyrene-d10	19.439	212	1053299	24.024	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.333	264	1110719	23.878	ng/ul	-0.01

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023400.D
Acq On : 12 Dec 2024 17:51
Operator : RC/JU
Sample : P5153-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Dec 13 02:03:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

