
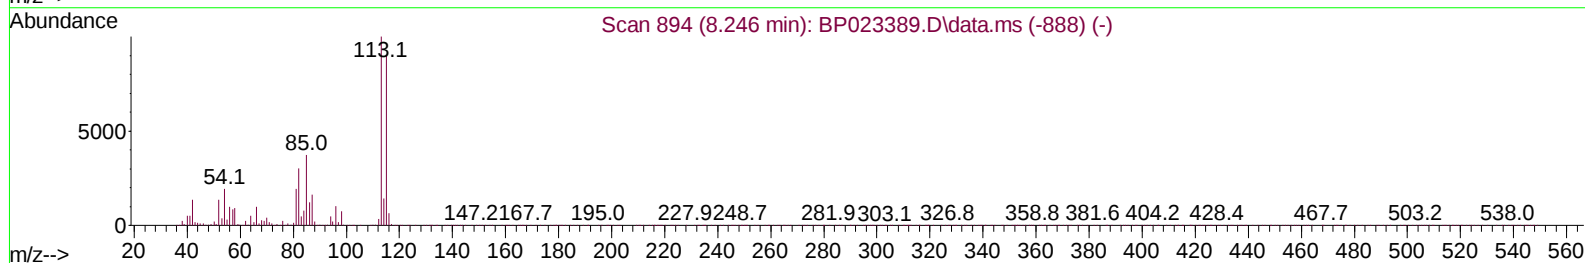
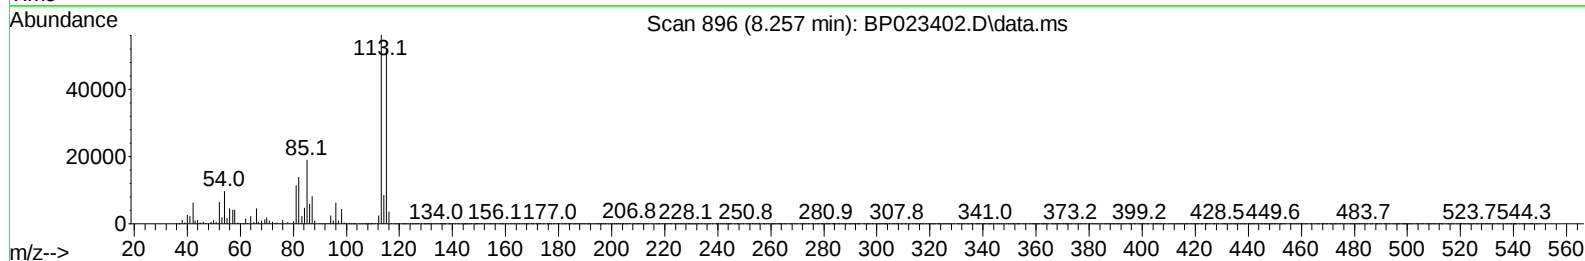


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

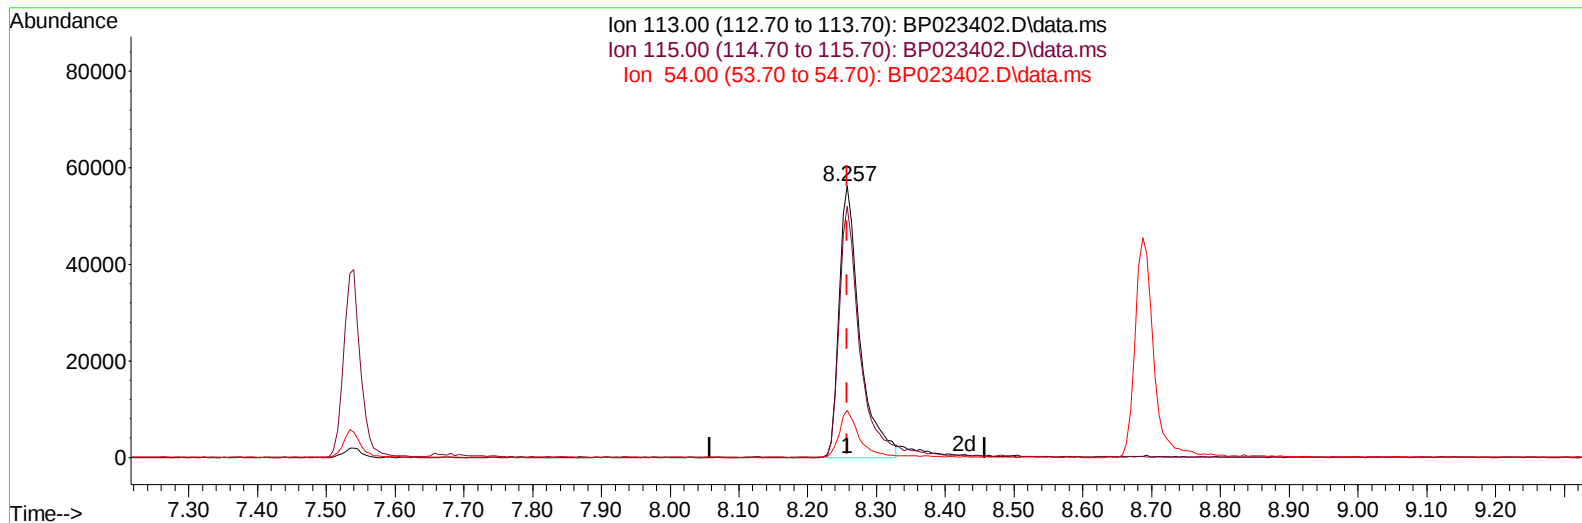

TIC: BP023402.D\data.ms

(15) 4-Methylphenol-d8 (S)




8.257min (-0.000) 17.72 ng/u1

response 117471

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	87.60	92.58
54.00	16.60	17.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

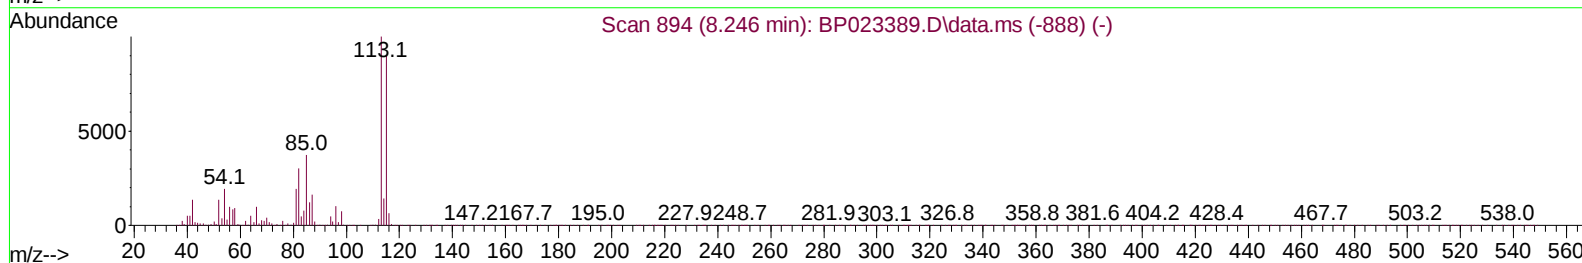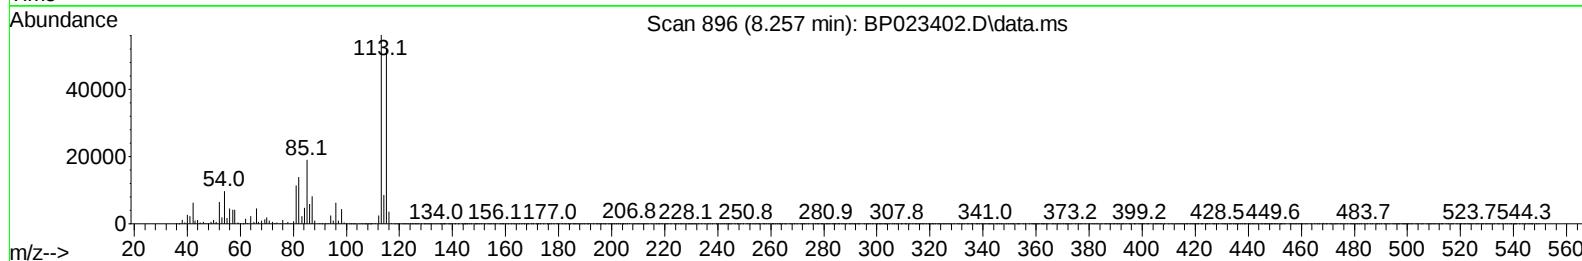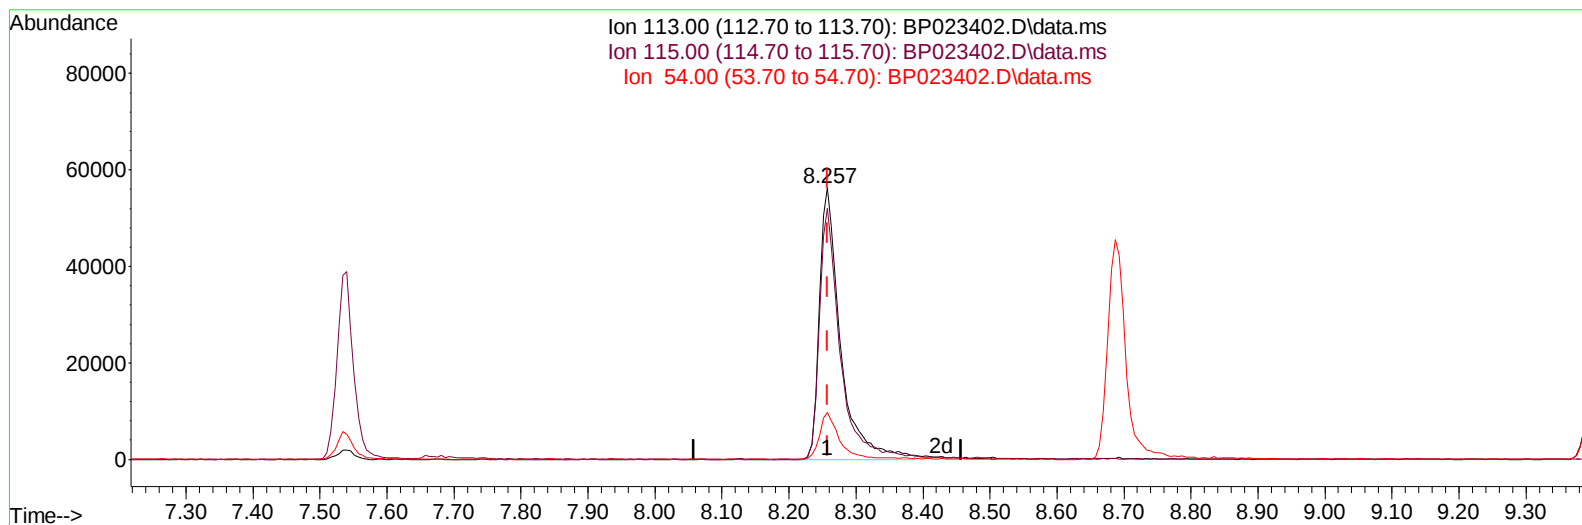




TIC: BP023402.D\data.ms

(15) 4-Methylphenol-d8 (S)**8.257min (-0.000) 18.55 ng/ul m****response 122939**

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	87.60	92.58
54.00	16.60	17.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

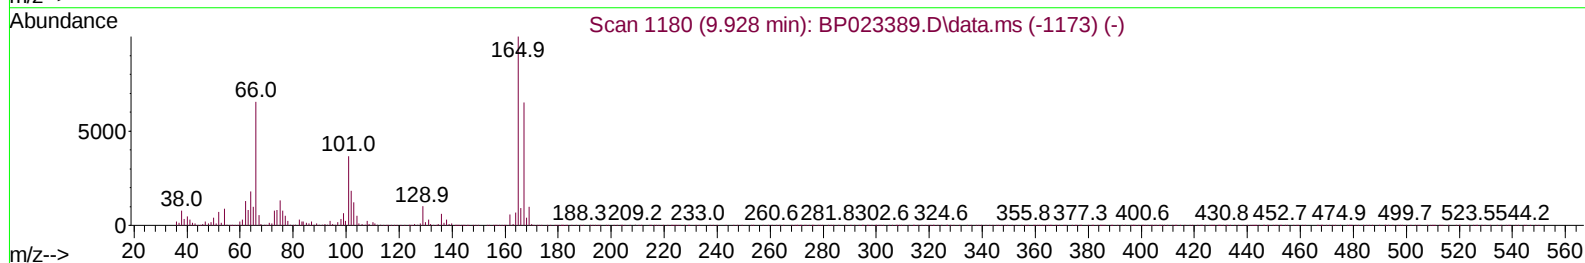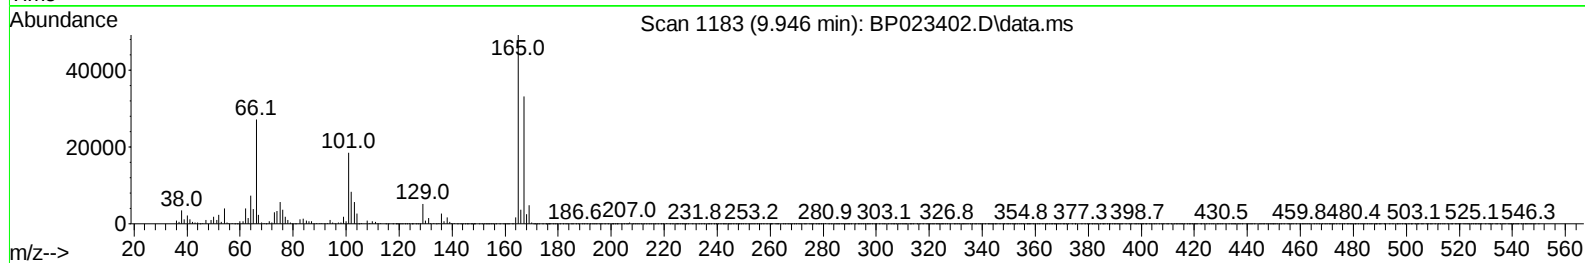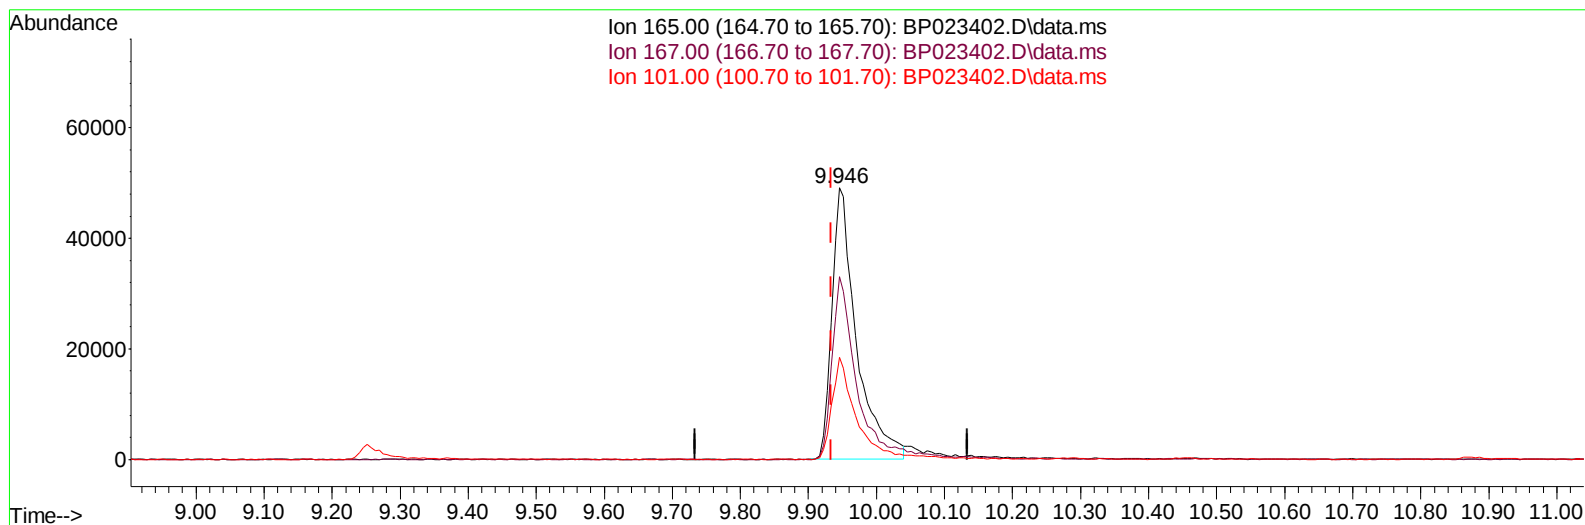

TIC: BP023402.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)




9.946min (+ 0.012) 17.82 ng/ul

response 123103

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.00	67.34
101.00	34.30	37.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

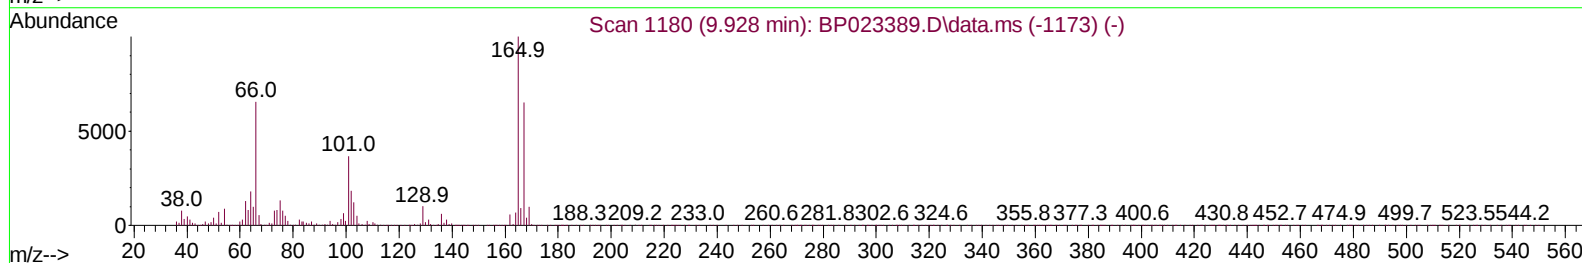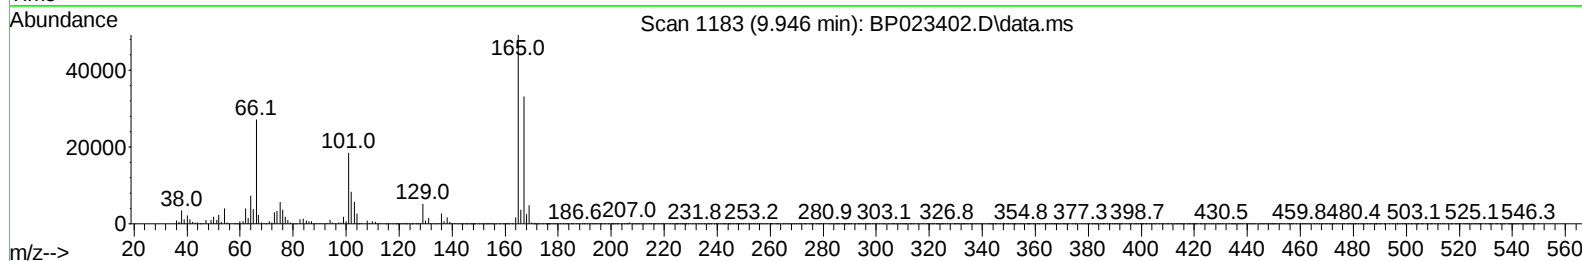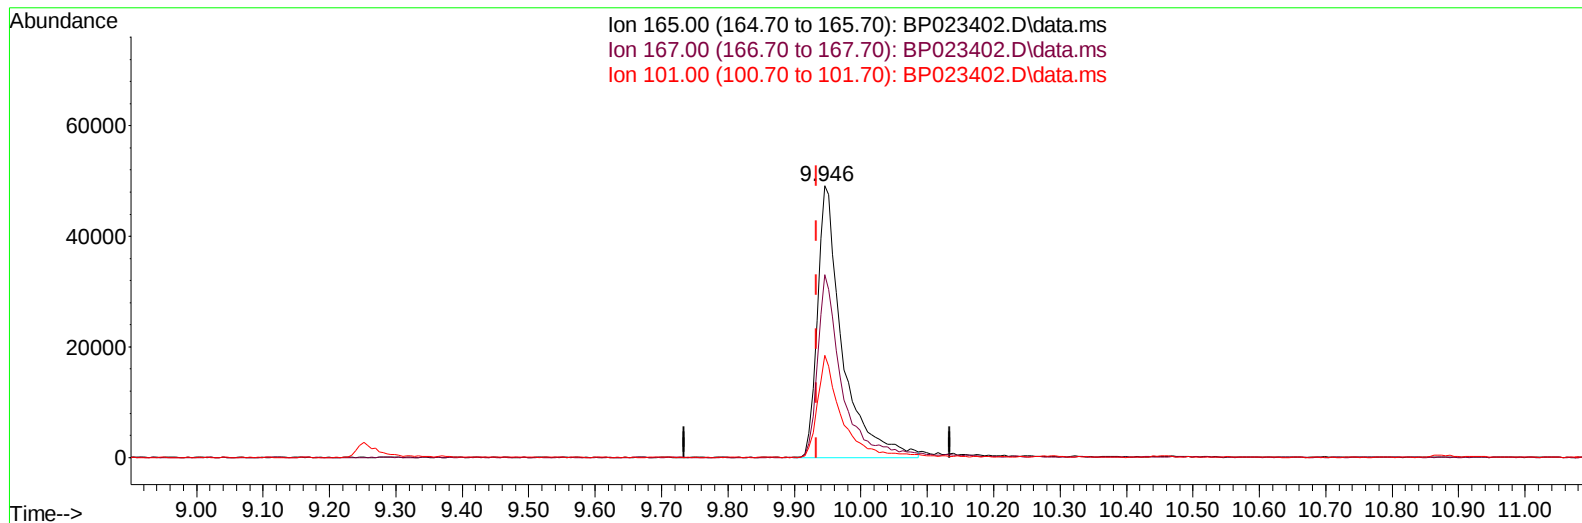

TIC: BP023402.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)




9.946min (+ 0.012) 18.58 ng/ul m

response 128302

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.00	67.34
101.00	34.30	37.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

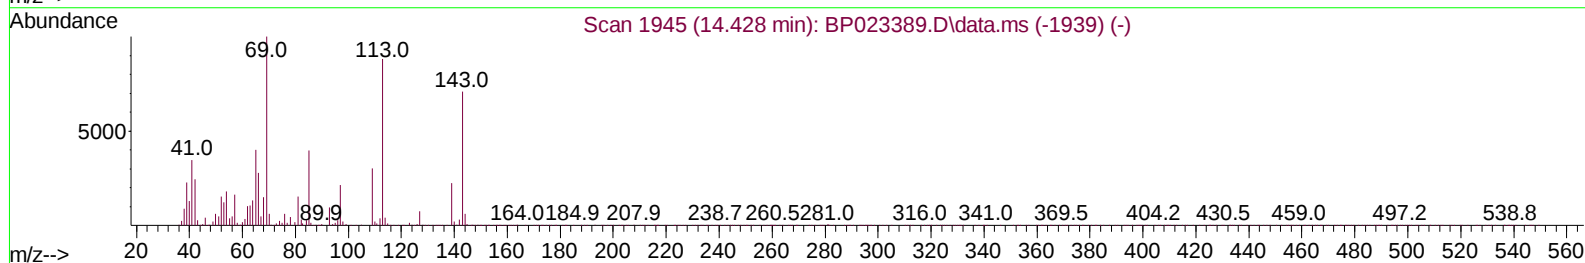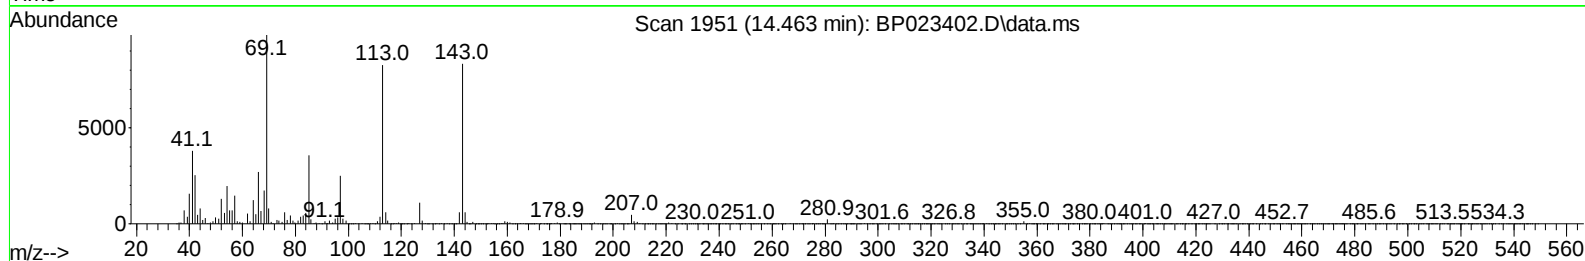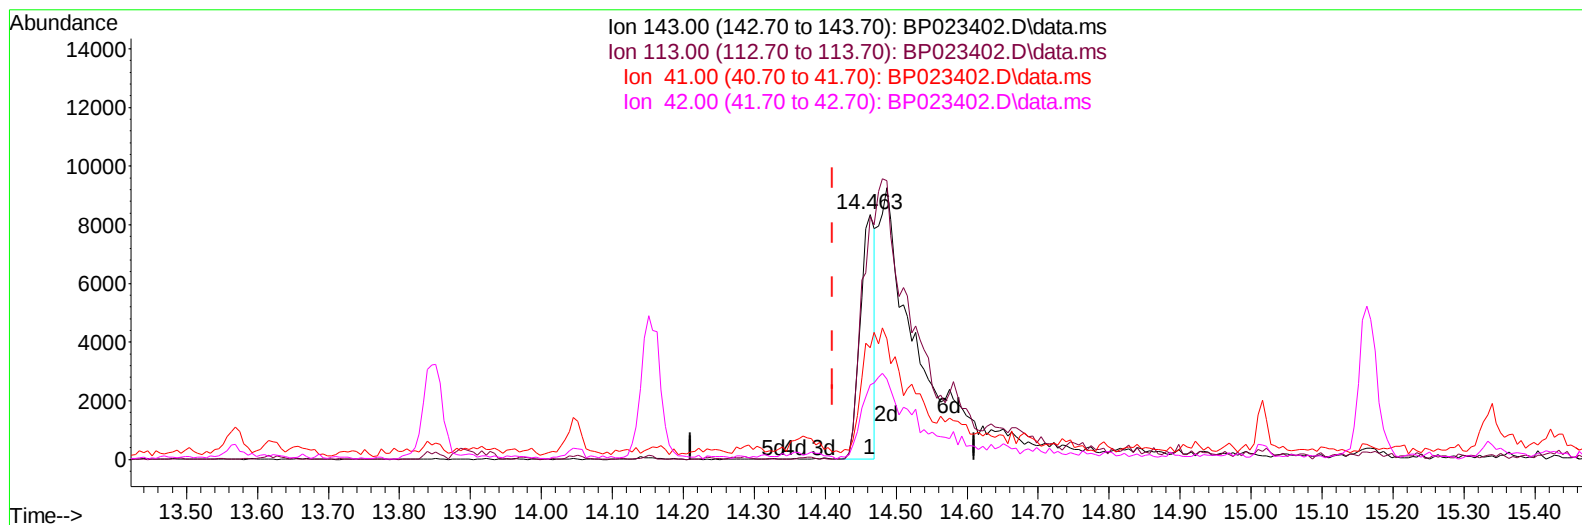

TIC: BP023402.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.463min (+ 0.053) 4.56 ng/ul

response 12001

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	99.15
41.00	45.60	45.60
42.00	31.70	30.45

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

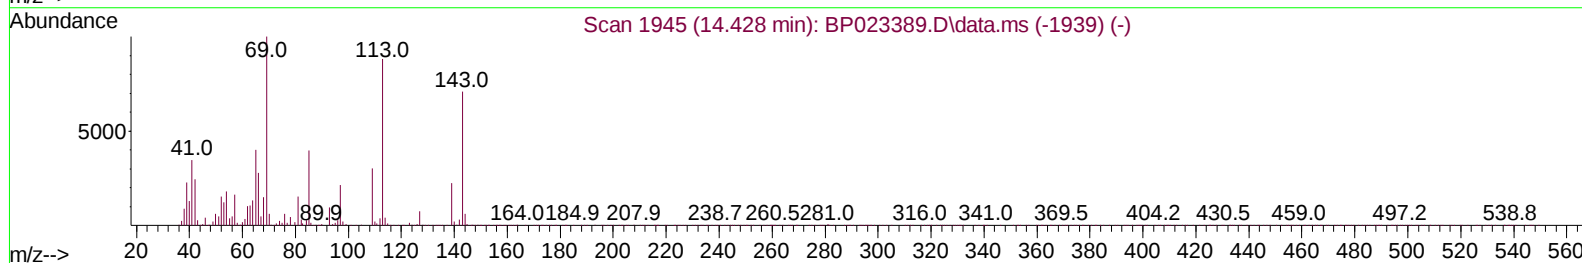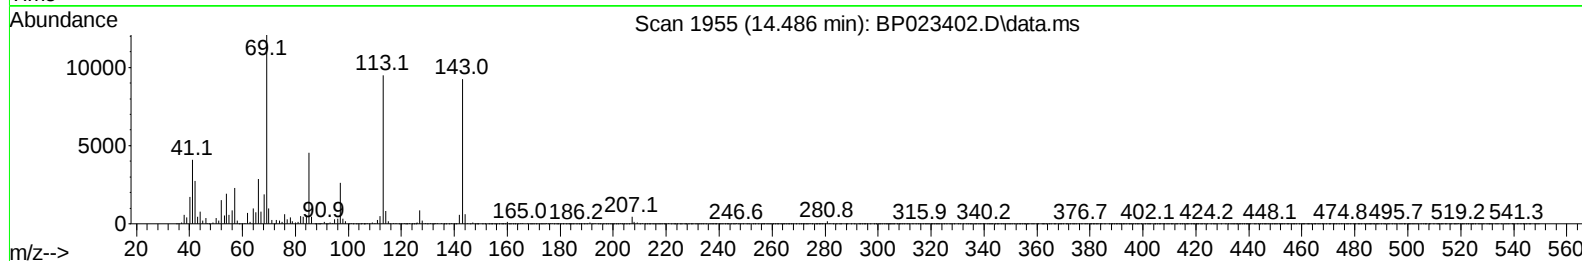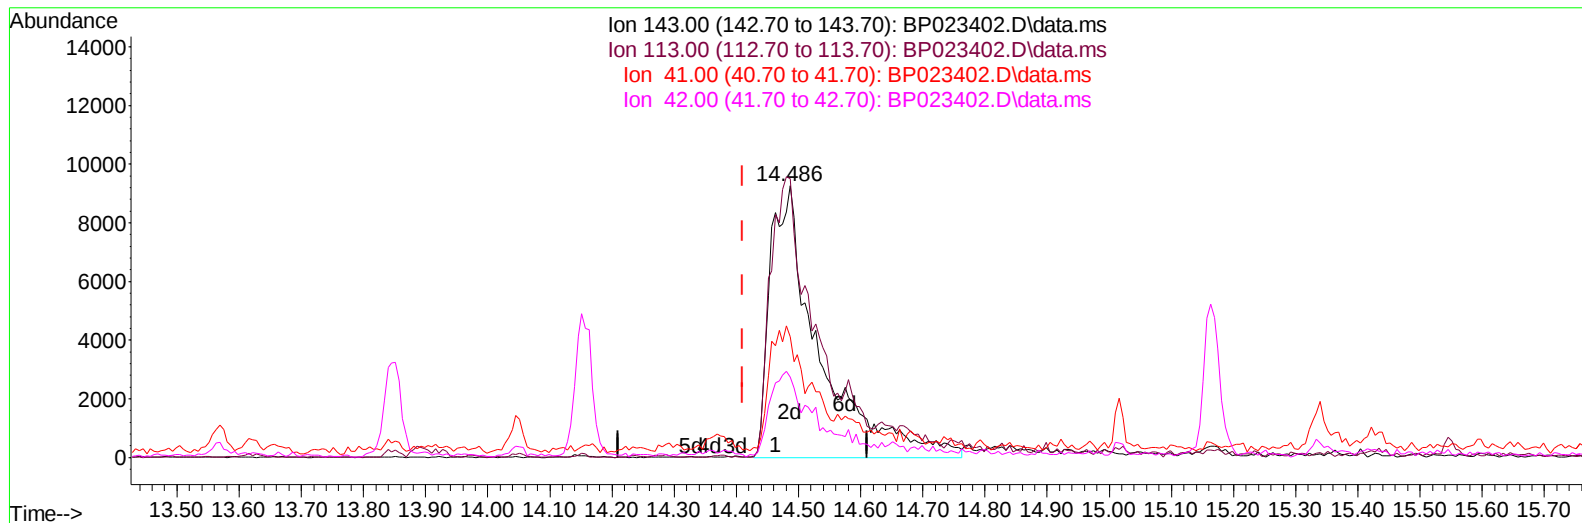

TIC: BP023402.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.486min (+ 0.076) 19.41 ng/ul m

response 51120

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	102.79
41.00	45.60	44.44
42.00	31.70	29.58

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

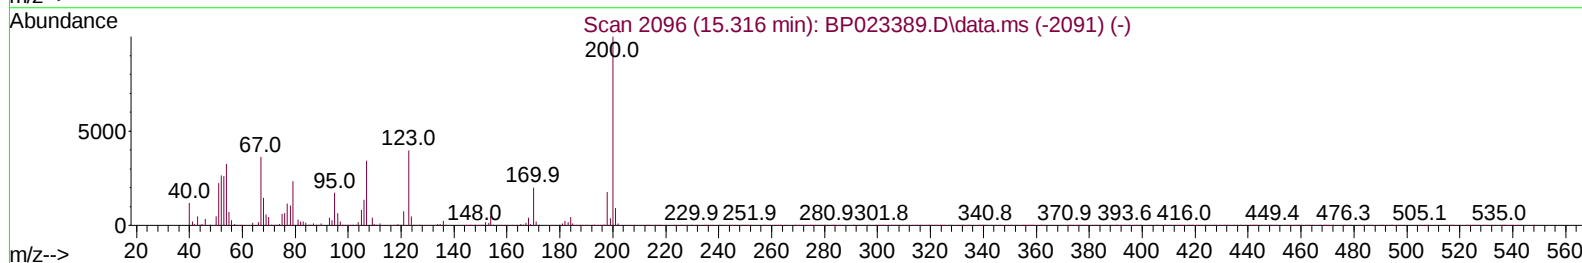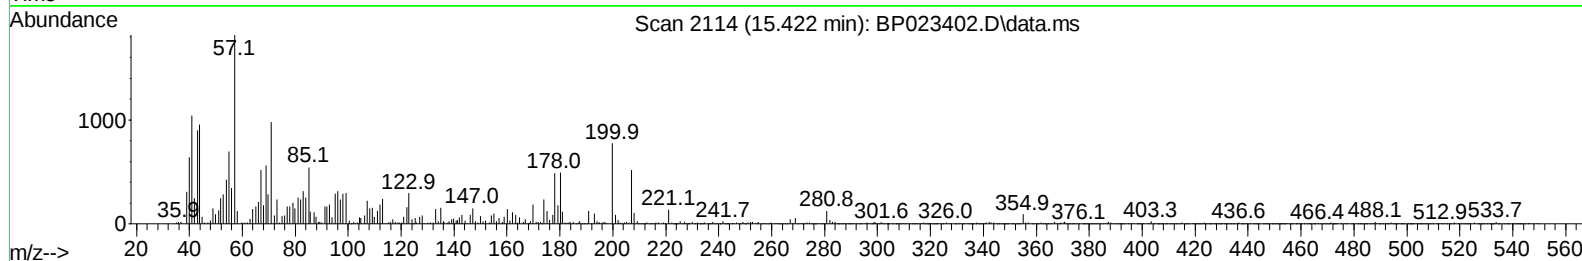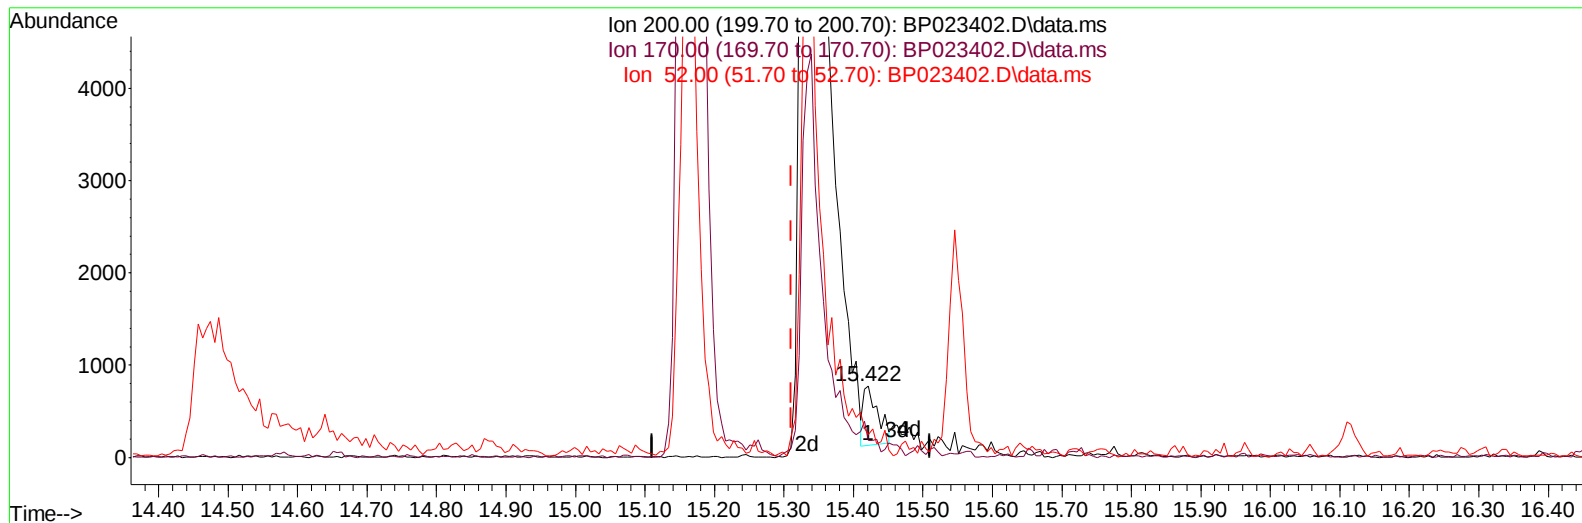

TIC: BP023402.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)




15.422min (+ 0.112) 0.25 ng/ul

response 952

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	23.61
52.00	37.90	32.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:09:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

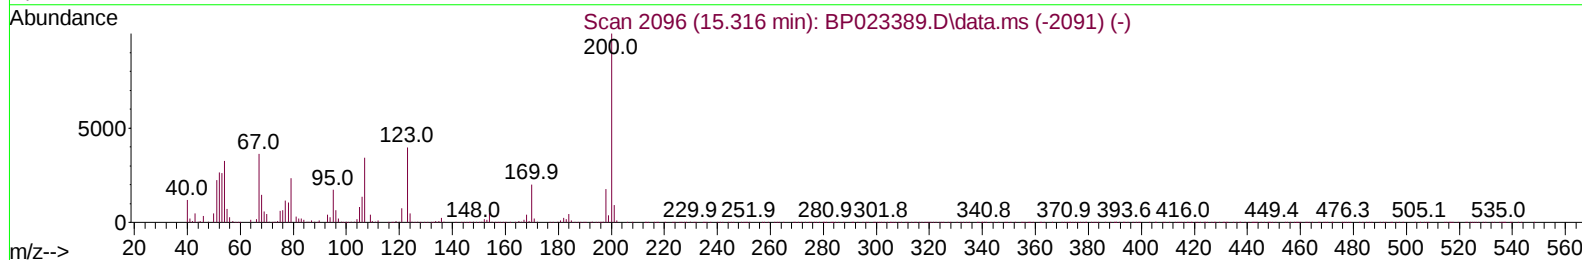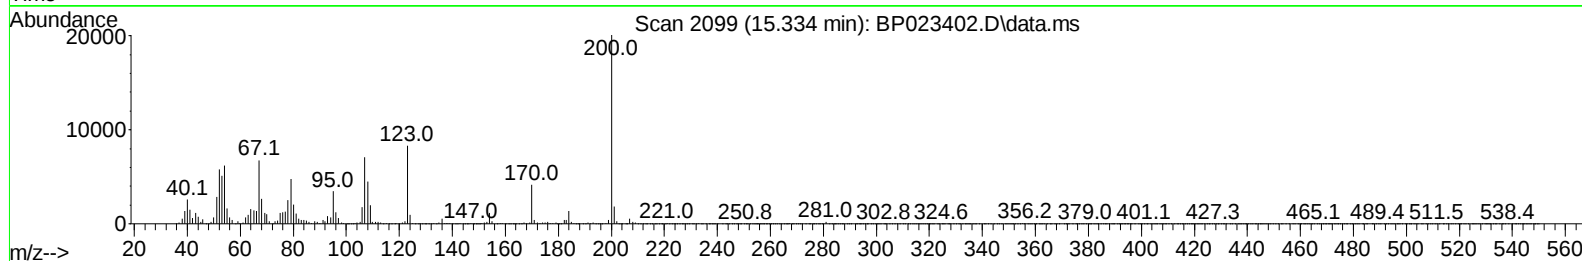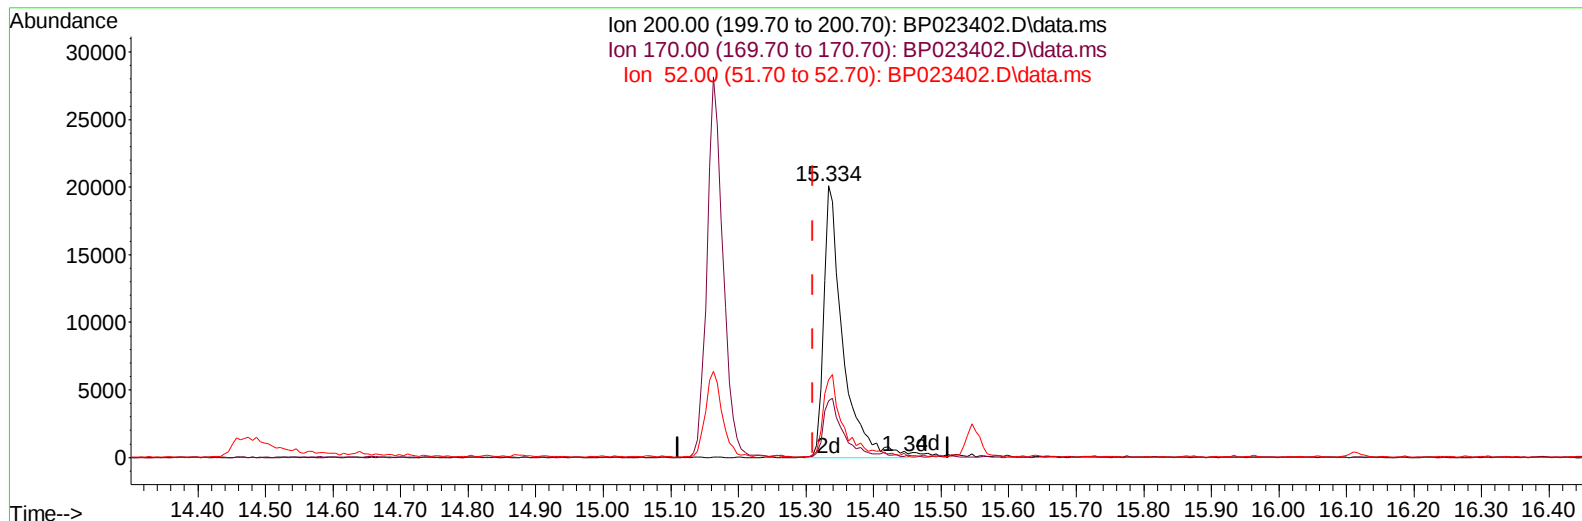

TIC: BP023402.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)**15.334min (+ 0.023) 10.21 ng/ul m****response 39485**

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	20.83
52.00	37.90	28.75#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
 Data File : BP023402.D
 Acq On : 12 Dec 2024 19:12
 Operator : RC/JU
 Sample : P5153-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:11:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.540	152	104683	20.000	ng/ul	0.00
20) Naphthalene-d8	10.287	136	380240	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.157	164	276811	20.000	ng/ul	0.01
64) Phenanthrene-d10	16.957	188	639781	20.000	ng/ul	0.00
79) Chrysene-d12	21.398	240	763783	20.000	ng/ul	0.01
88) Perylene-d12	24.568	264	863693	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.105	96	9774	3.437	ng/uL	0.00
4) Pyridine-d5	3.516	84	115468	15.792	ng/ul	0.00
7) Phenol-d5	6.752	99	154383	18.796	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.887	67	101638	19.613	ng/ul	0.00
11) 2-Chlorophenol-d4	7.087	132	115399	19.036	ng/ul	0.00
15) 4-Methylphenol-d8	8.257	113	122939m	18.545	ng/ul	0.00
21) Nitrobenzene-d5	8.687	128	54930	19.346	ng/ul	0.00
24) 2-Nitrophenol-d4	9.399	143	66782	20.407	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.946	165	128302m	18.577	ng/ul	0.01
31) 4-Chloroaniline-d4	10.446	131	142644	18.436	ng/ul	0.00
46) Dimethylphthalate-d6	13.569	166	449306	20.909	ng/ul	0.01
49) Acenaphthylene-d8	13.845	160	465178	20.523	ng/ul	0.01
54) 4-Nitrophenol-d4	14.486	143	51120m	19.413	ng/ul	0.08
60) Fluorene-d10	15.163	176	376145	19.901	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.334	200	39485m	10.212	ng/ul	0.02
73) Anthracene-d10	17.069	188	637215	21.823	ng/ul	0.02
81) Pyrene-d10	19.445	212	789308	19.780	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.357	264	837372	18.111	ng/ul	0.01

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023402.D
Acq On : 12 Dec 2024 19:12
Operator : RC/JU
Sample : P5153-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 13 02:11:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

