
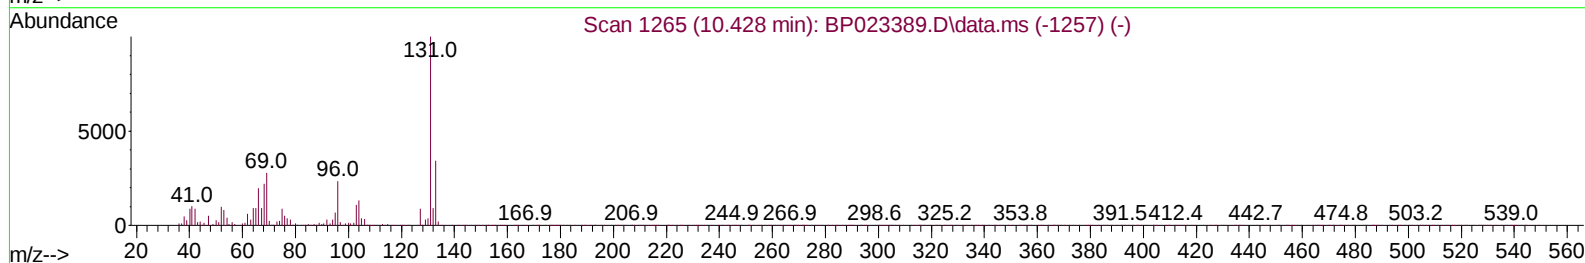
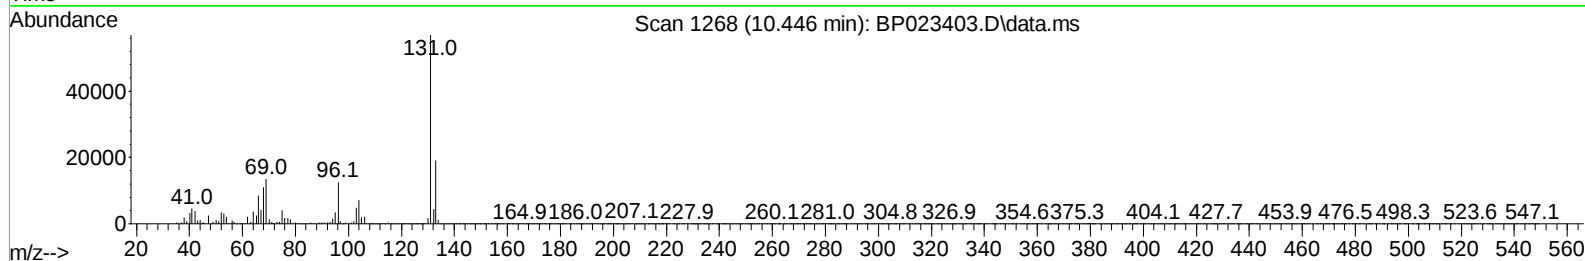


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023403.D
Acq On : 12 Dec 2024 19:52
Operator : RC/JU
Sample : P5153-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 13 02:13:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

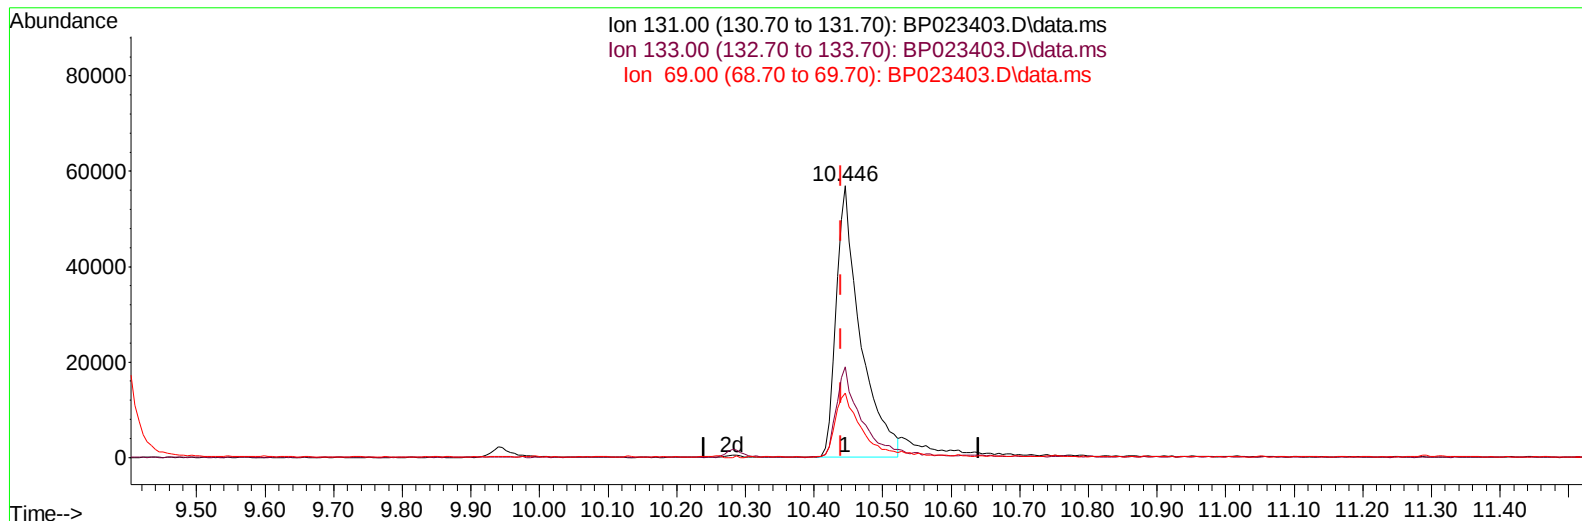

TIC: BP023403.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.446min (+ 0.006) 19.47 ng/u1

response 138902

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	33.40
69.00	24.30	23.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023403.D
Acq On : 12 Dec 2024 19:52
Operator : RC/JU
Sample : P5153-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 13 02:13:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

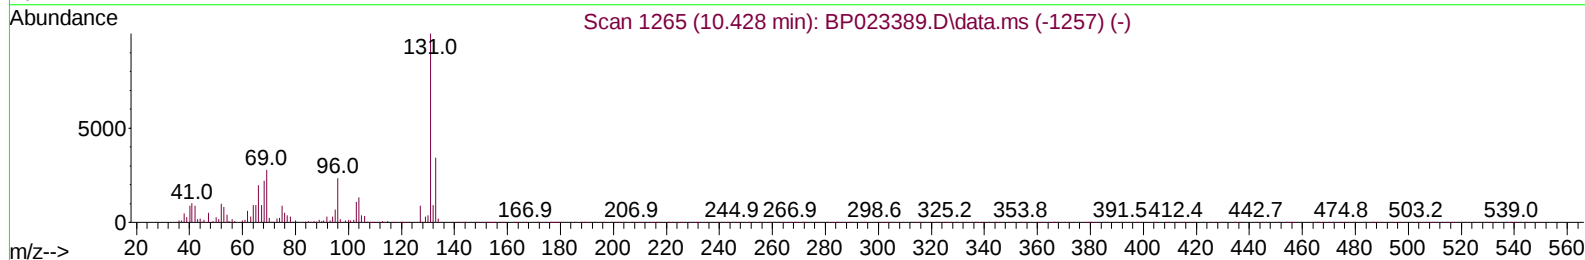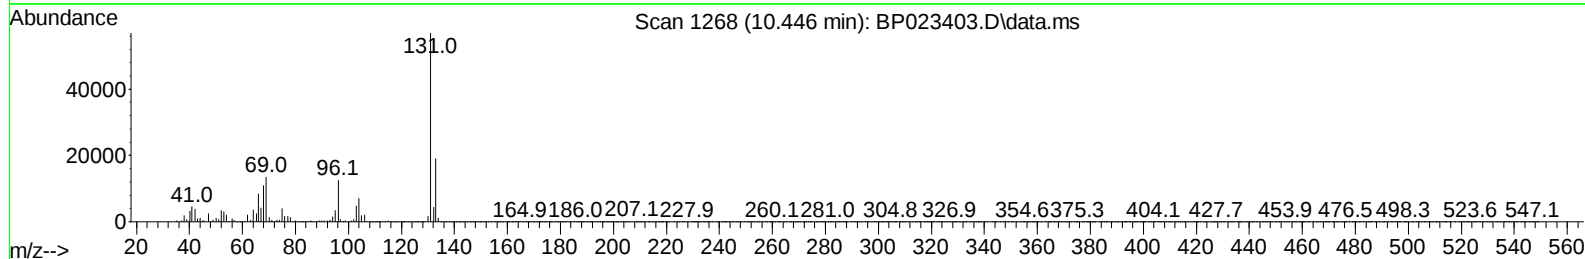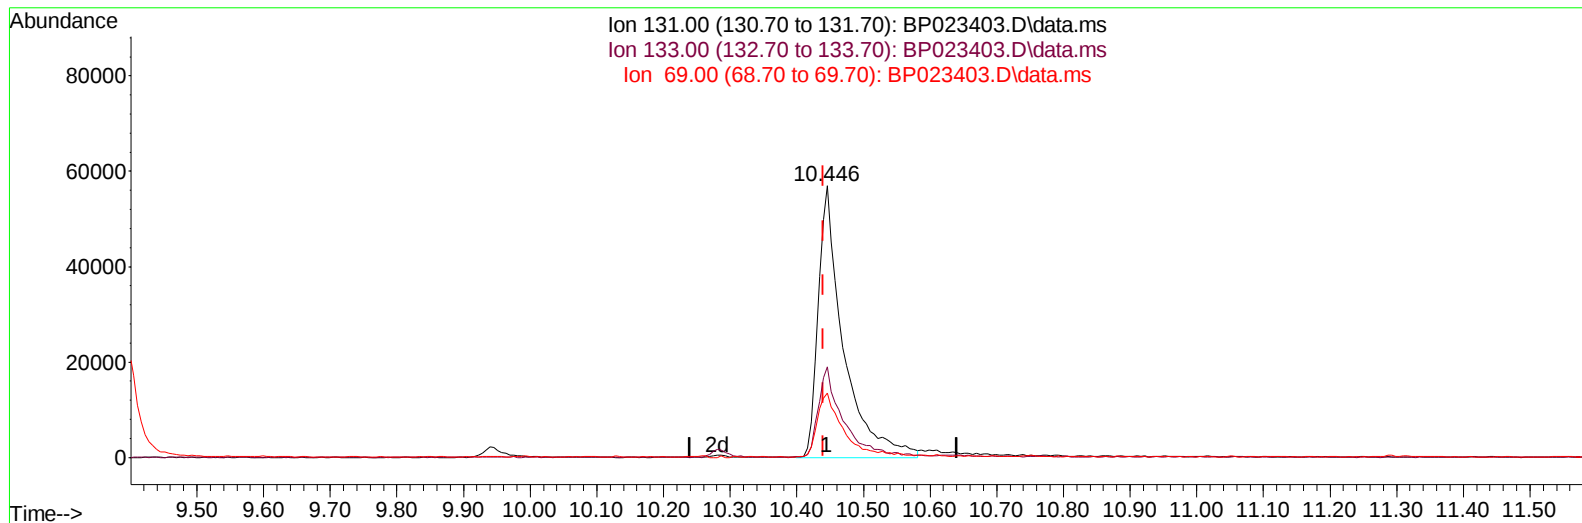

TIC: BP023403.D\data.ms

(31) 4-Chloroaniline-d4 (S)




10.446min (+ 0.006) 20.88 ng/ul m

response 148959

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.60	33.40
69.00	24.30	23.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023403.D
Acq On : 12 Dec 2024 19:52
Operator : RC/JU
Sample : P5153-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 13 02:13:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

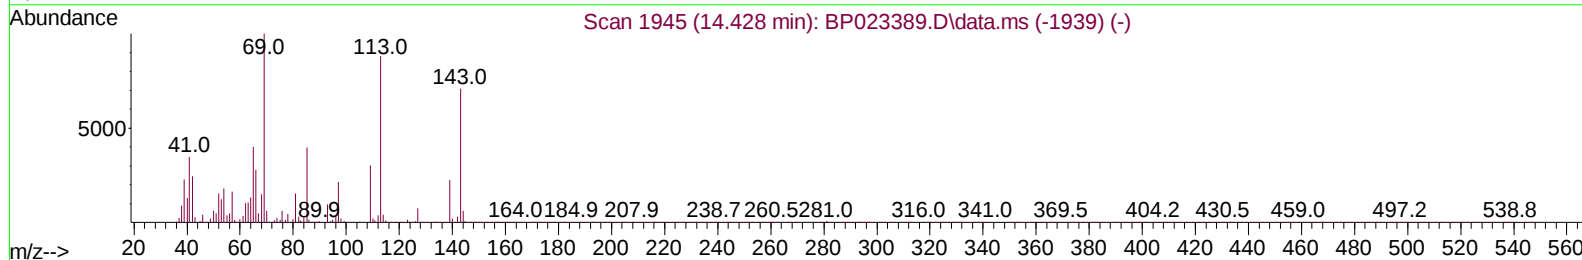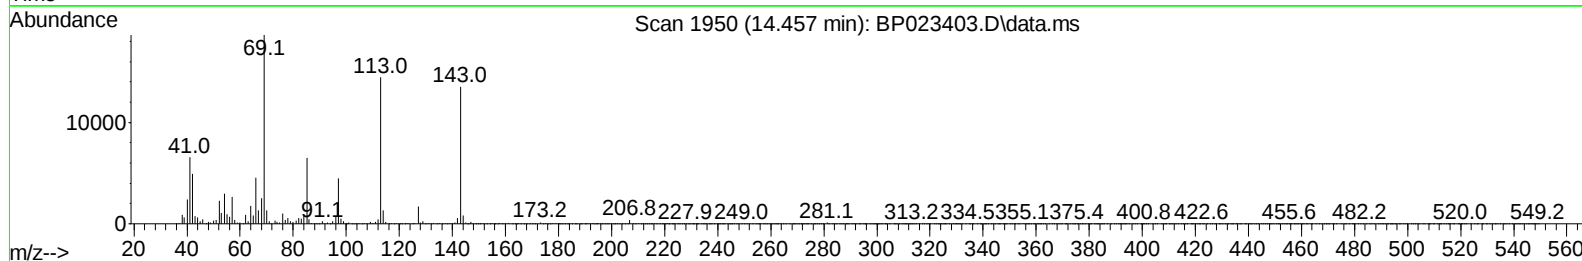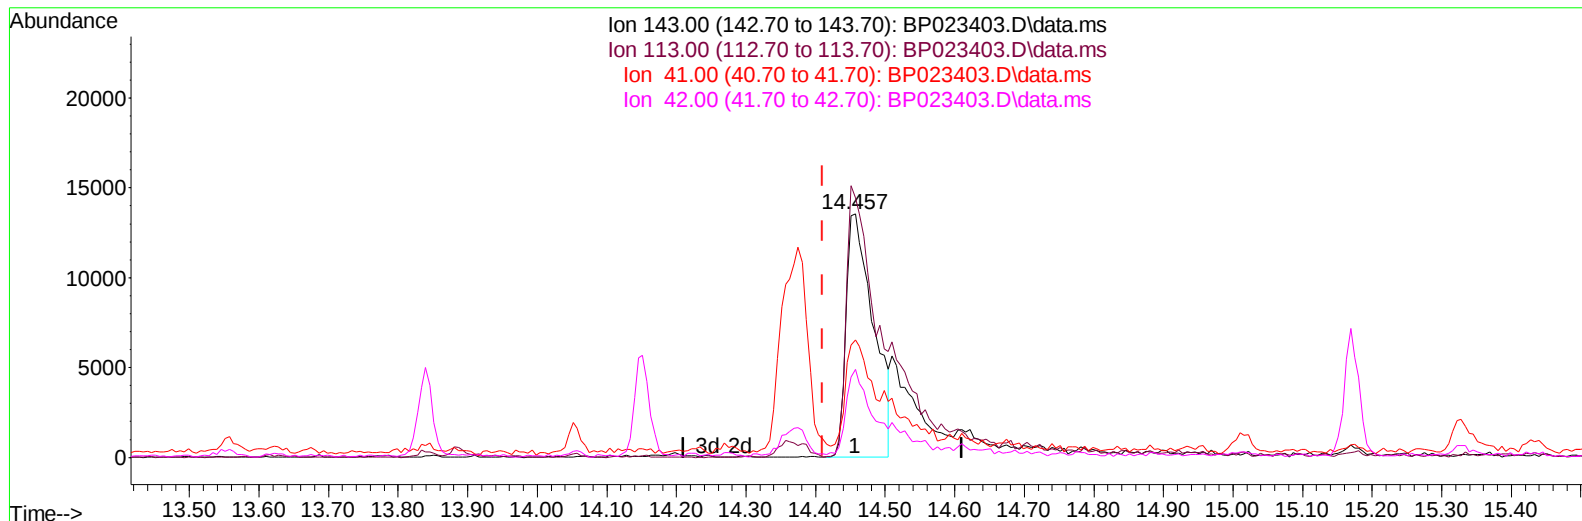

TIC: BP023403.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.457min (+ 0.047) 15.04 ng/u1

response 36878

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	106.66
41.00	45.60	48.31
42.00	31.70	36.26

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023403.D
Acq On : 12 Dec 2024 19:52
Operator : RC/JU
Sample : P5153-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 13 02:13:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

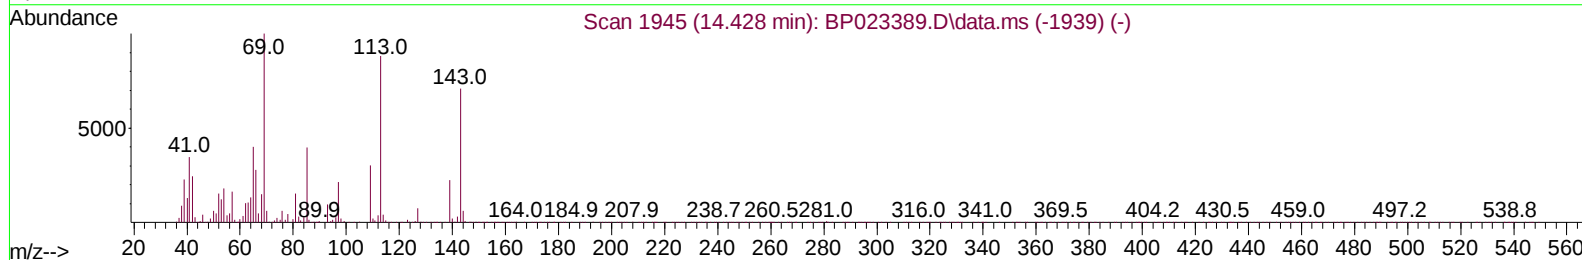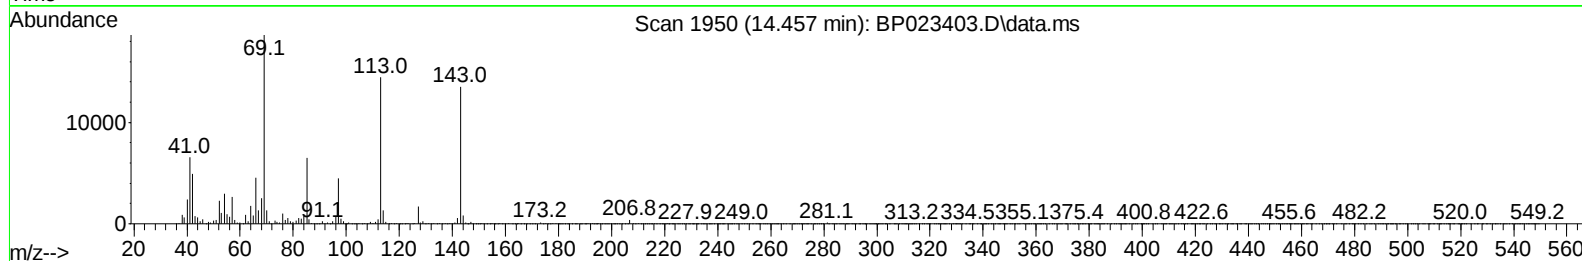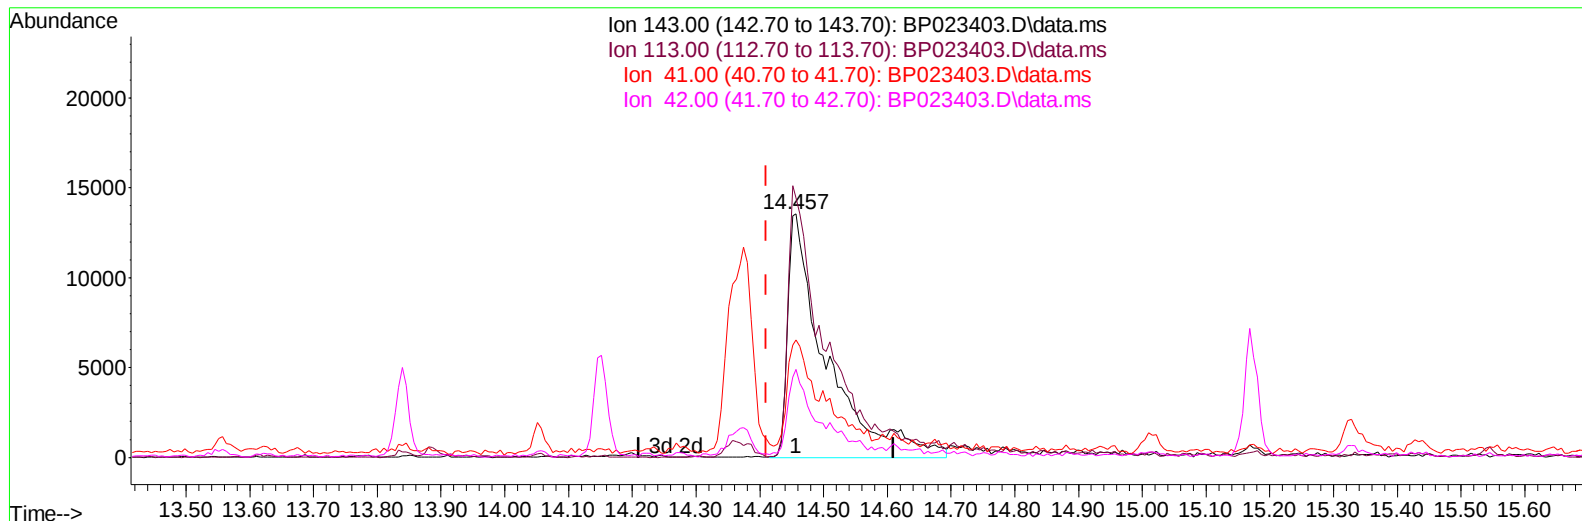

TIC: BP023403.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.457min (+ 0.047) 23.23 ng/ul m

response 56973

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	106.66
41.00	45.60	48.31
42.00	31.70	36.26

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023403.D
Acq On : 12 Dec 2024 19:52
Operator : RC/JU
Sample : P5153-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 13 02:13:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

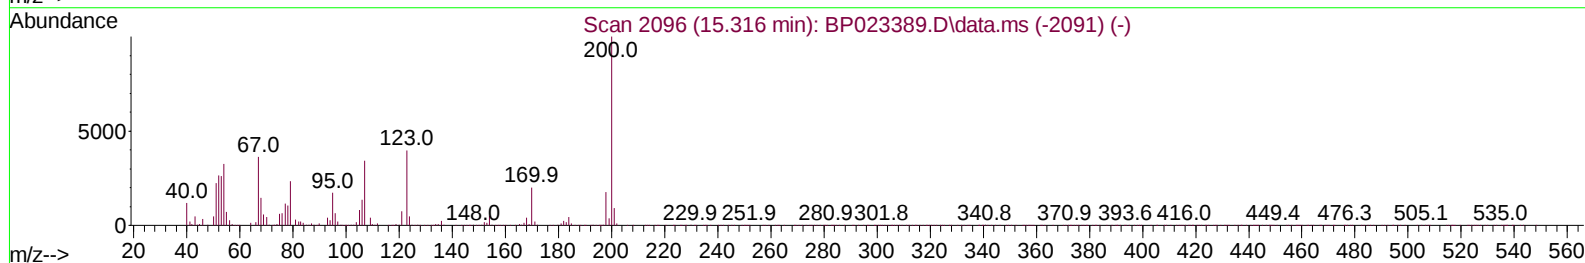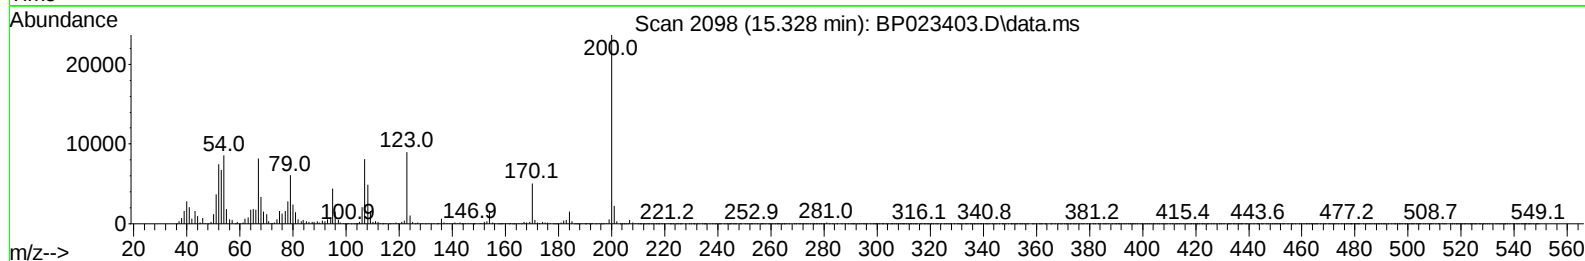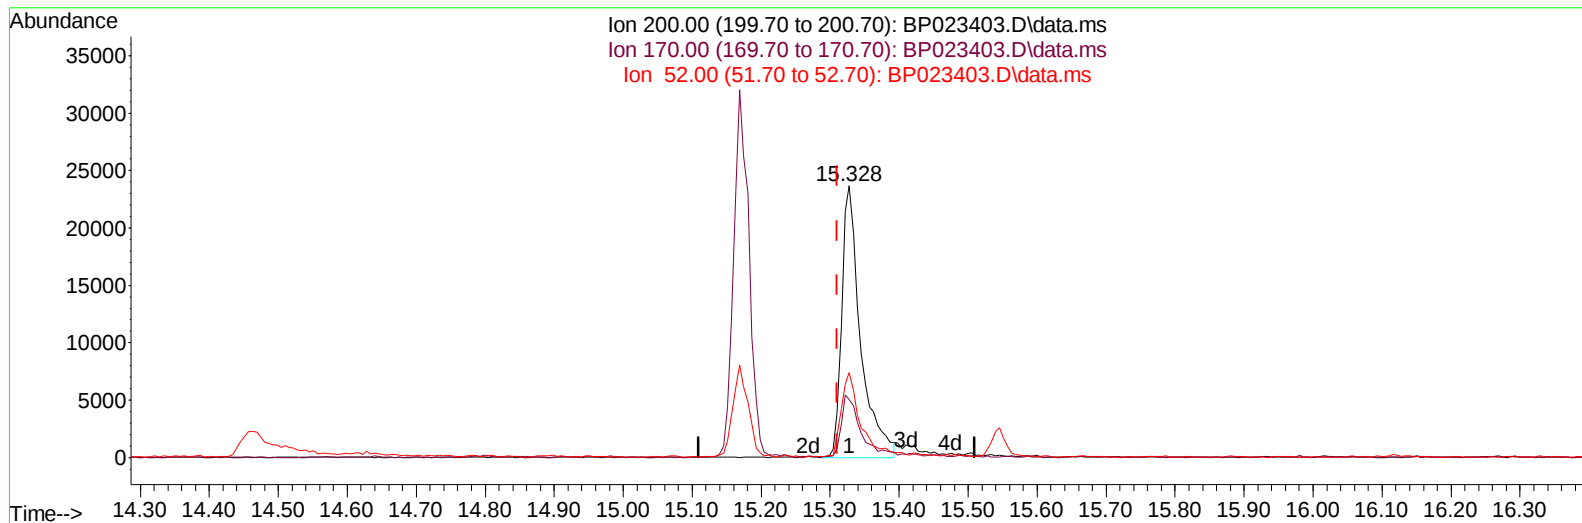

TIC: BP023403.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)




15.328min (+ 0.018) 12.26 ng/ul

response 44831

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	21.38
52.00	37.90	31.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023403.D
Acq On : 12 Dec 2024 19:52
Operator : RC/JU
Sample : P5153-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 13 02:13:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

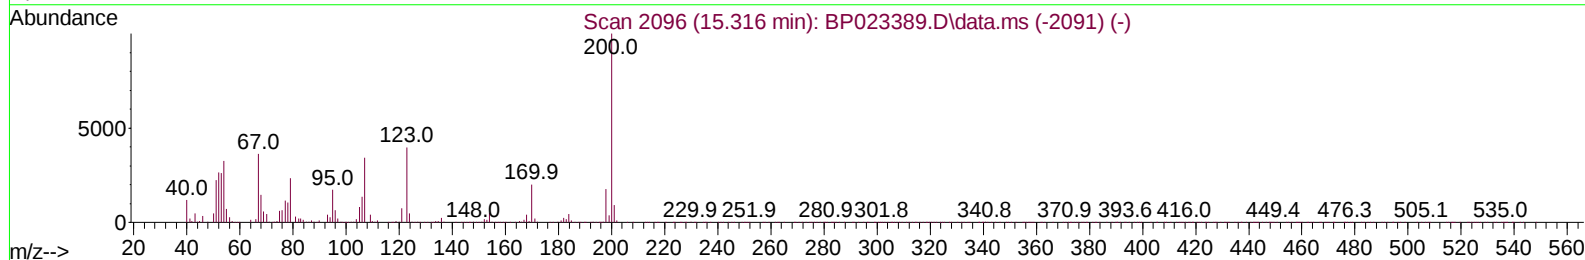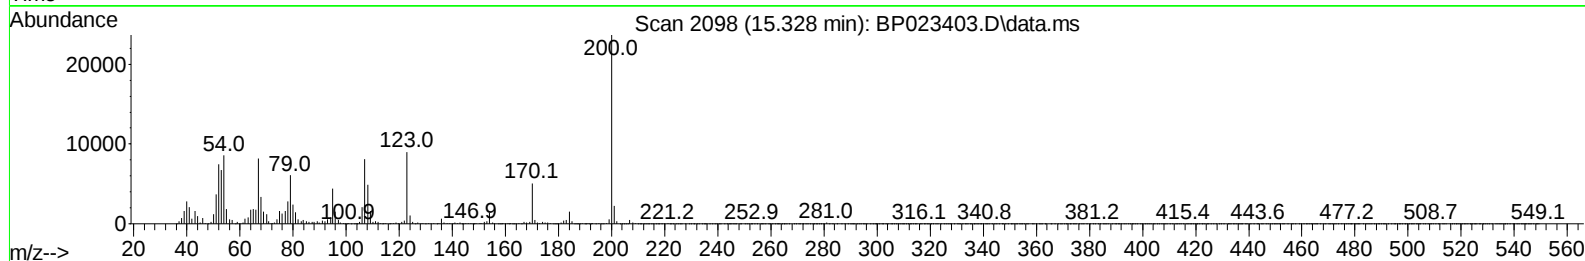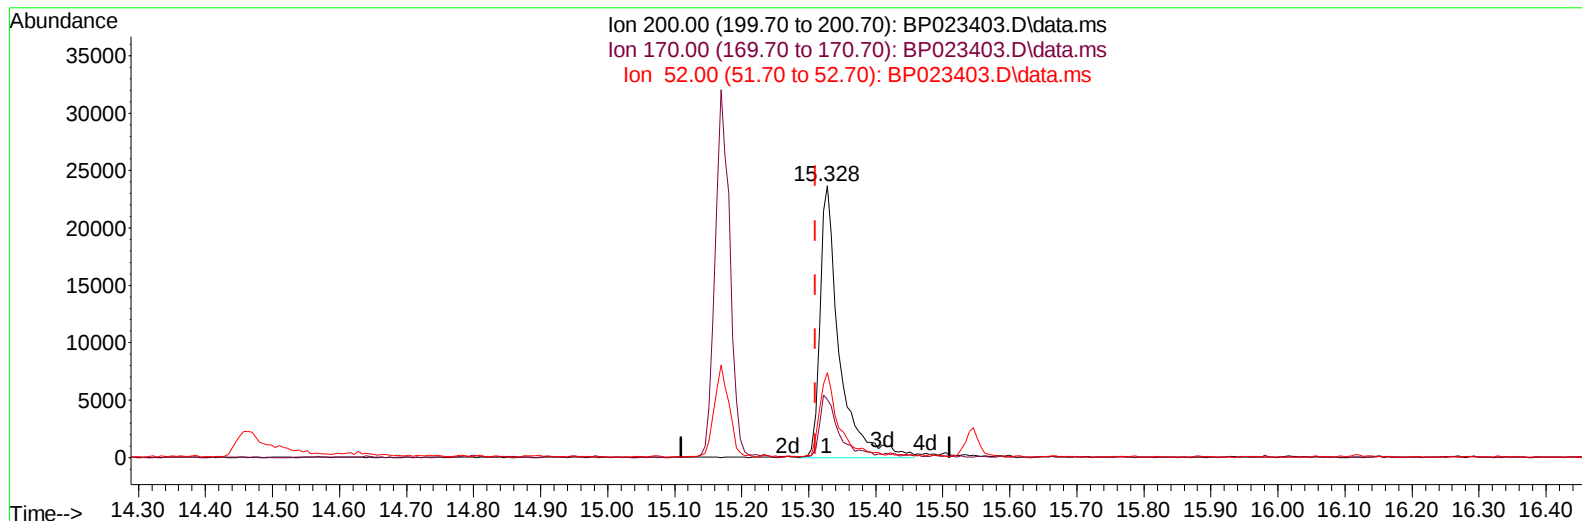

TIC: BP023403.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)**15.328min (+ 0.018) 13.01 ng/ul m****response 47576**

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	23.30	21.38
52.00	37.90	31.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
 Data File : BP023403.D
 Acq On : 12 Dec 2024 19:52
 Operator : RC/JU
 Sample : P5153-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 13 02:18:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.534	152	93718	20.000	ng/ul	0.00
20) Naphthalene-d8	10.281	136	350589	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	257795	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.963	188	605172	20.000	ng/ul	0.00
79) Chrysene-d12	21.386	240	761982	20.000	ng/ul	0.00
88) Perylene-d12	24.557	264	868554	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	10993	4.318	ng/uL	0.00
4) Pyridine-d5	3.511	84	129954	19.853	ng/ul	0.00
7) Phenol-d5	6.746	99	165801	22.548	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.887	67	109172	23.532	ng/ul	0.00
11) 2-Chlorophenol-d4	7.087	132	121768	22.437	ng/ul	0.00
15) 4-Methylphenol-d8	8.258	113	133099	22.427	ng/ul	0.00
21) Nitrobenzene-d5	8.681	128	59066	22.562	ng/ul	0.00
24) 2-Nitrophenol-d4	9.393	143	70684	23.427	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.940	165	139957	21.978	ng/ul	0.00
31) 4-Chloroaniline-d4	10.446	131	148959m	20.880	ng/ul	0.00
46) Dimethylphthalate-d6	13.557	166	469057	23.438	ng/ul	0.00
49) Acenaphthylene-d8	13.840	160	482700	22.867	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	56973m	23.231	ng/ul	0.05
60) Fluorene-d10	15.169	176	402419	22.861	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.328	200	47576m	13.008	ng/ul	0.02
73) Anthracene-d10	17.057	188	661632	23.955	ng/ul	0.00
81) Pyrene-d10	19.439	212	859382	21.587	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.333	264	1005006	21.615	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	6.775	94	7935	1.037	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023403.D
Acq On : 12 Dec 2024 19:52
Operator : RC/JU
Sample : P5153-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Dec 13 02:18:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

