
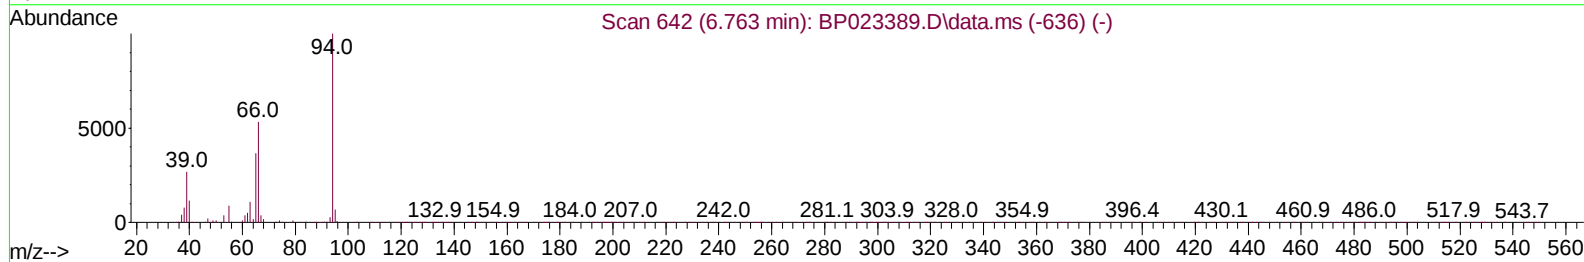
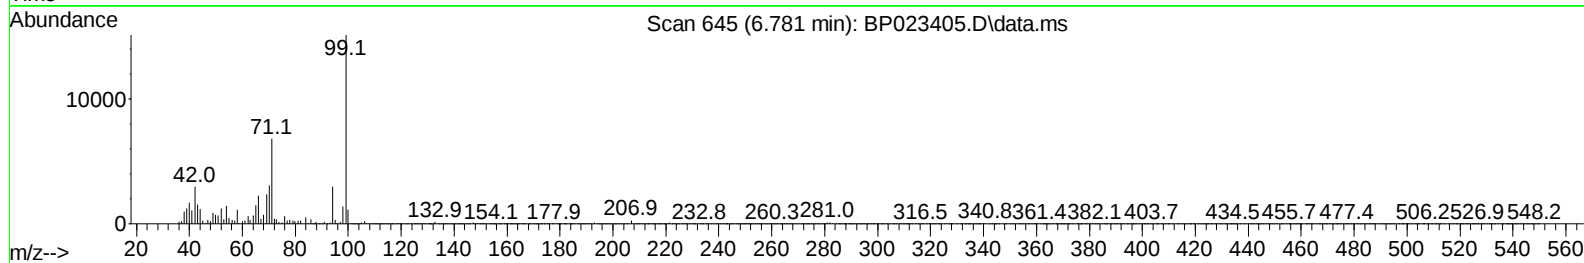


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023405.D
Acq On : 12 Dec 2024 21:13
Operator : RC/JU
Sample : P5232-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 13 03:14:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

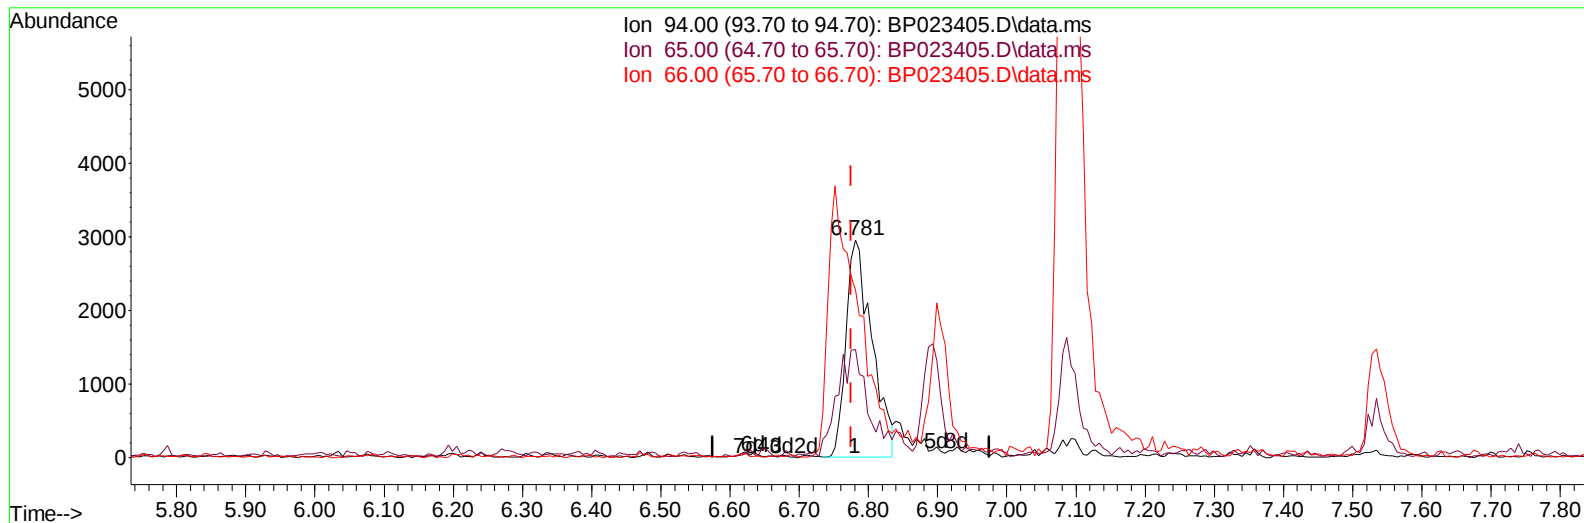

TIC: BP023405.D\data.ms

(8) Phenol




6.781min (+ 0.006) 0.92 ng/u1

response 7635

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	35.00	49.71#
66.00	52.50	77.12#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023405.D
Acq On : 12 Dec 2024 21:13
Operator : RC/JU
Sample : P5232-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 13 03:14:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

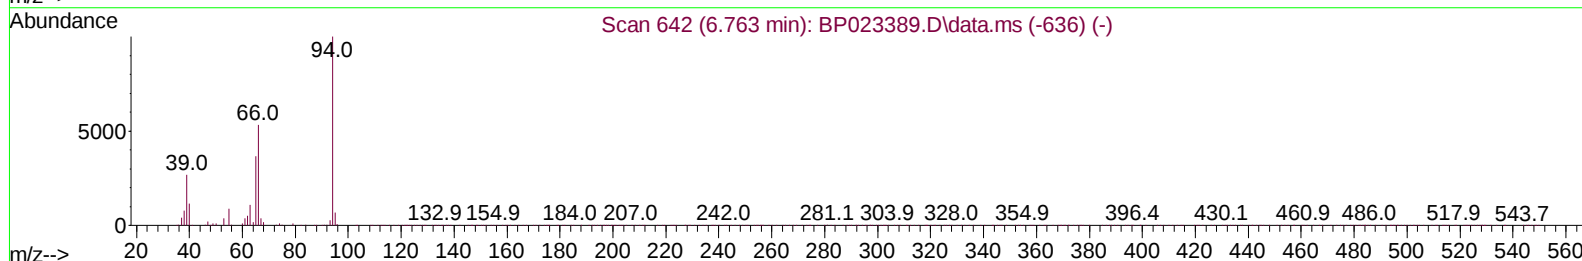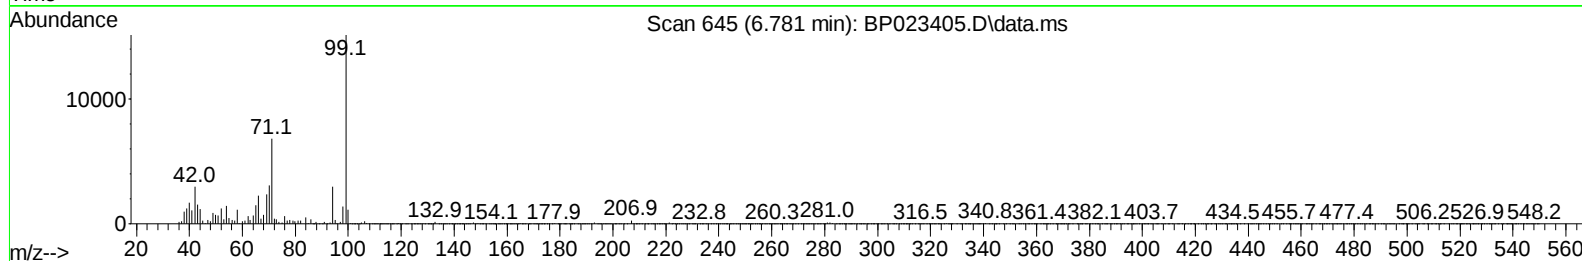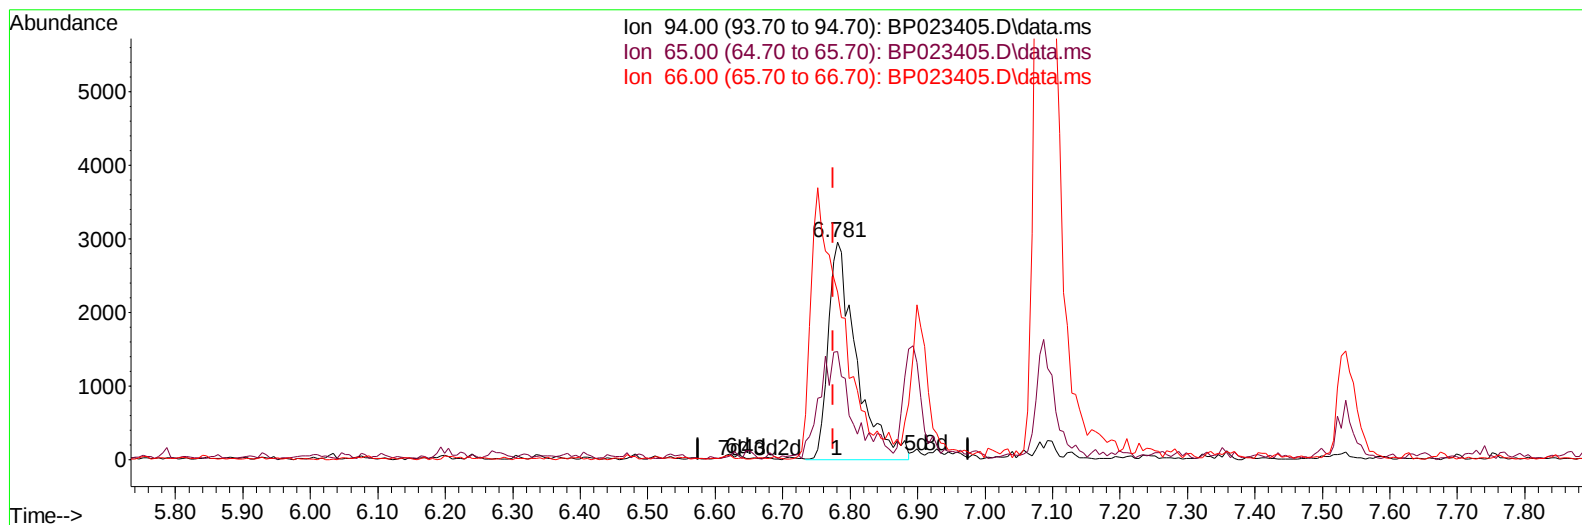

TIC: BP023405.D\data.ms

(8) Phenol




6.781min (+ 0.006) 1.03 ng/ul m

response 8512

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	35.00	49.71#
66.00	52.50	77.12#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023405.D
Acq On : 12 Dec 2024 21:13
Operator : RC/JU
Sample : P5232-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 13 03:14:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

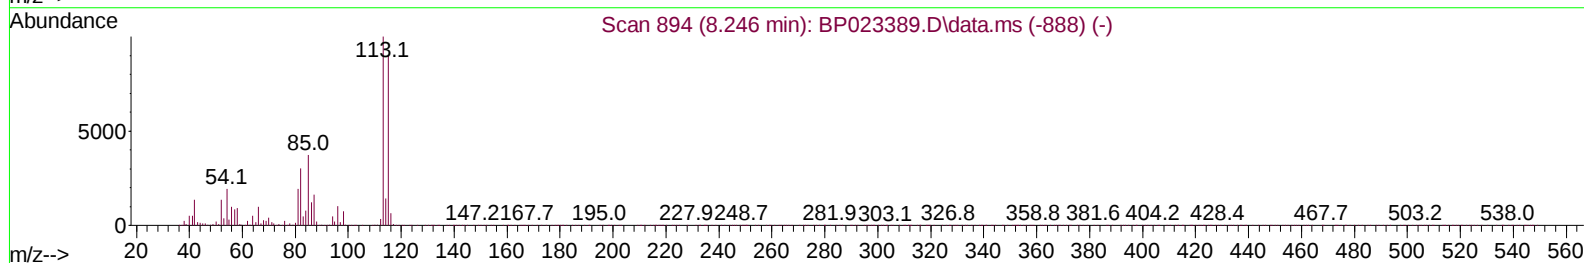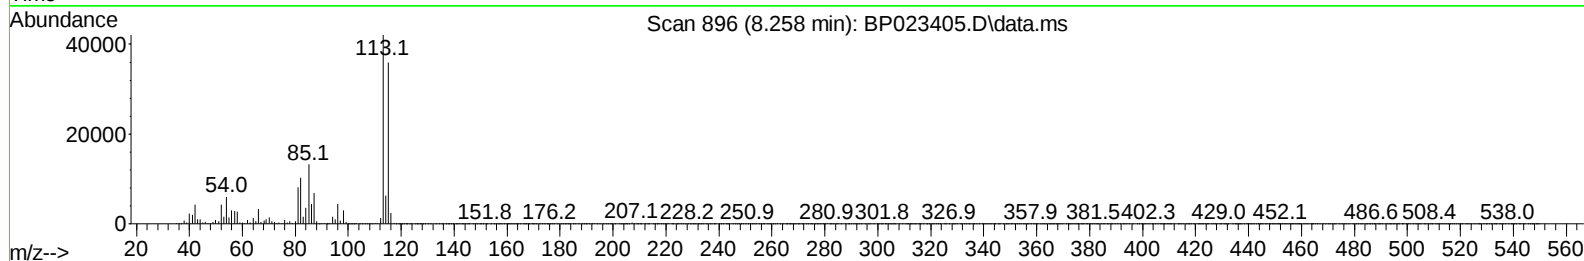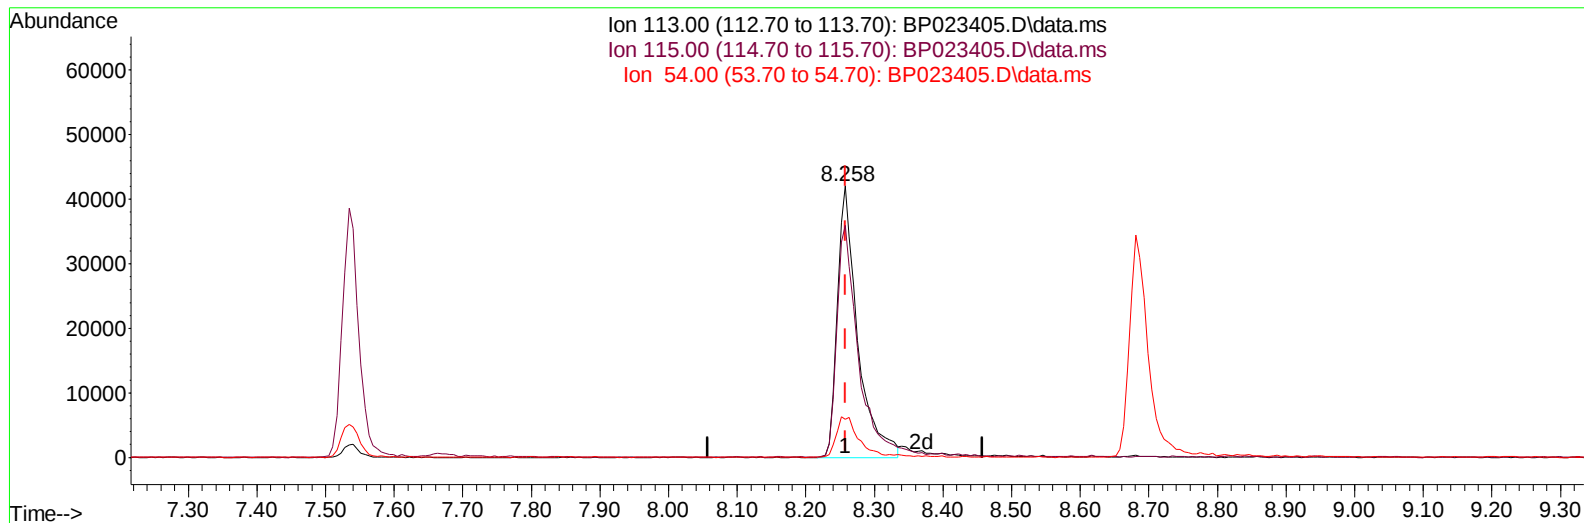

TIC: BP023405.D\data.ms

(15) 4-Methylphenol-d8 (S)




8.258min (-0.000) 13.56 ng/u1

response 86890

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	87.60	85.43
54.00	16.60	14.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023405.D
Acq On : 12 Dec 2024 21:13
Operator : RC/JU
Sample : P5232-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 13 03:14:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

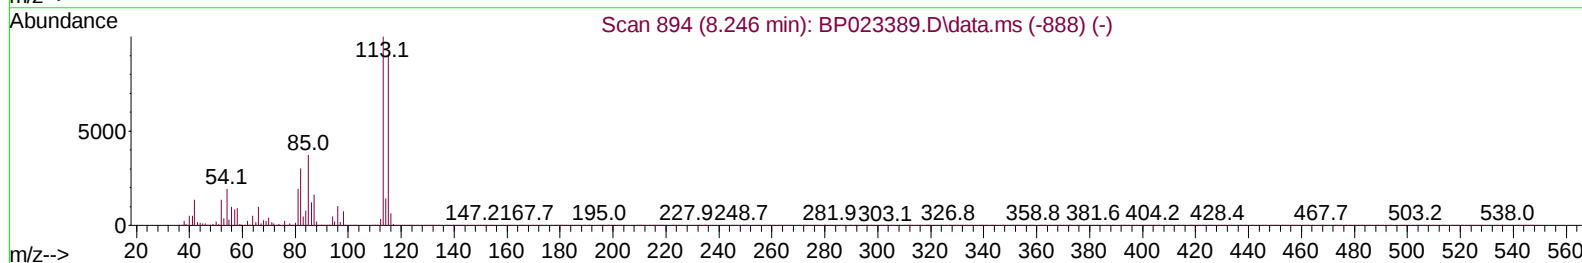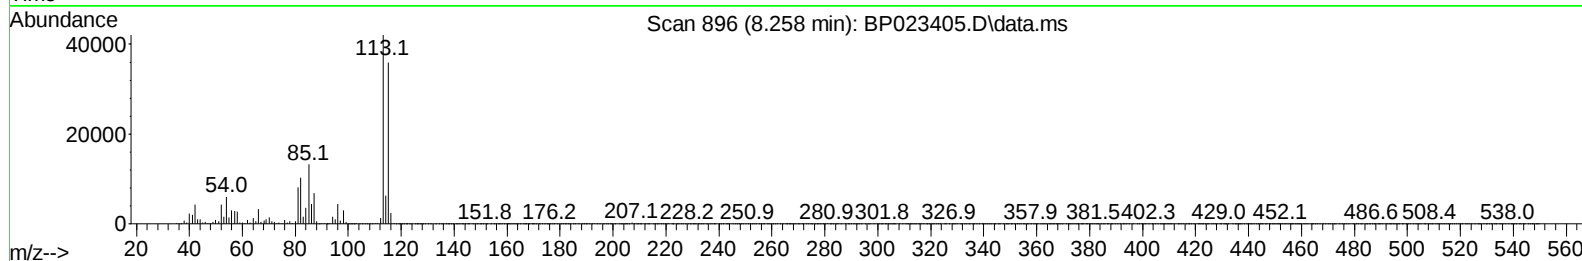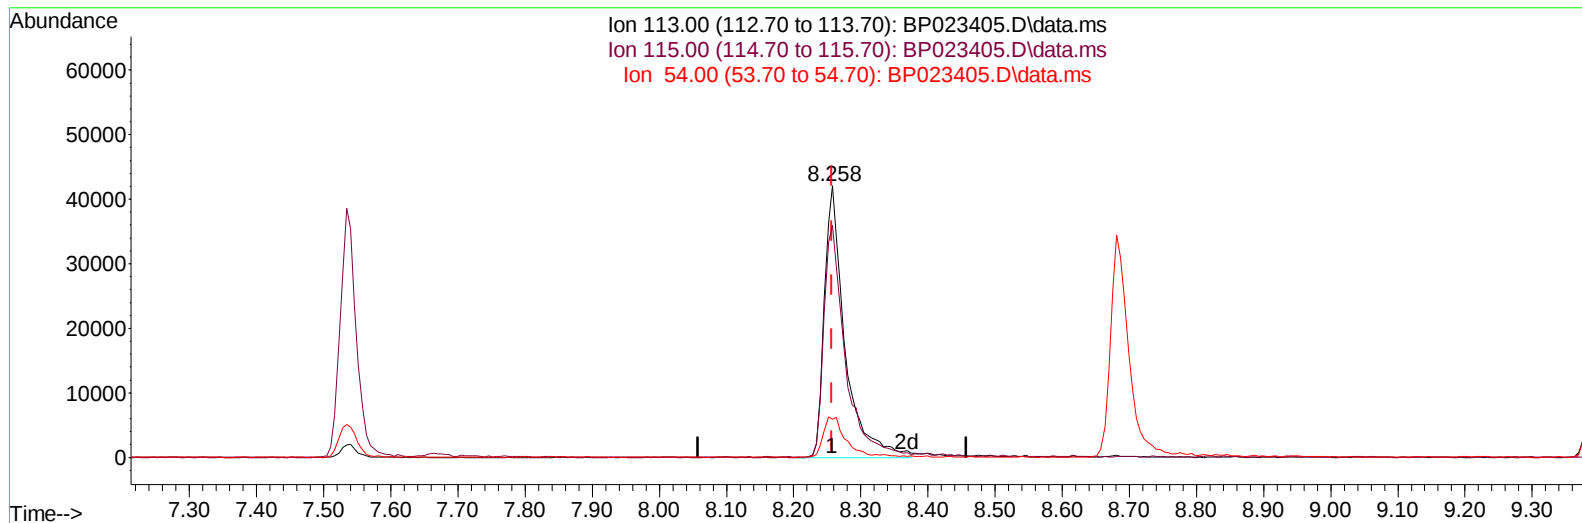

TIC: BP023405.D\data.ms

(15) 4-Methylphenol-d8 (S)




8.258min (-0.000) 14.01 ng/ul m

response 89758

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	87.60	85.43
54.00	16.60	14.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023405.D
Acq On : 12 Dec 2024 21:13
Operator : RC/JU
Sample : P5232-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 13 03:14:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

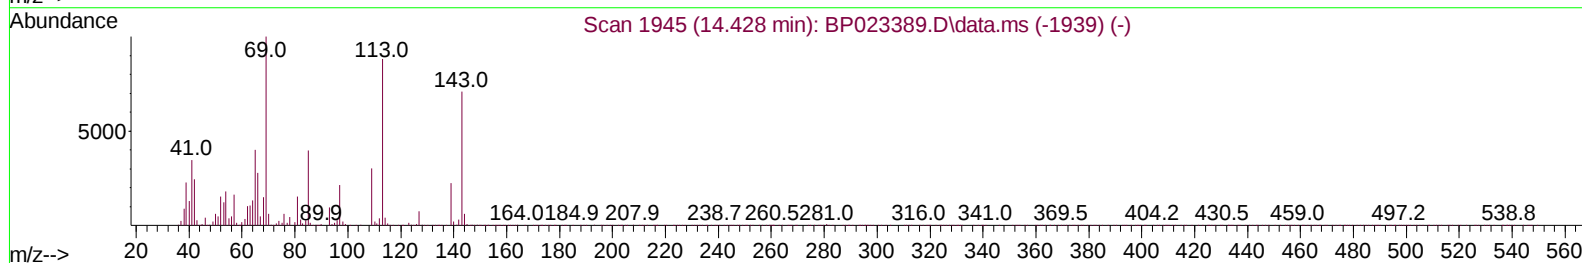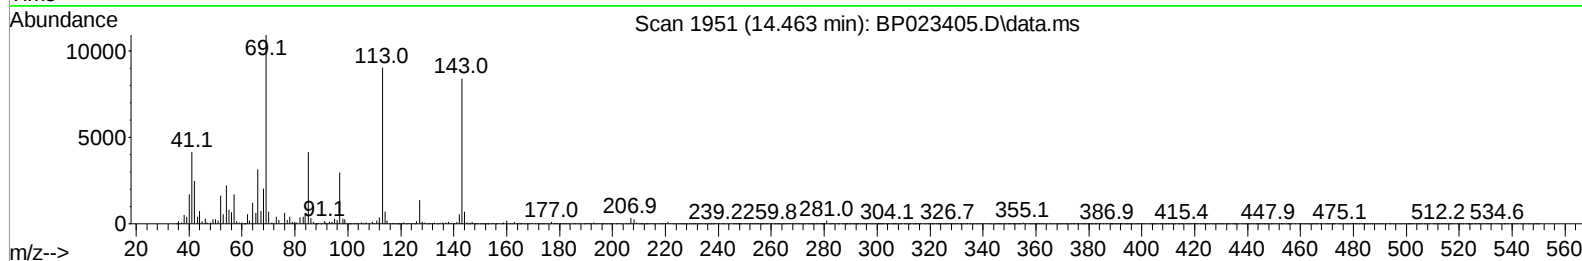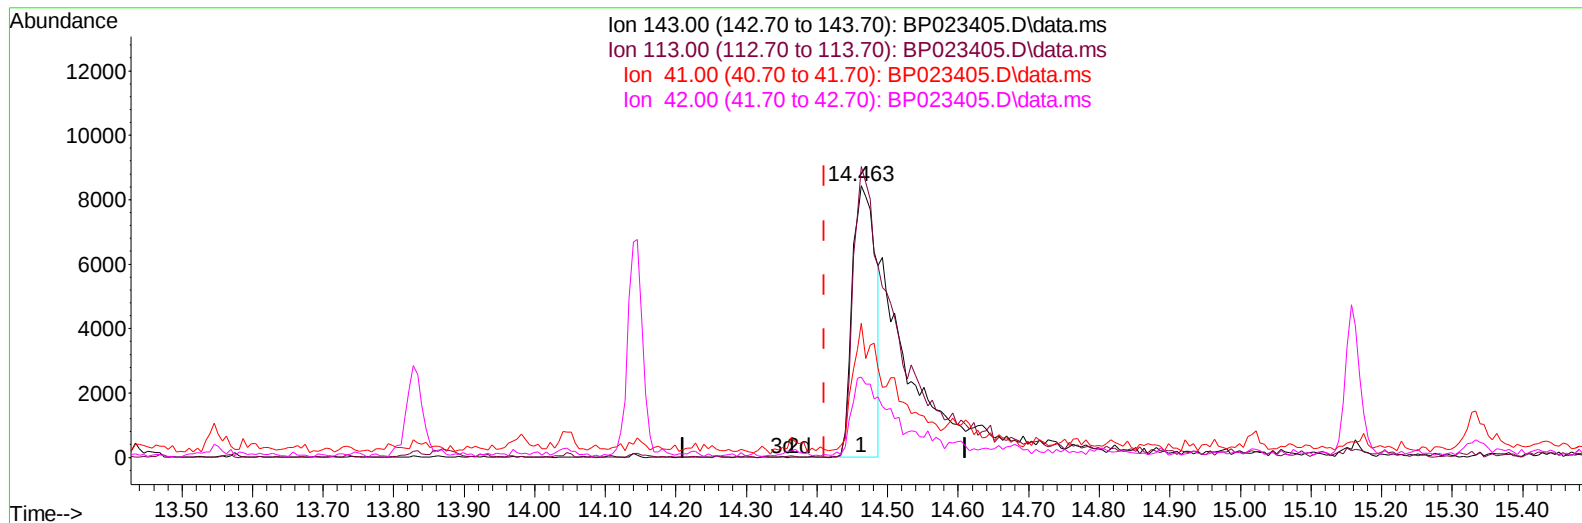

TIC: BP023405.D\data.ms

(54) 4-Nitrophenol-d4 (S)




14.463min (+ 0.053) 6.72 ng/ul

response 19134

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	107.24
41.00	45.60	49.50
42.00	31.70	29.62

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023405.D
Acq On : 12 Dec 2024 21:13
Operator : RC/JU
Sample : P5232-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 13 03:14:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

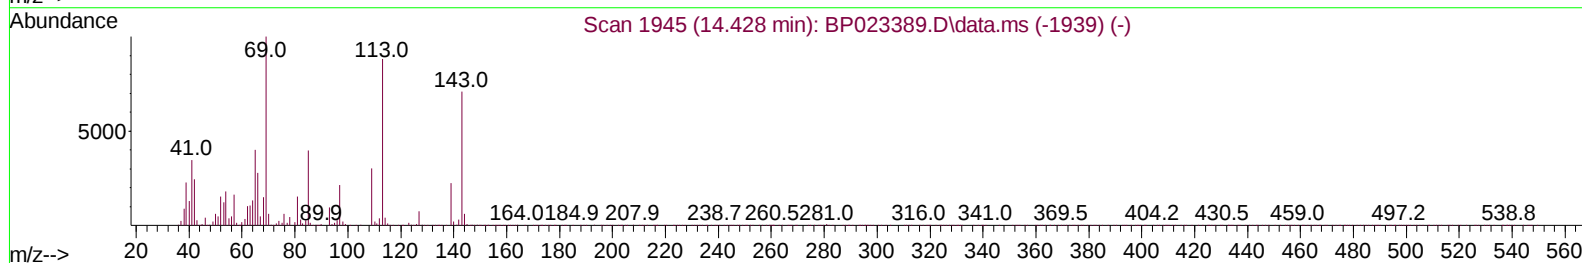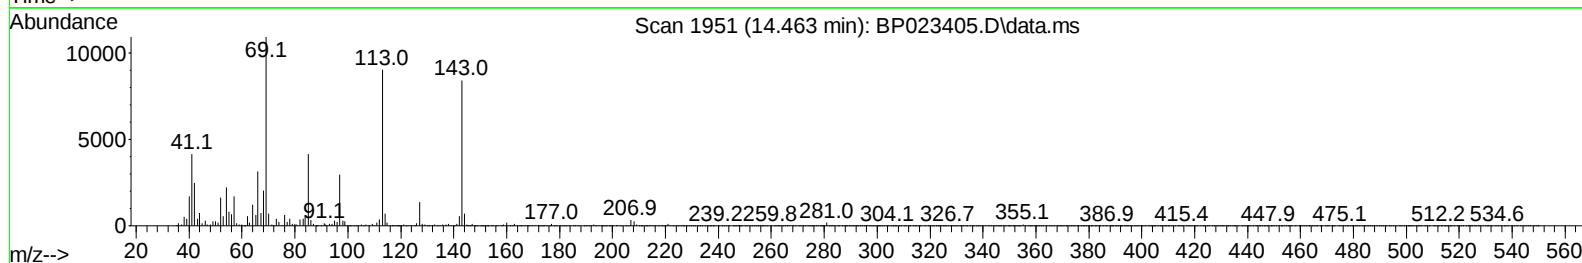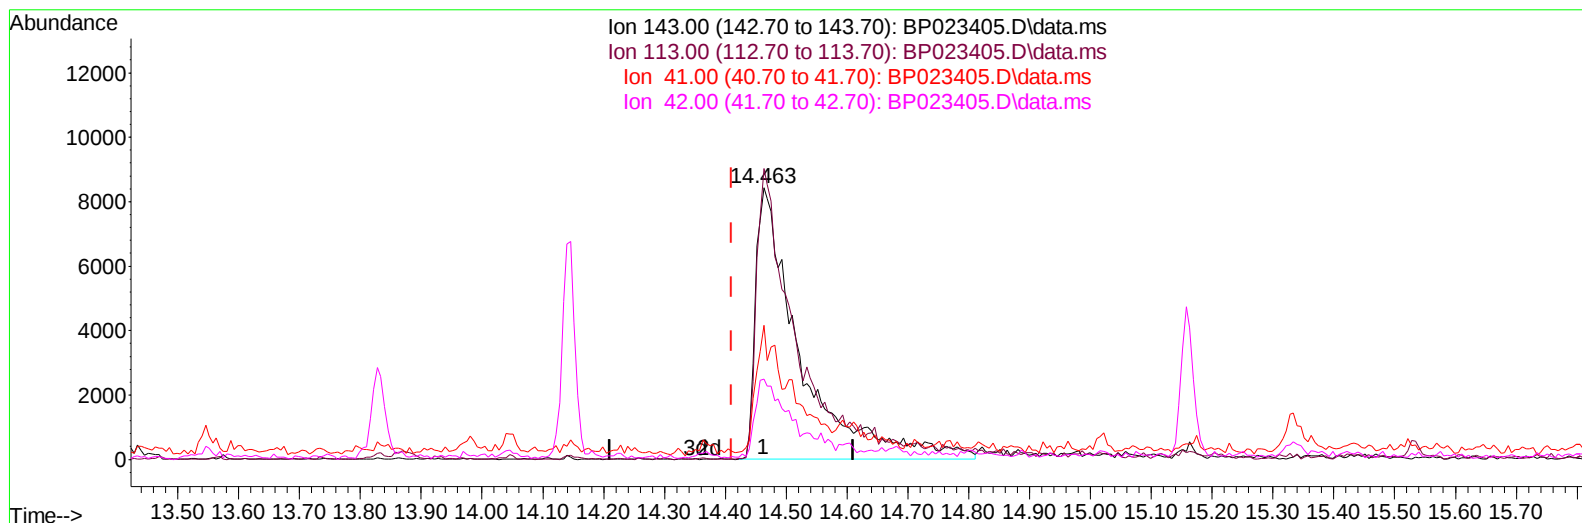

TIC: BP023405.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.463min (+ 0.053) 15.16 ng/ul m

response 43139

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	106.10	107.24
41.00	45.60	49.50
42.00	31.70	29.62

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
 Data File : BP023405.D
 Acq On : 12 Dec 2024 21:13
 Operator : RC/JU
 Sample : P5232-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 13 03:18:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.534	152	101195	20.000	ng/ul	0.00
20) Naphthalene-d8	10.275	136	393612	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.145	164	299170	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.945	188	671638	20.000	ng/ul	-0.01
79) Chrysene-d12	21.380	240	787333	20.000	ng/ul	0.00
88) Perylene-d12	24.551	264	890501	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.105	96	7212	2.624	ng/uL	0.00
4) Pyridine-d5	3.522	84	84687	11.982	ng/ul	0.00
7) Phenol-d5	6.752	99	120155	15.133	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.893	67	78806	15.731	ng/ul	0.00
11) 2-Chlorophenol-d4	7.087	132	89705	15.307	ng/ul	0.00
15) 4-Methylphenol-d8	8.258	113	89758m	14.007	ng/ul	0.00
21) Nitrobenzene-d5	8.681	128	42366	14.414	ng/ul	0.00
24) 2-Nitrophenol-d4	9.393	143	49791	14.698	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.940	165	108101	15.120	ng/ul	0.00
31) 4-Chloroaniline-d4	10.440	131	104086	12.996	ng/ul	0.00
46) Dimethylphthalate-d6	13.551	166	380060	16.364	ng/ul	0.00
49) Acenaphthylene-d8	13.828	160	335212	13.684	ng/ul	0.00
54) 4-Nitrophenol-d4	14.463	143	43139m	15.158	ng/ul	0.05
60) Fluorene-d10	15.157	176	255253	12.495	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.334	200	34578	8.519	ng/ul	0.02
73) Anthracene-d10	17.057	188	418473	13.652	ng/ul	0.00
81) Pyrene-d10	19.439	212	471286	11.457	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.333	264	471287	9.886	ng/ul	-0.01
Target Compounds						
						Qvalue
8) Phenol	6.781	94	8512m	1.030	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023405.D
Acq On : 12 Dec 2024 21:13
Operator : RC/JU
Sample : P5232-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Dec 13 03:18:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

