

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
 Data File : BP023403.D
 Acq On : 12 Dec 2024 19:52
 Operator : RC/JU
 Sample : P5153-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E28P7

Quant Time: Dec 13 02:18:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 11 00:30:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.534	152	93718	20.000	ng/ul	0.00
20) Naphthalene-d8	10.281	136	350589	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.151	164	257795	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.963	188	605172	20.000	ng/ul	0.00
79) Chrysene-d12	21.386	240	761982	20.000	ng/ul	0.00
88) Perylene-d12	24.557	264	868554	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	10993	4.318	ng/uL	0.00
4) Pyridine-d5	3.511	84	129954	19.853	ng/ul	0.00
7) Phenol-d5	6.746	99	165801	22.548	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.887	67	109172	23.532	ng/ul	0.00
11) 2-Chlorophenol-d4	7.087	132	121768	22.437	ng/ul	0.00
15) 4-Methylphenol-d8	8.258	113	133099	22.427	ng/ul	0.00
21) Nitrobenzene-d5	8.681	128	59066	22.562	ng/ul	0.00
24) 2-Nitrophenol-d4	9.393	143	70684	23.427	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.940	165	139957	21.978	ng/ul	0.00
31) 4-Chloroaniline-d4	10.446	131	148959m	20.880	ng/ul	0.00
46) Dimethylphthalate-d6	13.557	166	469057	23.438	ng/ul	0.00
49) Acenaphthylene-d8	13.840	160	482700	22.867	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	56973m	23.231	ng/ul	0.05
60) Fluorene-d10	15.169	176	402419	22.861	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.328	200	47576m	13.008	ng/ul	0.02
73) Anthracene-d10	17.057	188	661632	23.955	ng/ul	0.00
81) Pyrene-d10	19.439	212	859382	21.587	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.333	264	1005006	21.615	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	6.775	94	7935	1.037	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121224\
Data File : BP023403.D
Acq On : 12 Dec 2024 19:52
Operator : RC/JU
Sample : P5153-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E28P7

Quant Time: Dec 13 02:18:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 11 00:30:30 2024
Response via : Initial Calibration

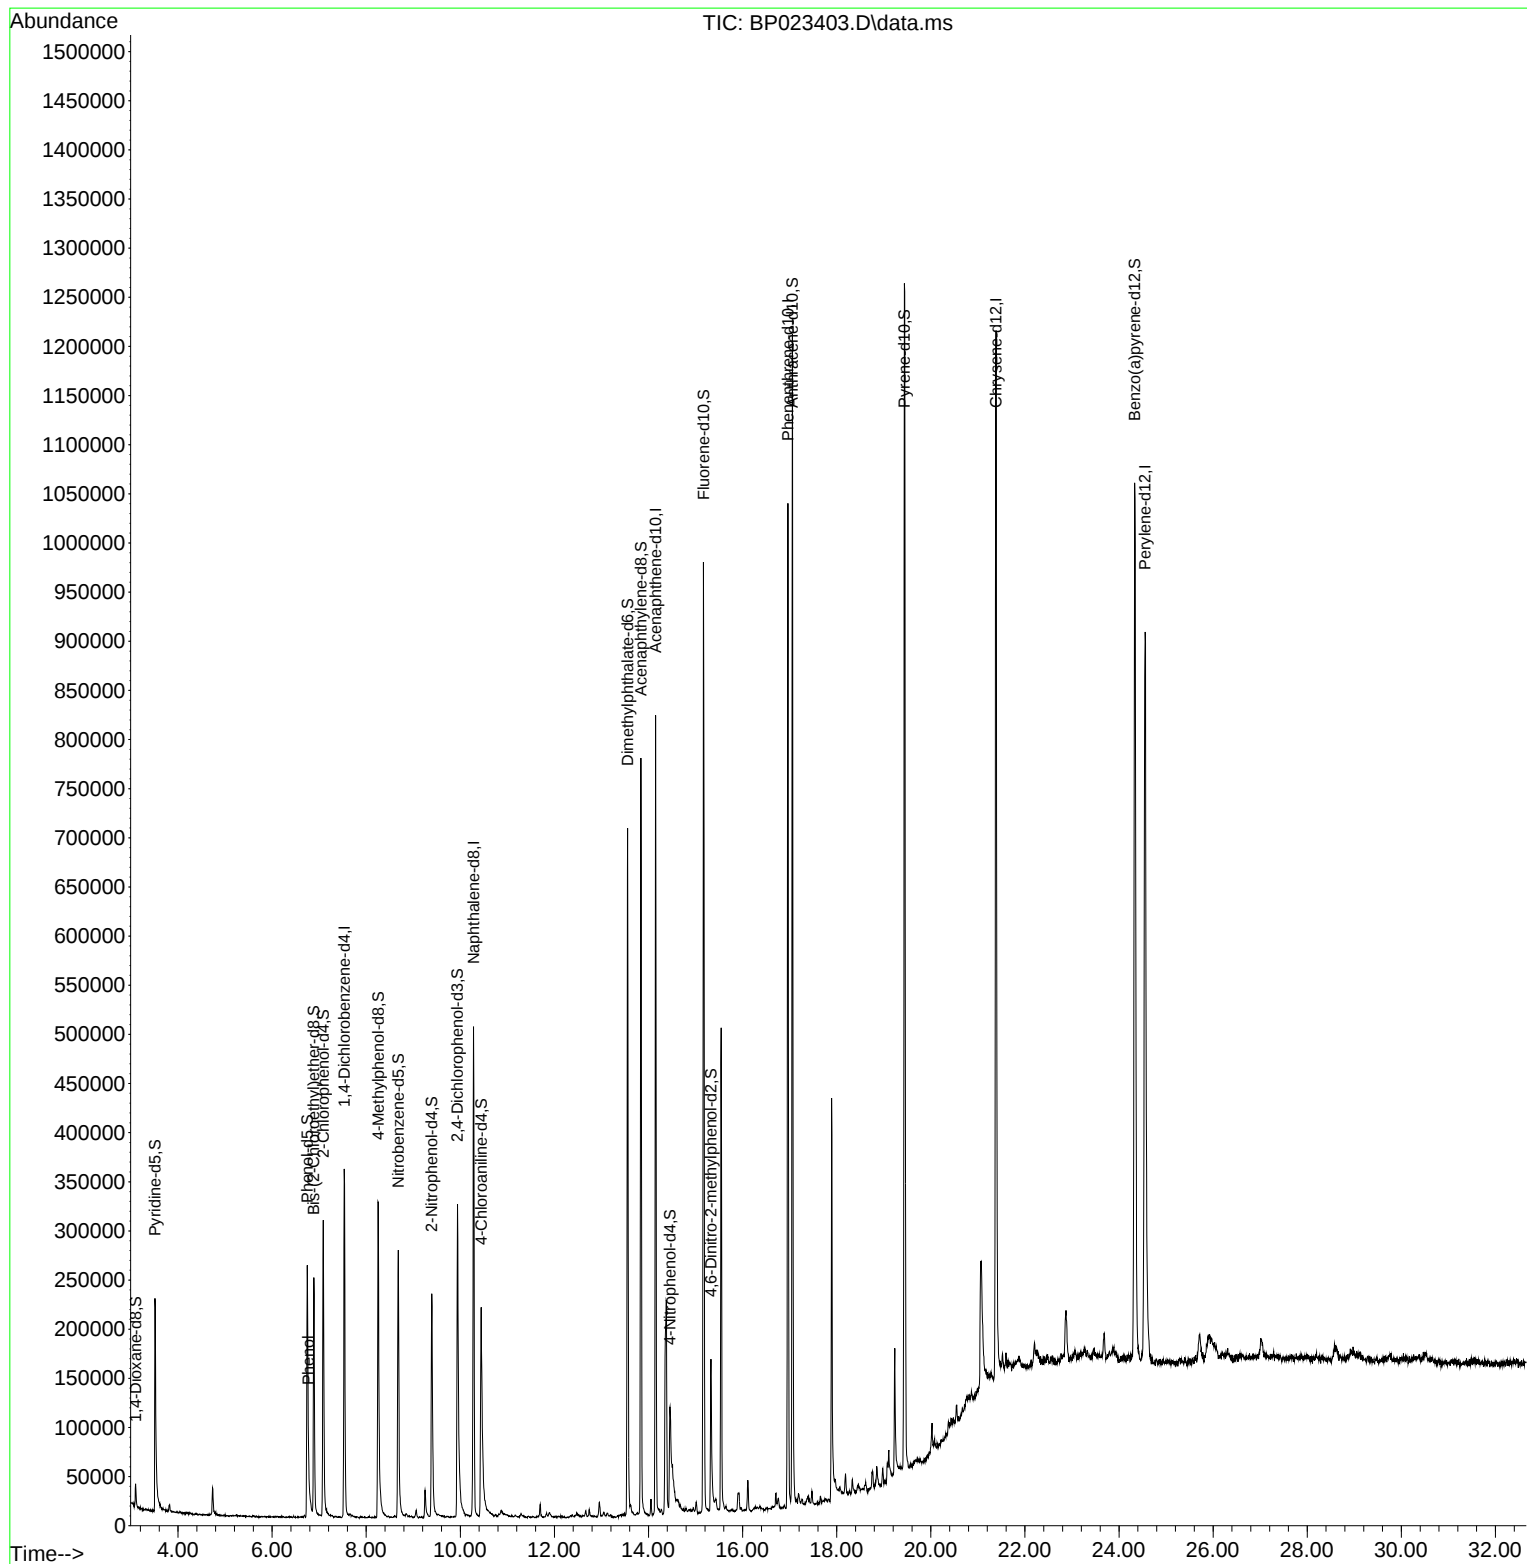

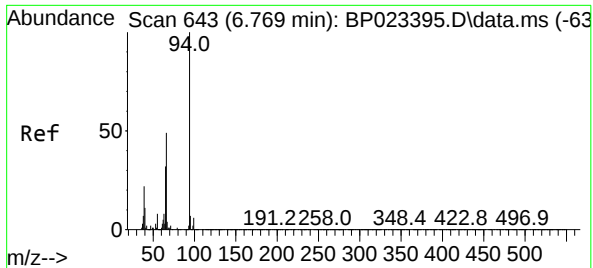

#8
Phenol
Concen: 1.037 ng/ul
RT: 6.775 min Scan# 64
Delta R.T. -0.000 min
Lab File: BP023403.D
Acq: 12 Dec 2024 19:52

Instrument :
BNA_P
ClientSampleId :
E28P7

Tgt Ion: 94	Resp:	7935
Ion	Ratio	Lower Upper
94	100	
65	34.9	28.0 42.0
66	74.9	42.0 63.0#

