

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121320\
 Data File : BP004251.D
 Acq On : 12 Dec 2020 10:03
 Operator : CG/JU
 Sample : PB133559BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK59

Quant Time: Dec 13 23:56:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 13 23:47:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	281904	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	1104393	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.47	164	638440	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.23	188	1353331	20.00	ng/ul	0.00
78) Chrysene-d12	21.32	240	1453831	20.00	ng/ul	0.00
86) Perylene-d12	23.67	264	1670740	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	38017	4.74	ng/uL	0.00
5) Phenol-d5	6.99	99	651303	27.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	398363	27.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	515989	29.15	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	492549	27.95	ng/ul	0.00
19) Nitrobenzene-d5	8.98	128	252480	27.91	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	236985	31.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	459624	28.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.75	131	675370	33.21	ng/ul	0.00
44) Dimethylphthalate-d6	13.88	166	1425398	29.21	ng/ul	0.00
47) Acenaphthylene-d8	14.16	160	1877036	30.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	199683	24.23	ng/ul	0.00
58) Fluorene-d10	15.47	176	1234011	27.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	138513	21.33	ng/ul	0.00
71) Anthracene-d10	17.33	188	1960160	29.72	ng/ul	0.00
79) Pyrene-d10	19.57	212	2268404	29.95	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.52	264	2639780	29.99	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.93	163	148612	2.990	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121320\
Data File : BP004251.D
Acq On : 12 Dec 2020 10:03
Operator : CG/JU
Sample : PB133559BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK59

Quant Time: Dec 13 23:56:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 13 23:47:32 2020
Response via : Initial Calibration

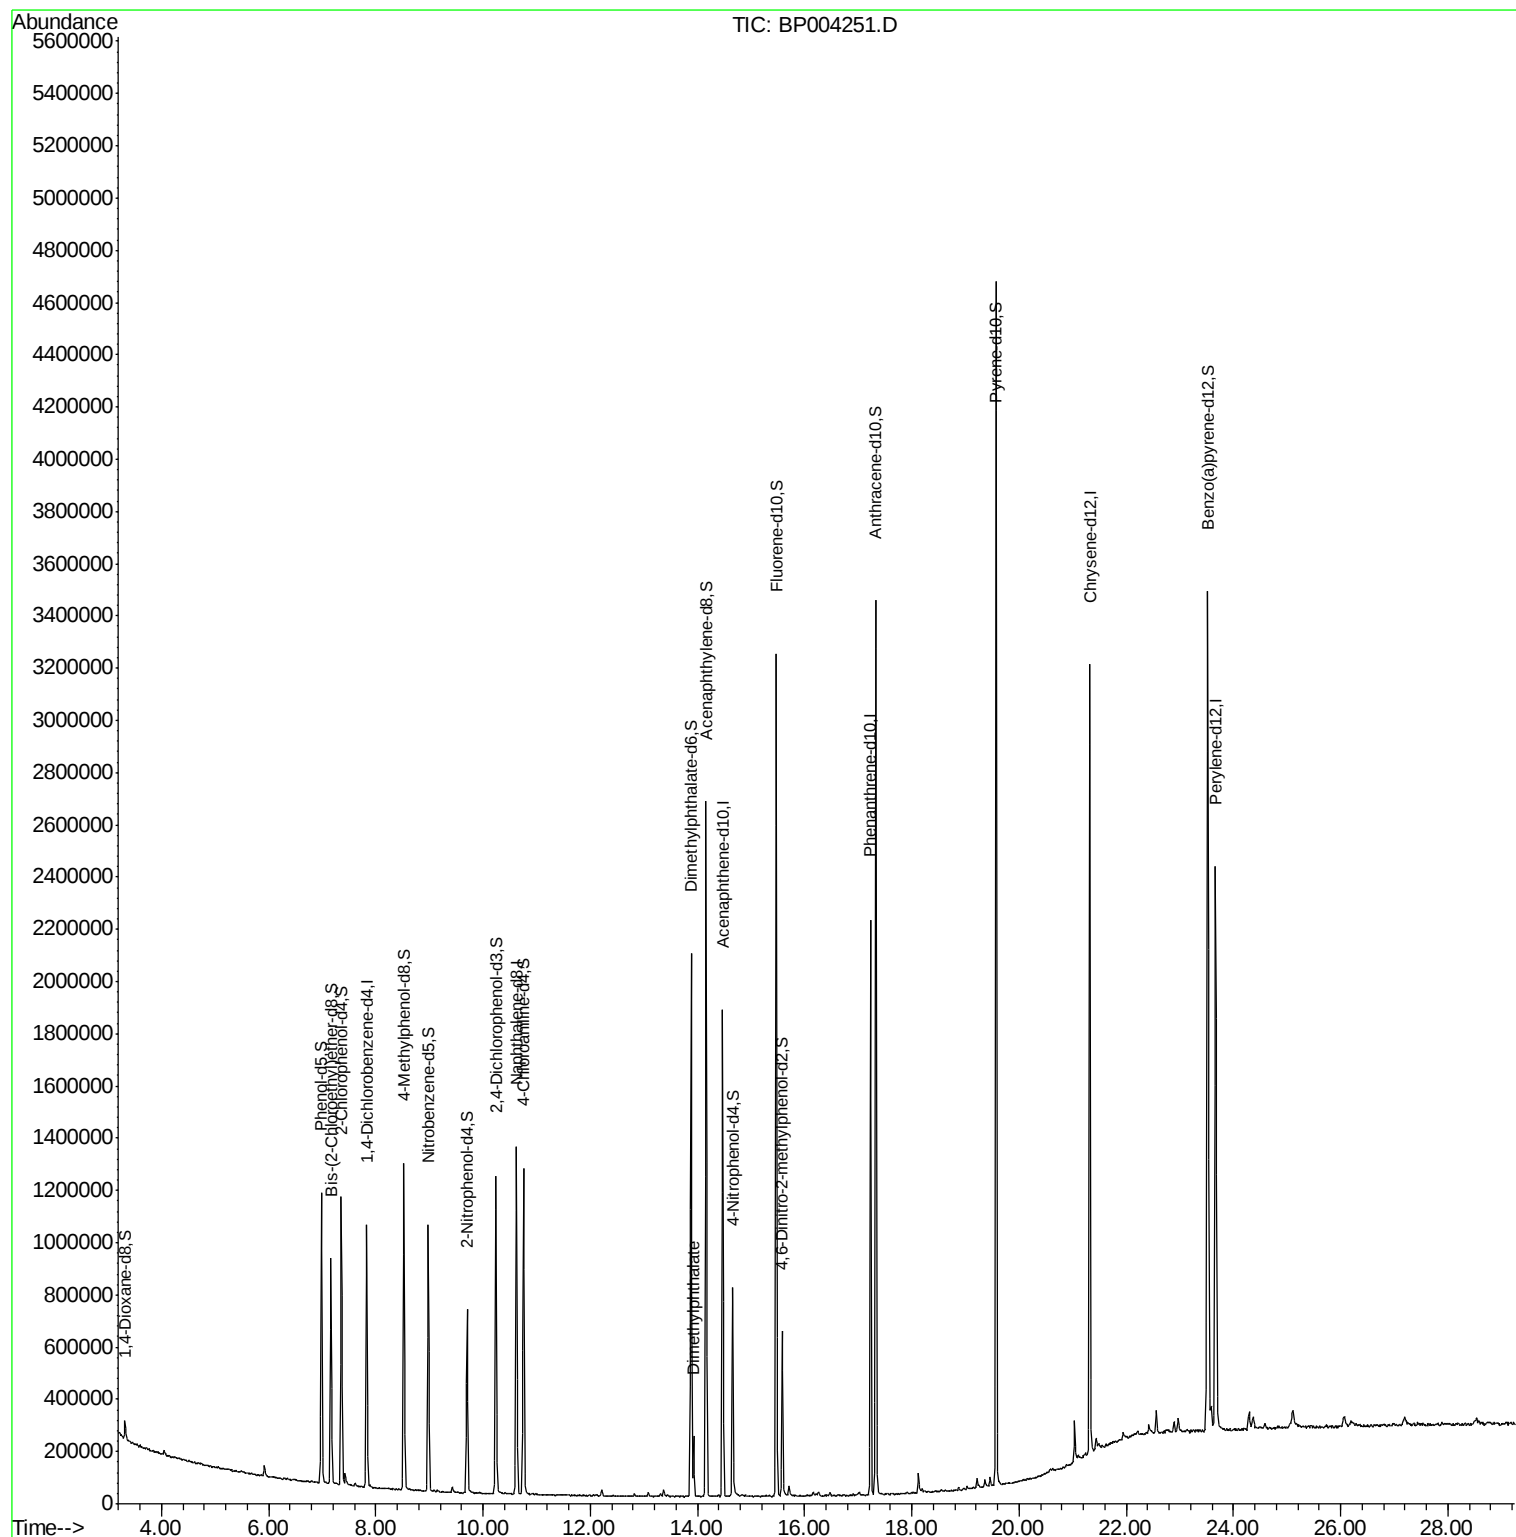

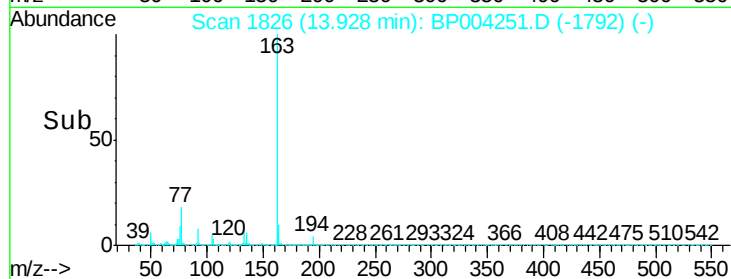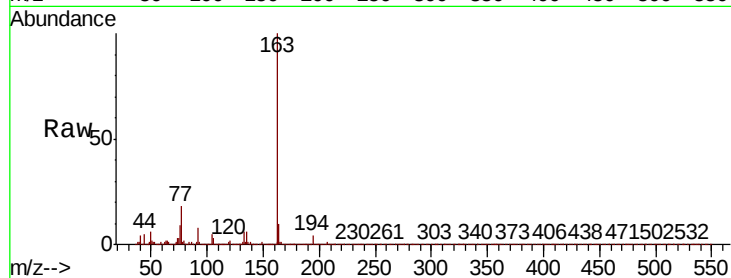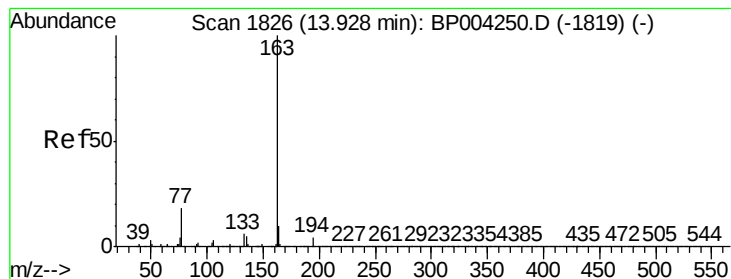

#45

Dimethylphthalate

Concen: 2.990 ng/ul

RT: 13.93 min Scan# 1826

Delta R.T. 0.00 min

Lab File: BP004251.D

Acq: 12 Dec 2020 10:03

Instrument :

BNA_P

ClientSampleId :

SBLK59

Tot Ion:163 Resp: 148612

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 9.8 8.4 12.6

