
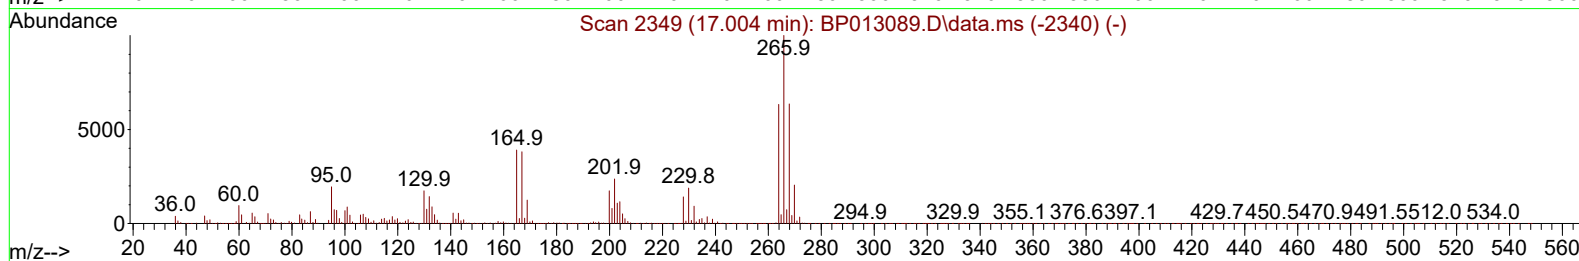
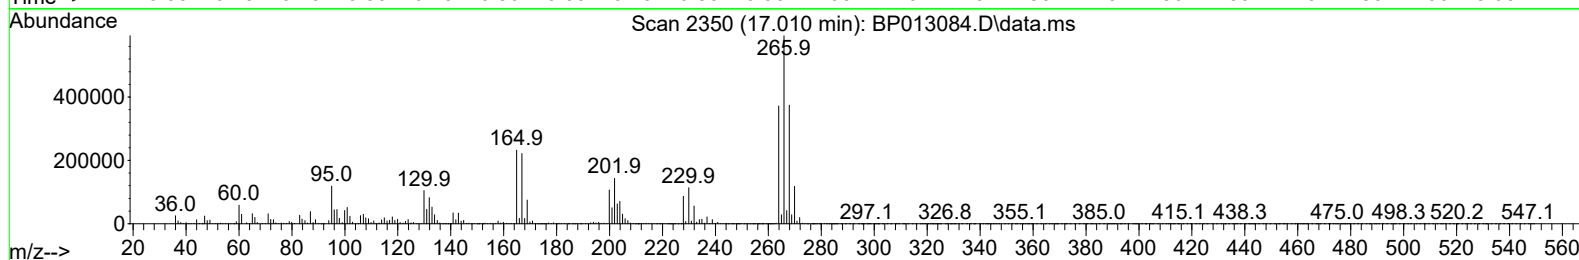


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121322\
 Data File : BP013084.D
 Acq On : 12 Dec 2022 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 07:49:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 03:29:24 2022
 Response via : Initial Calibration

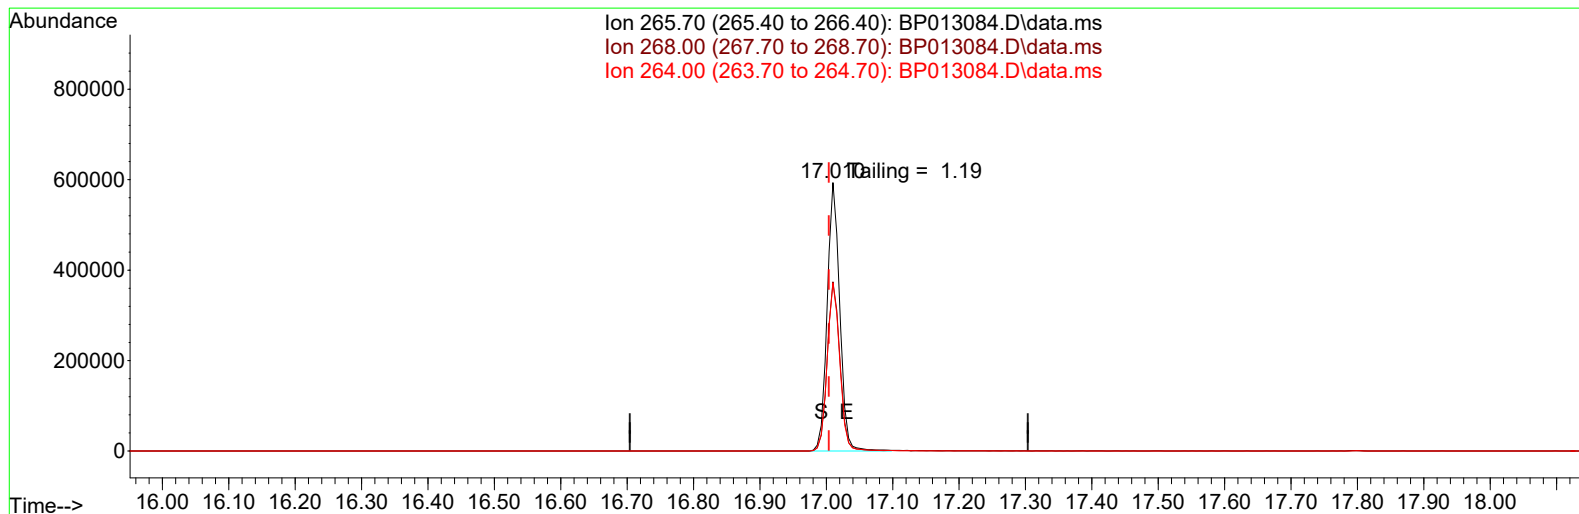

TIC: BP013084.D\data.ms

(70) Pentachlorophenol (C)




17.010min (+ 0.006) 269852.81 ng

response 785495

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.04
264.00	63.30	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121322\
 Data File : BP013084.D
 Acq On : 12 Dec 2022 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 13 07:49:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 03:29:24 2022
 Response via : Initial Calibration

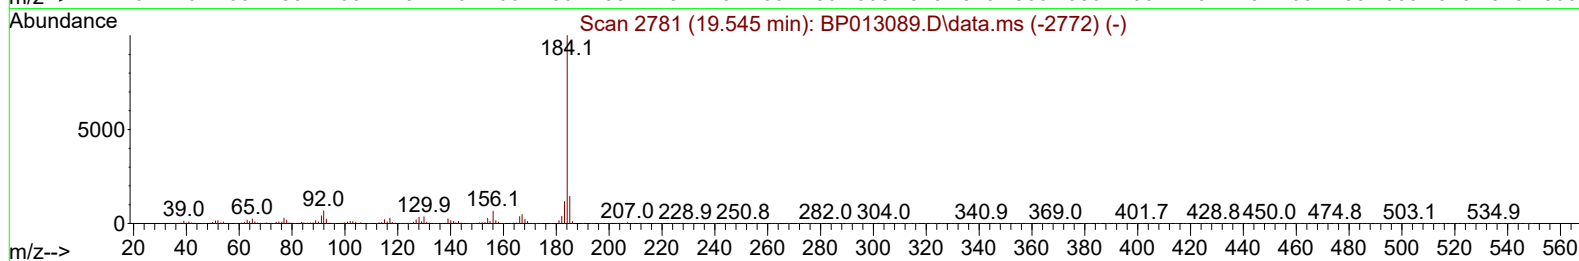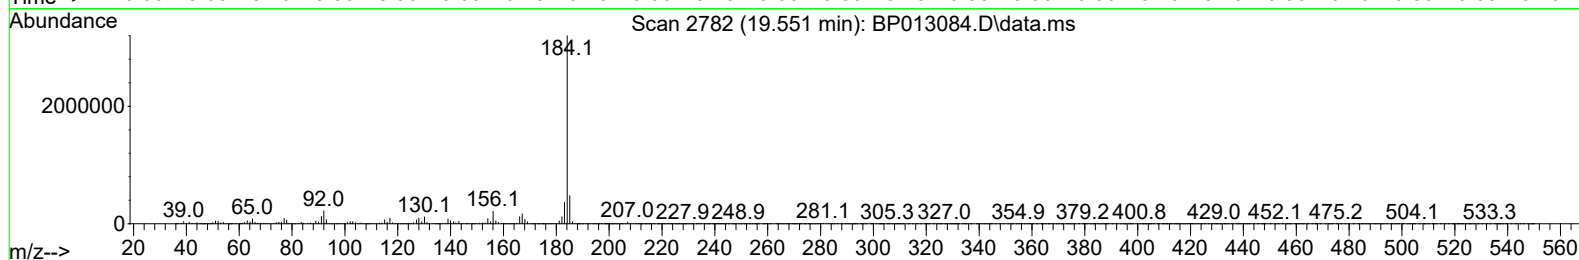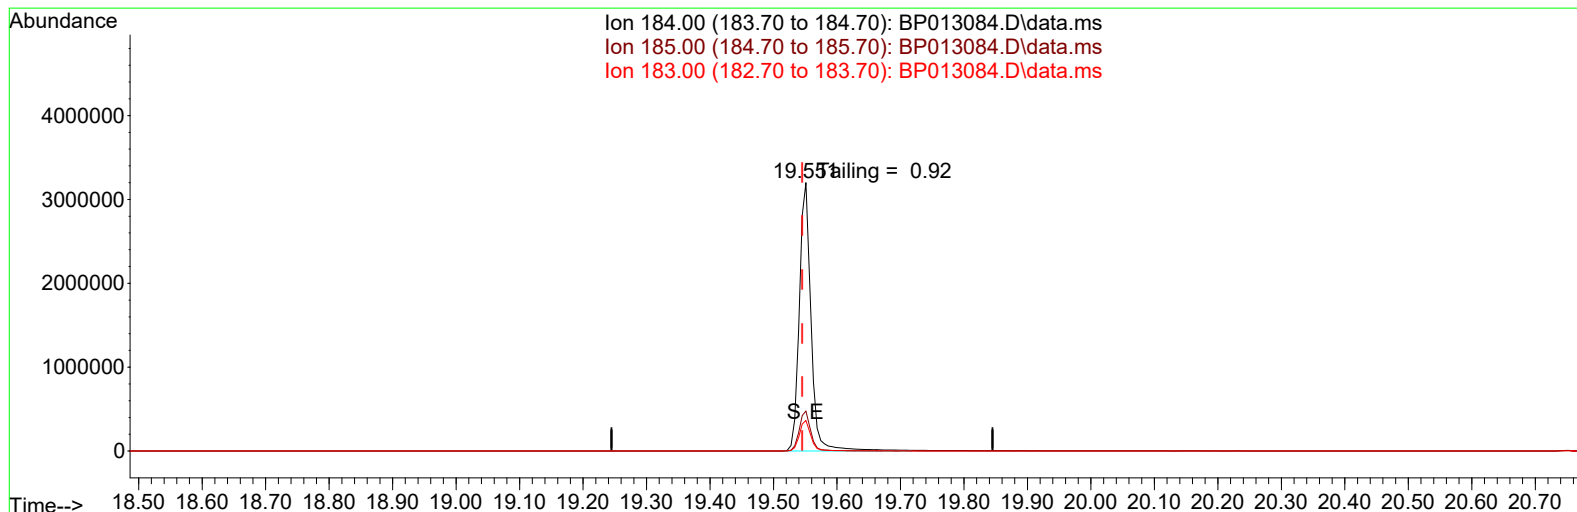

TIC: BP013084.D\data.ms

(77) Benzidine

19.551min (+ 0.006) 3295895.02 ng

response 4166552

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.95
183.00	11.70	11.40
0.00	0.00	0.00