
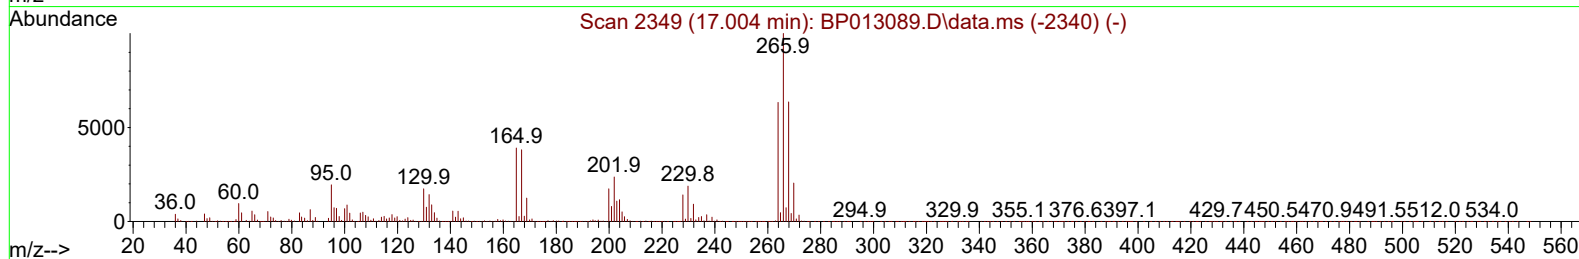
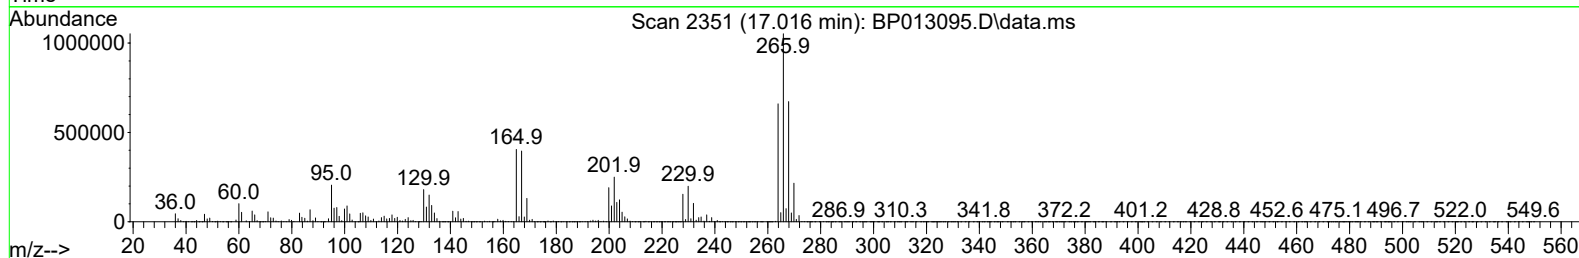


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121322\
Data File : BP013095.D
Acq On : 13 Dec 2022 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 06:37:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 03:29:24 2022
Response via : Initial Calibration

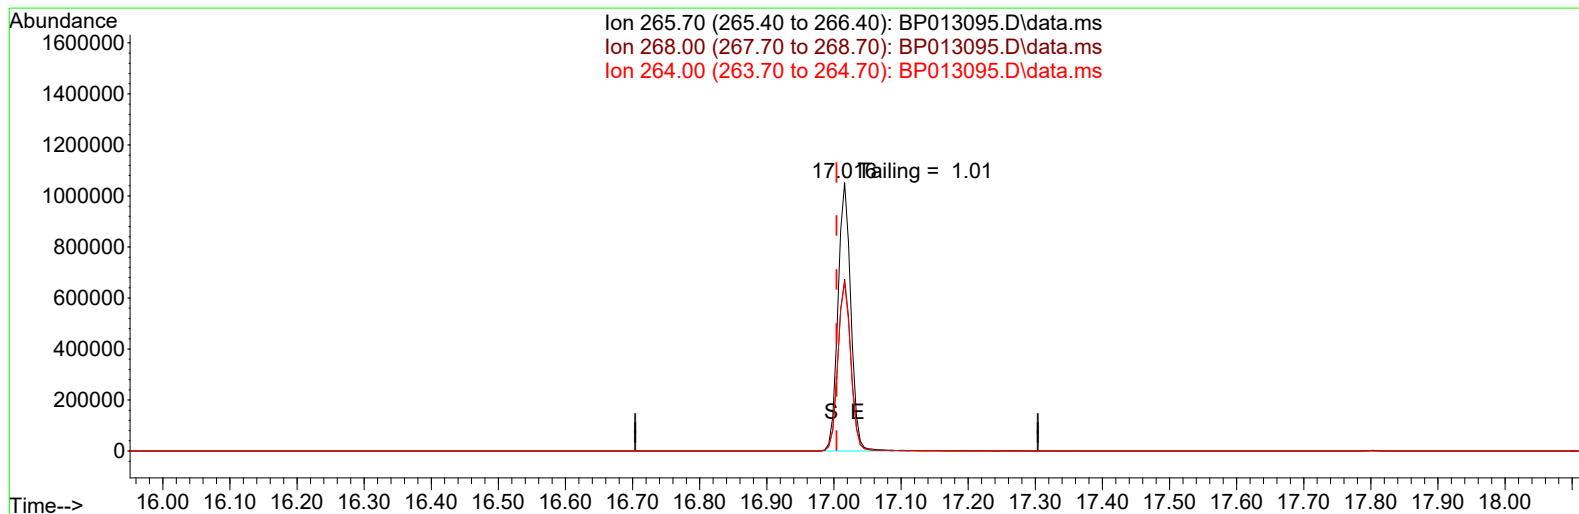

TIC: BP013095.D\data.ms

(70) Pentachlorophenol (C)




17.016min (+ 0.012) 164487.34 ng

response 1404195

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.91
264.00	63.30	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121322\
Data File : BP013095.D
Acq On : 13 Dec 2022 09:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 06:37:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 03:29:24 2022
Response via : Initial Calibration

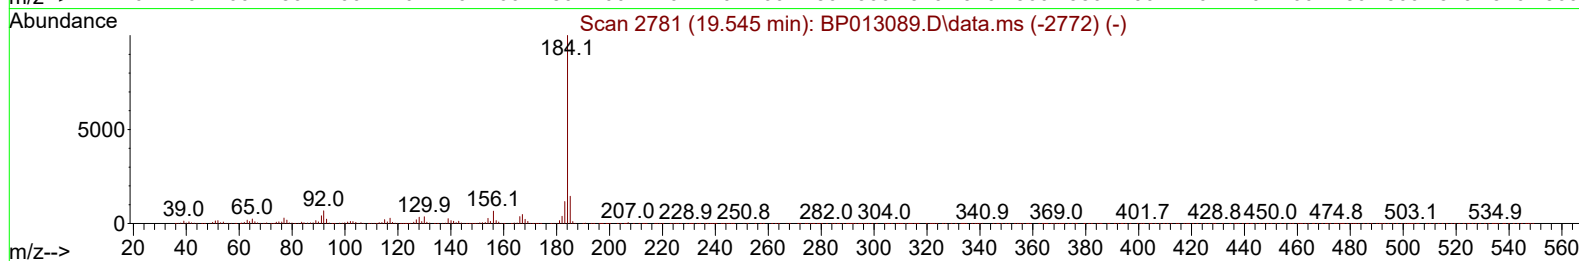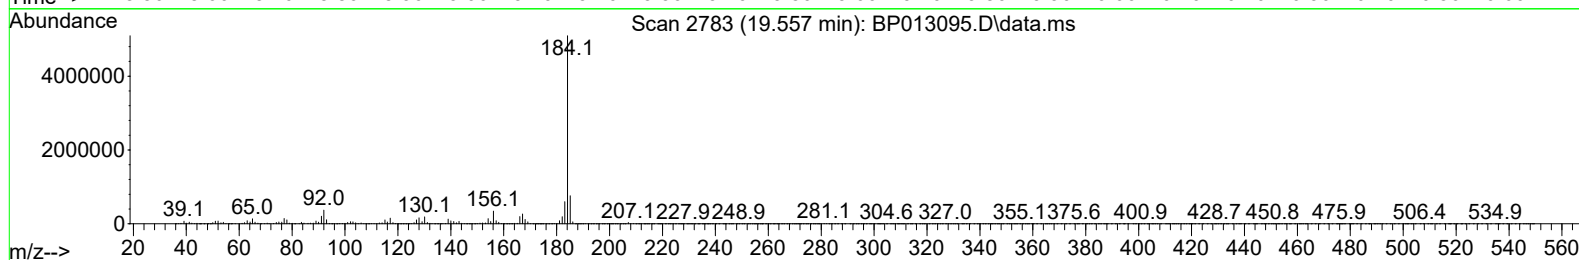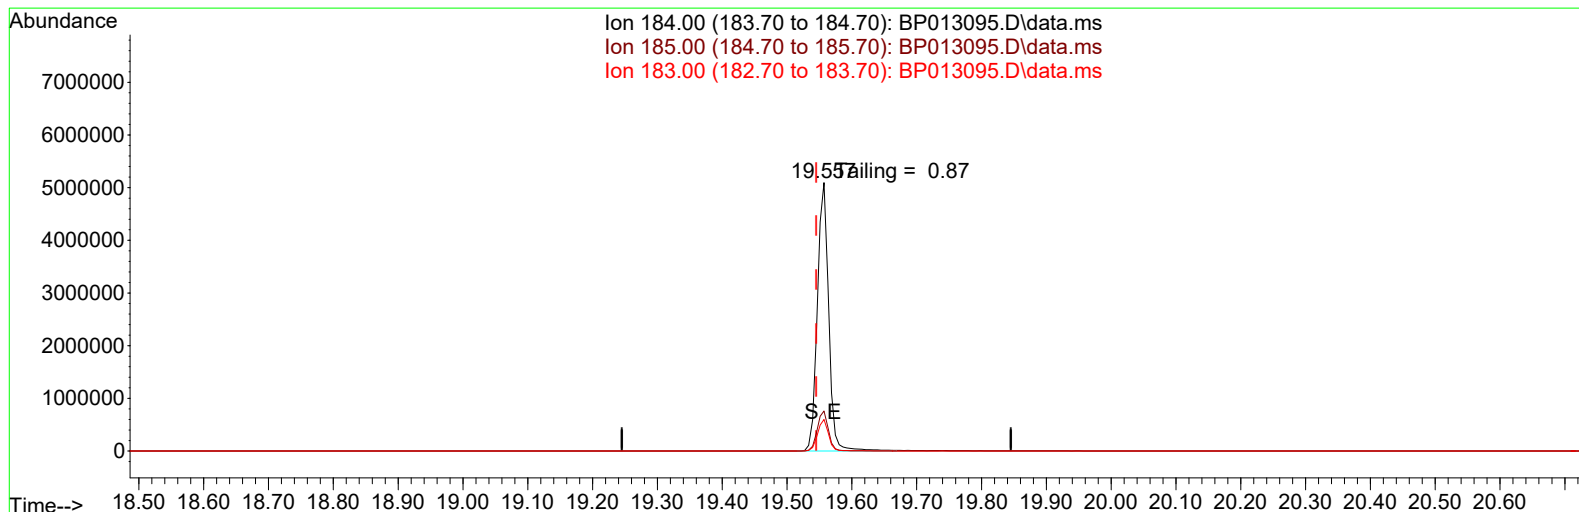

TIC: BP013095.D\data.ms

(77) Benzidine

19.557min (+ 0.012) 77450.74 ng

response 6233265

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.93
183.00	11.70	11.79
0.00	0.00	0.00