
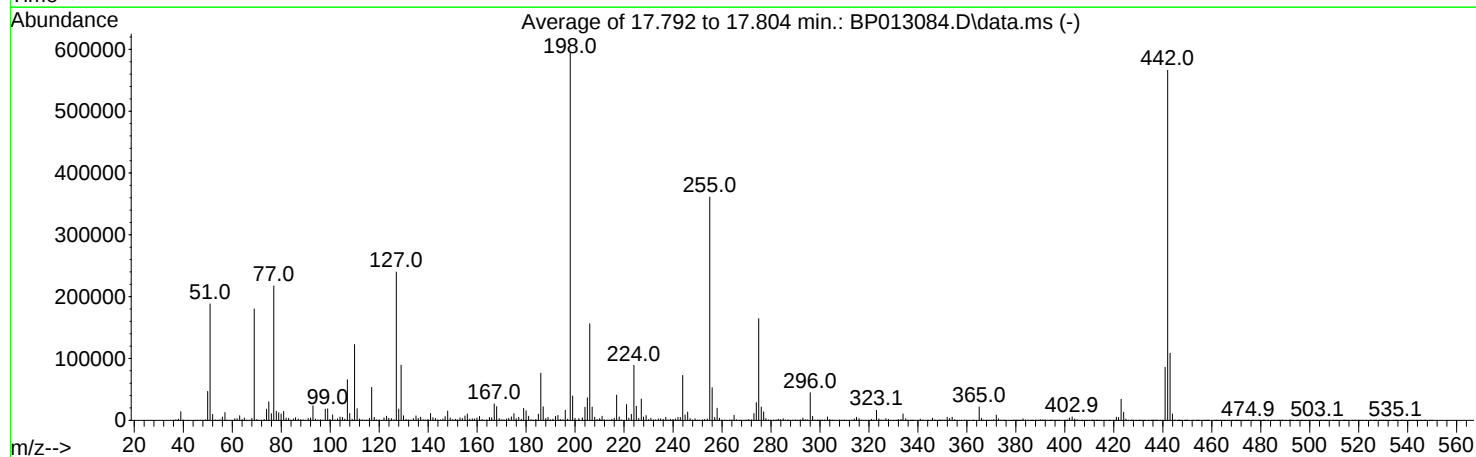


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121322\
 Data File : BP013084.D
 Acq On : 12 Dec 2022 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 13 03:29:24 2022

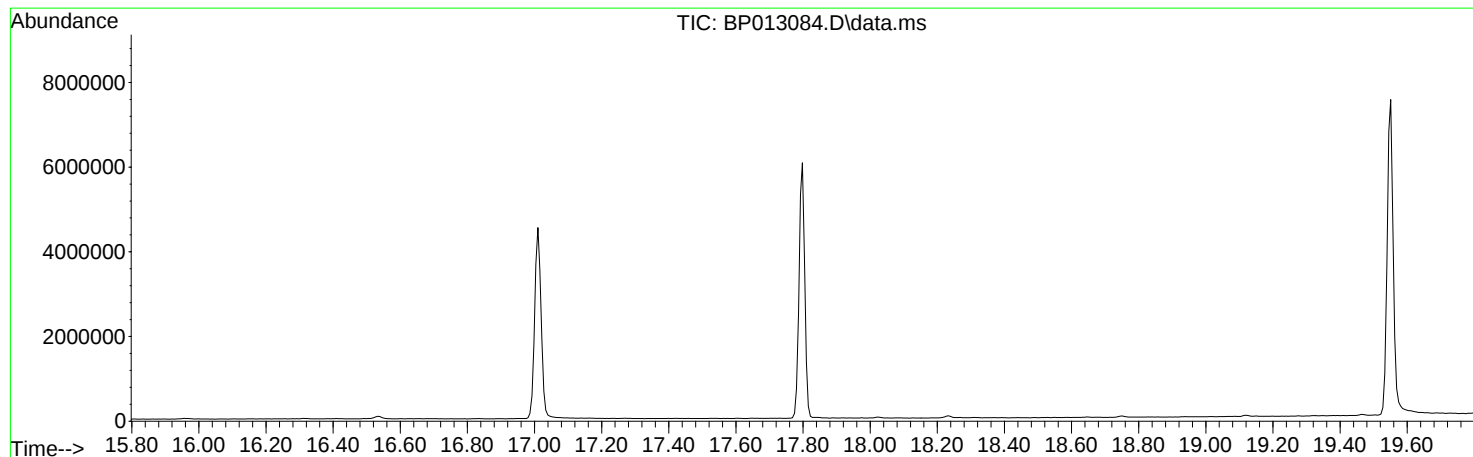




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	188339	PASS
68	69	0.00	2	1.8	3249	PASS
69	198	0.00	100	30.3	180059	PASS
70	69	0.00	2	0.7	1190	PASS
127	198	10	80	40.3	239750	PASS
197	198	0.00	2	0.3	1875	PASS
198	198	100	100	100.0	595103	PASS
199	198	5	9	6.6	39251	PASS
275	198	10	60	27.6	164411	PASS
365	198	1	100	3.6	21680	PASS
441	198	0.01	100	14.4	85876	PASS
442	442	100	100	100.0	566327	PASS
443	442	15	24	19.2	108647	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121322\
Data File : BP013084.D
Acq On : 12 Dec 2022 15:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 13 07:49:30 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 13 03:29:24 2022
Response via : Initial Calibration

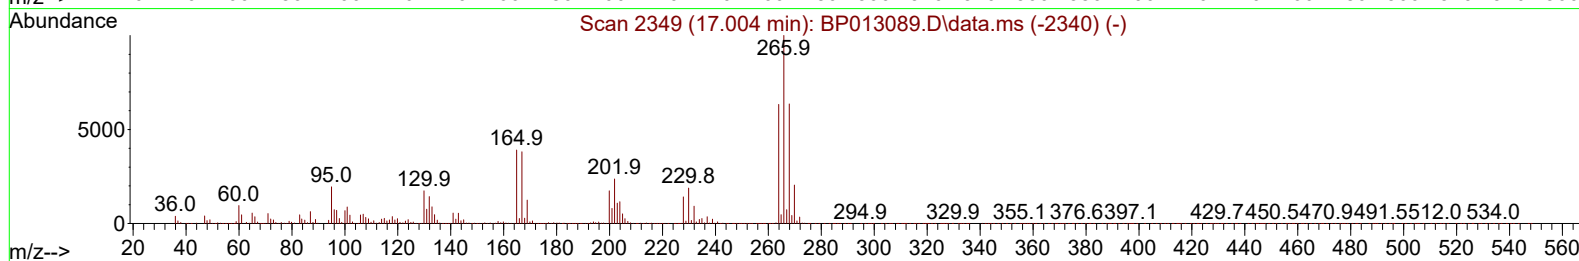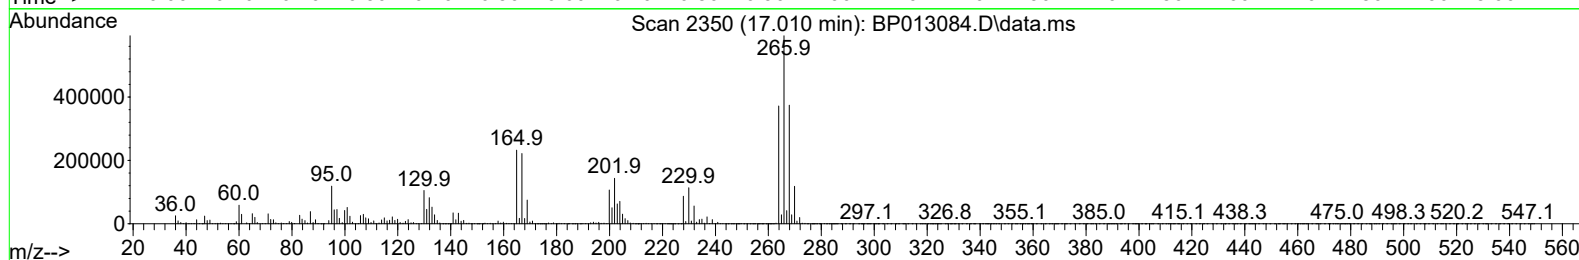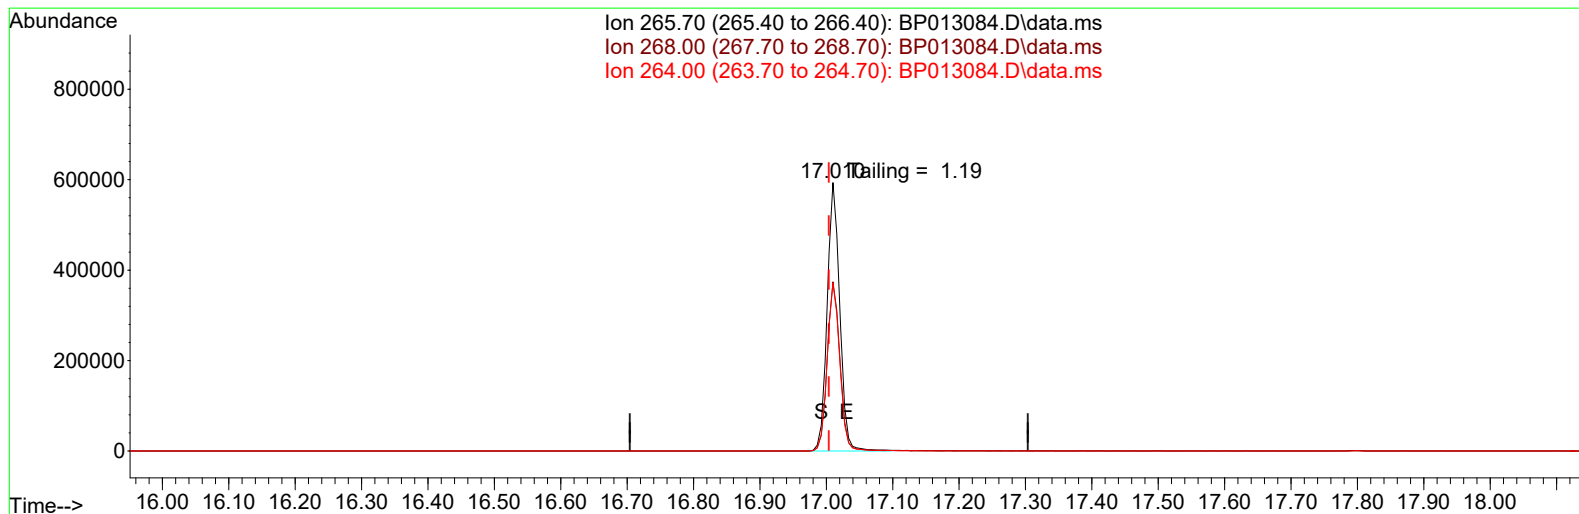

TIC: BP013084.D\data.ms

(70) Pentachlorophenol (C)

17.010min (+ 0.006) 269852.81 ng




response 785495

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.04
264.00	63.30	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121322\
 Data File : BP013084.D
 Acq On : 12 Dec 2022 15:06
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 13 07:49:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 13 03:29:24 2022
 Response via : Initial Calibration

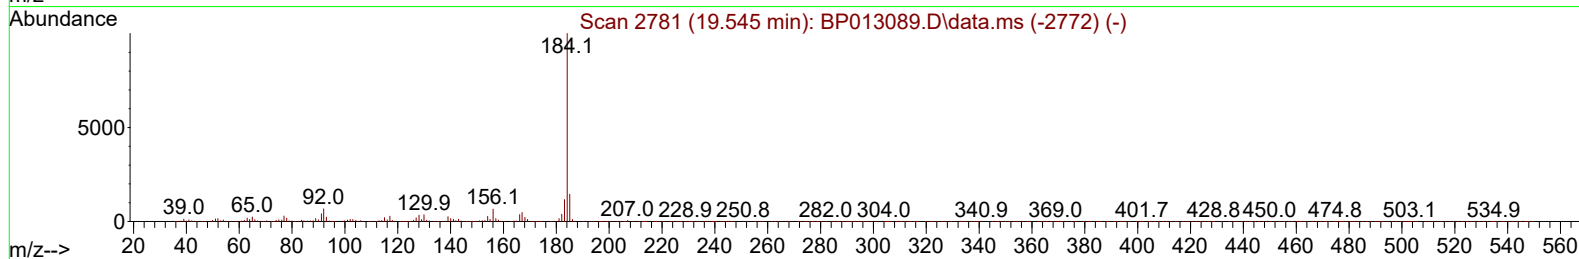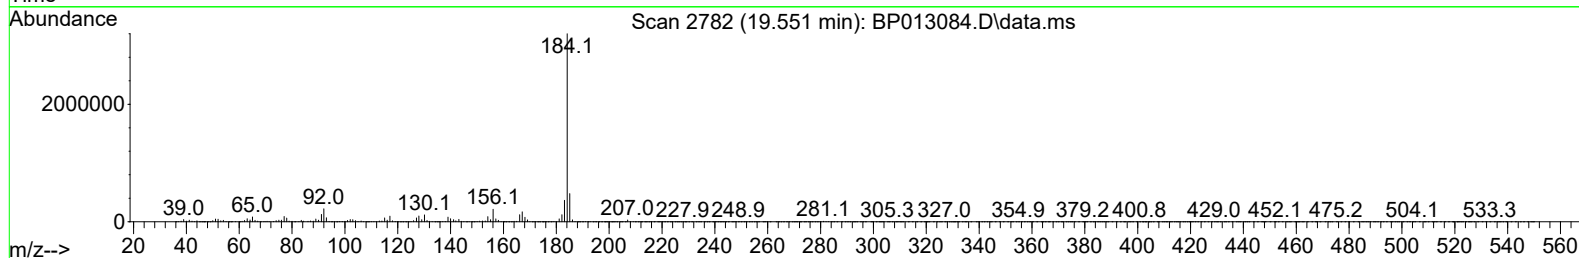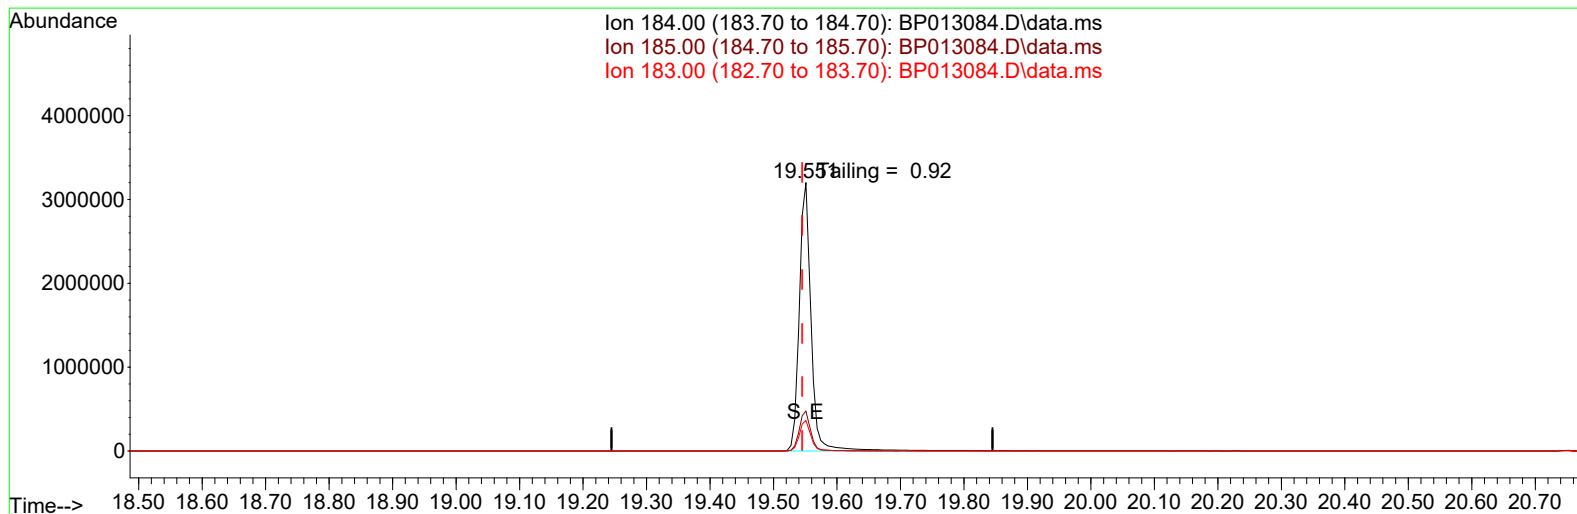

TIC: BP013084.D\data.ms

(77) Benzidine

19.551min (+ 0.006) 3295895.02 ng

response 4166552

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.95
183.00	11.70	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/13/2022	BNA_P	<u>BP013084.D</u>
Compound Name	Response	Retention Time
DDT	1999318	20.751
DDD	14858	20.369
DDE	312	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15170	2014488	0.75

Instrument :
BNA_P
ClientSampleId :
DFTPP