

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
 Data File : BP023414.D
 Acq On : 13 Dec 2024 09:59
 Operator : RC/JU
 Sample : PB165551BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK551

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	16	19	26	rVB	33140	41406	1.35%	0.153%
2	3.511	86	89	109	rBV	283160	501724	16.42%	1.850%
3	3.822	137	142	151	rBV3	9454	16762	0.55%	0.062%
4	6.116	528	532	539	rVB10	2179	4489	0.15%	0.017%
5	6.681	621	628	633	rBV4	4599	10348	0.34%	0.038%
6	6.746	633	639	658	rBV	298584	645810	21.13%	2.381%
7	6.887	658	663	675	rVB	309147	475624	15.56%	1.754%
8	7.087	689	697	712	rBV	389093	651268	21.31%	2.402%
9	7.540	766	774	786	rBV	308115	534966	17.50%	1.973%
10	8.252	888	895	915	rBV	376210	801155	26.21%	2.954%
11	8.681	962	968	989	rBV	350562	662545	21.68%	2.443%
12	9.063	1027	1033	1039	rVB10	2751	6639	0.22%	0.024%
13	9.393	1082	1089	1103	rBV	300876	567017	18.55%	2.091%
14	9.940	1175	1182	1206	rBV	349192	850899	27.84%	3.138%
15	10.275	1232	1239	1254	rVB	374074	685233	22.42%	2.527%
16	10.440	1260	1267	1290	rBV	320563	760270	24.88%	2.803%
17	11.904	1510	1516	1521	rBV7	4970	11263	0.37%	0.042%
18	13.563	1791	1798	1811	rBV	907381	1341001	43.88%	4.945%
19	13.834	1835	1844	1861	rBV	808413	1468254	48.04%	5.414%
20	14.140	1888	1896	1908	rBV	557381	990927	32.42%	3.654%
21	14.428	1939	1945	1949	rBV	130900	265994	8.70%	0.981%
22	15.151	2061	2068	2079	rBV	1244303	1951664	63.86%	7.197%
23	15.322	2091	2097	2117	rBV	251979	544470	17.82%	2.008%
24	15.969	2202	2207	2212	rBV8	3583	6647	0.22%	0.025%
25	16.622	2313	2318	2321	rBV7	2688	4136	0.14%	0.015%
26	16.739	2333	2338	2339	rBV5	3870	5228	0.17%	0.019%
27	16.957	2367	2375	2385	rBV	851348	1351843	44.23%	4.985%
28	17.057	2385	2392	2407	rVV	1558848	2319100	75.88%	8.552%
29	17.251	2422	2425	2428	rBV5	2520	3491	0.11%	0.013%
30	17.651	2490	2493	2498	rVB7	2355	3491	0.11%	0.013%
31	17.886	2529	2533	2544	rVB8	15114	25315	0.83%	0.093%
32	18.045	2557	2560	2565	rBV7	1671	3080	0.10%	0.011%
33	18.980	2715	2719	2726	rVB2	23438	30800	1.01%	0.114%
34	19.063	2729	2733	2737	rBV	16951	27668	0.91%	0.102%
35	19.228	2757	2761	2765	rBV4	21536	30628	1.00%	0.113%
36	19.433	2790	2796	2810	rBV	1902508	2920218	95.55%	10.768%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
Data File : BP023414.D
Acq On : 13 Dec 2024 09:59
Operator : RC/JU
Sample : PB165551BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK551

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Title : SVOA CALIBRATION

37	21.374	3120	3126	3138	rBV	1038053	1758681	57.54%	6.485%
38	24.321	3618	3627	3641	rVB	1257993	3056227	100.00%	11.270%
39	24.533	3655	3663	3680	rVB	627433	1782771	58.33%	6.574%




Sum of corrected areas: 27119052

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
Data File : BP023414.D
Acq On : 13 Dec 2024 09:59
Operator : RC/JU
Sample : PB165551BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

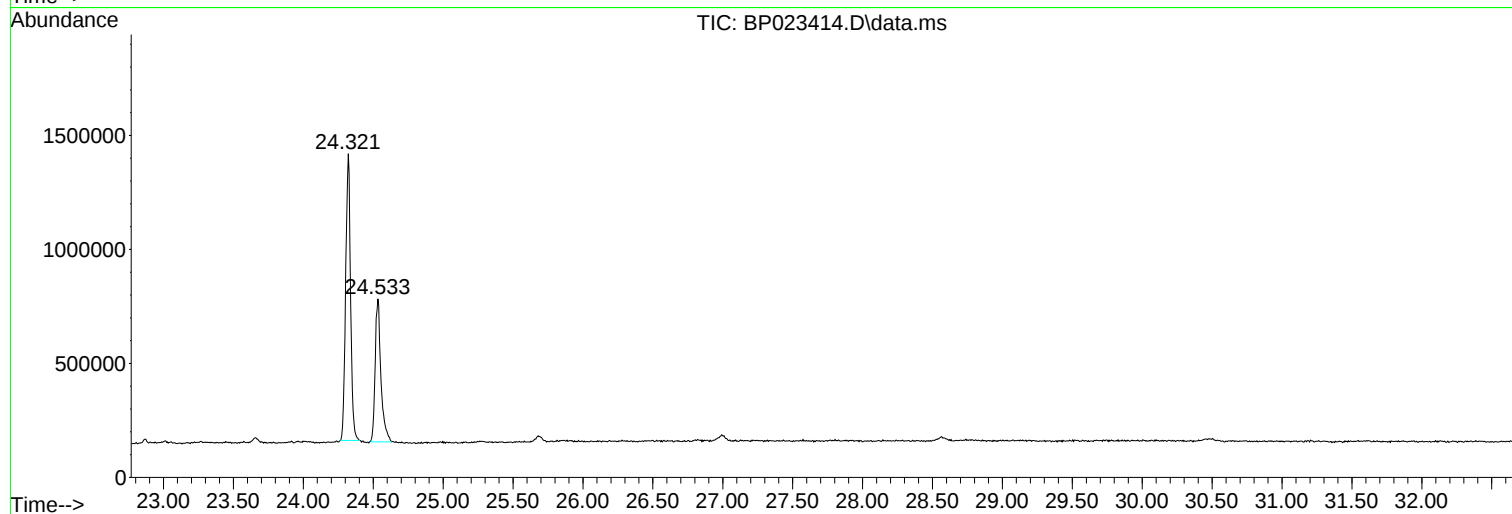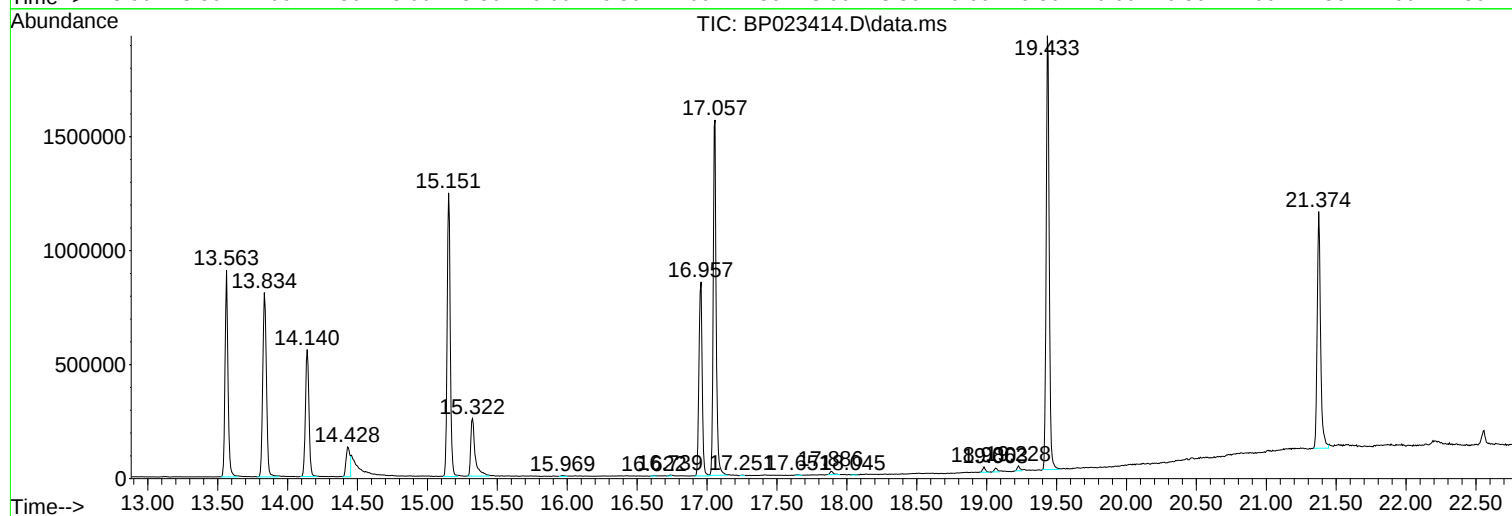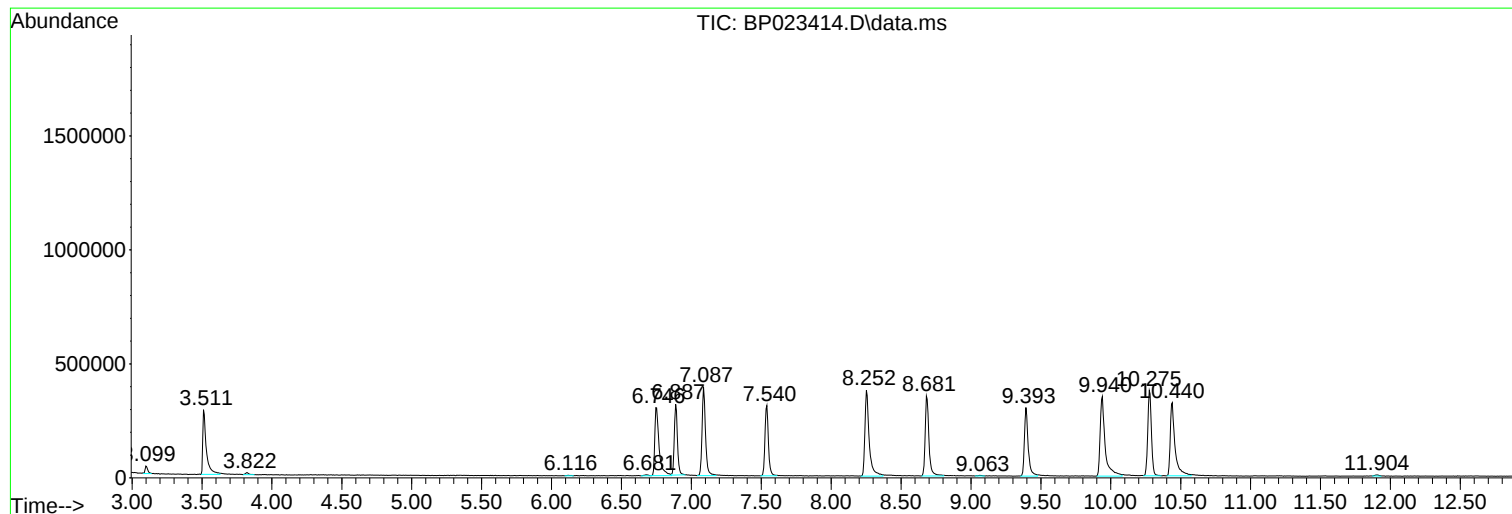

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
Data File : BP023414.D
Acq On : 13 Dec 2024 09:59
Operator : RC/JU
Sample : PB165551BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
Data File : BP023414.D
Acq On : 13 Dec 2024 09:59
Operator : RC/JU
Sample : PB165551BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK551

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc