

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
 Data File : BP023426.D
 Acq On : 13 Dec 2024 18:52
 Operator : RC/JU
 Sample : PB165624BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK624

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP023426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	15	19	29	rVB	33250	46004	1.22%	0.132%
2	3.511	85	89	109	rBV	369583	620657	16.42%	1.783%
3	3.817	138	141	149	rVB	11361	17657	0.47%	0.051%
4	6.381	574	577	583	rBV7	1983	4606	0.12%	0.013%
5	6.675	621	627	631	rVB4	5581	8597	0.23%	0.025%
6	6.752	633	640	657	rBV	421742	825361	21.83%	2.372%
7	6.887	657	663	675	rVB	391364	599956	15.87%	1.724%
8	7.087	690	697	713	rBV	477466	809338	21.41%	2.326%
9	7.534	765	773	784	rBV	417637	689958	18.25%	1.983%
10	8.252	889	895	918	rBV	512528	1043586	27.60%	2.999%
11	8.681	960	968	984	rBV	477931	835765	22.11%	2.402%
12	9.058	1029	1032	1038	rVB8	3838	5121	0.14%	0.015%
13	9.387	1082	1088	1101	rBV	340931	664623	17.58%	1.910%
14	9.934	1174	1181	1213	rBV	518411	1175834	31.10%	3.379%
15	10.281	1233	1240	1253	rBV	587631	933809	24.70%	2.683%
16	10.434	1259	1266	1286	rBV	461238	1021594	27.02%	2.936%
17	11.887	1507	1513	1521	rBV4	7998	18757	0.50%	0.054%
18	13.110	1715	1721	1725	rBV9	3029	5202	0.14%	0.015%
19	13.551	1790	1796	1808	rBV	1203395	1777194	47.00%	5.107%
20	13.840	1837	1845	1859	rBV2	1320044	2020973	53.45%	5.807%
21	14.151	1890	1898	1906	rBV	1048106	1466635	38.79%	4.214%
22	14.445	1939	1948	1965	rBV	232926	755030	19.97%	2.170%
23	14.869	2016	2020	2022	rBV4	4526	6619	0.18%	0.019%
24	15.163	2062	2070	2083	rBV	1779553	2688037	71.10%	7.724%
25	15.322	2091	2097	2107	rBV	139264	272818	7.22%	0.784%
26	15.804	2175	2179	2181	rBV4	2987	4058	0.11%	0.012%
27	16.122	2228	2233	2237	rVB7	3442	5794	0.15%	0.017%
28	16.622	2314	2318	2320	rBV5	4481	7192	0.19%	0.021%
29	16.734	2333	2337	2344	rVB3	7177	13232	0.35%	0.038%
30	16.951	2368	2374	2384	rBV2	1289463	1922382	50.84%	5.524%
31	17.051	2384	2391	2403	rVV	2290642	3126890	82.70%	8.985%
32	17.357	2440	2443	2444	rBV3	3822	4692	0.12%	0.013%
33	17.892	2530	2534	2542	rVB8	16495	29392	0.78%	0.084%
34	18.981	2715	2719	2725	rBV2	27784	43664	1.15%	0.125%
35	19.069	2731	2734	2741	rBV	23247	38038	1.01%	0.109%
36	19.439	2790	2797	2810	rBV	2536634	3780881	100.00%	10.865%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
Data File : BP023426.D
Acq On : 13 Dec 2024 18:52
Operator : RC/JU
Sample : PB165624BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK624

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Title : SVOA CALIBRATION

37	21.369	3120	3125	3135	rBV	1203745	2063824	54.59%	5.931%
38	24.304	3616	3624	3636	rBV	1312953	3513071	92.92%	10.095%
39	24.527	3653	3662	3670	rBV	693193	1933212	51.13%	5.555%


Sum of corrected areas: 34800053

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
Data File : BP023426.D
Acq On : 13 Dec 2024 18:52
Operator : RC/JU
Sample : PB165624BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

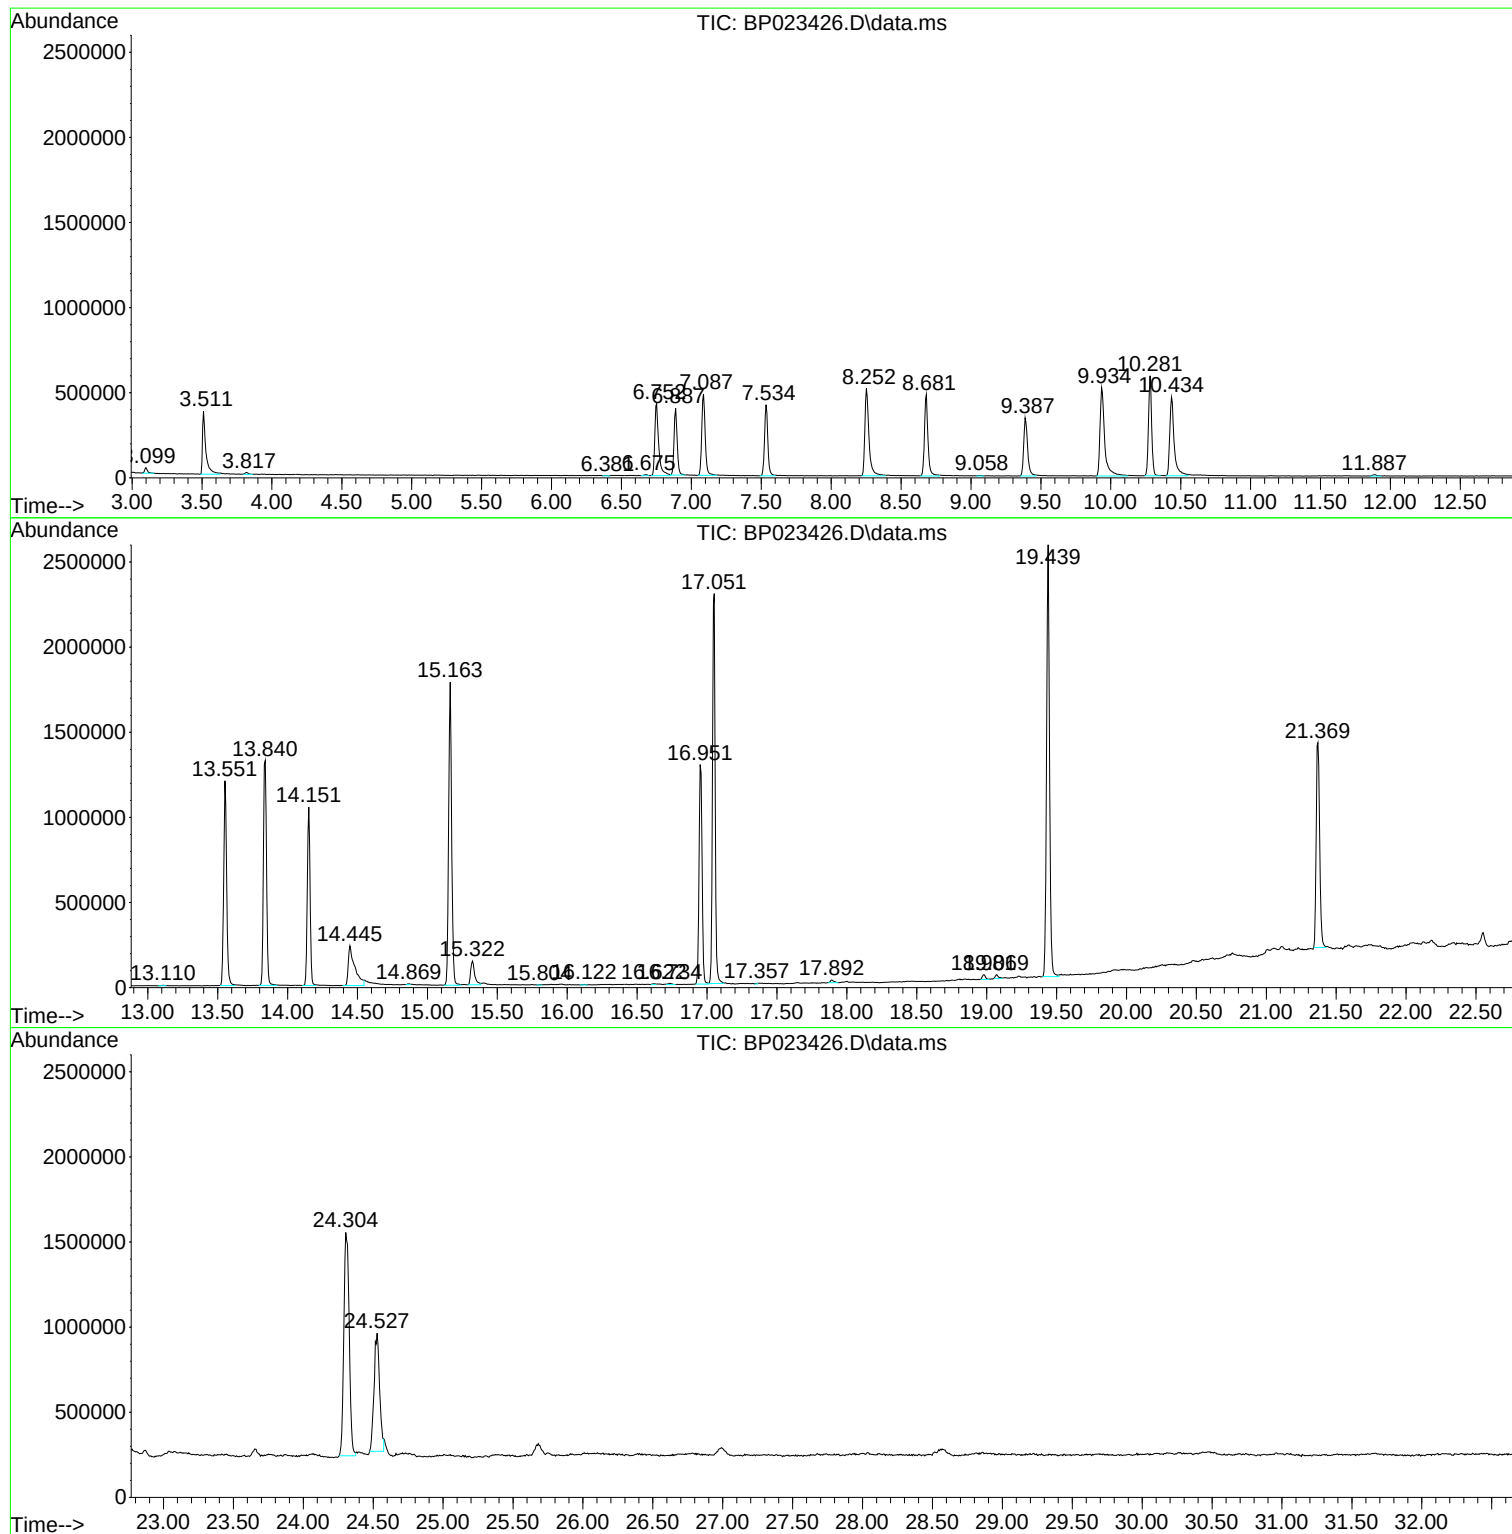

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
Data File : BP023426.D
Acq On : 13 Dec 2024 18:52
Operator : RC/JU
Sample : PB165624BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121324\
Data File : BP023426.D
Acq On : 13 Dec 2024 18:52
Operator : RC/JU
Sample : PB165624BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP112624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------