

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
 Data File : BP004274.D
 Acq On : 14 Dec 2020 15:11
 Operator : CG/JU
 Sample : L5000-02MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54A1MS

Manual Integrations
 APPROVED

mohammad
 12/17/2020 9:51:32 AM

Quant Time: Dec 15 00:18:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 10 13:52:32 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	328325	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	1394648	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.49	164	907675	20.00	ng/ul	0.01
62) Phenanthrene-d10	17.25	188	1973758	20.00	ng/ul	0.01
78) Chrysene-d12	21.34	240	1917260	20.00	ng/ul	0.02
86) Perylene-d12	23.70	264	2176918	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	24267	2.60	ng/uL	0.00
5) Phenol-d5	7.00	99	534780	19.69	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.17	67	284182	16.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	440918	21.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.54	113	417232	20.33	ng/ul	0.01
19) Nitrobenzene-d5	8.99	128	220429	19.30	ng/ul	0.01
22) 2-Nitrophenol-d4	9.72	143	245708	26.08	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.25	165	466830	22.54	ng/ul	0.01
29) 4-Chloroaniline-d4	10.76	131	447973	17.45	ng/ul	0.00
44) Dimethylphthalate-d6	13.89	166	1356359	19.55	ng/ul	0.01
47) Acenaphthylene-d8	14.17	160	1780306	20.11	ng/ul	0.01
52) 4-Nitrophenol-d4	14.68	143	202130	17.25	ng/ul	0.02
58) Fluorene-d10	15.48	176	1224202	19.48	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	15.60	200	108249	11.43	ng/ul	0.02
71) Anthracene-d10	17.35	188	1935449	20.12	ng/ul	0.01
79) Pyrene-d10	19.59	212	2207025	22.10	ng/ul	0.02
90) Benzo(a)pyrene-d12	23.56	264	2388684	20.83	ng/ul	0.04

Target Compounds

					Ovalue
6) Phenol	7.03	94	538242	18.980	ng/ul 100
10) 2-Chlorophenol	7.40	128	400903	18.551	ng/ul 96
15) N-Nitroso-di-n-propylamine	8.64	70	295413	18.792	ng/ul 97
33) 4-Chloro-3-methylphenol	11.92	107	440175	22.273	ng/ul 99
45) Dimethylphthalate	13.93	163	288778	4.087	ng/ul 100
50) Acenaphthene	14.55	153	1089074	17.505	ng/ul 99
53) 4-Nitrophenol	14.69	109	151557	17.526	ng/ul 96
55) 2,4-Dinitrotoluene	14.85	165	366532	19.629	ng/ul 97
69) Pentachlorophenol	16.89	266	265762	20.995	ng/ul 99
70) Phenanthrene	17.29	178	1485545	12.758	ng/ul 100
72) Anthracene	17.38	178	191476	1.662	ng/ul 99
75) Carbazole	17.65	167	187536	2.000	ng/ul 97
77) Fluoranthene	19.26	202	4963729	39.922	ng/ul 96
80) Pyrene	19.62	202	6335208	48.985	ng/ul 96
83) Benzo(a)anthracene	21.32	228	1926261	15.242	ng/ul 98
85) Chrysene	21.37	228	2544522	20.524	ng/ul 98
88) Benzo(b)fluoranthene	22.99	252	3828354	27.731	ng/ul 97
89) Benzo(k)fluoranthene	23.03	252	1206688m	8.511	ng/ul
91) Benzo(a)pyrene	23.60	252	2326407	18.059	ng/ul 98
92) Indeno(1,2,3-cd)pyrene	26.14	276	2004843	12.409	ng/ul 98
93) Dibenzo(a,h)anthracene	26.15	278	451051	3.331	ng/ul# 90
94) Benzo(a,h,i)perylene	26.89	276	1647381	12.154	ng/ul 95

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
Data File : BP004274.D
Acq On : 14 Dec 2020 15:11
Operator : CG/JU
Sample : L5000-02MS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54A1MS

Manual Integrations
APPROVED

mohammad
12/17/2020 9:51:32 AM

Quant Time: Dec 15 00:18:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 10 13:52:32 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
 Data File : BP004274.D
 Acq On : 14 Dec 2020 15:11
 Operator : CG/JU
 Sample : L5000-02MS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 A54A1MS

Manual Integrations
 APPROVED

mohammad
 12/17/2020 9:51:32 AM

Quant Time: Dec 15 00:18:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 10 13:52:32 2020
 Response via : Initial Calibration

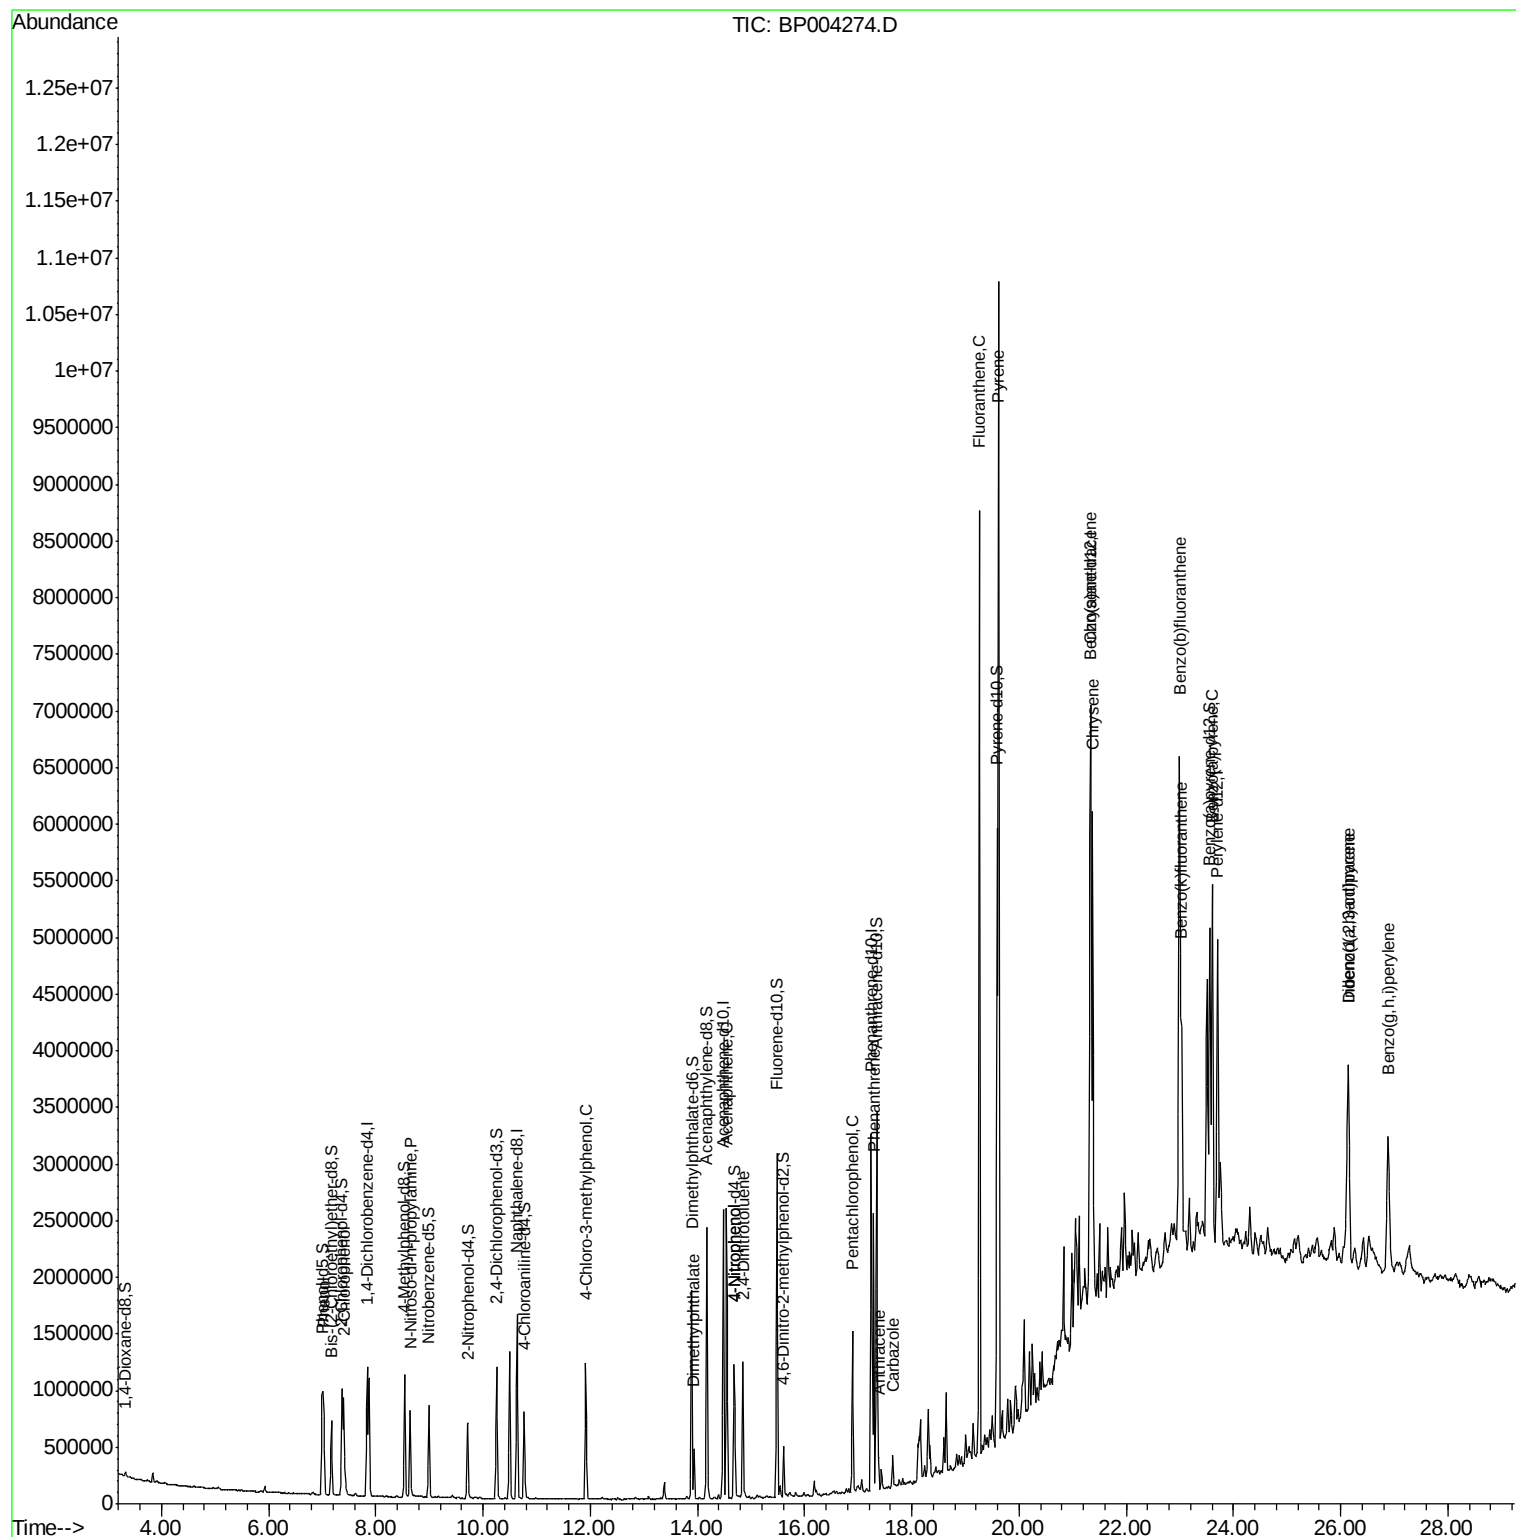

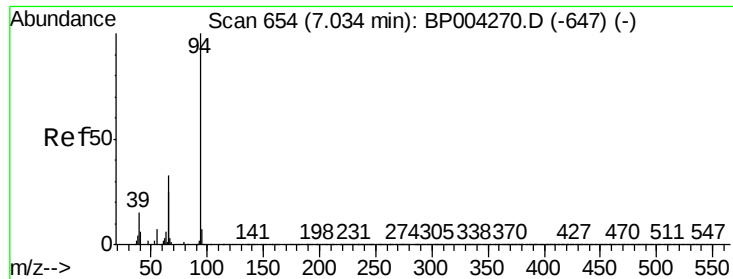

#6

Phenol

Concen: 18.980 ng/ul

RT: 7.03 min Scan# 653

Delta R.T. 0.01 min

Lab File: BP004274.D

Acq: 14 Dec 2020 15:11

Instrument :

BNA_P





ClientSampleId :

A54A1MS

Tot Ion:	94	Resp:	538242
Ion Ratio	Lower	Upper	
94	100		
65	25.5	20.8	31.2
66	33.1	26.5	39.7

Manual Integrations
APPROVED

mohammad
12/17/2020 9:51:32 AM

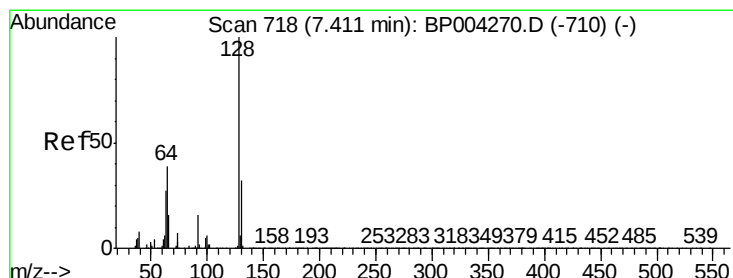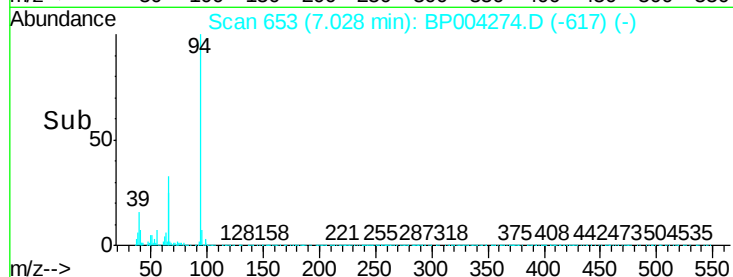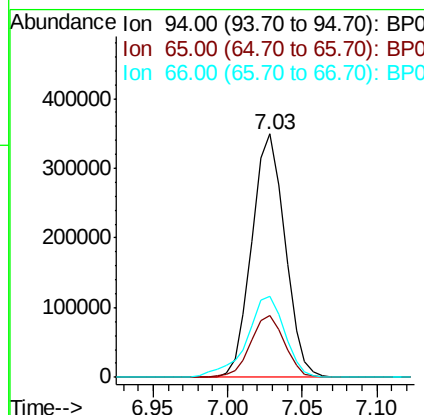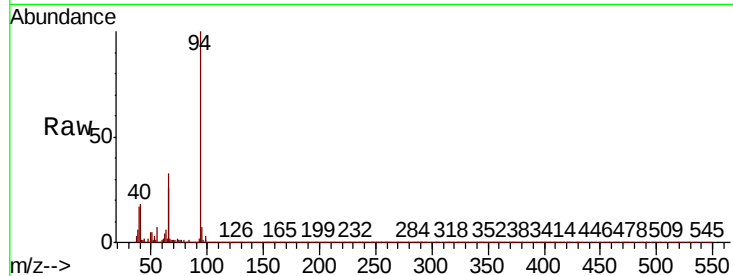

#10

2-Chlorophenol

Concen: 18.551 ng/ul




RT: 7.40 min Scan# 716


Delta R.T. 0.01 min

Lab File: BP004274.D

Acq: 14 Dec 2020 15:11

Tgt Ion:	128	Resp:	400903
Ion Ratio	Lower	Upper	
128	100		
64	42.2	36.9	55.3
130	33.3	25.9	38.9

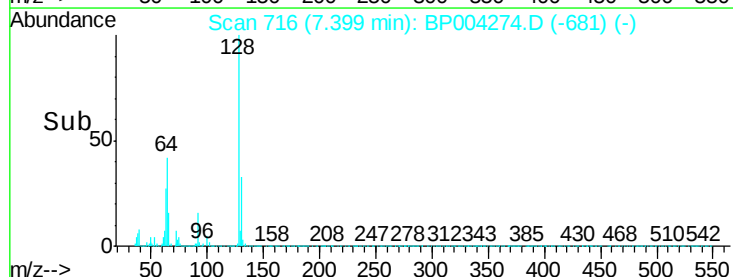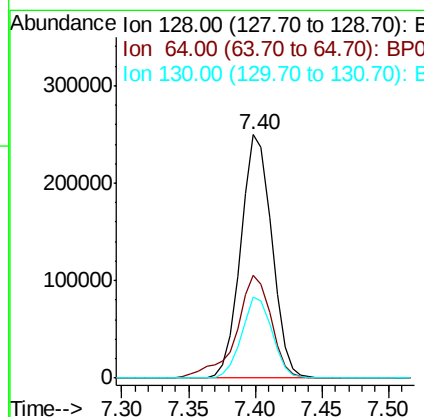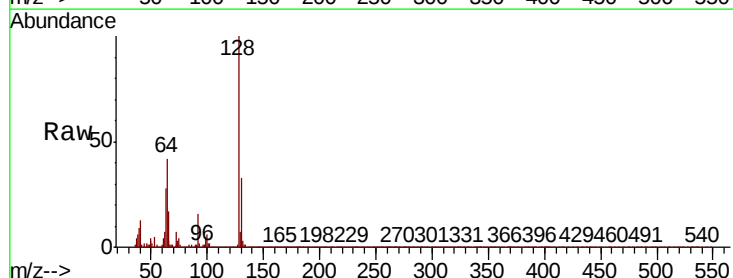







#15
N-Nitroso-di-n-propylamine
Concen: 18.792 ng/ul
RT: 8.64 min Scan# 927
Delta R.T. 0.01 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Instrument :
BNA_P
ClientSampleId :
A54A1MS

Tot Ion	Ratio	Lower	Upper
70	100		
42	47.1	39.0	58.6
101	10.4	7.6	11.4
130	23.8	16.6	25.0




Manual Integrations
APPROVED


mohammad
12/17/2020 9:51:32 AM

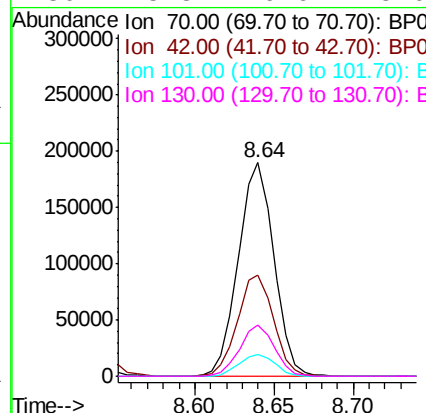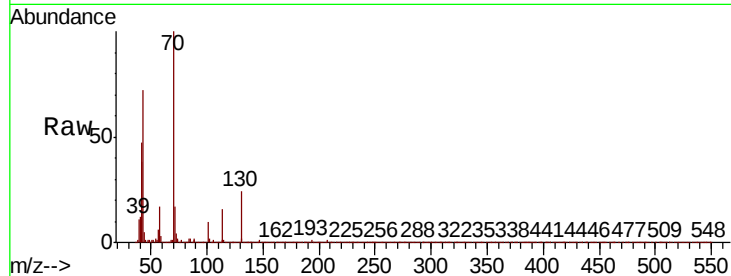

#33
4-Chloro-3-methylphenol
Concen: 22.273 ng/ul
RT: 11.92 min Scan# 1484
Delta R.T. 0.01 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Tgt Ion	Ratio	Lower	Upper
107	100		
144	26.1	22.0	33.0
142	82.4	66.2	99.2

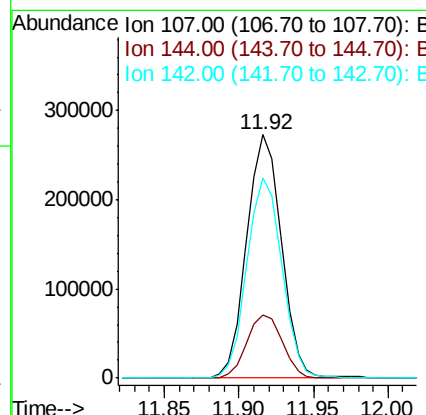







#45
Dimethylphthalate
Concen: 4.087 ng/ul
RT: 13.93 min Scan# 1827
Delta R.T. 0.01 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Instrument :
BNA_P
ClientSampled :
A54A1MS

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.2
164	10.3	8.4	12.6




Manual Integrations
APPROVED


mohammad
12/17/2020 9:51:32 AM

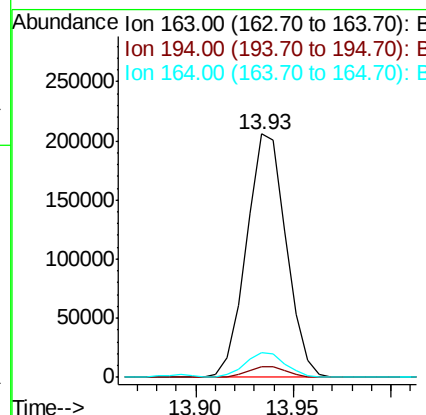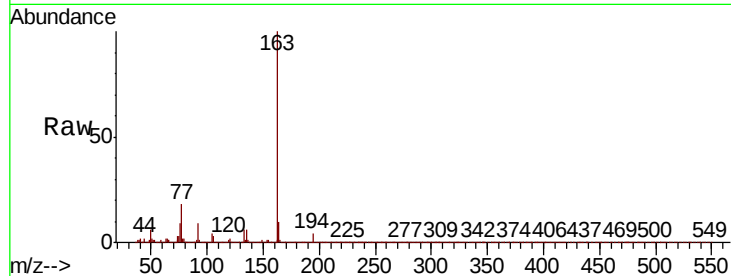

#50
Acenaphthene
Concen: 17.505 ng/ul
RT: 14.55 min Scan# 1931
Delta R.T. 0.01 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Tgt Ion	Ratio	Lower	Upper
153	100		
152	47.2	37.8	56.6
154	88.6	69.8	104.8

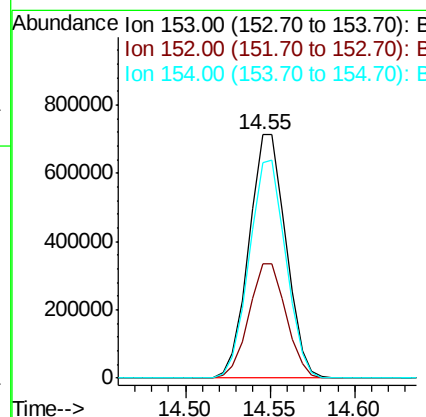







#53
4-Nitrophenol
Concen: 17.526 ng/ul
RT: 14.69 min Scan# 1956
Delta R.T. 0.02 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Instrument :
BNA_P
ClientSampleId :
A54A1MS

Tot Ion	Ratio	Resp Lower	Resp Upper
109	100		
139	142.4	113.5	170.3
65	123.1	105.1	157.7




Manual Integrations
APPROVED


mohammad
12/17/2020 9:51:32 AM

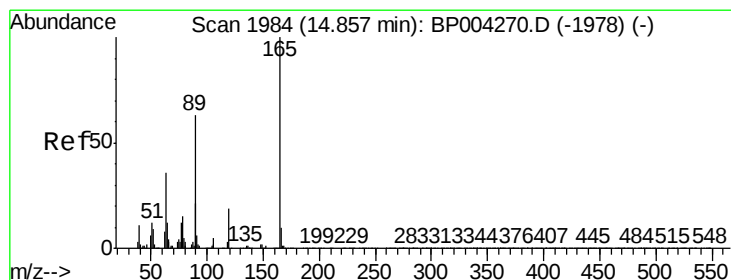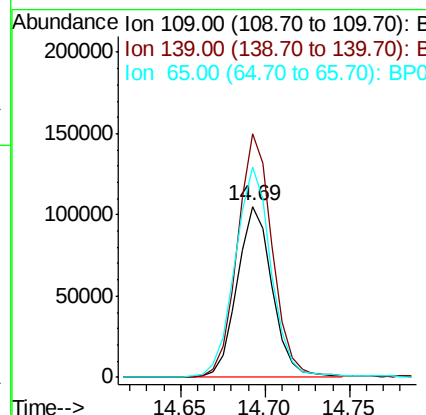

#55
2,4-Dinitrotoluene
Concen: 19.629 ng/ul
RT: 14.85 min Scan# 1983
Delta R.T. 0.02 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Tgt Ion	Ratio	Resp Lower	Resp Upper
165	100		
63	35.0	29.4	44.2
182	3.2	2.6	3.8

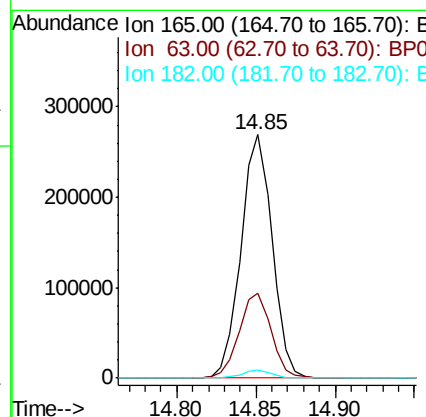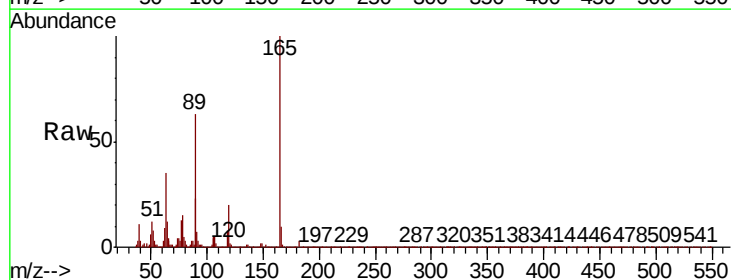







#69
 Pentachlorophenol
 Concen: 20.995 ng/ul
 RT: 16.89 min Scan# 2330
 Delta R.T. 0.01 min
 Lab File: BP004274.D
 Acq: 14 Dec 2020 15:11

Instrument :
 BNA_P
 ClientSampleID :
 A54A1MS

Tot Ion	Ratio	Resp	Lower	Upper
266	100	265762		
264	63.1	49.8	74.6	
268	63.8	52.0	78.0	




Manual Integrations
 APPROVED


mohammad
 12/17/2020 9:51:32 AM

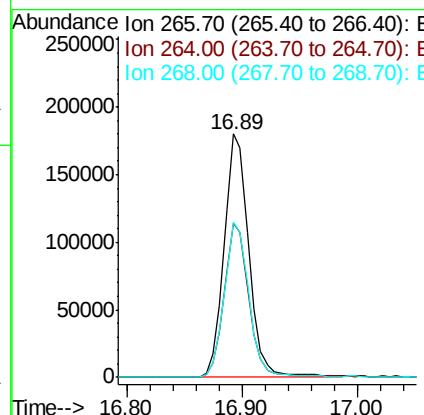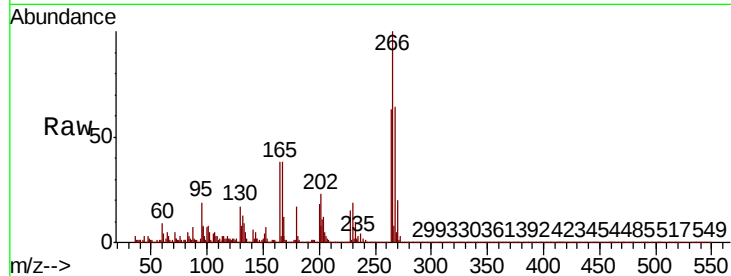

#70
 Phenanthrene
 Concen: 12.758 ng/ul
 RT: 17.29 min Scan# 2397
 Delta R.T. 0.01 min
 Lab File: BP004274.D
 Acq: 14 Dec 2020 15:11

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	1485545		
179	15.4	12.4	18.6	
176	19.1	15.4	23.0	

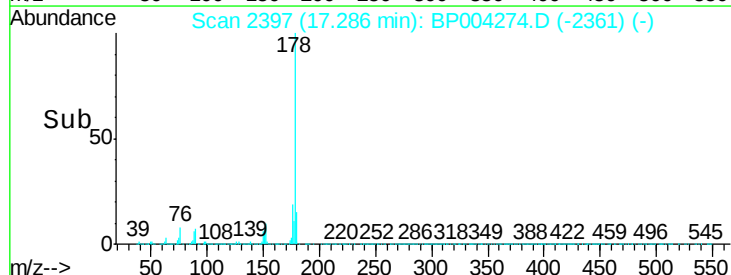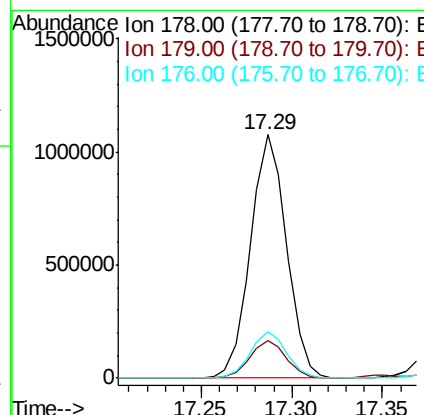



#72

Anthracene

Concen: 1.662 ng/ul

RT: 17.38 min Scan# 2413

Delta R.T. 0.01 min

Lab File: BP004274.D

Acq: 14 Dec 2020 15:11

Instrument :

BNA_P


ClientSampleId :

A54A1MS

Tot Ion:	178	Resp:	191476
Ion Ratio	Lower	Upper	
178	100		
179	14.8	12.3	18.5
176	18.8	14.9	22.3

Manual Integrations
APPROVED

mohammad
12/17/2020 9:51:32 AM



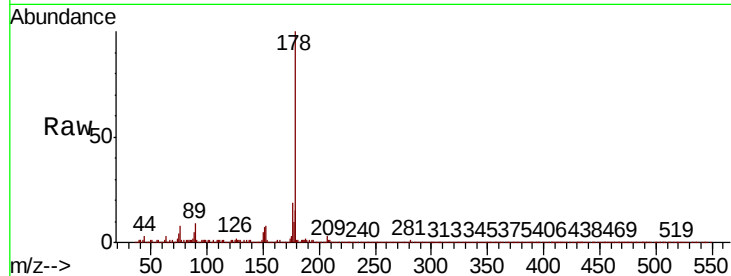


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

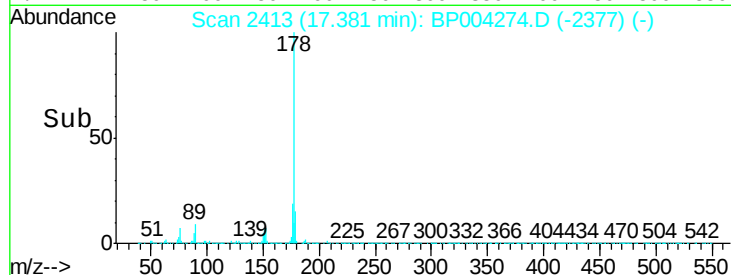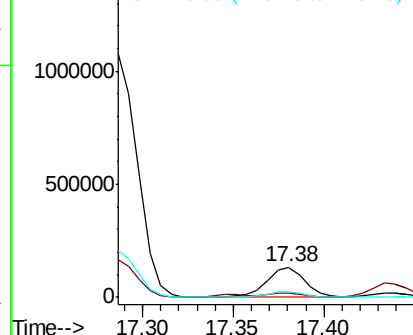

#75

Carbazole

Concen: 2.000 ng/ul

RT: 17.65 min Scan# 2458

Delta R.T. 0.01 min

Lab File: BP004274.D

Acq: 14 Dec 2020 15:11




Tgt Ion:	167	Resp:	187536
Ion Ratio	Lower	Upper	
167	100		
166	22.9	17.1	25.7
139	13.4	9.8	14.6


Abundance

Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

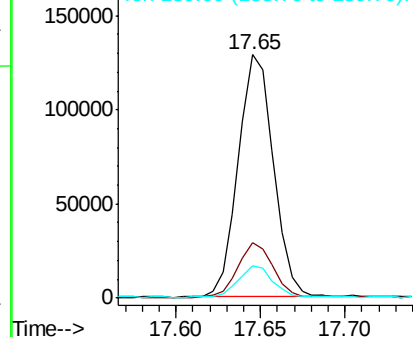







#77
 Fluoranthene
 Concen: 39.922 ng/ul
 RT: 19.26 min Scan# 2733
 Delta R.T. 0.02 min
 Lab File: BP004274.D
 Acq: 14 Dec 2020 15:11

Instrument :
 BNA_P
 ClientSampleId :
 A54A1MS

Tot Ion:	202	Resp:	4963729
Ion Ratio	Lower	Upper	
202	100		
101	9.9	9.1	13.7
100	7.5	7.1	10.7




Manual Integrations
 APPROVED


mohammad
 12/17/2020 9:51:32 AM

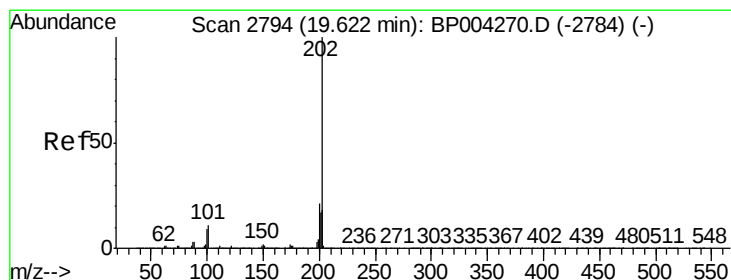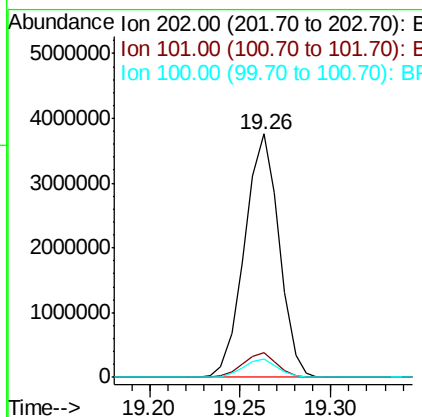

#80
 Pyrene
 Concen: 48.985 ng/ul
 RT: 19.62 min Scan# 2793
 Delta R.T. 0.02 min
 Lab File: BP004274.D
 Acq: 14 Dec 2020 15:11

Tgt Ion:	202	Resp:	6335208
Ion Ratio	Lower	Upper	
202	100		
101	11.5	10.6	15.8
100	9.4	8.6	12.8

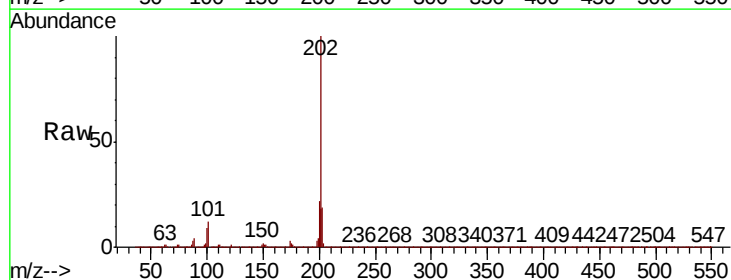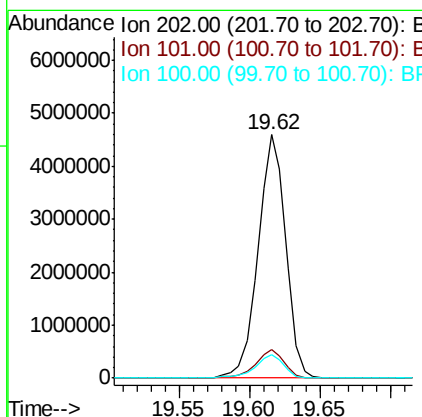







#83
Benzo(a)anthracene
Concen: 15.242 ng/ul
RT: 21.32 min Scan# 3083
Delta R.T. 0.01 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Instrument :
BNA_P
ClientSampleId :
A54A1MS

Tot Ion	Ratio	Lower	Upper
228	100		
229	21.1	15.8	23.8
226	28.2	21.7	32.5




Manual Integrations
APPROVED


mohammad
12/17/2020 9:51:32 AM

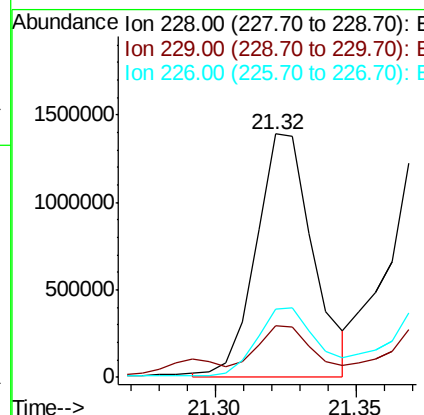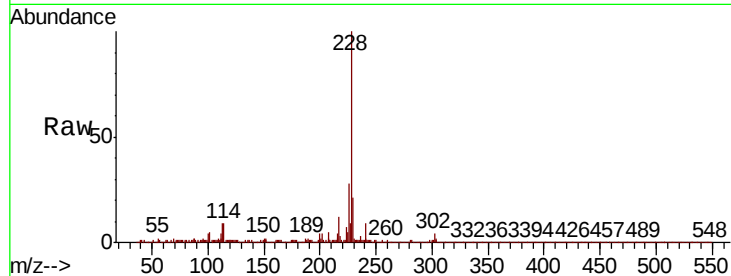

#85
Chrysene
Concen: 20.524 ng/ul
RT: 21.37 min Scan# 3092
Delta R.T. 0.01 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.4	24.2	36.2
229	21.9	15.8	23.8

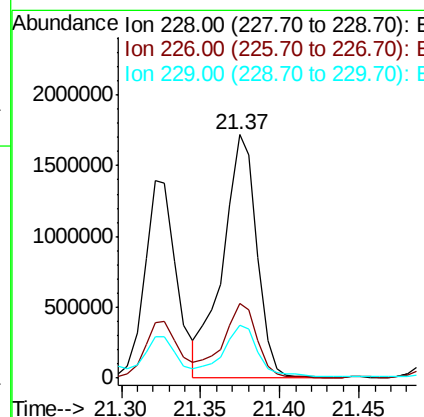







#88
Benzo(b)fluoranthene
Concen: 27.731 ng/ul
RT: 22.99 min Scan# 3367
Delta R.T. 0.03 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Instrument :
BNA_P
ClientSampleId :
A54A1MS

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.3	17.6	26.4
125	8.7	7.7	11.5




Manual Integrations
APPROVED


mohammad
12/17/2020 9:51:32 AM

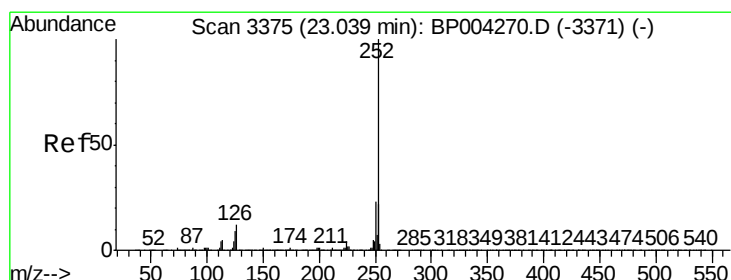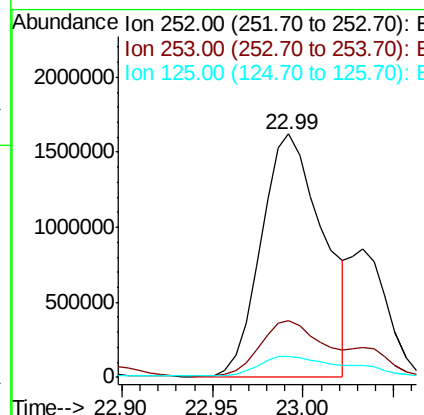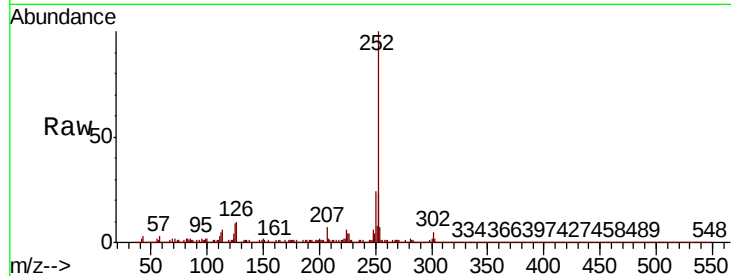

#89
Benzo(k)fluoranthene
Concen: 8.511 ng/ul m
RT: 23.03 min Scan# 3374
Delta R.T. 0.02 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.8	17.4	26.2
125	9.2	7.3	10.9

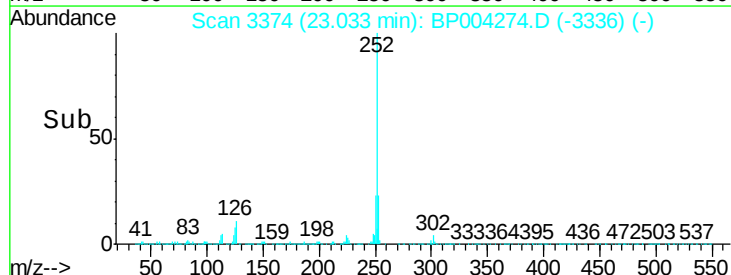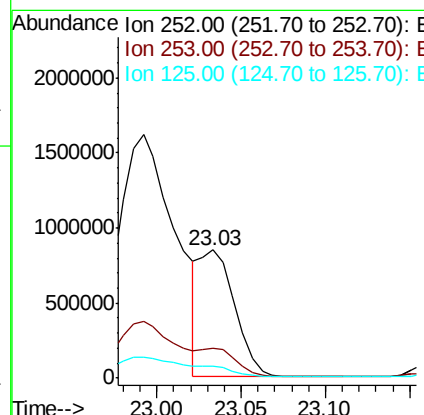







#91
Benzo(a)pyrene
Concen: 18.059 ng/ul
RT: 23.60 min Scan# 3471
Delta R.T. 0.03 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Instrument :
BNA_P
ClientSampleId :
A54A1MS

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.3	25.9
125	9.4	7.8	11.6




Manual Integrations
APPROVED


mohammad
12/17/2020 9:51:32 AM

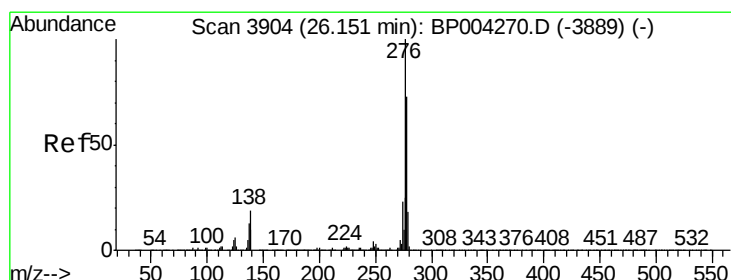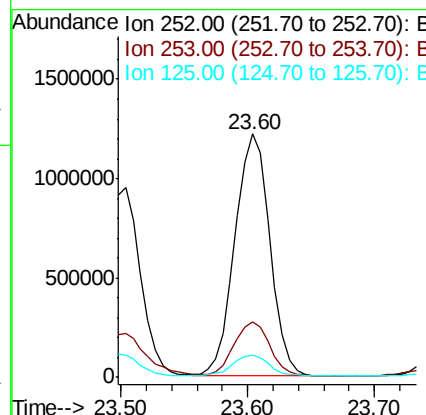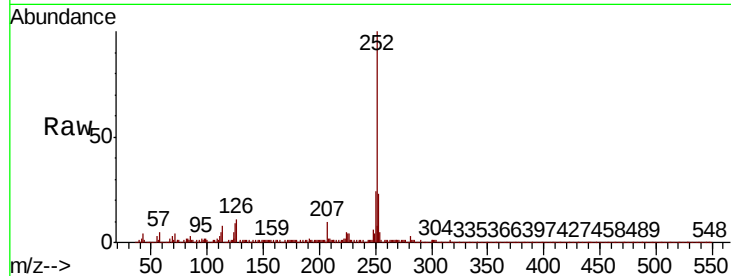

#92
Indeno(1,2,3-cd)pyrene
Concen: 12.409 ng/ul
RT: 26.14 min Scan# 3903
Delta R.T. 0.06 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Tgt Ion	Ratio	Lower	Upper
276	100		
138	20.3	17.8	26.6
277	24.6	19.8	29.6

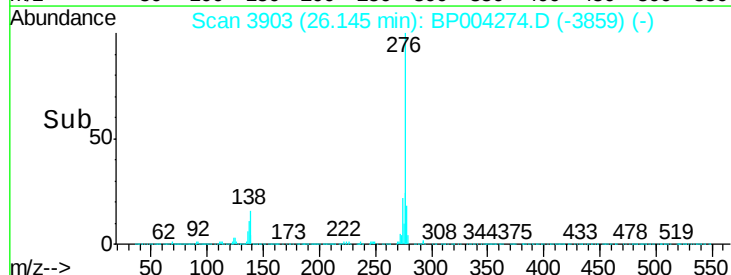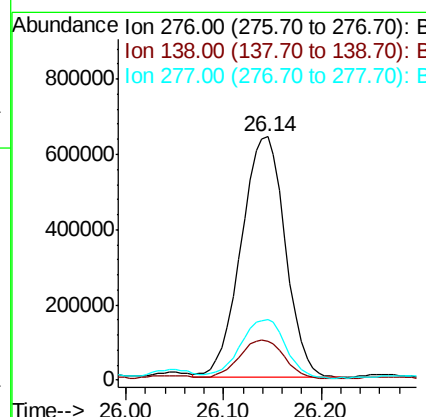







#93
Dibenzo(a,h)anthracene
Concen: 3.331 ng/ul
RT: 26.15 min Scan# 3904
Delta R.T. 0.05 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Instrument :
BNA_P
ClientSampleId :
A54A1MS

Tot Ion	Ratio	Lower	Upper
278	100		
139	19.5	11.9	17.9#
279	27.6	18.6	28.0

Manual Integrations
APPROVED

mohammad
12/17/2020 9:51:32 AM

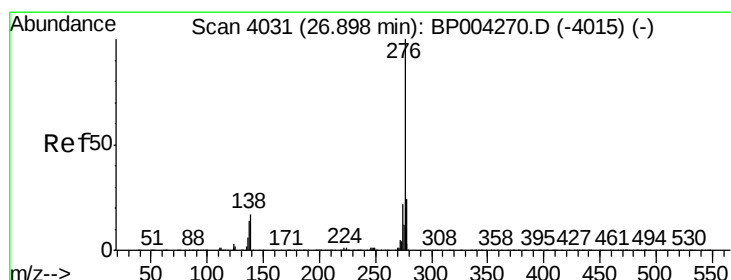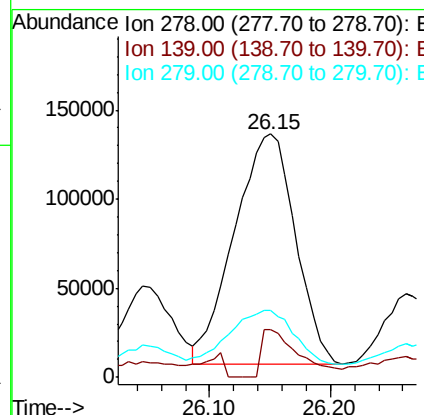

#94
Benzo(g,h,i)perylene
Concen: 12.154 ng/ul
RT: 26.89 min Scan# 4029
Delta R.T. 0.06 min
Lab File: BP004274.D
Acq: 14 Dec 2020 15:11

Tgt Ion	Ratio	Lower	Upper
276	100		
138	17.6	16.6	25.0
277	24.8	18.5	27.7

