

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
 Data File : BP004306.D
 Acq On : 15 Dec 2020 16:11
 Operator : CG/JU
 Sample : L5001-04
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54C2

Manual Integrations
 APPROVED

mohammad
 12/17/2020 9:52:51 AM

Quant Time: Dec 15 17:36:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 15 09:00:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.85	152	349159	20.00	ng/ul	0.01
18) Naphthalene-d8	10.64	136	1458848	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.49	164	895710	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.26	188	1851474	20.00	ng/ul	0.01
78) Chrysene-d12	21.35	240	1712461	20.00	ng/ul	0.01
86) Perylene-d12	23.73	264	1933805	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.33	96	11851	1.19	ng/uL	0.00
5) Phenol-d5	7.01	99	291439	10.09	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.17	67	157323	8.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.38	132	234985	10.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.55	113	216616	9.93	ng/ul	0.00
19) Nitrobenzene-d5	9.00	128	116816	9.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.72	143	102864	10.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.26	165	243107	11.22	ng/ul	0.01
29) 4-Chloroaniline-d4	10.78	131	230385	8.58	ng/ul	0.01
44) Dimethylphthalate-d6	13.89	166	704270	10.29	ng/ul	0.00
47) Acenaphthylene-d8	14.18	160	952677	10.90	ng/ul	0.00
52) 4-Nitrophenol-d4	14.69	143	89107	7.71	ng/ul	0.01
58) Fluorene-d10	15.49	176	637336	10.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.62	200	2394	0.27	ng/ul	0.01
71) Anthracene-d10	17.35	188	966865	10.72	ng/ul	0.00
79) Pyrene-d10	19.60	212	1001897	11.23	ng/ul	0.01
90) Benzo(a)pyrene-d12	23.57	264	1104229	10.84	ng/ul	0.03

Target Compounds

					Ovalue	
6) Phenol	7.03	94	58940	1.954	ng/ul	95
45) Dimethylphthalate	13.94	163	133660	1.917	ng/ul	99
70) Phenanthrene	17.30	178	173178	1.585	ng/ul	97
77) Fluoranthene	19.27	202	674302	5.781	ng/ul	96
80) Pyrene	19.62	202	650216	5.629	ng/ul	97
83) Benzo(a)anthracene	21.33	228	314383	2.785	ng/ul#	87
85) Chrysene	21.39	228	429310	3.877	ng/ul#	90
88) Benzo(b)fluoranthene	23.00	252	710844	5.796	ng/ul#	80
89) Benzo(k)fluoranthene	23.05	252	201237m	1.598	ng/ul	
91) Benzo(a)pyrene	23.62	252	424630	3.711	ng/ul#	75
92) Indeno(1,2,3-cd)pyrene	26.17	276	370227	2.580	ng/ul#	92
94) Benzo(g,h,i)perylene	26.92	276	286197	2.377	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
Data File : BP004306.D
Acq On : 15 Dec 2020 16:11
Operator : CG/JU
Sample : L5001-04
Misc :
ALS Vial : 41 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
A54C2

Manual Integrations
APPROVED

mohammad
12/17/2020 9:52:51 AM

Quant Time: Dec 15 17:36:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 15 09:00:06 2020
Response via : Initial Calibration

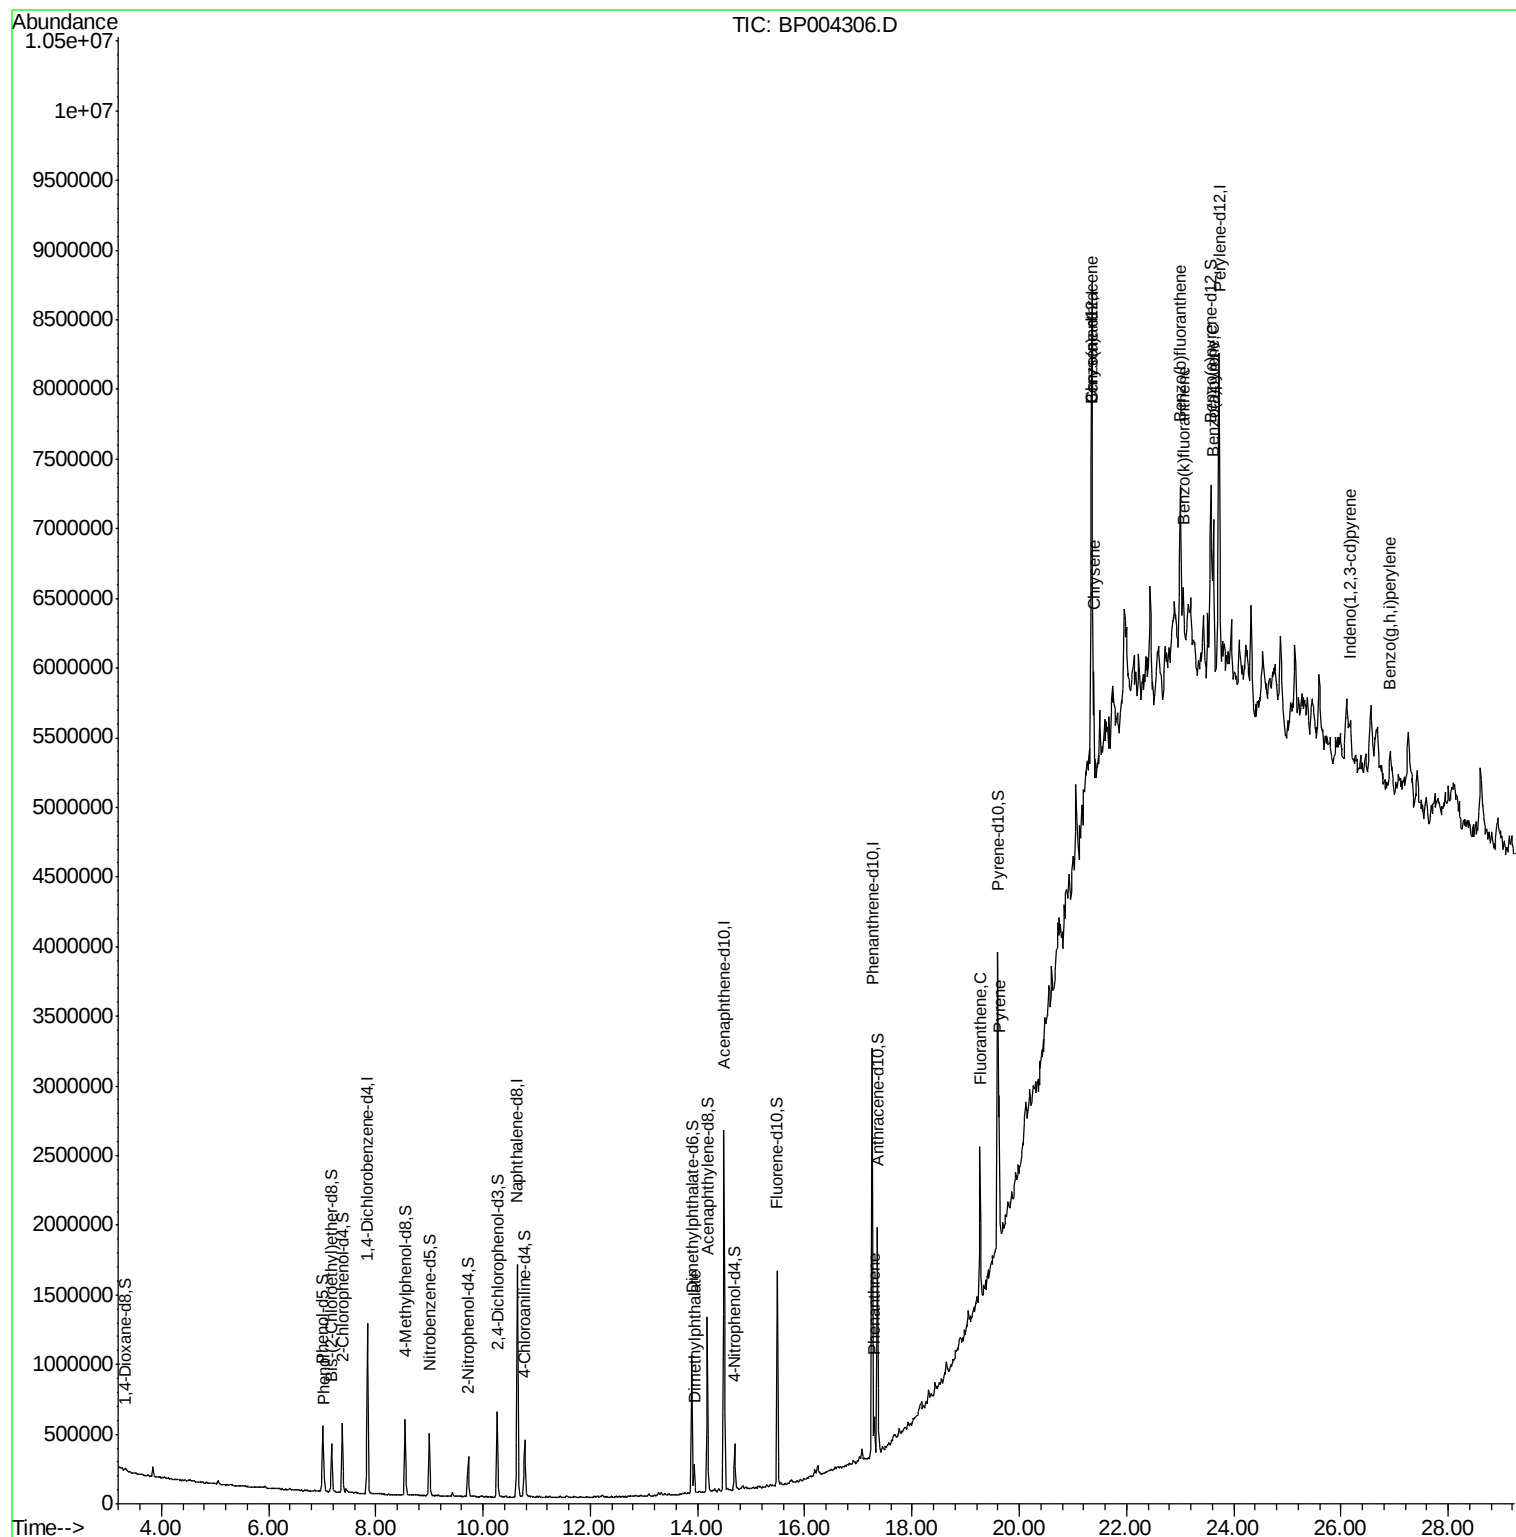

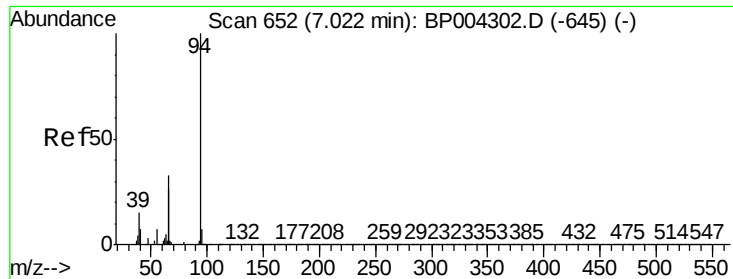

#6

Phenol

Concen: 1.954 ng/ul

RT: 7.03 min Scan# 654

Delta R.T. 0.01 min

Lab File: BP004306.D

Acq: 15 Dec 2020 16:11

Instrument :

BNA_P





ClientSampleId :

A54C2

Tot Ion:	94	Resp:	58940
Ion Ratio	Lower	Upper	
94	100		
65	28.7	20.8	31.2
66	36.1	26.5	39.7

Manual Integrations
APPROVED

mohammad
12/17/2020 9:52:51 AM

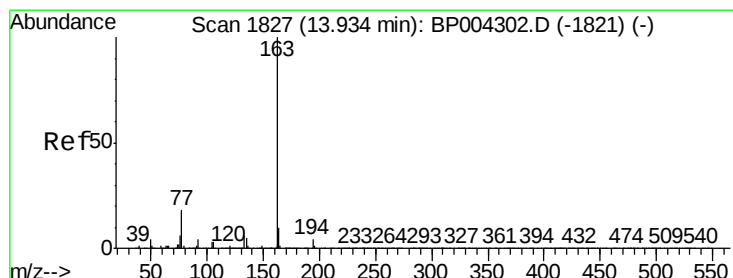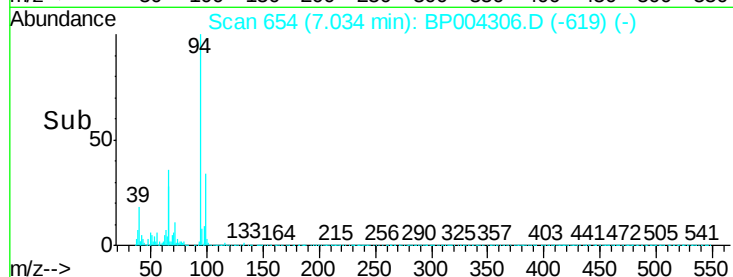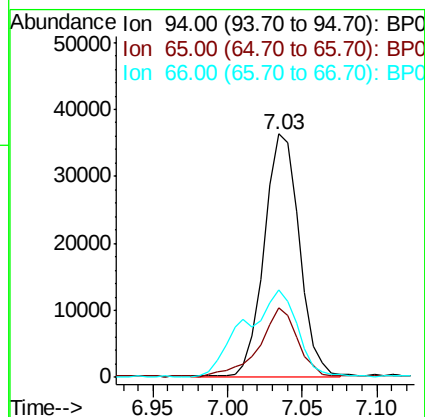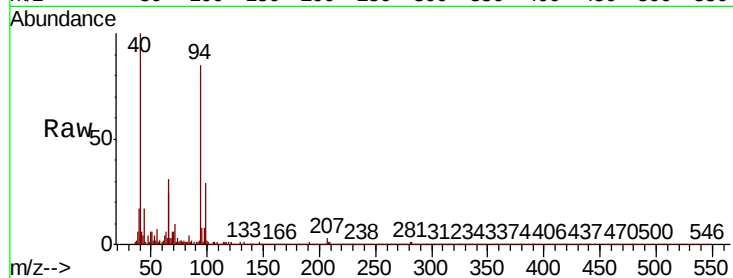

#45

Dimethylphthalate

Concen: 1.917 ng/ul




RT: 13.94 min Scan# 1828


Delta R.T. 0.00 min

Lab File: BP004306.D

Acq: 15 Dec 2020 16:11

Tgt Ion:	163	Resp:	133660
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.4	5.2
164	9.9	8.4	12.6

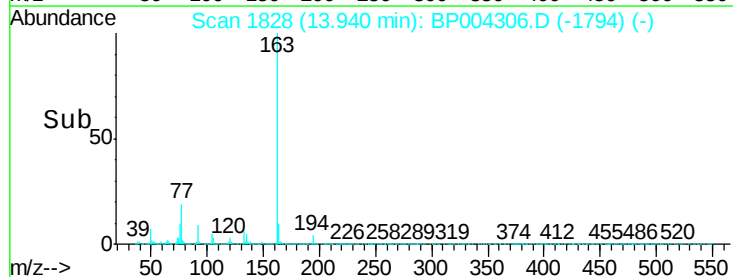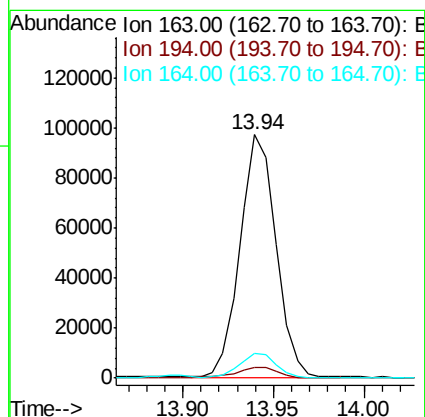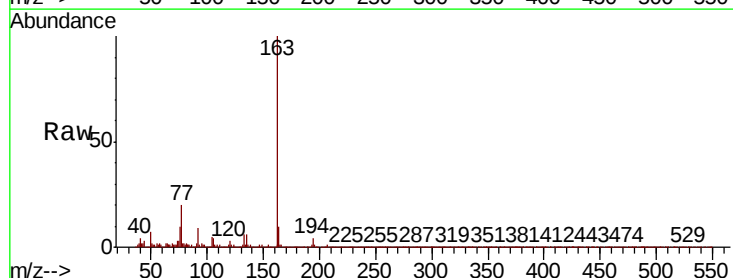

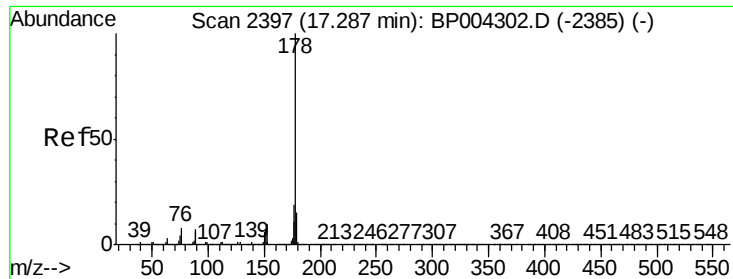





#70
Phenanthrene
Concen: 1.585 ng/ul
RT: 17.30 min Scan# 2399
Delta R.T. 0.01 min
Lab File: BP004306.D
Acq: 15 Dec 2020 16:11

Instrument :
BNA_P
ClientSampleId :
A54C2

Tot Ion:	178	Resp:	173178
Ion Ratio	Lower	Upper	
178	100		
179	16.8	12.4	18.6
176	20.5	15.4	23.0




Manual Integrations
APPROVED


mohammad
12/17/2020 9:52:51 AM

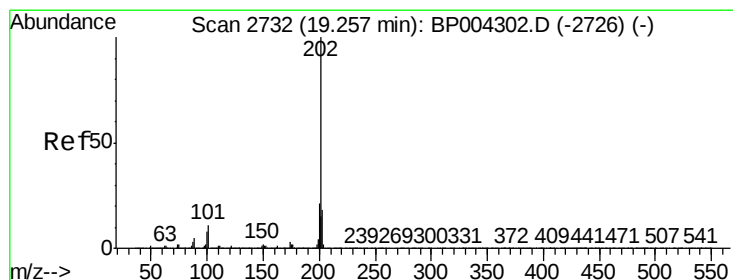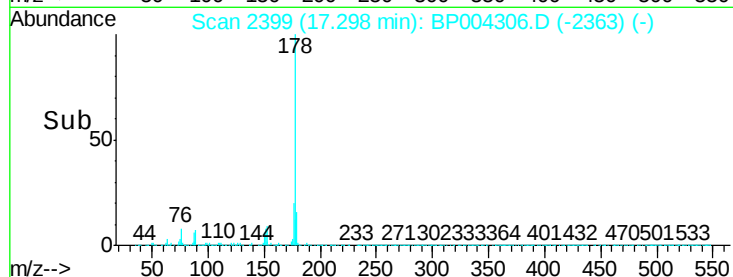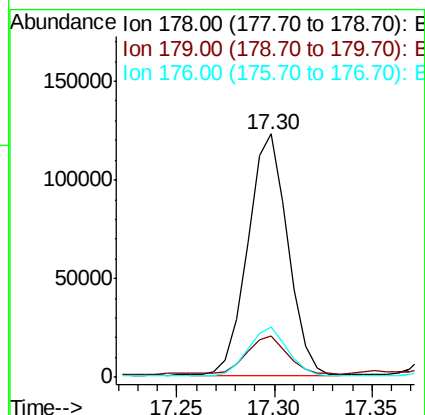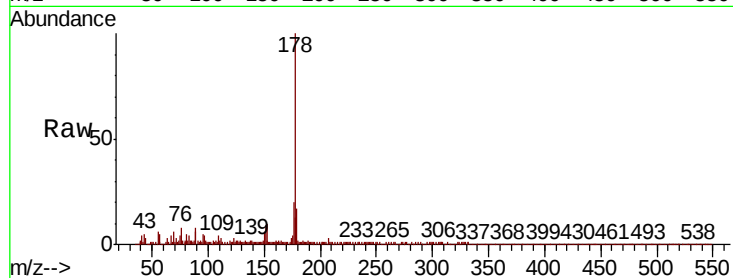

#77
Fluoranthene
Concen: 5.781 ng/ul
RT: 19.27 min Scan# 2734
Delta R.T. 0.01 min
Lab File: BP004306.D
Acq: 15 Dec 2020 16:11

Tgt Ion:	202	Resp:	674302
Ion Ratio	Lower	Upper	
202	100		
101	10.0	9.1	13.7
100	7.7	7.1	10.7

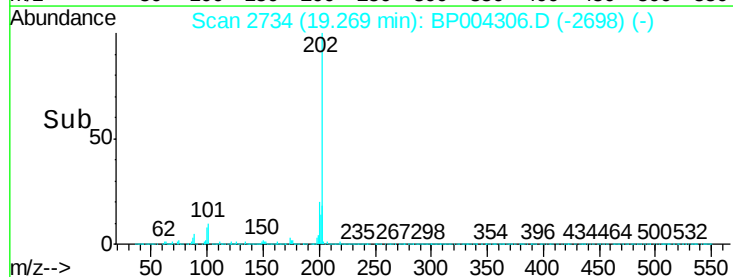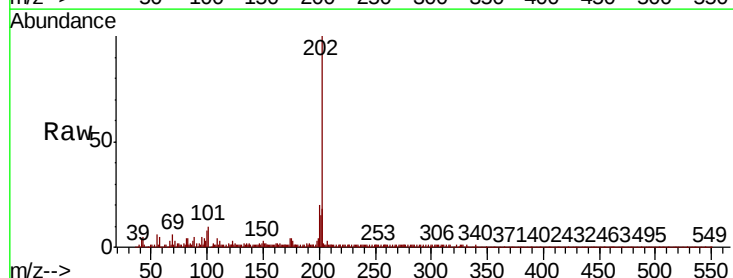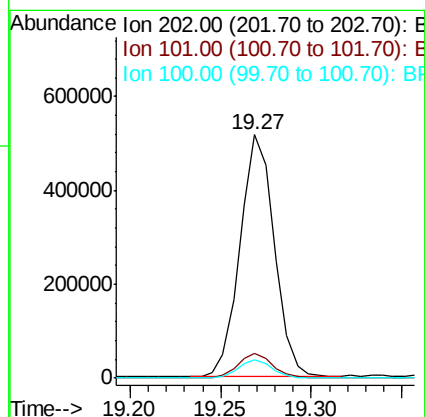

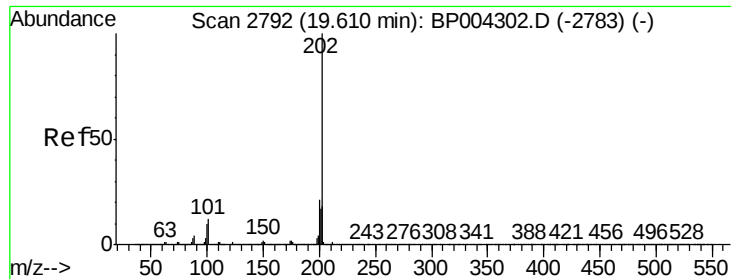





#80
Pvrene
Concen: 5.629 ng/ul
RT: 19.62 min Scan# 2794
Delta R.T. 0.01 min
Lab File: BP004306.D
Acq: 15 Dec 2020 16:11

Instrument :
BNA_P
ClientSampleId :
A54C2

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	11.8	10.6	15.8
100	9.5	8.6	12.8




Manual Integrations
APPROVED


mohammad
12/17/2020 9:52:51 AM

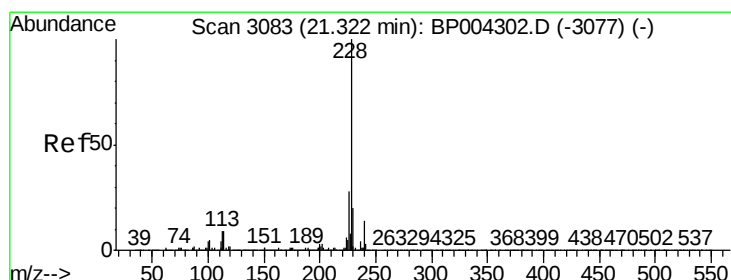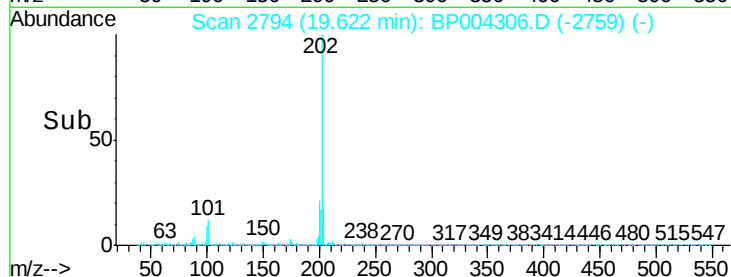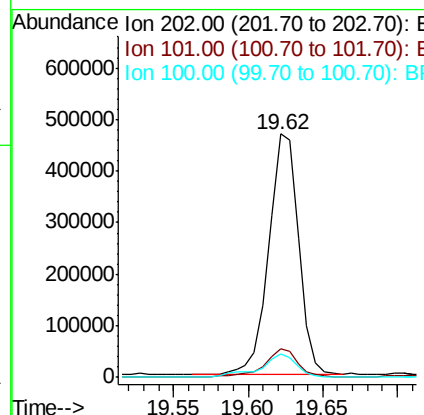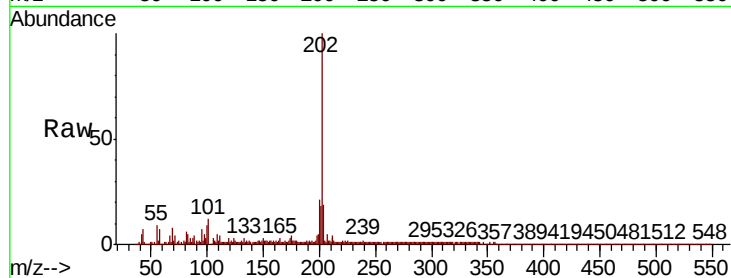

#83
Benzo(a)anthracene
Concen: 2.785 ng/ul
RT: 21.33 min Scan# 3085
Delta R.T. 0.01 min
Lab File: BP004306.D
Acq: 15 Dec 2020 16:11

Tgt Ion	Ratio	Resp Lower	Upper
228	100		
229	27.7	15.8	23.8#
226	32.2	21.7	32.5

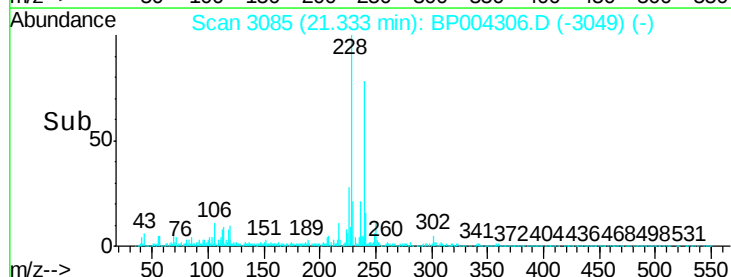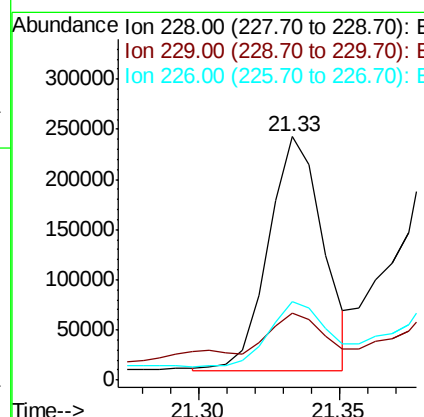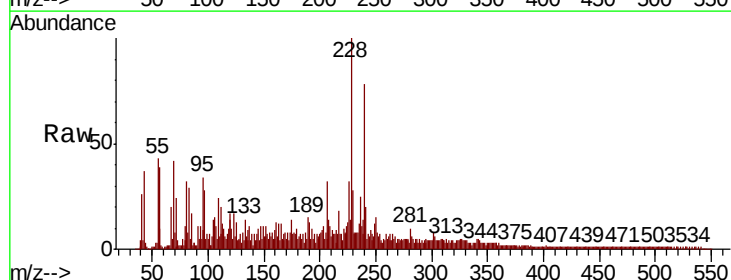

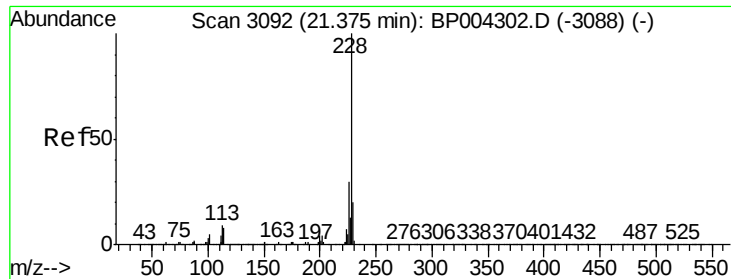

#85

Chrysene

Concen: 3.877 ng/ul

RT: 21.39 min Scan# 3094

Delta R.T. 0.01 min

Lab File: BP004306.D

Acq: 15 Dec 2020 16:11

Instrument :

BNA_P





ClientSampleId :

A54C2

Tot Ion:	228	Resp:	429310
Ion Ratio	Lower	Upper	
228	100		
226	34.2	24.2	36.2
229	26.6	15.8	23.8

Manual Integrations
APPROVED

mohammad
12/17/2020 9:52:51 AM

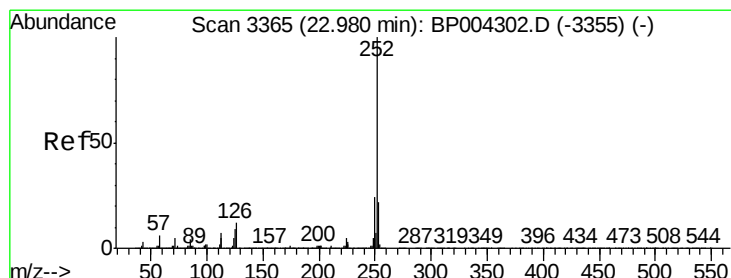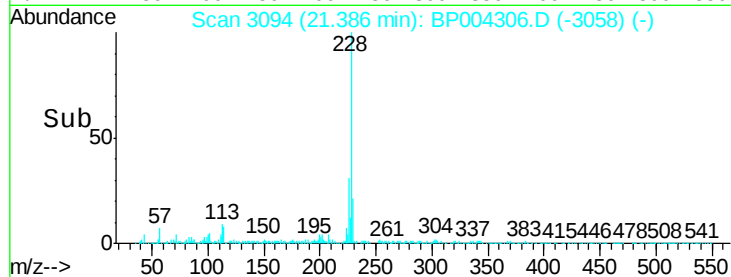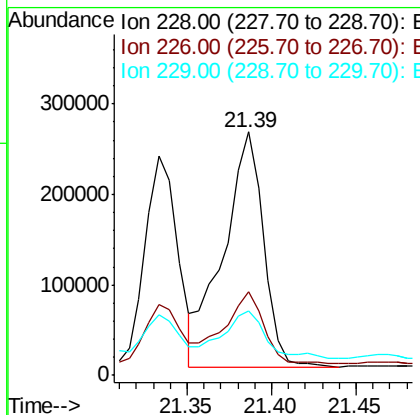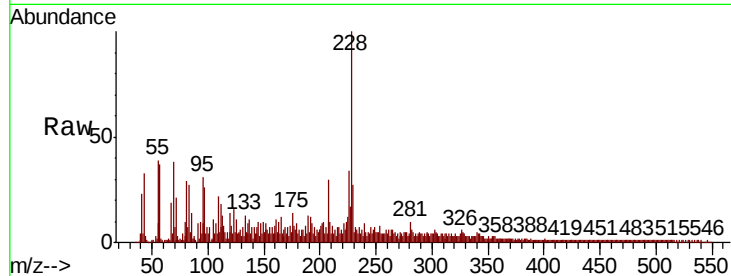

#88

Benzo(b)fluoranthene

Concen: 5.796 ng/ul




RT: 23.00 min Scan# 3369


Delta R.T. 0.02 min

Lab File: BP004306.D

Acq: 15 Dec 2020 16:11

Tgt Ion:	252	Resp:	710844
Ion Ratio	Lower	Upper	
252	100		
253	30.8	17.6	26.4
125	18.2	7.7	11.5

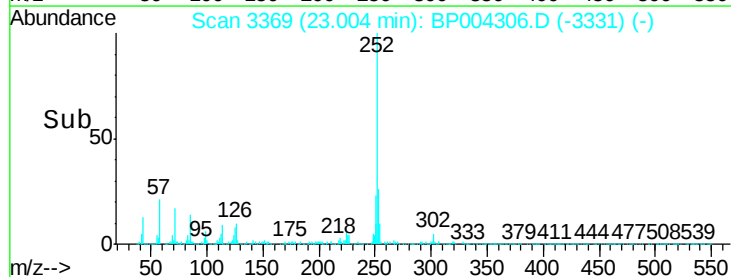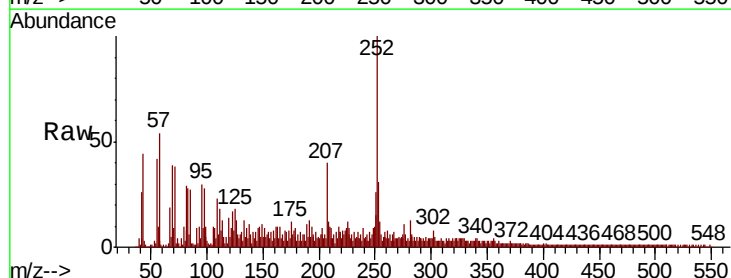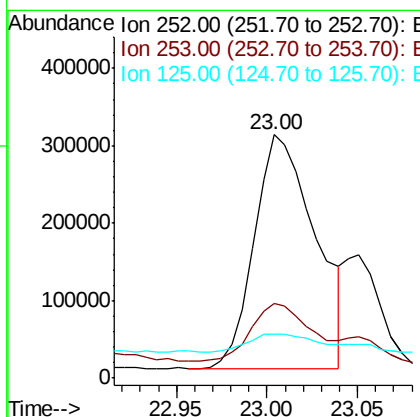

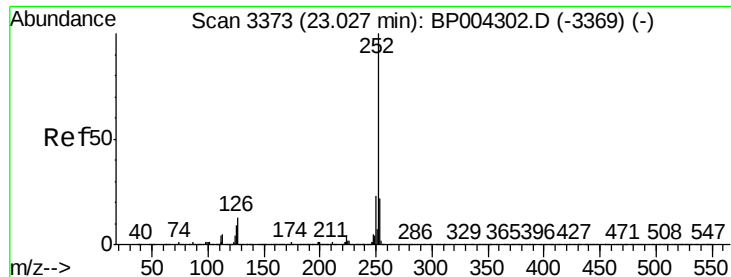





#89
Benzo(k)fluoranthene
Concen: 1.598 ng/ul m
RT: 23.05 min Scan# 3377
Delta R.T. 0.02 min
Lab File: BP004306.D
Acq: 15 Dec 2020 16:11

Instrument :
BNA_P
ClientSampleId :
A54C2

Tot Ion	Ratio	Lower	Upper
252	100		
253	33.3	17.4	26.2#
125	27.1	7.3	10.9#




Manual Integrations
APPROVED


mohammad
12/17/2020 9:52:51 AM

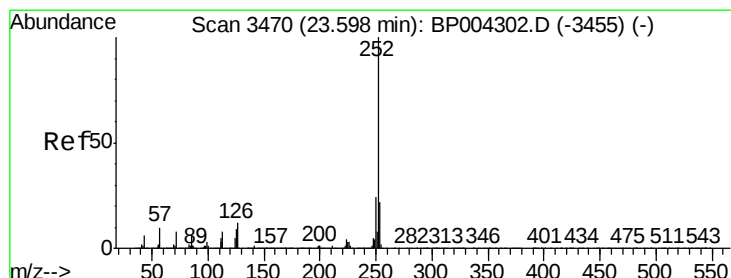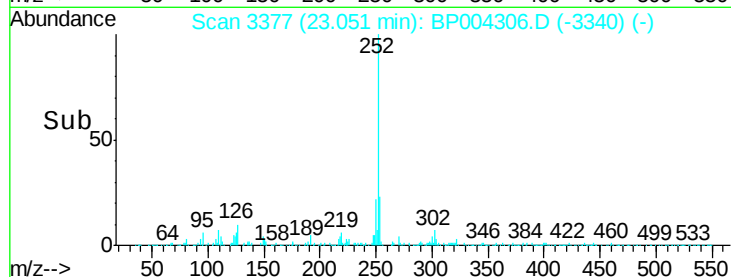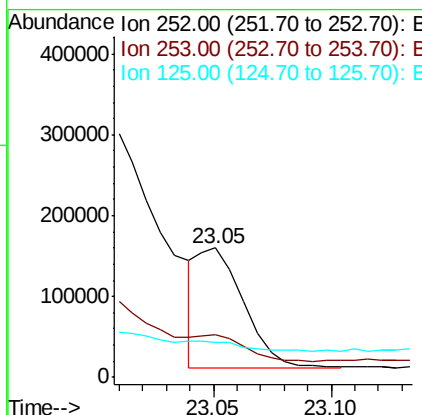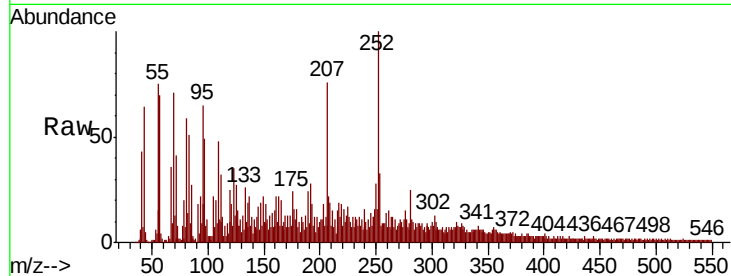

#91
Benzo(a)pyrene
Concen: 3.711 ng/ul
RT: 23.62 min Scan# 3474
Delta R.T. 0.02 min
Lab File: BP004306.D
Acq: 15 Dec 2020 16:11

Tgt Ion	Ratio	Lower	Upper
252	100		
253	30.2	17.3	25.9#
125	24.7	7.8	11.6#

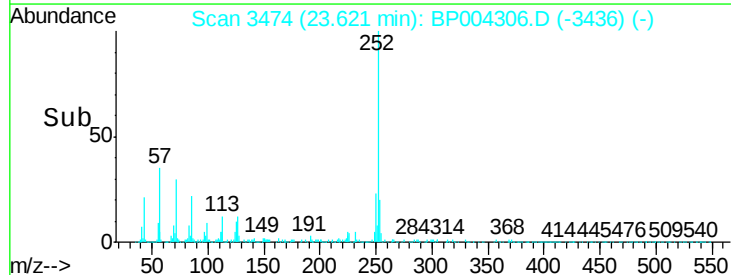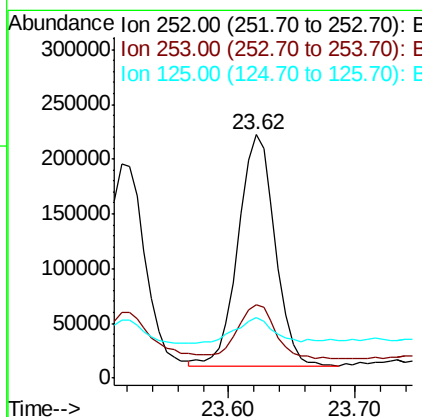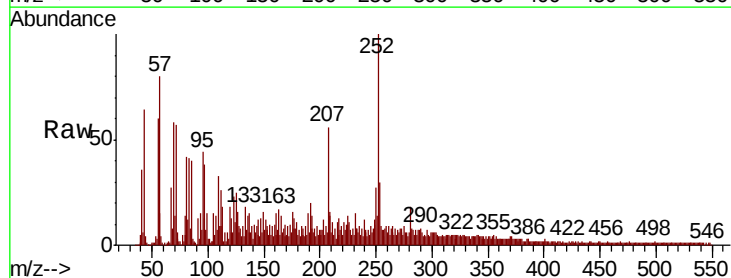

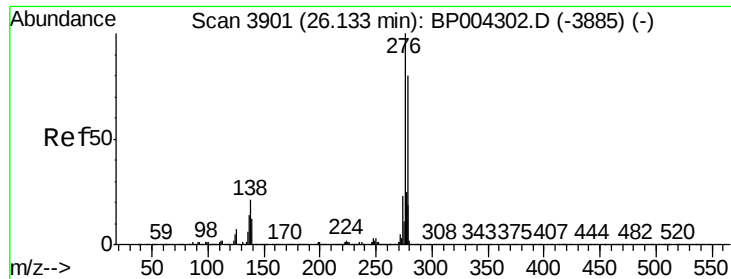





#92
 Indeno(1,2,3-cd)pyrene
 Concen: 2.580 ng/ul
 RT: 26.17 min Scan# 3908
 Delta R.T. 0.04 min
 Lab File: BP004306.D
 Acq: 15 Dec 2020 16:11

Instrument :
 BNA_P
 ClientSampleId :
 A54C2

Tot Ion	Ratio	Lower	Upper
276	100		
138	21.5	17.8	26.6
277	31.9	19.8	29.6

Manual Integrations
 APPROVED

mohammad
 12/17/2020 9:52:51 AM

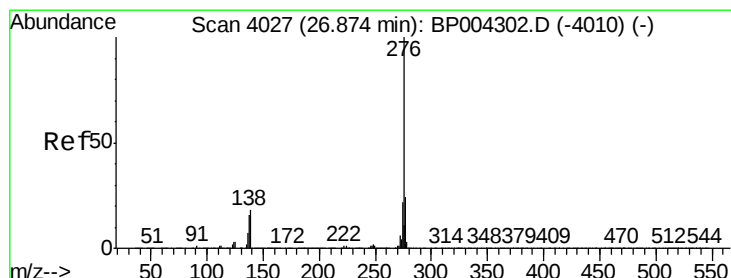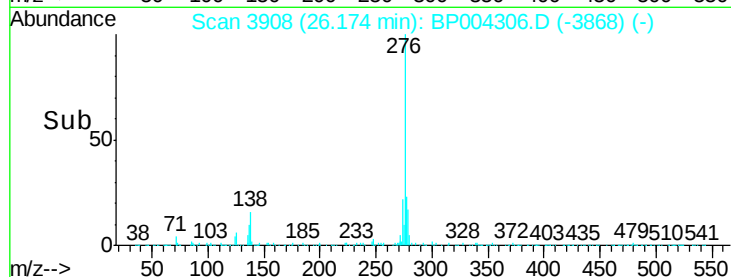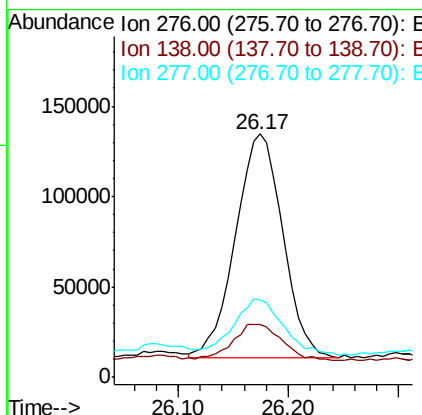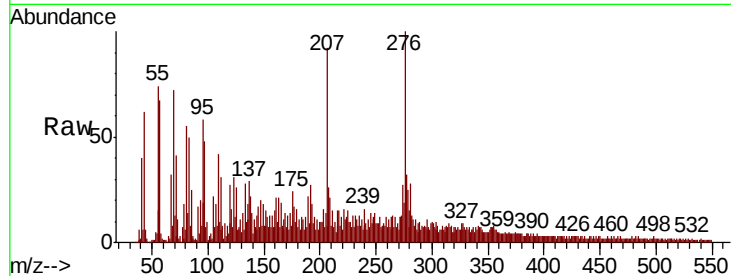

#94
 Benzo(g,h,i)perylene
 Concen: 2.377 ng/ul
 RT: 26.92 min Scan# 4035
 Delta R.T. 0.04 min
 Lab File: BP004306.D
 Acq: 15 Dec 2020 16:11

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.3	16.6	25.0
277	34.3	18.5	27.7

