

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
 Data File : BP004293.D
 Acq On : 15 Dec 2020 02:32
 Operator : CG/JU
 Sample : L5001-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54D7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.999	642	648	666	rVB2	690582	1273472	19.94%	2.001%
2	7.169	671	677	685	rBV	536815	865013	13.55%	1.359%
3	7.369	705	711	718	rBV	726978	1166407	18.27%	1.832%
4	7.434	718	722	735	rVB3	39772	87816	1.38%	0.138%
5	7.840	784	791	798	rBV	1432621	2276751	35.65%	3.577%
6	8.540	903	910	918	rBV	778414	1281353	20.07%	2.013%
7	8.993	980	987	996	rVB	670855	1125937	17.63%	1.769%
8	9.428	1056	1061	1069	rVB	48757	79807	1.25%	0.125%
9	9.716	1102	1110	1122	rBV	518055	900395	14.10%	1.415%
10	10.251	1194	1201	1212	rBV	908167	1516509	23.75%	2.382%
11	10.634	1258	1266	1280	rBV	2076491	3453044	54.07%	5.425%
12	10.763	1281	1288	1303	rVV	806599	1408990	22.06%	2.214%
13	10.987	1322	1326	1330	rVB6	5502	10792	0.17%	0.017%
14	11.228	1363	1367	1371	rBV5	4812	6621	0.10%	0.010%
15	11.428	1396	1401	1402	rBV5	4529	6858	0.11%	0.011%
16	11.540	1415	1420	1434	rVV5	4710	16144	0.25%	0.025%
17	11.669	1437	1442	1447	rVB8	4161	7709	0.12%	0.012%
18	12.069	1506	1510	1513	rBV4	9007	13045	0.20%	0.020%
19	12.128	1516	1520	1523	rBV4	4601	6591	0.10%	0.010%
20	12.222	1532	1536	1543	rVB	17311	28516	0.45%	0.045%
21	12.840	1637	1641	1645	rVV6	4774	6914	0.11%	0.011%
22	12.887	1645	1649	1654	rVB8	4535	7552	0.12%	0.012%
23	13.028	1670	1673	1679	rVV8	4487	7016	0.11%	0.011%
24	13.087	1679	1683	1690	rVB5	10267	15769	0.25%	0.025%
25	13.316	1718	1722	1726	rBV3	21589	31857	0.50%	0.050%
26	13.381	1729	1733	1738	rVV2	18213	33626	0.53%	0.053%
27	13.445	1738	1744	1750	rVB2	5298	9804	0.15%	0.015%
28	13.757	1793	1797	1800	rBV6	6316	7390	0.12%	0.012%
29	13.804	1800	1805	1809	rBV8	5053	9337	0.15%	0.015%
30	13.887	1811	1819	1824	rBV	1504232	2137835	33.48%	3.359%
31	13.934	1824	1827	1833	rVB	342913	452160	7.08%	0.710%
32	14.175	1857	1868	1878	rBV	1926130	2876091	45.04%	4.518%
33	14.392	1901	1905	1911	rVV	15556	21358	0.33%	0.034%
34	14.486	1911	1921	1928	rVV	3108667	4675754	73.22%	7.346%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
 Data File : BP004293.D
 Acq On : 15 Dec 2020 02:32
 Operator : CG/JU
 Sample : L5001-19
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54D7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

35	14.551	1928	1932	1939	rVB3	14689	27809	0.44%	0.044%
36	14.681	1947	1954	1970	rBV	585747	908702	14.23%	1.428%
37	14.834	1975	1980	1984	rVV8	8797	19792	0.31%	0.031%
38	14.892	1986	1990	1998	rVV8	13597	33321	0.52%	0.052%
39	14.963	1998	2002	2007	rVB6	6740	11214	0.18%	0.018%
40	15.016	2007	2011	2017	rVB8	5041	8449	0.13%	0.013%
41	15.110	2023	2027	2034	rVB10	4124	7728	0.12%	0.012%
42	15.304	2052	2060	2064	rBV10	6319	14535	0.23%	0.023%
43	15.351	2064	2068	2072	rBV3	14879	18284	0.29%	0.029%
44	15.481	2083	2090	2097	rBV	2289676	3310370	51.84%	5.201%
45	15.533	2097	2099	2104	rVB2	13992	15301	0.24%	0.024%
46	15.604	2106	2111	2119	rBV	203077	315747	4.94%	0.496%
47	15.722	2126	2131	2141	rVB3	28259	56308	0.88%	0.088%
48	15.833	2145	2150	2157	rVB9	8843	20481	0.32%	0.032%
49	16.057	2185	2188	2193	rVB7	3716	7508	0.12%	0.012%
50	16.169	2202	2207	2211	rBV7	9780	20204	0.32%	0.032%
51	16.216	2211	2215	2220	rVV6	19561	35476	0.56%	0.056%
52	16.275	2222	2225	2231	rVB8	14447	21142	0.33%	0.033%
53	16.480	2257	2260	2265	rBV	18786	23260	0.36%	0.037%
54	16.816	2315	2317	2321	rVB5	7300	6512	0.10%	0.010%
55	16.898	2327	2331	2340	rVB3	13656	29389	0.46%	0.046%
56	16.975	2340	2344	2346	rBV5	10191	17077	0.27%	0.027%
57	17.245	2383	2390	2395	rBV	3754314	5360630	83.94%	8.421%
58	17.286	2395	2397	2401	rVV	234604	278031	4.35%	0.437%
59	17.345	2401	2407	2418	rVB	2493476	3657997	57.28%	5.747%
60	17.439	2419	2423	2427	rBV3	15254	20973	0.33%	0.033%
61	17.486	2427	2431	2440	rBV	51230	101321	1.59%	0.159%
62	17.651	2456	2459	2462	rVB	20443	23242	0.36%	0.037%
63	18.133	2535	2541	2543	rBV2	52733	112340	1.76%	0.176%
64	18.163	2543	2546	2551	rVB	66987	92119	1.44%	0.145%
65	18.304	2565	2570	2574	rBV3	71488	131076	2.05%	0.206%
66	18.598	2617	2620	2623	rBV	36630	45656	0.71%	0.072%
67	18.639	2624	2627	2633	rVB2	44800	63789	1.00%	0.100%
68	19.257	2728	2732	2738	rVB	672820	869524	13.62%	1.366%
69	19.586	2782	2788	2799	rBV2	3345926	5310984	83.17%	8.343%
70	21.051	3034	3037	3044	rVB5	217555	334321	5.24%	0.525%
71	21.339	3080	3086	3090	rBV	4563986	6291617	98.52%	9.884%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
Data File : BP004293.D
Acq On : 15 Dec 2020 02:32
Operator : CG/JU
Sample : L5001-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54D7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Title : SVOA CALIBRATION

72	23.551	3456	3462	3467	rBV	1976956	3821981	59.85%	6.004%
73	23.698	3481	3487	3505	rVB	3023871	6385892	100.00%	10.032%


Sum of corrected areas: 63654335

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
Data File : BP004293.D
Acq On : 15 Dec 2020 02:32
Operator : CG/JU
Sample : L5001-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54D7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

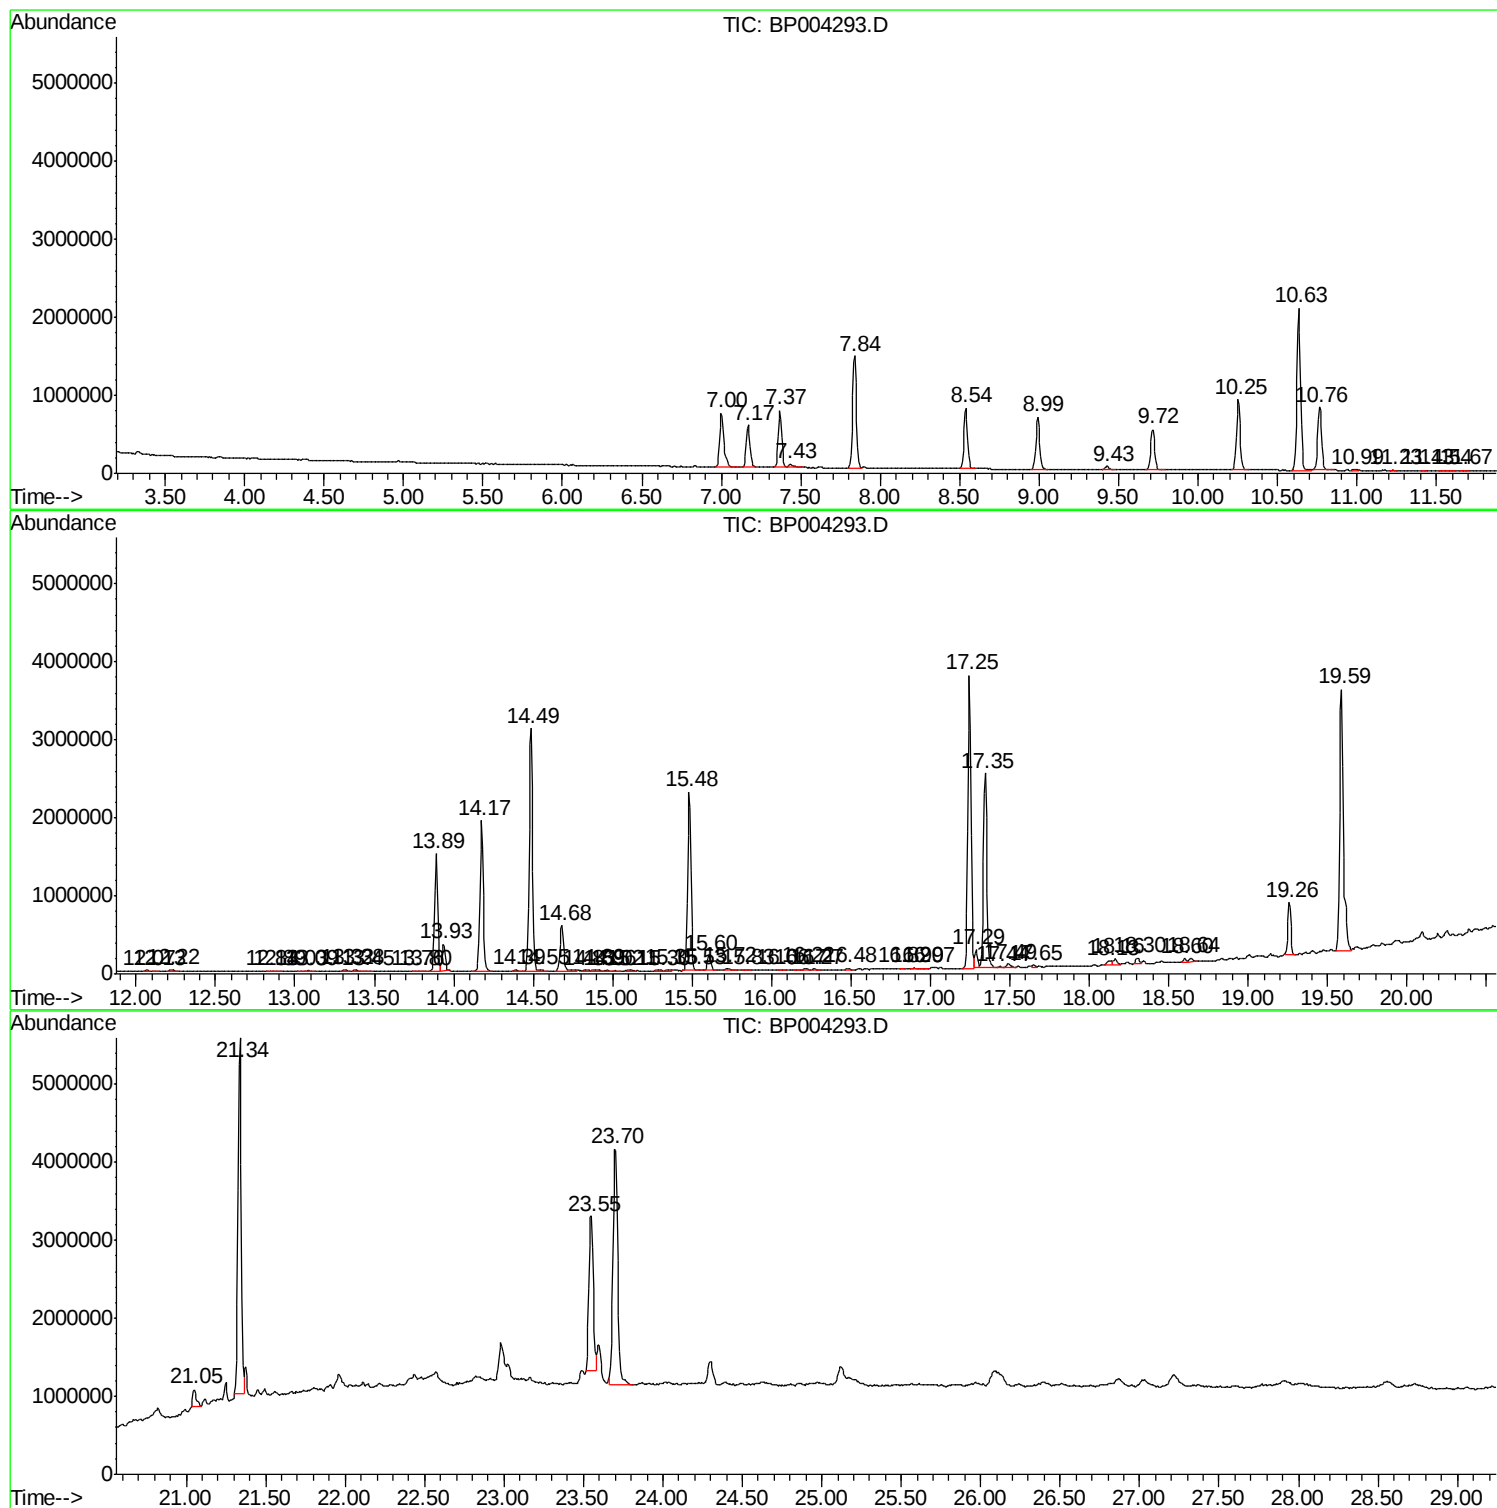

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121420\
Data File : BP004293.D
Acq On : 15 Dec 2020 02:32
Operator : CG/JU
Sample : L5001-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54D7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121420\
Data File : BP004293.D
Acq On : 15 Dec 2020 02:32
Operator : CG/JU
Sample : L5001-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54D7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc