

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
 Data File : BP004311.D
 Acq On : 15 Dec 2020 19:08
 Operator : CG/JU
 Sample : L5001-04
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54C2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.840	108	111	117	rVB	55025	74343	2.03%	0.217%
2	7.005	643	649	663	rVB	528642	961919	26.29%	2.807%
3	7.169	672	677	690	rVB	410006	655784	17.92%	1.914%
4	7.375	705	712	719	rBV	552873	894535	24.44%	2.610%
5	7.846	785	792	799	rVB	802486	1316569	35.98%	3.842%
6	8.546	904	911	924	rBV	646667	1060596	28.98%	3.095%
7	8.999	980	988	998	rBV	492802	834847	22.81%	2.436%
8	9.169	1013	1017	1023	rVB8	8192	12990	0.35%	0.038%
9	9.428	1056	1061	1067	rVB	18699	32036	0.88%	0.093%
10	9.722	1103	1111	1118	rBV	390200	683713	18.68%	1.995%
11	10.257	1196	1202	1217	rBV	654600	1137412	31.08%	3.319%
12	10.422	1226	1230	1234	rBV7	3724	5473	0.15%	0.016%
13	10.640	1257	1267	1276	rBV	1130411	1890605	51.66%	5.517%
14	10.769	1279	1289	1300	rBV	508335	895165	24.46%	2.612%
15	11.175	1355	1358	1363	rVV5	7454	9310	0.25%	0.027%
16	11.240	1363	1369	1373	rVB4	6518	11428	0.31%	0.033%
17	11.810	1460	1466	1471	rBV8	5634	13640	0.37%	0.040%
18	11.928	1481	1486	1491	rBV9	3340	6152	0.17%	0.018%
19	12.075	1505	1511	1512	rBV6	3646	5451	0.15%	0.016%
20	12.128	1515	1520	1525	rVB7	4937	10069	0.28%	0.029%
21	12.228	1525	1537	1541	rBV10	8809	24741	0.68%	0.072%
22	12.298	1548	1549	1555	rVB6	3966	6193	0.17%	0.018%
23	12.375	1555	1562	1568	rBV6	3662	9986	0.27%	0.029%
24	12.845	1638	1642	1648	rVB9	6439	10946	0.30%	0.032%
25	12.934	1653	1657	1662	rVB8	5438	7784	0.21%	0.023%
26	13.092	1680	1684	1689	rBV3	12061	19822	0.54%	0.058%
27	13.275	1710	1715	1720	rBV5	16009	21134	0.58%	0.062%
28	13.316	1720	1722	1727	rVB5	10992	14014	0.38%	0.041%
29	13.387	1729	1734	1740	rVV10	8445	13789	0.38%	0.040%
30	13.451	1742	1745	1750	rVB7	6636	10535	0.29%	0.031%
31	13.804	1802	1805	1810	rBV6	4265	7784	0.21%	0.023%
32	13.892	1814	1820	1825	rVV	1131059	1533128	41.90%	4.474%
33	13.939	1825	1828	1833	rVV	133635	182674	4.99%	0.533%
34	13.981	1833	1835	1839	rVB4	6149	5838	0.16%	0.017%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121420\
 Data File : BP004311.D
 Acq On : 15 Dec 2020 19:08
 Operator : CG/JU
 Sample : L5001-04
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A54C2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
 Title : SVOA CALIBRATION

35	14.016	1839	1841	1845	rBV5	5143	6969	0.19%	0.020%
36	14.181	1857	1869	1882	rBV	1409129	2108415	57.62%	6.152%
37	14.322	1890	1893	1901	rVB6	21446	35480	0.97%	0.104%
38	14.398	1901	1906	1910	rBV4	18242	29233	0.80%	0.085%
39	14.492	1912	1922	1928	rBV	1662069	2520948	68.89%	7.356%
40	14.687	1949	1955	1967	rBV	418762	672338	18.37%	1.962%
41	14.839	1975	1981	1986	rBV6	13818	29037	0.79%	0.085%
42	14.898	1988	1991	1998	rVB7	7093	14607	0.40%	0.043%
43	15.022	2009	2012	2015	rBV4	5585	7422	0.20%	0.022%
44	15.128	2026	2030	2031	rBV4	8057	9119	0.25%	0.027%
45	15.351	2065	2068	2071	rVB4	12730	11458	0.31%	0.033%
46	15.486	2083	2091	2098	rBV	1646509	2462668	67.30%	7.186%
47	15.545	2098	2101	2104	rVV4	13972	18944	0.52%	0.055%
48	15.616	2108	2113	2122	rBV	254194	384175	10.50%	1.121%
49	15.733	2127	2133	2135	rBV	18644	30984	0.85%	0.090%
50	16.181	2206	2209	2212	rBV3	16818	20725	0.57%	0.060%
51	16.239	2217	2219	2223	rVB	34010	41601	1.14%	0.121%
52	17.069	2357	2360	2370	rVB2	49269	86860	2.37%	0.253%
53	17.251	2385	2391	2396	rBV	2065573	2950465	80.63%	8.610%
54	17.292	2396	2398	2402	rVV	193488	238423	6.52%	0.696%
55	17.351	2402	2408	2420	rVB2	1800316	2681420	73.27%	7.824%
56	19.269	2730	2734	2739	rVB	768411	983690	26.88%	2.870%
57	19.592	2784	2789	2793	rBV	2347906	3659426	100.00%	10.678%
58	21.345	3083	3087	3091	rVB2	2252639	2884920	78.84%	8.418%


Sum of corrected areas: 34269732

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP121420\
Data File : BP004311.D
Acq On : 15 Dec 2020 19:08
Operator : CG/JU
Sample : L5001-04
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54C2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

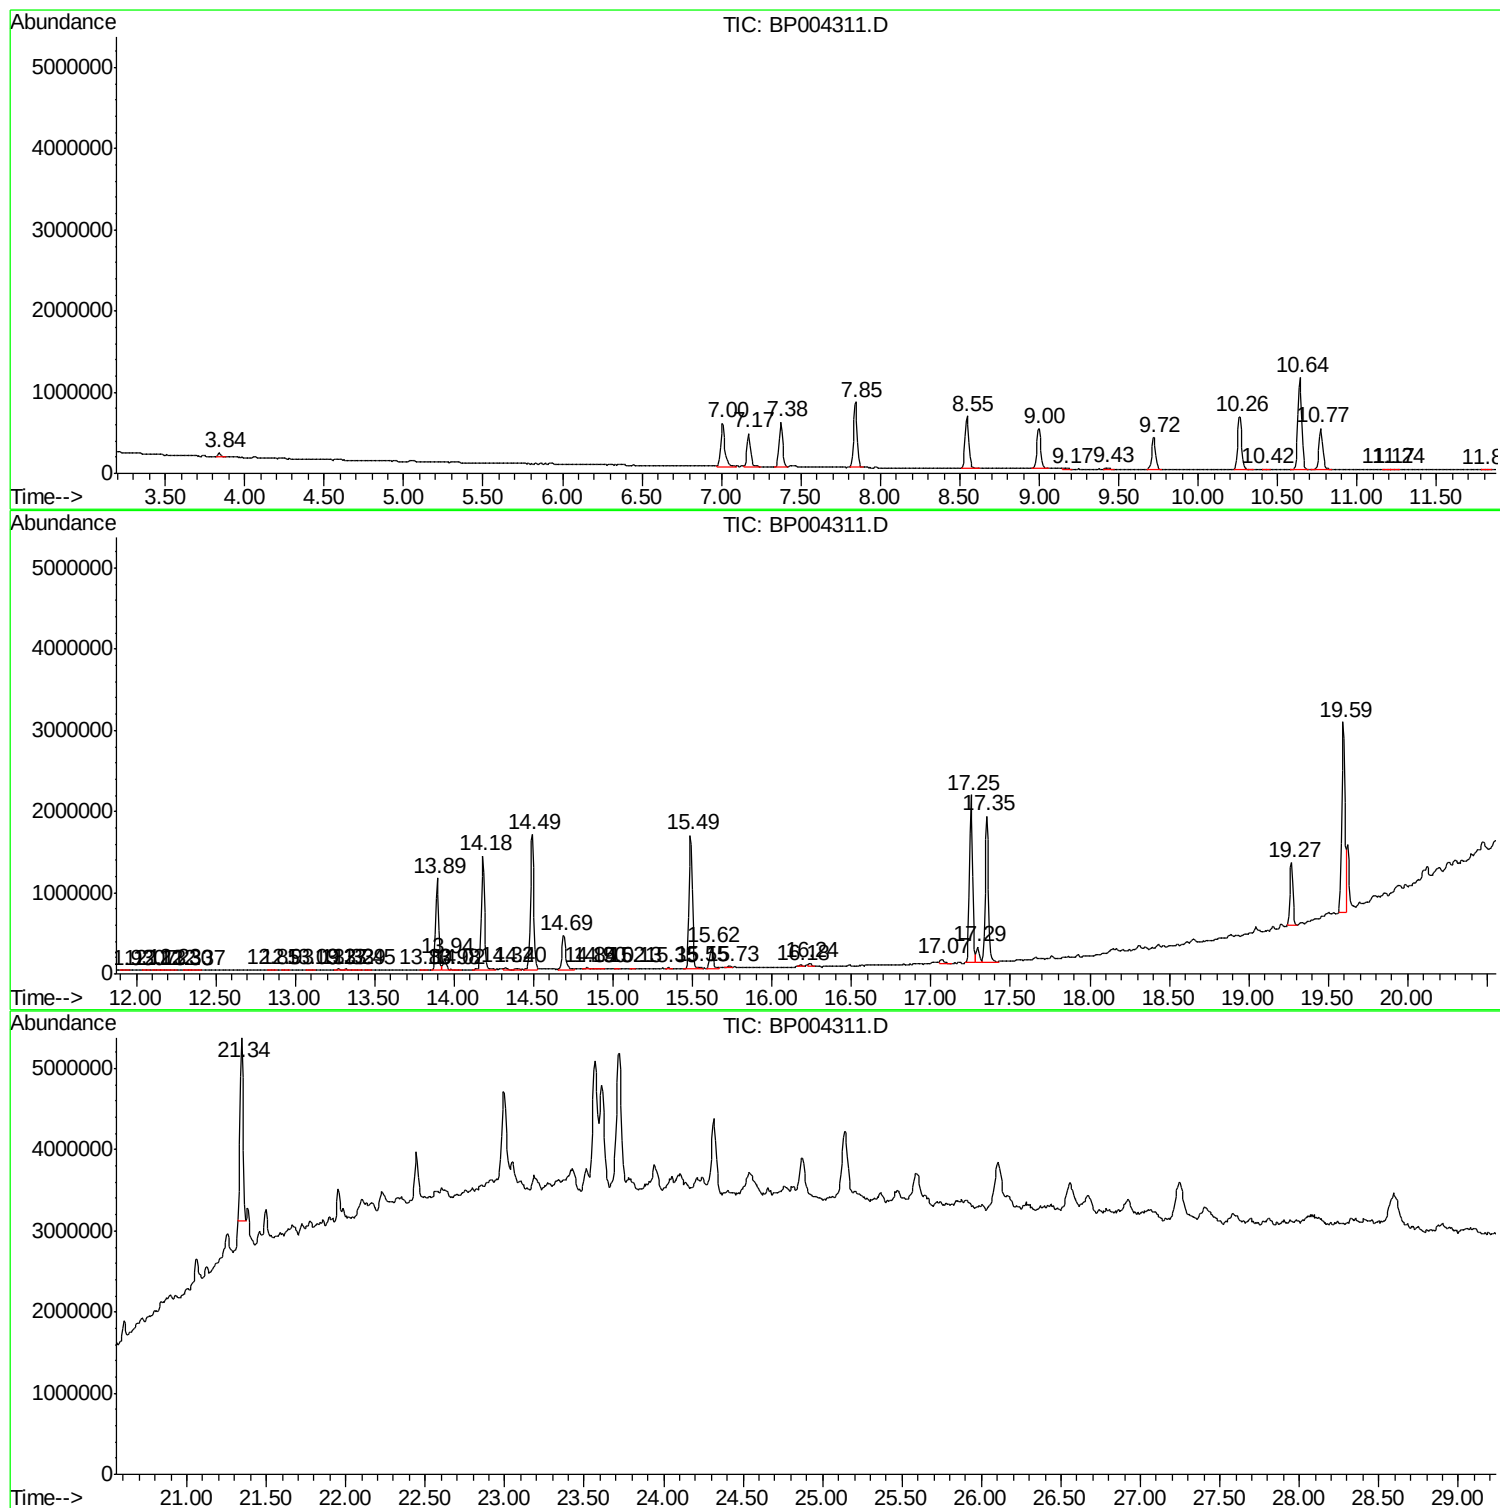

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121420\
Data File : BP004311.D
Acq On : 15 Dec 2020 19:08
Operator : CG/JU
Sample : L5001-04
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54C2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP121420\
Data File : BP004311.D
Acq On : 15 Dec 2020 19:08
Operator : CG/JU
Sample : L5001-04
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A54C2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP121020MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc