
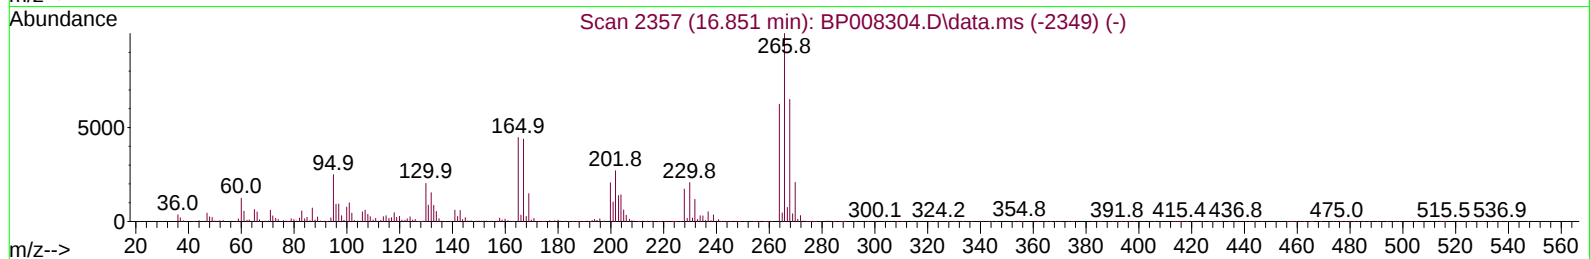
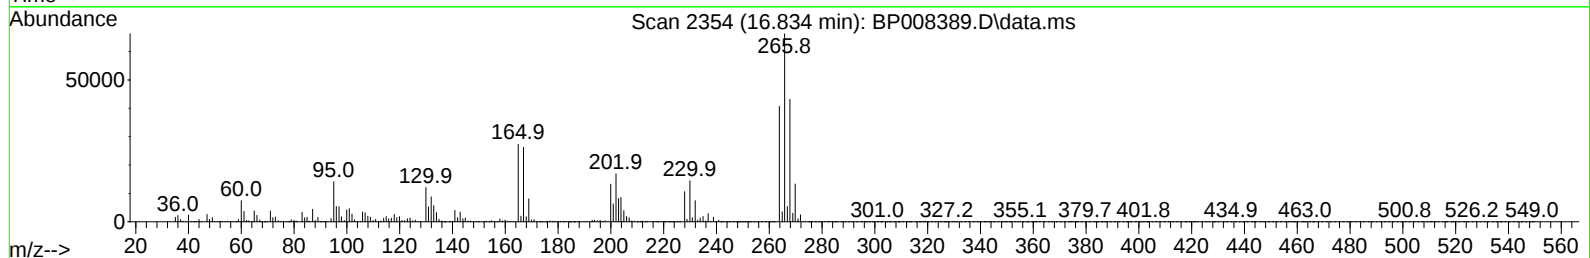


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121421\
Data File : BP008389.D
Acq On : 14 Dec 2021 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 14:41:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 14:37:17 2021
Response via : Initial Calibration

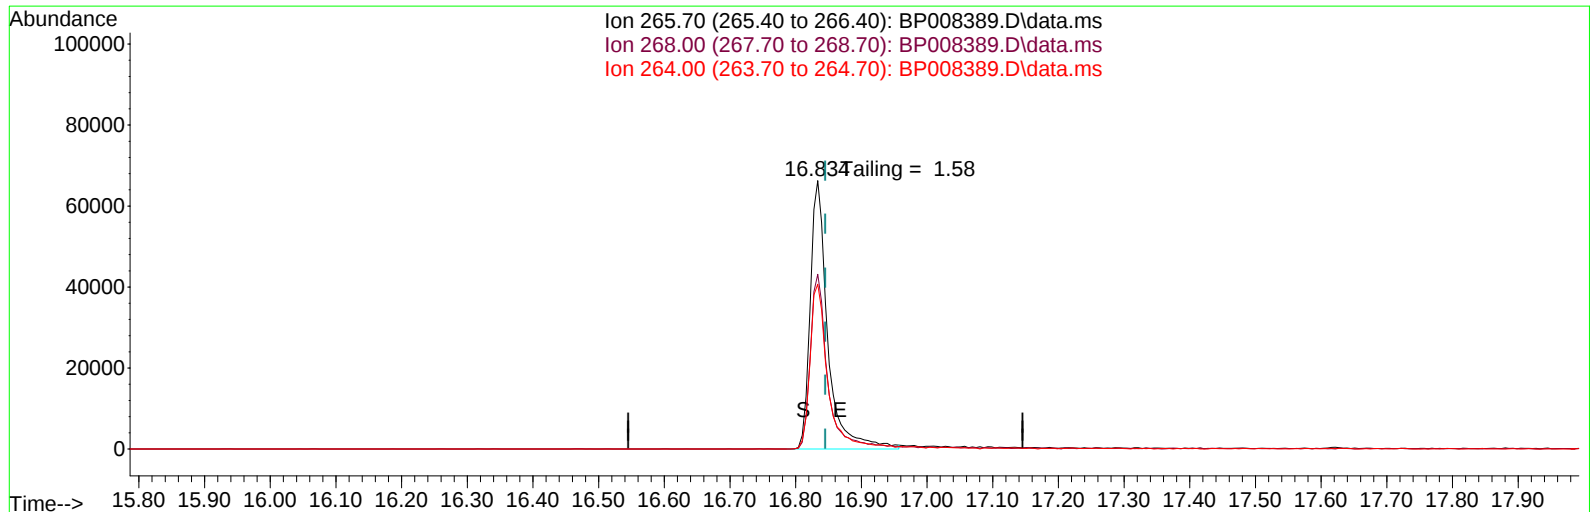

TIC: BP008389.D\data.ms

(70) Pentachlorophenol (C)




16.834min (-0.012) 189428.26 ng

response 124517

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	65.11
264.00	61.90	61.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121421\
 Data File : BP008389.D
 Acq On : 14 Dec 2021 11:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 14 14:41:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 14:37:17 2021
 Response via : Initial Calibration

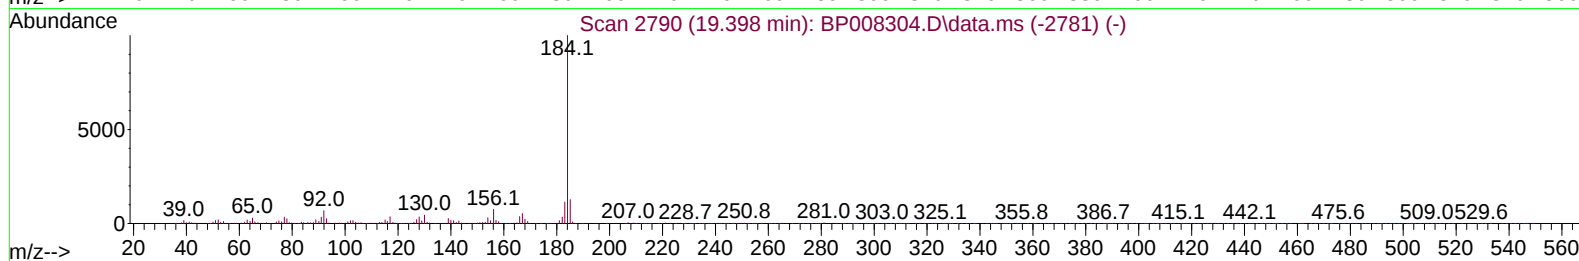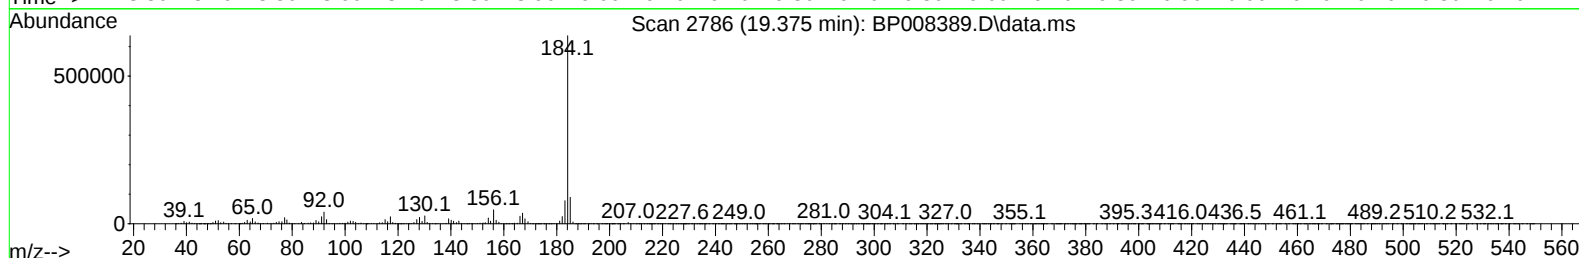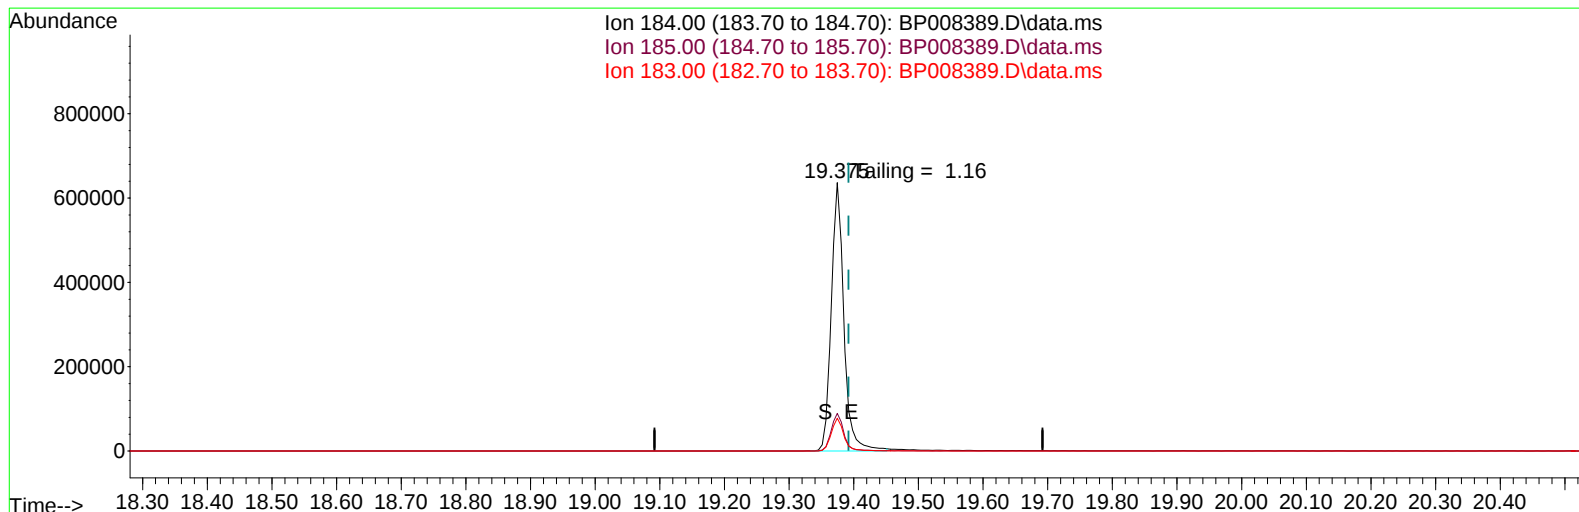

TIC: BP008389.D\data.ms

(77) Benzidine**19.375min (-0.018) 786671.81 ng****response 874067**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.05
183.00	11.40	12.24
0.00	0.00	0.00