

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121421\
 Data File : BP008405.D
 Acq On : 14 Dec 2021 21:55
 Operator : CG/JU
 Sample : M5076-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-20-G

Quant Time: Dec 15 02:00:44 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 17:59:47 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.746	152	62273	20.000	ng	0.00
21) Naphthalene-d8	10.540	136	233547	20.000	ng	0.00
39) Acenaphthene-d10	14.398	164	145605	20.000	ng	0.00
64) Phenanthrene-d10	17.163	188	262441	20.000	ng	# 0.00
76) Chrysene-d12	21.269	240	261410	20.000	ng	# 0.00
86) Perylene-d12	23.633	264	311750	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.346	112	501234	127.113	ng	0.00
7) Phenol-d6	6.940	99	652120	123.134	ng	0.00
23) Nitrobenzene-d5	8.911	82	437924	79.438	ng	0.00
42) 2,4,6-Tribromophenol	15.898	330	244496	114.262	ng	0.00
45) 2-Fluorobiphenyl	13.016	172	918140	80.158	ng	0.00
79) Terphenyl-d14	19.733	244	1090220	72.583	ng	0.00
Target Compounds						
10) Phenol	6.969	94	13723	2.552	ng	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121421\
Data File : BP008405.D
Acq On : 14 Dec 2021 21:55
Operator : CG/JU
Sample : M5076-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-20-G

Quant Time: Dec 15 02:00:44 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 17:59:47 2021
Response via : Initial Calibration




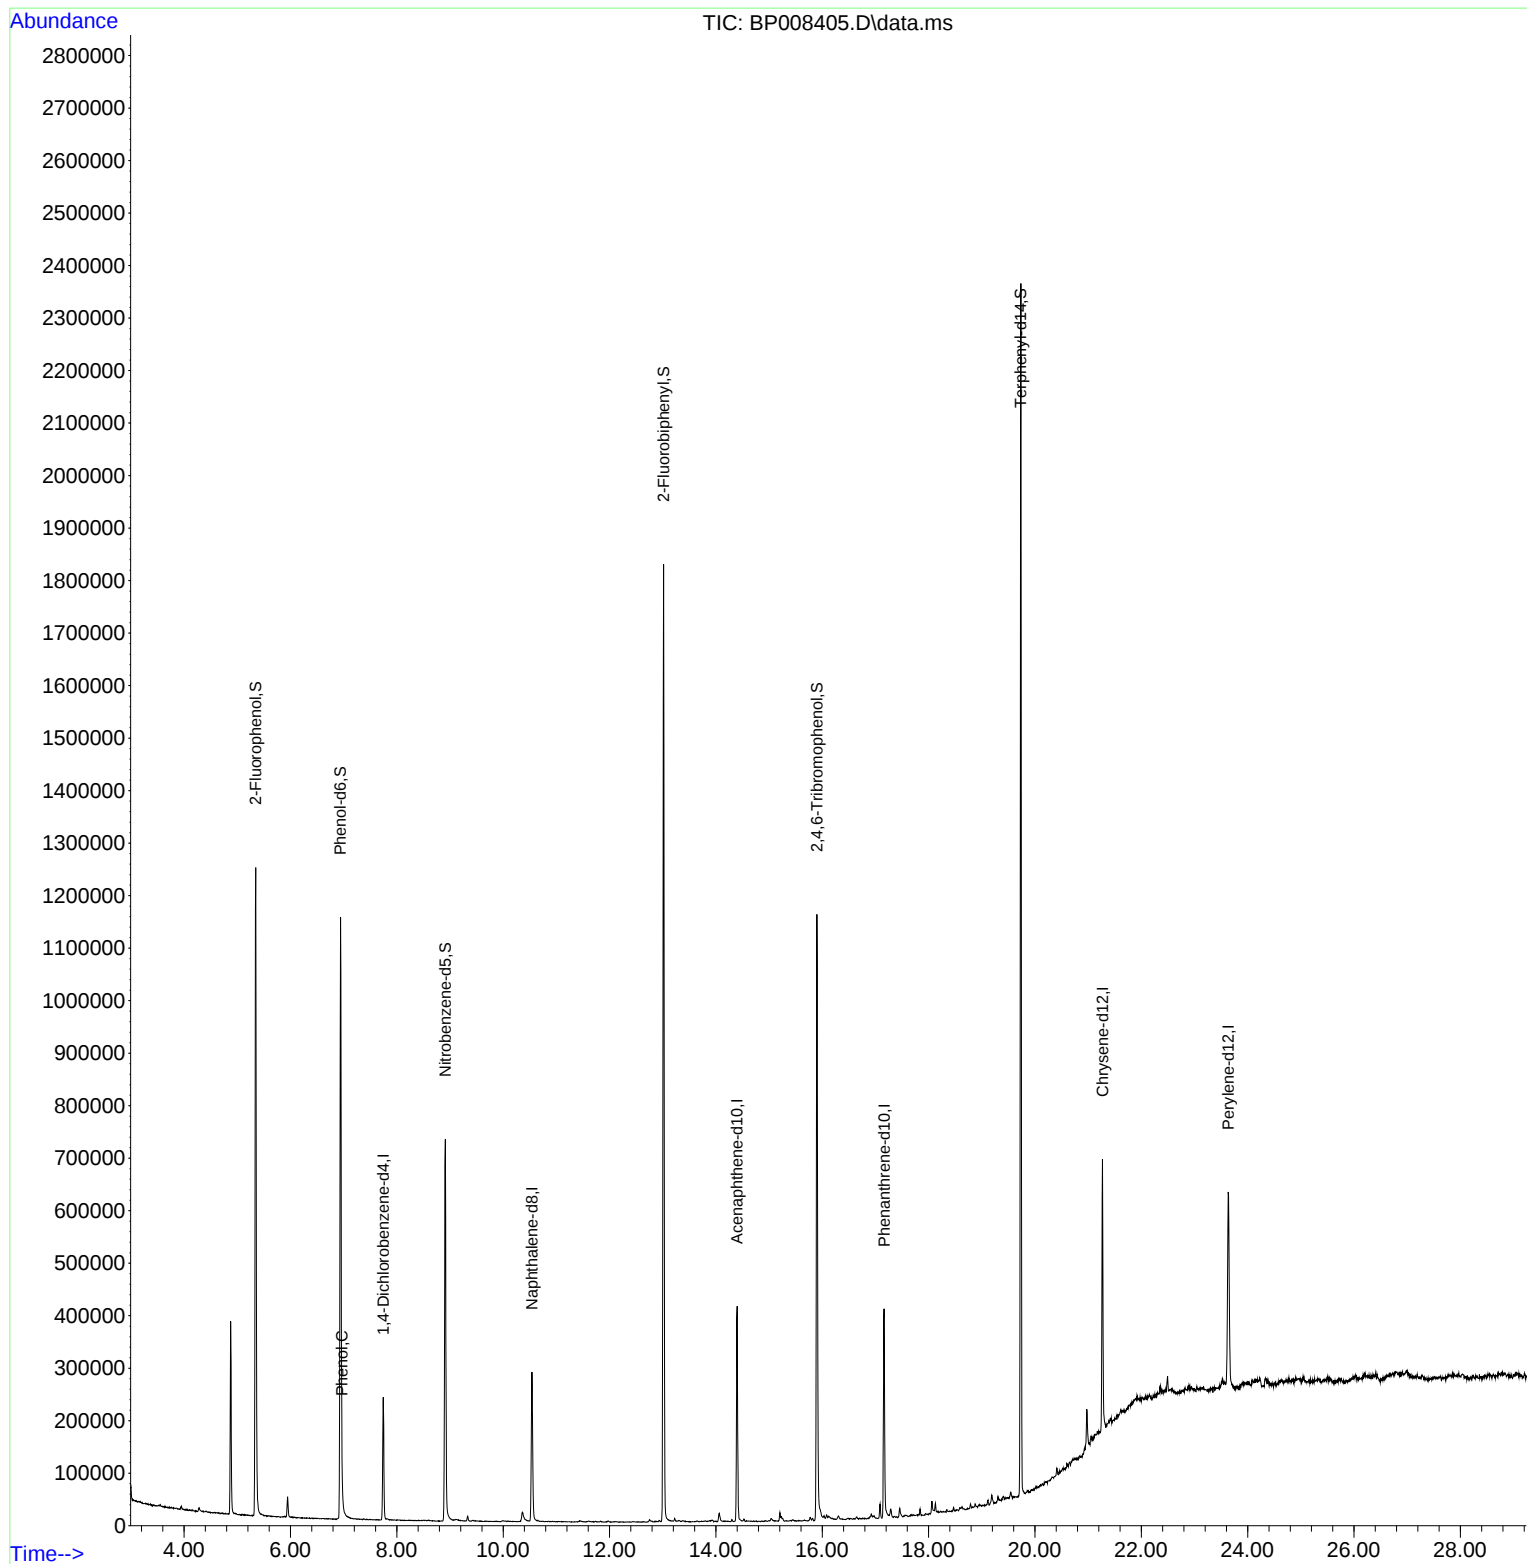




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.746 min Scan# 809
Delta R.T. -0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55




Instrument :
BNA_P
ClientSampleId :
SB-20-G


Tgt Ion:152 Resp: 62273
Ion Ratio Lower Upper
152 100
150 151.7 125.7 188.5
115 59.0 50.7 76.1

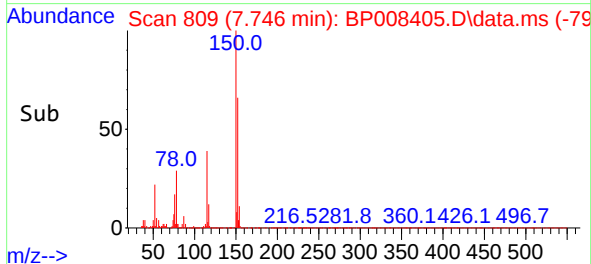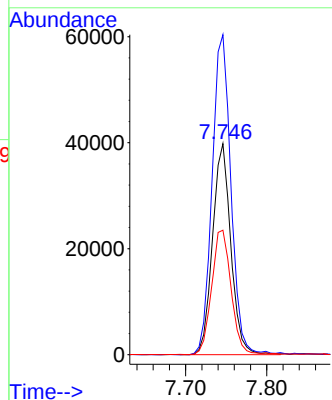

#5
2-Fluorophenol
Concen: 127.113 ng
RT: 5.346 min Scan# 401
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55

Tgt Ion:112 Resp: 501234
Ion Ratio Lower Upper
112 100
64 62.4 53.4 80.2
63 32.7 27.8 41.8


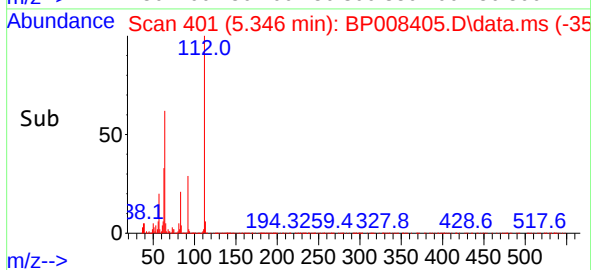
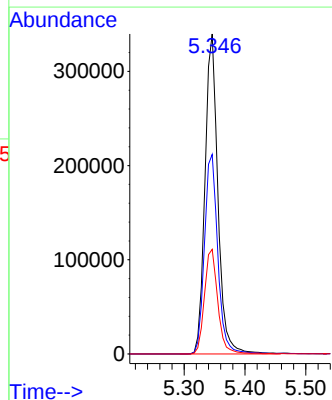
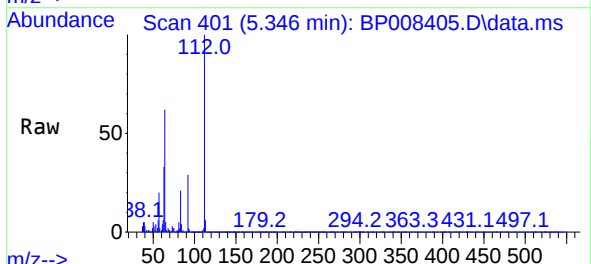


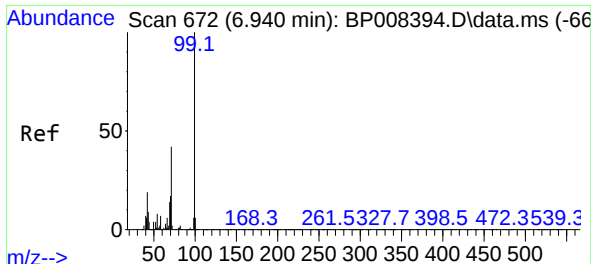

#7
Phenol-d6
Concen: 123.134 ng
RT: 6.940 min Scan# 672
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55




Instrument :
BNA_P
ClientSampleId :
SB-20-G


Tgt Ion: 99 Resp: 652120
Ion Ratio Lower Upper
99 100
42 18.1 14.6 22.0
71 41.6 31.1 46.7

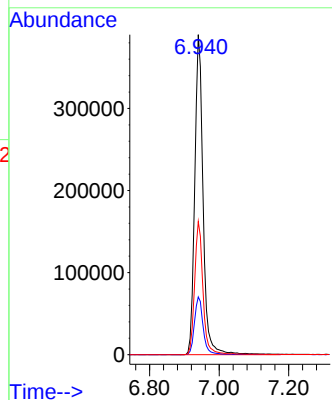

#10
Phenol
Concen: 2.552 ng
RT: 6.969 min Scan# 677
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55

Tgt Ion: 94 Resp: 13723
Ion Ratio Lower Upper
94 100
65 36.5 10.9 50.9
66 64.7 24.3 64.3#


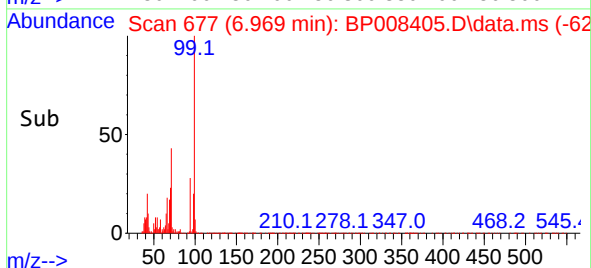
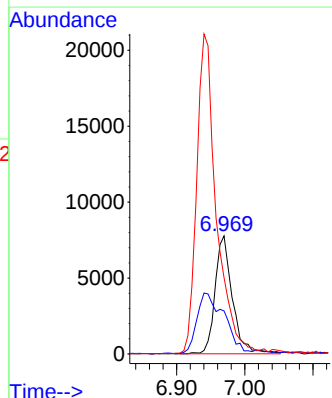
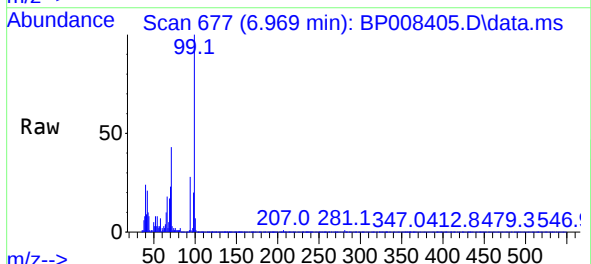


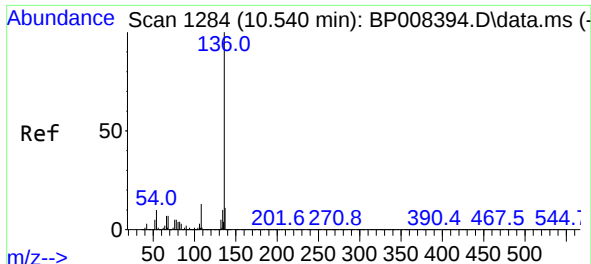

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.540 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55




Instrument :
BNA_P
ClientSampleId :
SB-20-G


Tgt Ion:	136	Resp:	233547
Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.0	13.6
54	9.7	8.2	12.4
68	6.5	5.8	8.8

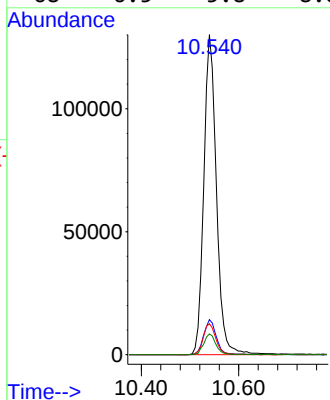

#23
Nitrobenzene-d5
Concen: 79.438 ng
RT: 8.911 min Scan# 1007
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55

Tgt Ion:	82	Resp:	437924
Ion	Ratio	Lower	Upper
82	100		
128	39.6	29.6	44.4
54	53.4	42.7	64.1


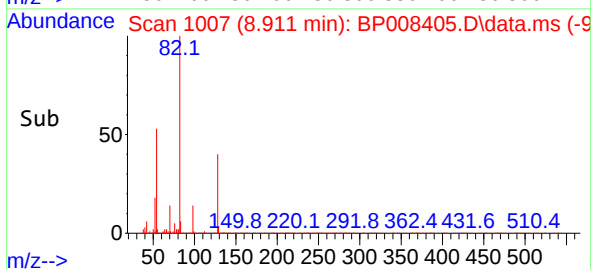
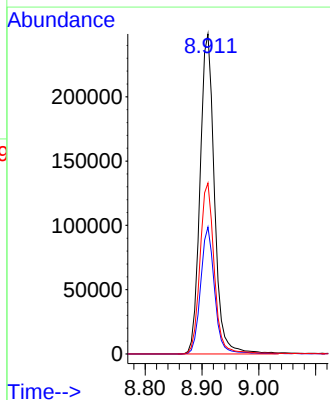
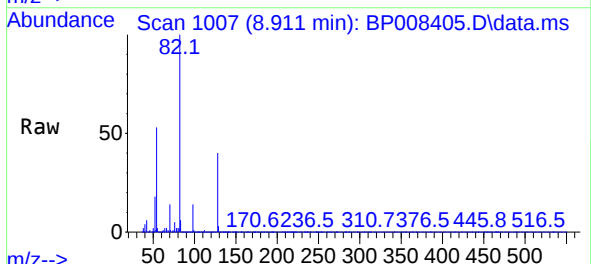


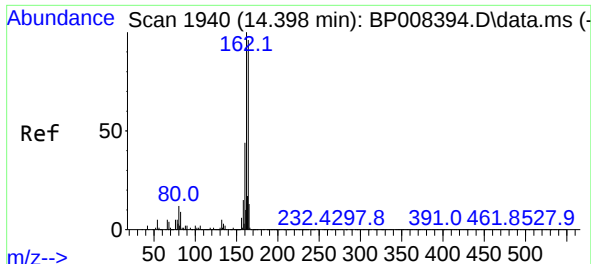

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.398 min Scan# 1940
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55




Instrument :
BNA_P
ClientSampleId :
SB-20-G


Tgt Ion:164 Resp: 145605
Ion Ratio Lower Upper
164 100
162 101.1 81.9 122.9
160 43.1 35.4 53.0

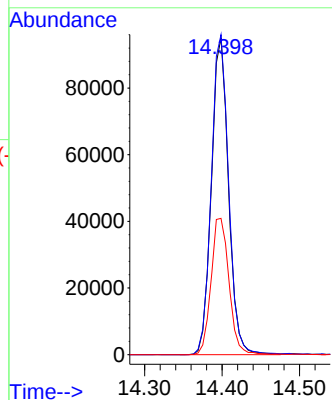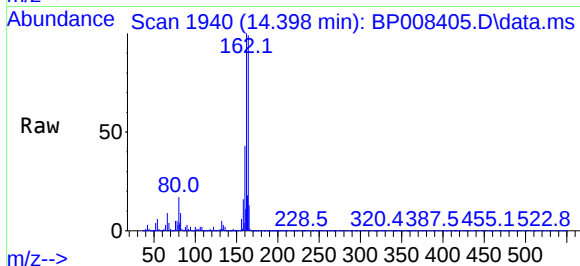

#42
2,4,6-Tribromophenol
Concen: 114.262 ng
RT: 15.898 min Scan# 2195
Delta R.T. -0.006 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55

Tgt Ion:330 Resp: 244496
Ion Ratio Lower Upper
330 100
332 96.2 77.0 115.4
141 30.1 28.4 42.6


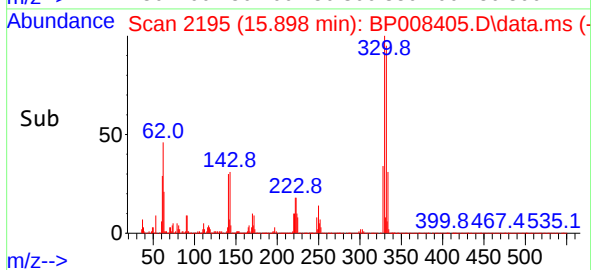
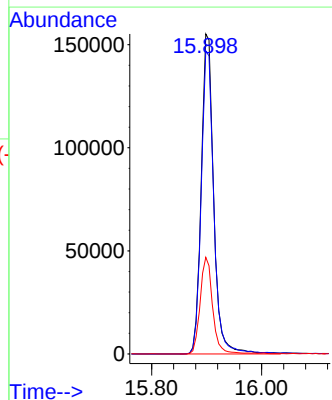
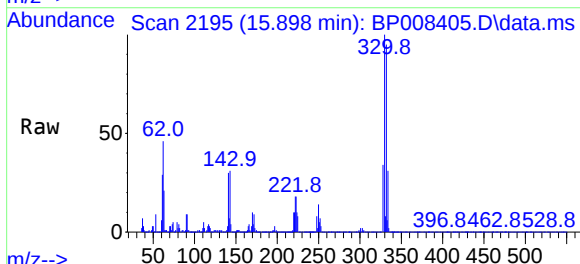


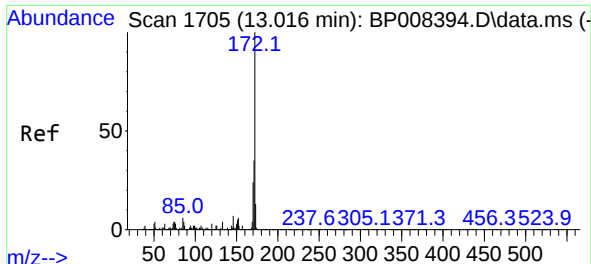

#45
2-Fluorobiphenyl
Concen: 80.158 ng
RT: 13.016 min Scan# 1705
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55




Instrument :
BNA_P
ClientSampleId :
SB-20-G


Tgt Ion:172 Resp: 918140
Ion Ratio Lower Upper
172 100
171 34.9 28.0 42.0
170 23.2 18.9 28.3

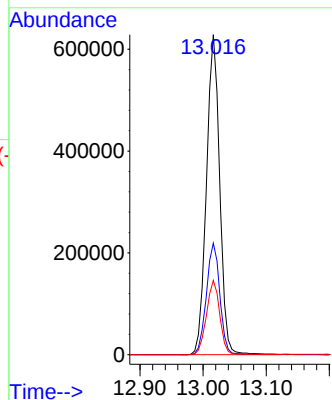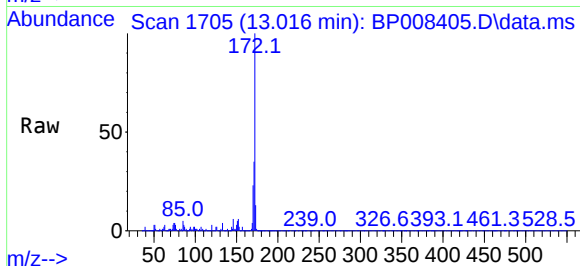

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.163 min Scan# 2410
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55

Tgt Ion:188 Resp: 262441
Ion Ratio Lower Upper
188 100
94 7.1 7.2 10.8#
80 9.1 8.2 12.4


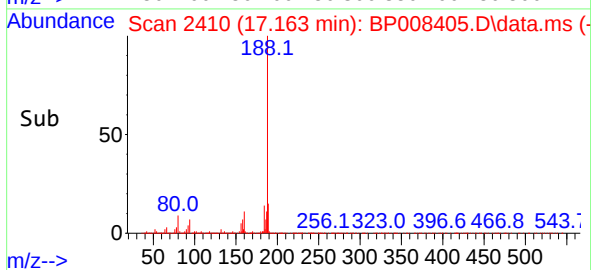
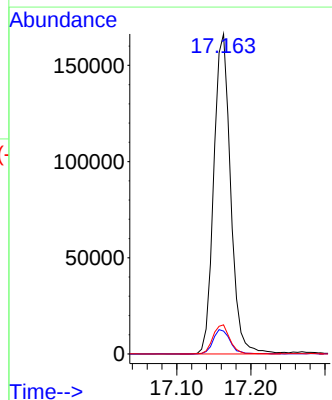
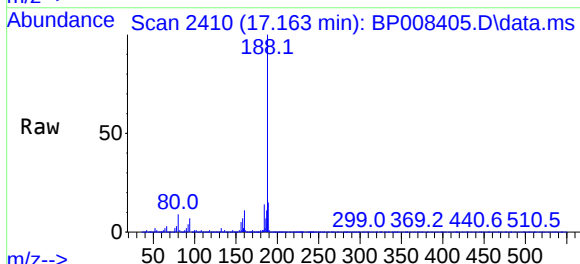




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.269 min Scan# 3108
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55




Instrument :
BNA_P
ClientSampleId :
SB-20-G


Tgt Ion:240 Resp: 261410
Ion Ratio Lower Upper
240 100
120 6.8 7.3 10.9#
236 25.6 21.4 32.2

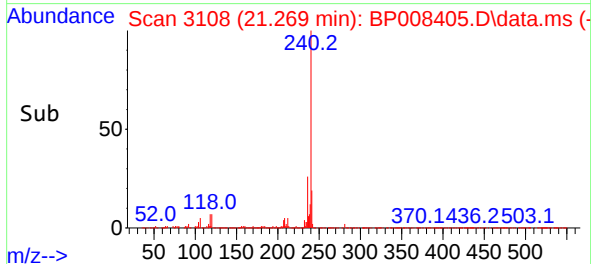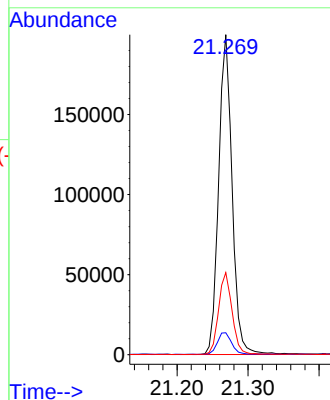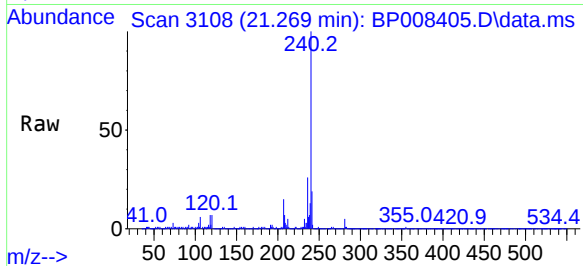

#79
Terphenyl-d14
Concen: 72.583 ng
RT: 19.733 min Scan# 2847
Delta R.T. 0.000 min
Lab File: BP008405.D
Acq: 14 Dec 2021 21:55


Tgt Ion:244 Resp: 1090220
Ion Ratio Lower Upper
244 100
212 7.4 6.0 9.0
122 7.3 6.6 9.8

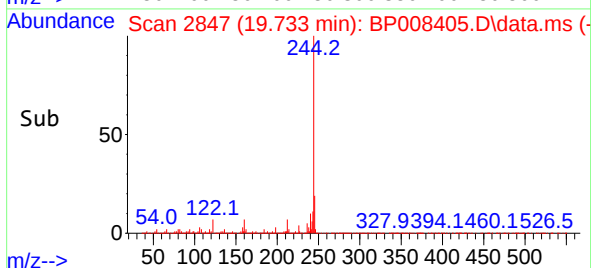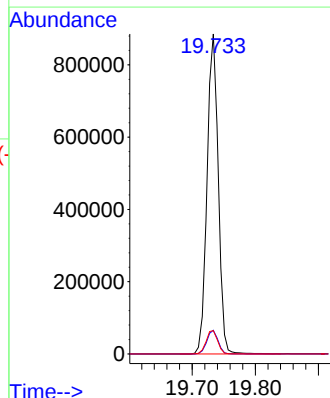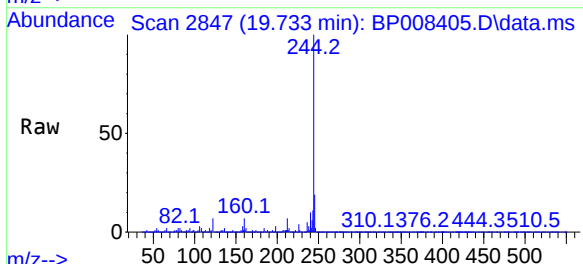



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.633 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BP008405.D
 Acq: 14 Dec 2021 21:55

Instrument :
 BNA_P
 ClientSampleId :
 SB-20-G



Tgt Ion:264 Resp: 311750
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.4 29.2
 265 22.3 17.6 26.4

