


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121421\
 Data File : BP008389.D
 Acq On : 14 Dec 2021 11:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 14 17:59:47 2021

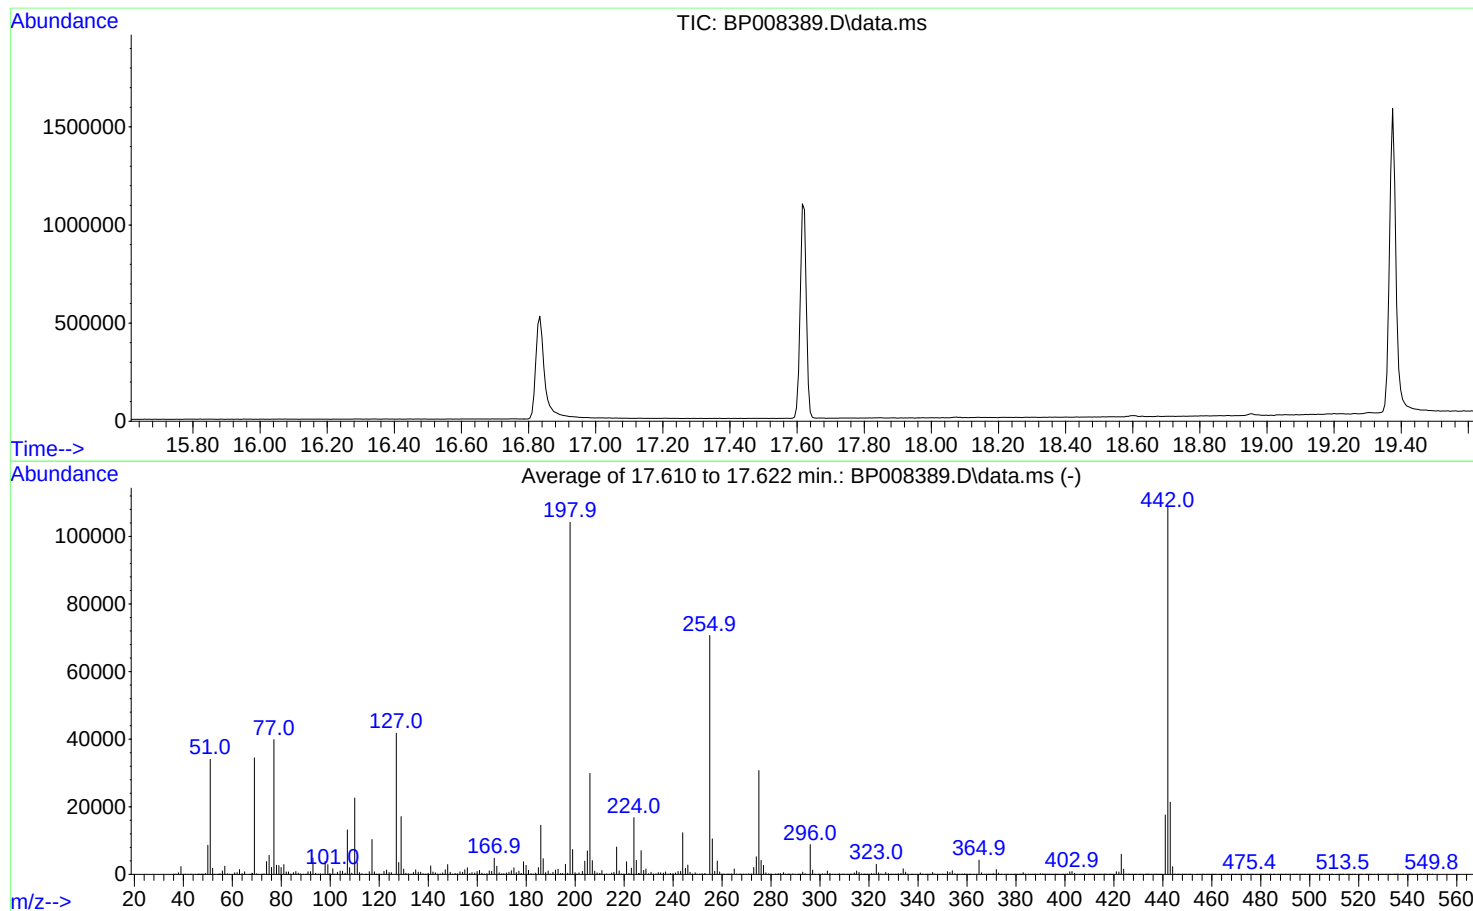


AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	34044	PASS
68	69	0.00	2	1.1	381	PASS
69	198	0.00	100	33.1	34462	PASS
70	69	0.00	2	0.6	206	PASS
127	198	10	80	40.1	41743	PASS
197	198	0.00	2	0.3	328	PASS
198	198	100	100	100.0	104197	PASS
199	198	5	9	7.0	7333	PASS
275	198	10	60	29.5	30720	PASS
365	198	1	100	4.1	4221	PASS
441	198	0.01	100	16.9	17577	PASS
442	442	100	100	100.0	108860	PASS
443	442	15	24	19.6	21372	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121421\
Data File : BP008389.D
Acq On : 14 Dec 2021 11:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 14 14:41:31 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 14 14:37:17 2021
Response via : Initial Calibration

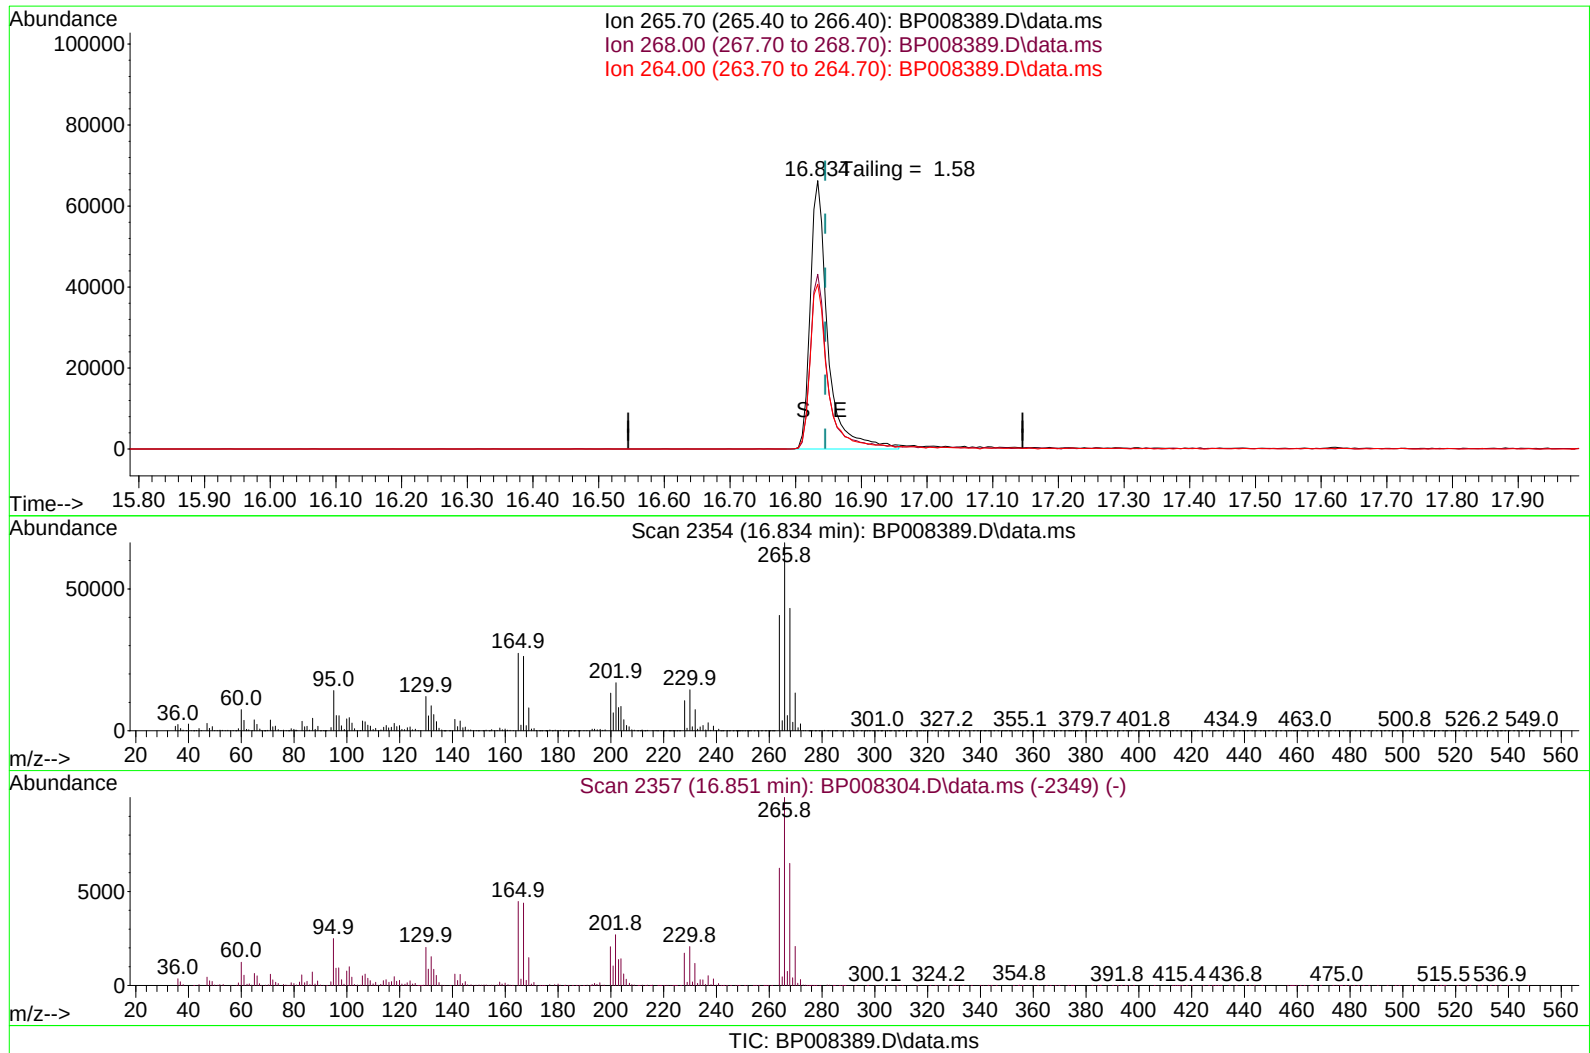

(70) Pentachlorophenol (C)

16.834min (-0.012) 189428.26 ng




response 124517

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	65.11
264.00	61.90	61.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121421\
 Data File : BP008389.D
 Acq On : 14 Dec 2021 11:24
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 14 14:41:31 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP121421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 14 14:37:17 2021
 Response via : Initial Calibration

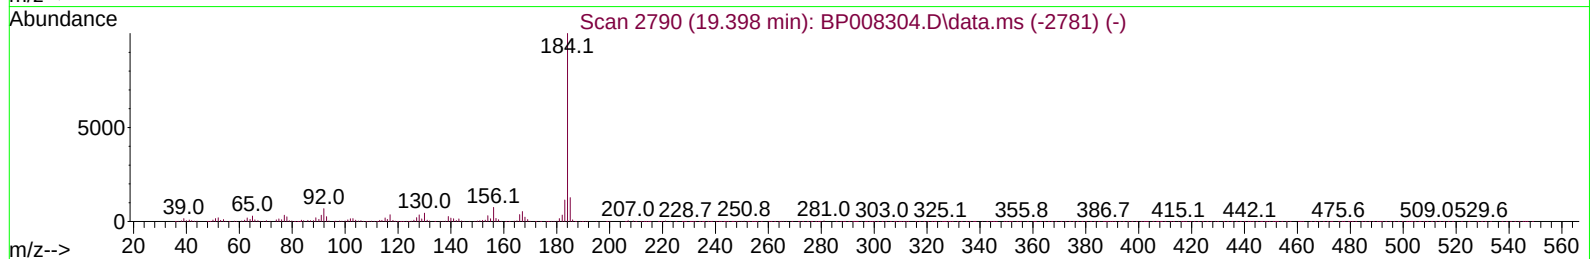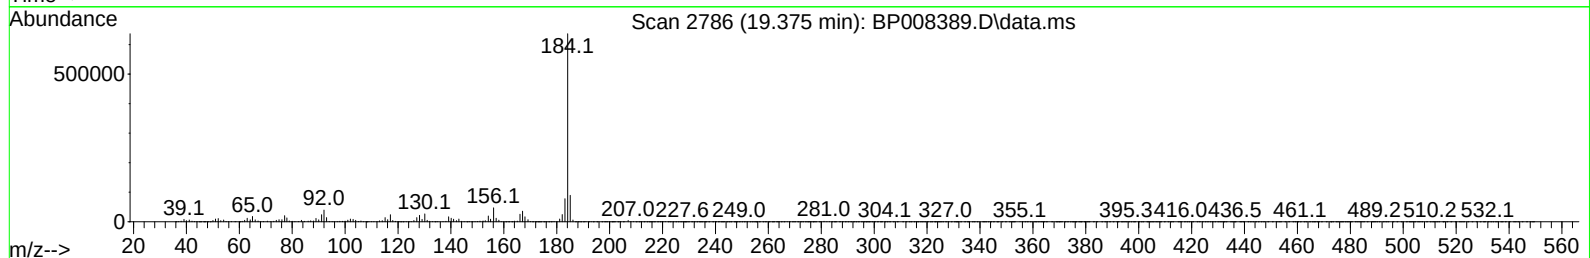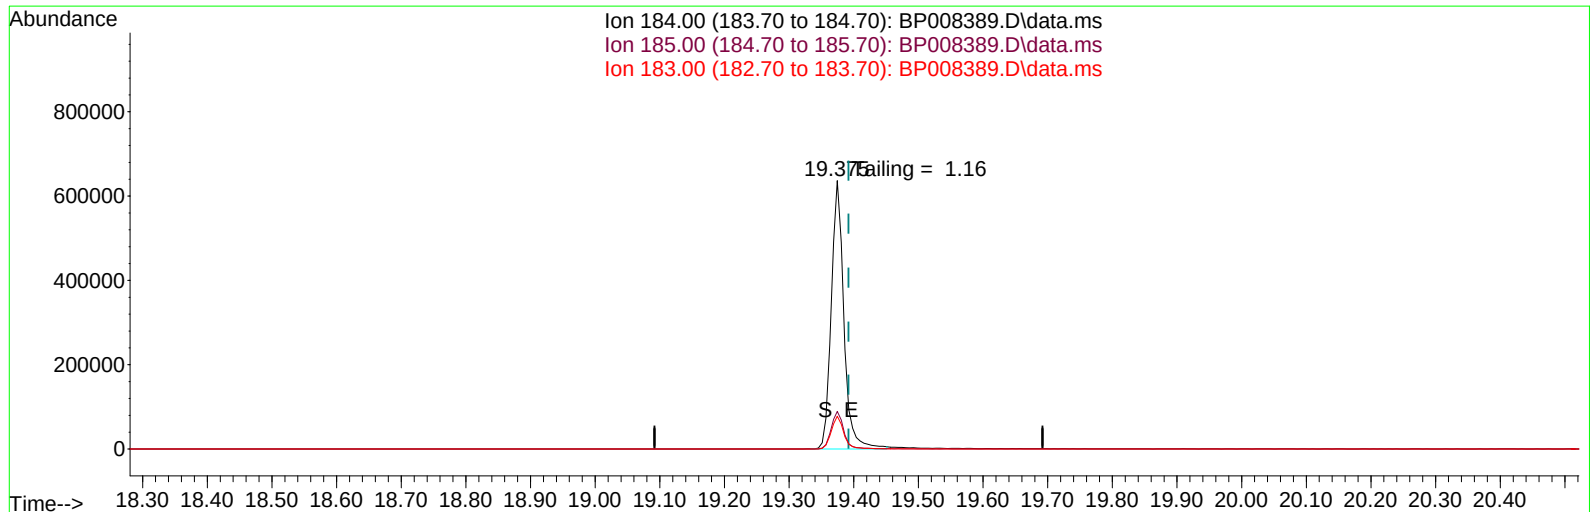

TIC: BP008389.D\data.ms

(77) Benzidine

19.375min (-0.018) 786671.81 ng

response 874067

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	14.05
183.00	11.40	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/14/2021	BNA_P	BP008389.D
Compound Name	Response	Retention Time
DDT	425743	20.57
DDD	5619	20.15
DDE	971	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6590	432333	1.52