

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018891.D
 Acq On : 15 Dec 2023 21:44
 Operator : MA/JU
 Sample : 05627-14DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC6DL

Quant Time: Dec 15 23:25:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	304651	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	1130776	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	613599	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	1245147	20.000	ng/ul	-0.01
79) Chrysene-d12	21.292	240	1271152	20.000	ng/ul	-0.01
88) Perylene-d12	23.651	264	1531978	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	7974	0.892	ng/uL	0.00
4) Pyridine-d5	3.687	84	36502	1.524	ng/ul	0.01
7) Phenol-d5	6.999	99	38119	1.247	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.164	67	100616	5.553	ng/ul	0.00
11) 2-Chlorophenol-d4	7.358	132	96451	4.043	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	63443	2.564	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	48200	4.789	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	39367	3.773	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	97868	4.587	ng/ul	0.00
31) 4-Chloroaniline-d4	10.769	131	101387	3.636	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	355407	6.490	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	363867	6.034	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	6644	0.739	ng/ul	0.01
60) Fluorene-d10	15.451	176	317326	6.903	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	21027	2.816	ng/ul	-0.01
73) Anthracene-d10	17.304	188	484208	7.397	ng/ul	0.00
81) Pyrene-d10	19.539	212	593091	5.994	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.498	264	627722	7.027	ng/ul	-0.02
Target Compounds						
78) Di-n-butylphthalate	18.169	149	4131556	51.647	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018891.D
Acq On : 15 Dec 2023 21:44
Operator : MA/JU
Sample : 05627-14DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC6DL


Quant Time: Dec 15 23:25:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

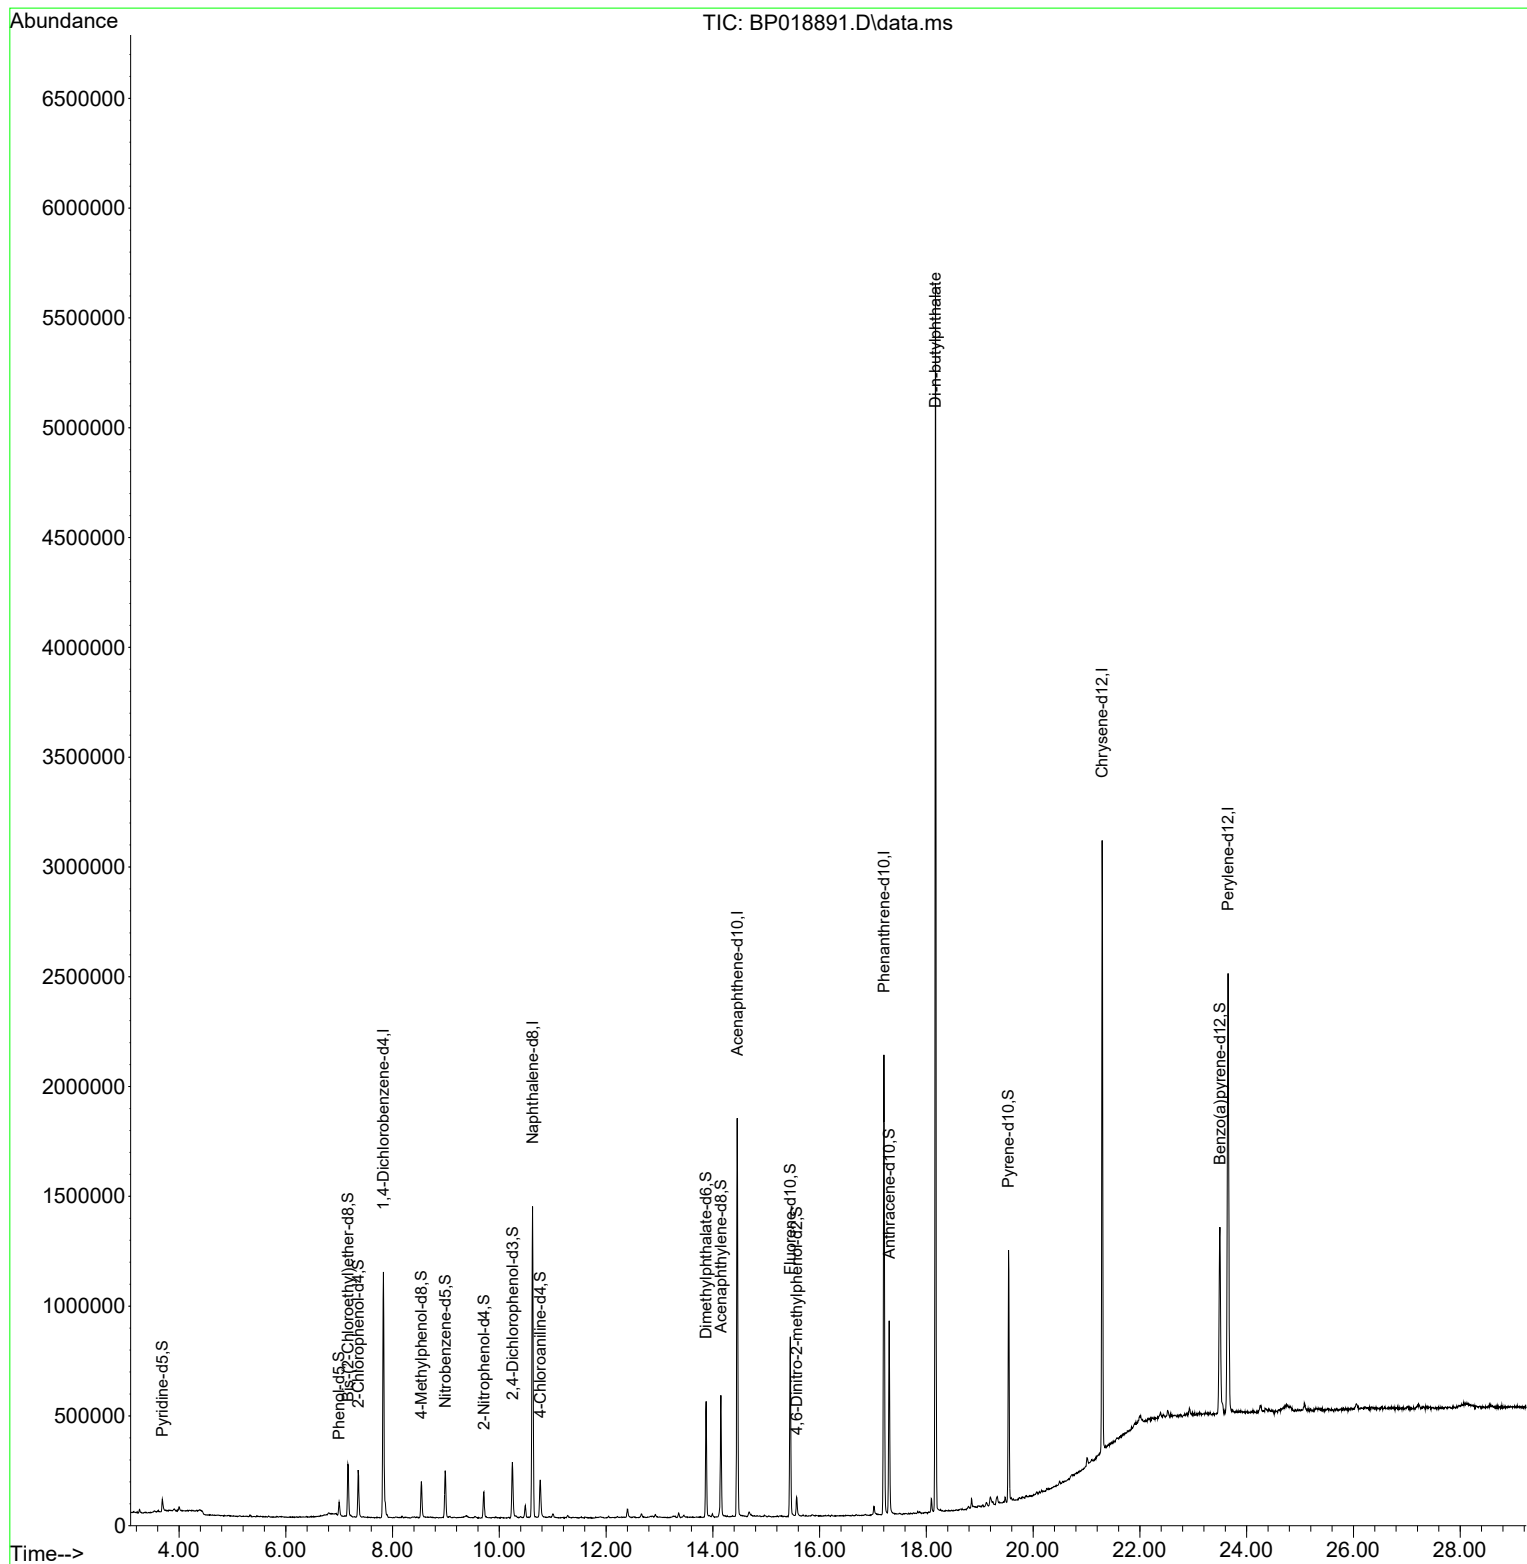

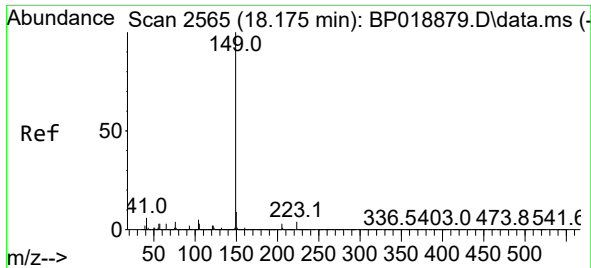

#78
 Di-n-butylphthalate
 Concen: 51.647 ng/ul
 RT: 18.169 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP018891.D
 Acq: 15 Dec 2023 21:44

Instrument :
 BNA_P
 ClientSampleId :
 DCLC6DL

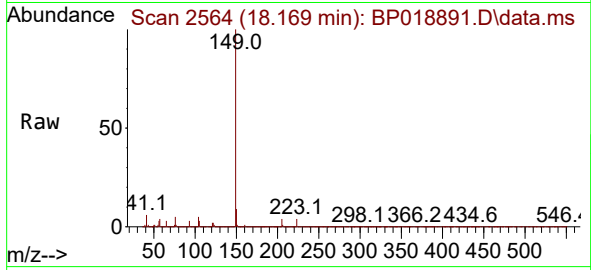

Tgt Ion:149 Resp: 4131556
 Ion Ratio Lower Upper
 149 100
 150 9.5 7.4 11.2
 104 5.0 3.9 5.9

