

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018892.D
 Acq On : 15 Dec 2023 22:18
 Operator : MA/JU
 Sample : 05627-15DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC7DL

Quant Time: Dec 15 23:25:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 13 23:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.828	152	268904	20.000	ng/ul	0.00
20) Naphthalene-d8	10.622	136	977187	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	558865	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	1290388	20.000	ng/ul	-0.01
79) Chrysene-d12	21.292	240	1397576	20.000	ng/ul	-0.01
88) Perylene-d12	23.651	264	1627244	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	6176	0.783	ng/uL	0.00
4) Pyridine-d5	3.687	84	35177	1.664	ng/ul	0.01
7) Phenol-d5	6.999	99	35376	1.311	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.163	67	91121	5.697	ng/ul	0.00
11) 2-Chlorophenol-d4	7.358	132	89382	4.245	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	56215	2.574	ng/ul	0.00
21) Nitrobenzene-d5	8.987	128	43815	5.038	ng/ul	0.00
24) 2-Nitrophenol-d4	9.710	143	35709	3.960	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.246	165	86918	4.714	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	94885	3.938	ng/ul	0.00
46) Dimethylphthalate-d6	13.875	166	309144	6.198	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	334425	6.089	ng/ul	0.00
54) 4-Nitrophenol-d4	14.675	143	5722	0.699	ng/ul	0.00
60) Fluorene-d10	15.451	176	290289	6.933	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.569	200	22353	2.889	ng/ul	-0.01
73) Anthracene-d10	17.304	188	505166	7.447	ng/ul	0.00
81) Pyrene-d10	19.539	212	669994	6.159	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.498	264	679880	7.166	ng/ul	-0.02
Target Compounds						
78) Di-n-butylphthalate	18.169	149	3147388	37.965	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018892.D
Acq On : 15 Dec 2023 22:18
Operator : MA/JU
Sample : 05627-15DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC7DL

Quant Time: Dec 15 23:25:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 13 23:34:47 2023
Response via : Initial Calibration

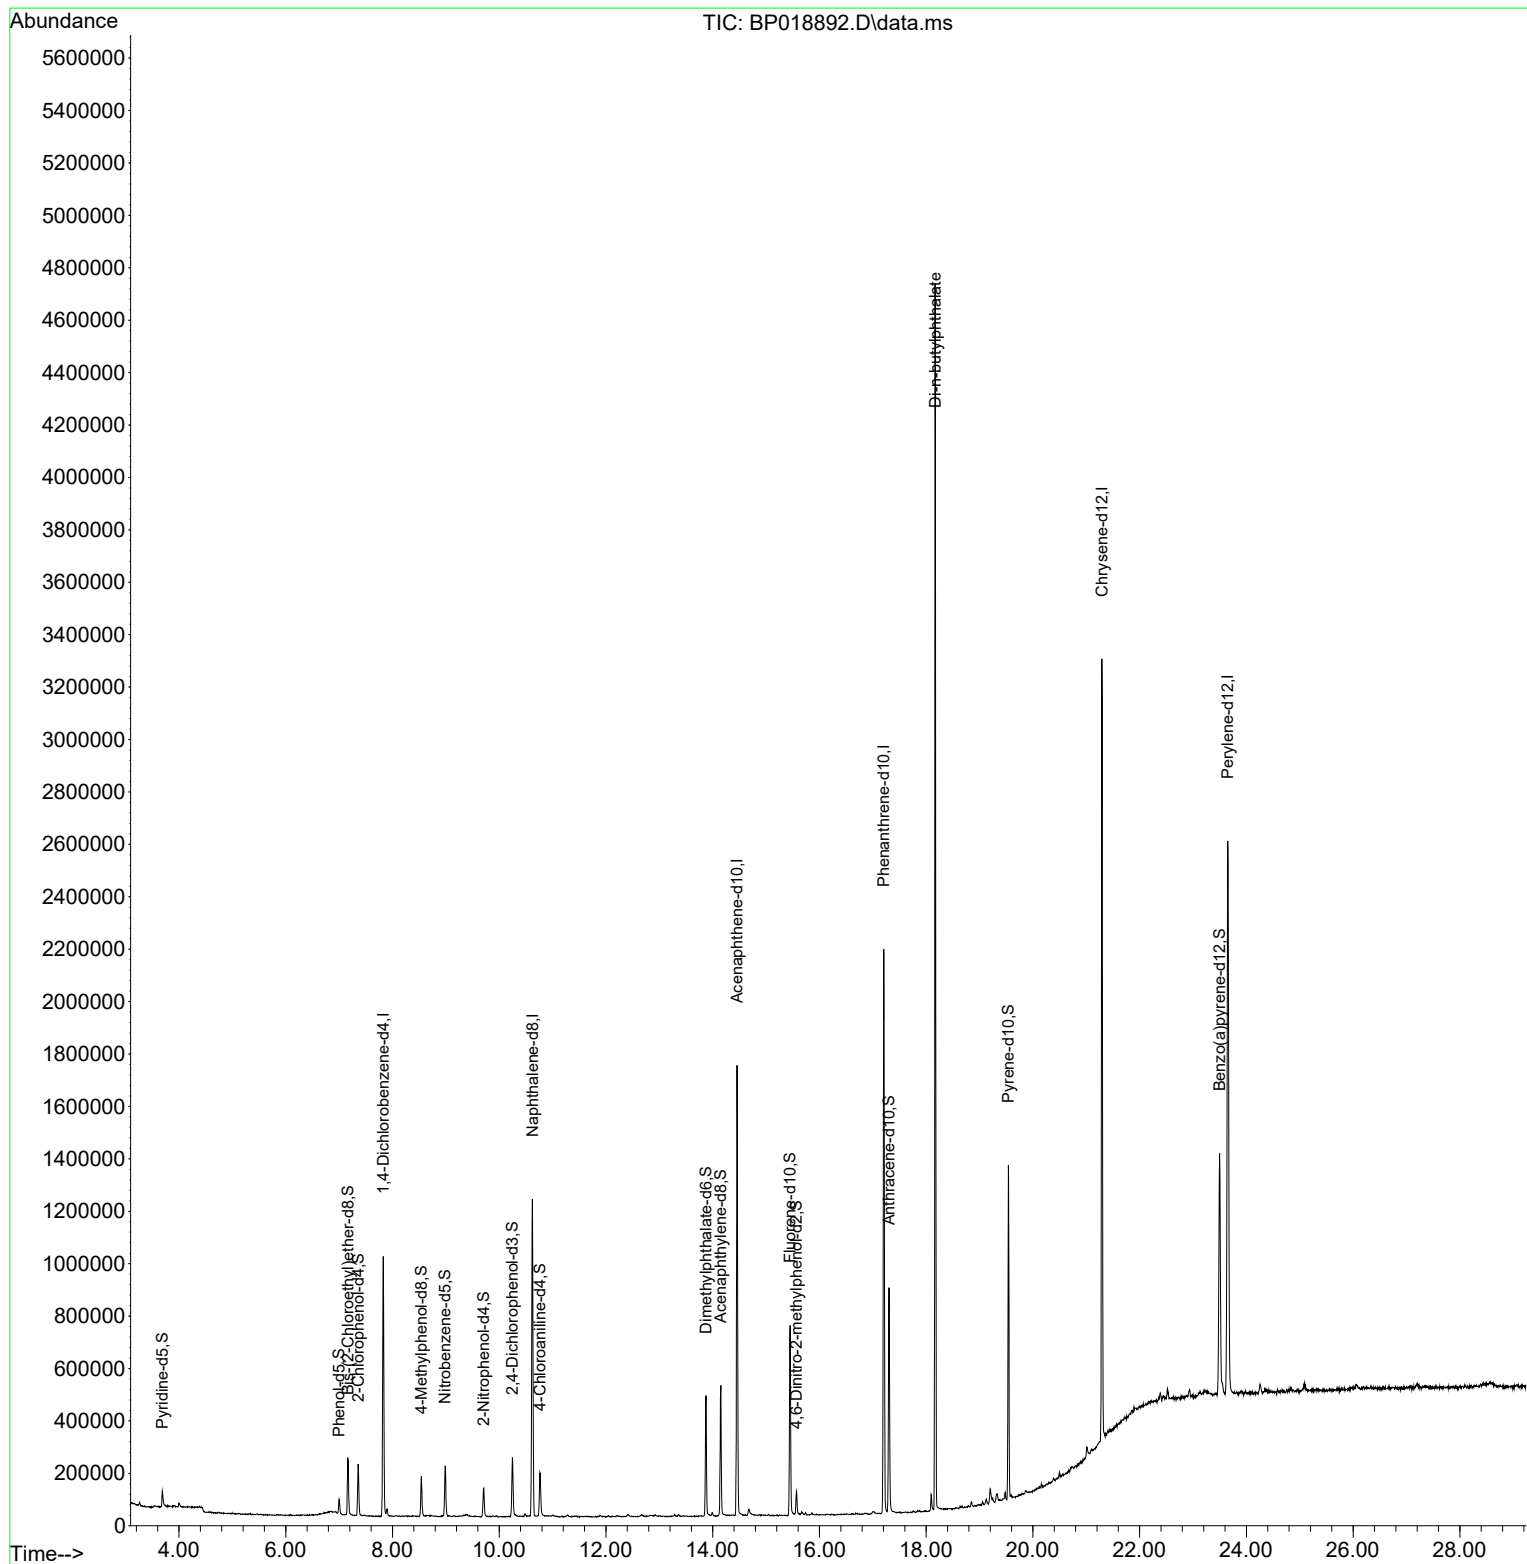

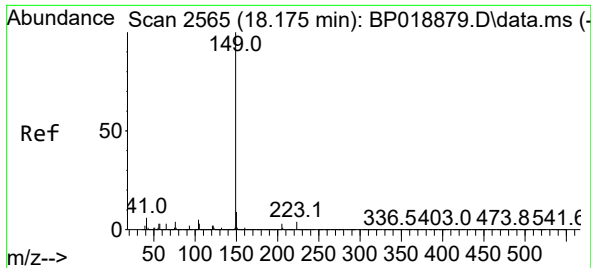

#78
 Di-n-butylphthalate
 Concen: 37.965 ng/ul
 RT: 18.169 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BP018892.D
 Acq: 15 Dec 2023 22:18

Instrument :
 BNA_P
 ClientSampleId :
 DCLC7DL

Tgt Ion:149 Resp: 3147388
 Ion Ratio Lower Upper
 149 100
 150 9.4 7.4 11.2
 104 5.0 3.9 5.9

