

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018880.D
 Acq On : 15 Dec 2023 14:41
 Operator : MA/JU
 Sample : PB157656BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	37	rBV	88083	113751	1.87%	0.193%
2	3.540	73	77	82	rBV5	11496	21562	0.36%	0.037%
3	3.675	96	100	115	rBV	937246	1456413	23.99%	2.472%
4	4.005	153	156	161	rVB	16783	20429	0.34%	0.035%
5	6.999	659	665	678	rVB	1097958	1685139	27.76%	2.861%
6	7.163	687	693	705	rVV	925670	1436687	23.67%	2.439%
7	7.357	719	726	736	rBV	1141182	1741462	28.69%	2.956%
8	7.828	799	806	815	rVB	1019201	1577723	25.99%	2.678%
9	8.540	920	927	936	rBV	1328182	2038334	33.58%	3.460%
10	8.987	995	1003	1014	rBV	955328	1559619	25.69%	2.648%
11	9.710	1117	1126	1138	rBV	710500	1205220	19.86%	2.046%
12	10.246	1209	1217	1235	rBV	1238198	2050804	33.79%	3.481%
13	10.622	1273	1281	1288	rBV	1244982	2045988	33.71%	3.473%
14	10.675	1288	1290	1294	rVB	18483	19531	0.32%	0.033%
15	10.763	1294	1305	1325	rBV	1170303	2007409	33.07%	3.408%
16	11.881	1491	1495	1499	rBV7	5086	7266	0.12%	0.012%
17	12.210	1546	1551	1559	rVB2	22372	38164	0.63%	0.065%
18	12.287	1559	1564	1571	rVB2	16269	28828	0.47%	0.049%
19	12.504	1596	1601	1606	rBV2	12288	19858	0.33%	0.034%
20	12.640	1619	1624	1626	rBV6	4912	6796	0.11%	0.012%
21	12.828	1652	1656	1658	rVV5	3795	6822	0.11%	0.012%
22	13.257	1725	1729	1731	rBV5	6697	9745	0.16%	0.017%
23	13.298	1731	1736	1740	rVV2	11804	23015	0.38%	0.039%
24	13.357	1742	1746	1752	rVV7	11949	28694	0.47%	0.049%
25	13.428	1756	1758	1764	rVB7	5907	7830	0.13%	0.013%
26	13.875	1828	1834	1846	rBV	1581795	2196316	36.18%	3.728%
27	14.151	1873	1881	1897	rBV	2246489	3299040	54.35%	5.600%
28	14.457	1927	1933	1940	rBV	1689272	2489541	41.01%	4.226%
29	14.522	1940	1944	1953	rVB	40326	63539	1.05%	0.108%
30	14.663	1962	1968	1983	rBV	589763	1054508	17.37%	1.790%
31	14.857	1997	2001	2009	rVB2	30680	52667	0.87%	0.089%
32	15.451	2093	2102	2108	rBV	2880144	4072571	67.09%	6.914%
33	15.504	2108	2111	2116	rVV2	45852	66704	1.10%	0.113%
34	15.569	2117	2122	2131	rVV	560632	754688	12.43%	1.281%
35	15.692	2140	2143	2146	rVB4	9594	9542	0.16%	0.016%
36	15.804	2158	2162	2166	rVB5	4151	6165	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018880.D
Acq On : 15 Dec 2023 14:41
Operator : MA/JU
Sample : PB157656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	16.404	2259	2264	2268	rBV8	6505	9809	0.16%	0.017%
38	16.510	2277	2282	2286	rBV7	9241	15320	0.25%	0.026%
39	16.686	2310	2312	2317	rVB5	7561	9754	0.16%	0.017%
40	17.204	2394	2400	2405	rBV	1885576	2731438	45.00%	4.637%
41	17.245	2405	2407	2411	rVV	91865	120451	1.98%	0.204%
42	17.304	2411	2417	2432	rVB2	2882006	4234066	69.75%	7.188%
43	17.616	2468	2470	2474	rVB3	10994	13444	0.22%	0.023%
44	18.104	2549	2553	2556	rBV6	9383	15659	0.26%	0.027%
45	19.122	2722	2726	2731	rVB	41565	49736	0.82%	0.084%
46	19.186	2734	2737	2740	rBV	35759	48802	0.80%	0.083%
47	19.216	2740	2742	2747	rVB	44962	56599	0.93%	0.096%
48	19.545	2792	2798	2808	rBV	3874250	5157368	84.96%	8.755%
49	21.298	3091	3096	3101	rBV	2623584	3356433	55.30%	5.698%
50	23.504	3464	3471	3486	rVB2	3200469	6070036	100.00%	10.304%
51	23.657	3490	3497	3509	rVB	1955587	3795795	62.53%	6.444%




Sum of corrected areas: 58907080

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018880.D
Acq On : 15 Dec 2023 14:41
Operator : MA/JU
Sample : PB157656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

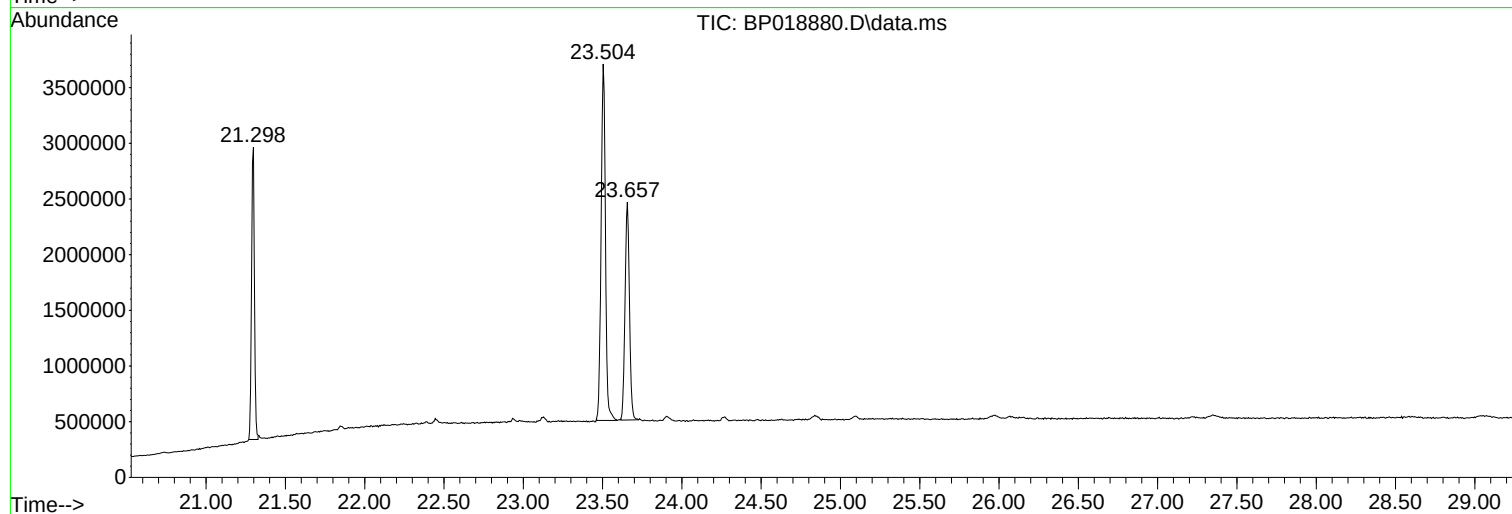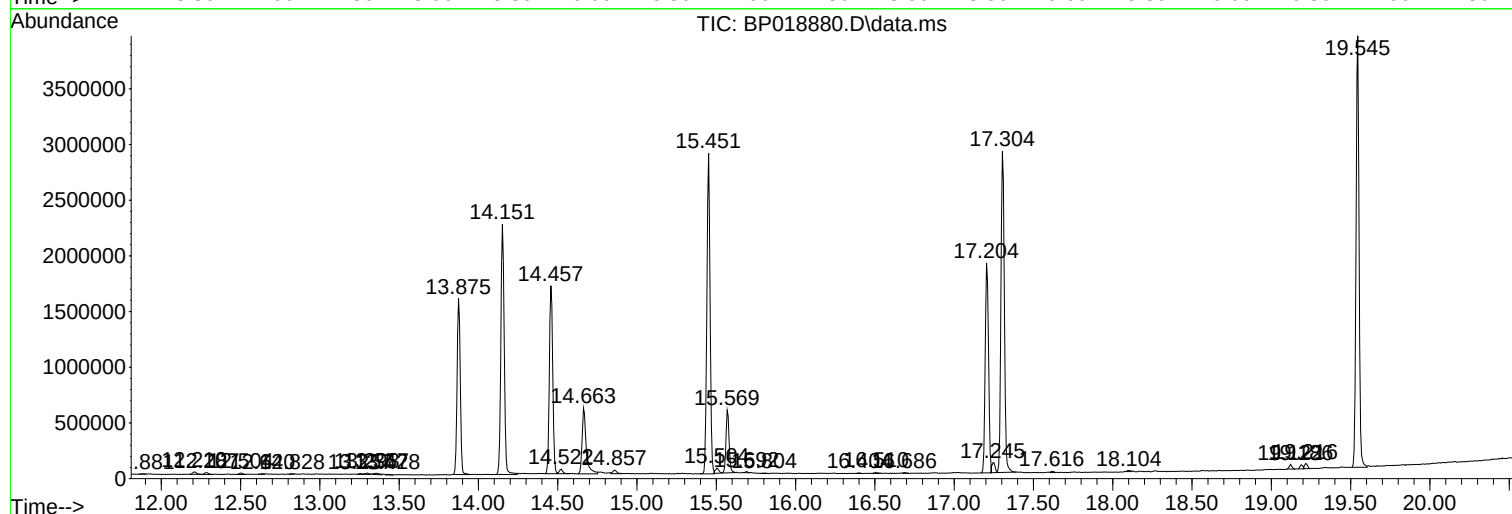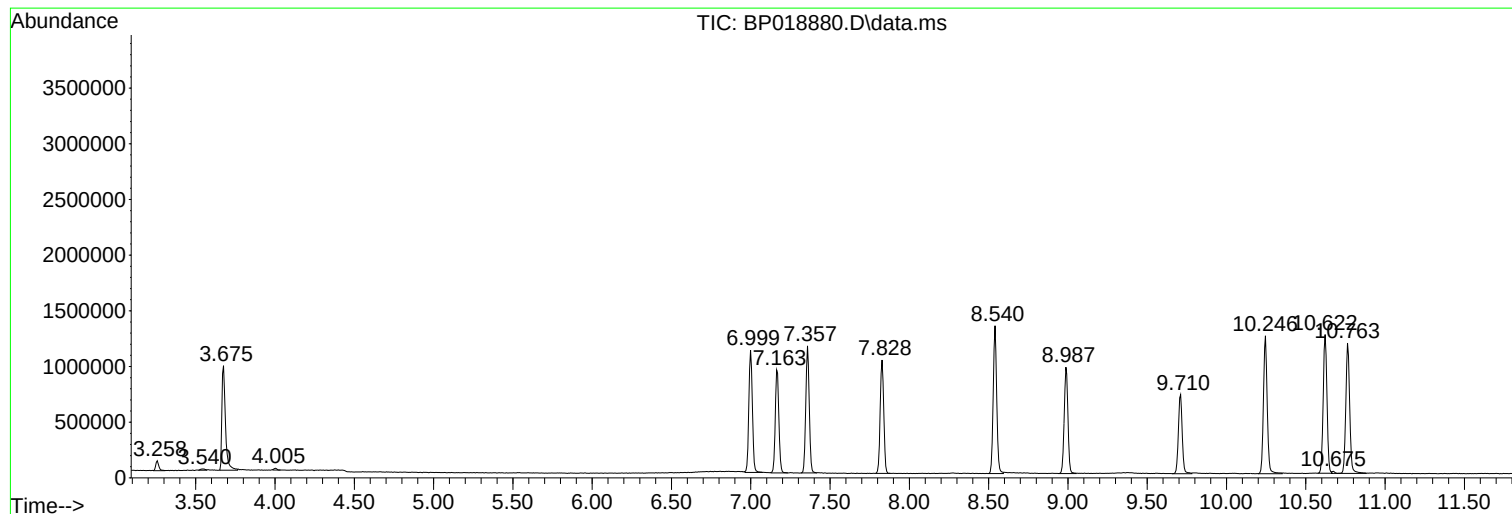

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018880.D
Acq On : 15 Dec 2023 14:41
Operator : MA/JU
Sample : PB157656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018880.D
Acq On : 15 Dec 2023 14:41
Operator : MA/JU
Sample : PB157656BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc