

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018884.D
 Acq On : 15 Dec 2023 17:46
 Operator : MA/JU
 Sample : PB157656BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK656

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.699	265	269	274	rBV2	17623	38424	0.66%	0.074%
2	2.905	468	474	484	rVV3	105927	223464	3.85%	0.430%
3	2.993	484	489	498	rVB	44903	66901	1.15%	0.129%
4	3.258	530	534	541	rVB2	43262	58426	1.01%	0.112%
5	3.676	600	605	619	rBV	539805	828733	14.29%	1.595%
6	6.999	1163	1170	1186	rVB	962018	1490010	25.68%	2.867%
7	7.164	1192	1198	1208	rVB	790612	1214487	20.93%	2.337%
8	7.358	1224	1231	1247	rBV	948264	1463583	25.23%	2.816%
9	7.828	1304	1311	1320	rVB	883286	1353228	23.33%	2.604%
10	8.540	1425	1432	1446	rBV	1128980	1798883	31.01%	3.461%
11	8.987	1501	1508	1522	rBV	772718	1231785	21.23%	2.370%
12	9.711	1623	1631	1639	rBV	348573	594066	10.24%	1.143%
13	10.246	1715	1722	1732	rBV	999307	1697725	29.26%	3.267%
14	10.622	1779	1786	1792	rBV	1109515	1829163	31.53%	3.520%
15	10.763	1803	1810	1834	rVB	1050288	1822427	31.41%	3.507%
16	12.210	2049	2056	2062	rBV2	17994	32610	0.56%	0.063%
17	12.281	2064	2068	2075	rBV2	16088	27671	0.48%	0.053%
18	13.875	2333	2339	2350	rBV	1731665	2285533	39.40%	4.398%
19	14.151	2379	2386	2401	rBV	2085371	3016691	52.00%	5.805%
20	14.457	2431	2438	2445	rBV	1526778	2224628	38.35%	4.280%
21	14.522	2445	2449	2455	rVB2	35382	53839	0.93%	0.104%
22	14.663	2467	2473	2488	rBV	371801	718072	12.38%	1.382%
23	14.857	2502	2506	2517	rVB2	27736	49570	0.85%	0.095%
24	15.451	2600	2607	2613	rBV	2674202	3675121	63.35%	7.071%
25	15.504	2613	2616	2622	rVV	45477	68388	1.18%	0.132%
26	15.569	2622	2627	2641	rVB	257170	377681	6.51%	0.727%
27	17.204	2899	2905	2910	rBV	1748798	2473061	42.63%	4.759%
28	17.245	2910	2912	2916	rVV	82200	108021	1.86%	0.208%
29	17.304	2916	2922	2935	rVB2	2672850	3830659	66.03%	7.371%
30	19.122	3227	3231	3237	rVB3	33741	43512	0.75%	0.084%
31	19.187	3239	3242	3245	rVV2	30840	44011	0.76%	0.085%
32	19.222	3245	3248	3252	rVB	43980	58854	1.01%	0.113%
33	19.545	3297	3303	3315	rBV	3554826	4661570	80.35%	8.969%
34	21.298	3596	3601	3613	rBV	2465793	3084014	53.16%	5.934%
35	23.504	3969	3976	3990	rVB2	2928503	5801257	100.00%	11.162%
36	23.657	3995	4002	4020	rVB	1809461	3625359	62.49%	6.976%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018884.D
Acq On : 15 Dec 2023 17:46
Operator : MA/JU
Sample : PB157656BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 51971427

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018884.D
Acq On : 15 Dec 2023 17:46
Operator : MA/JU
Sample : PB157656BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

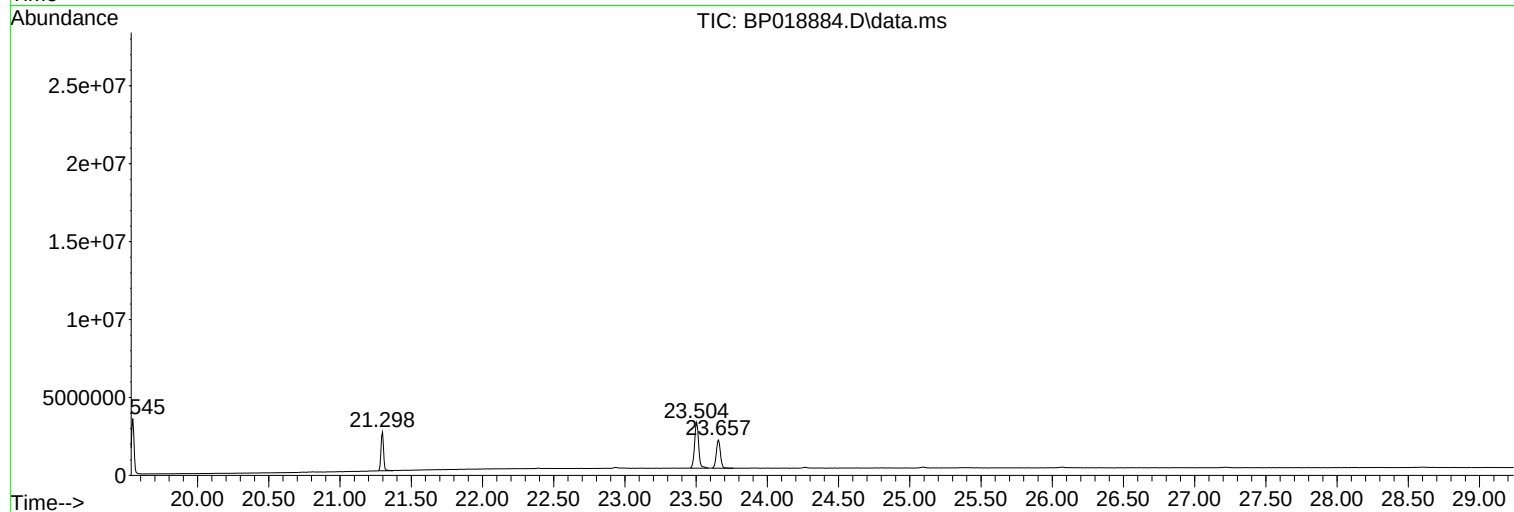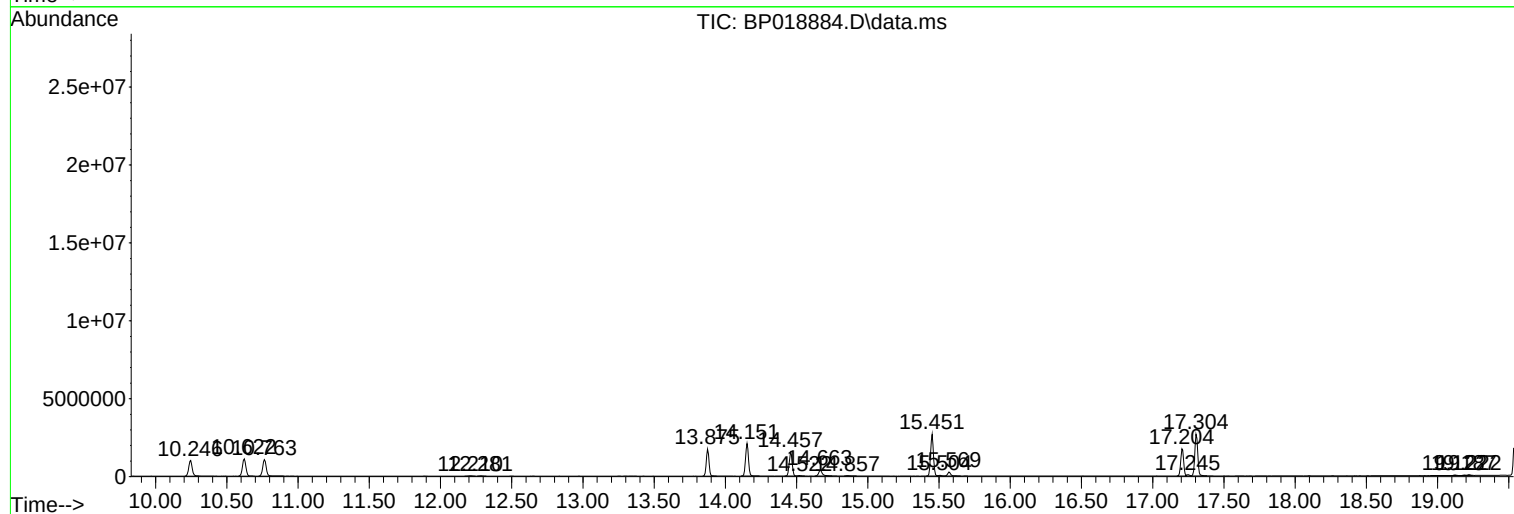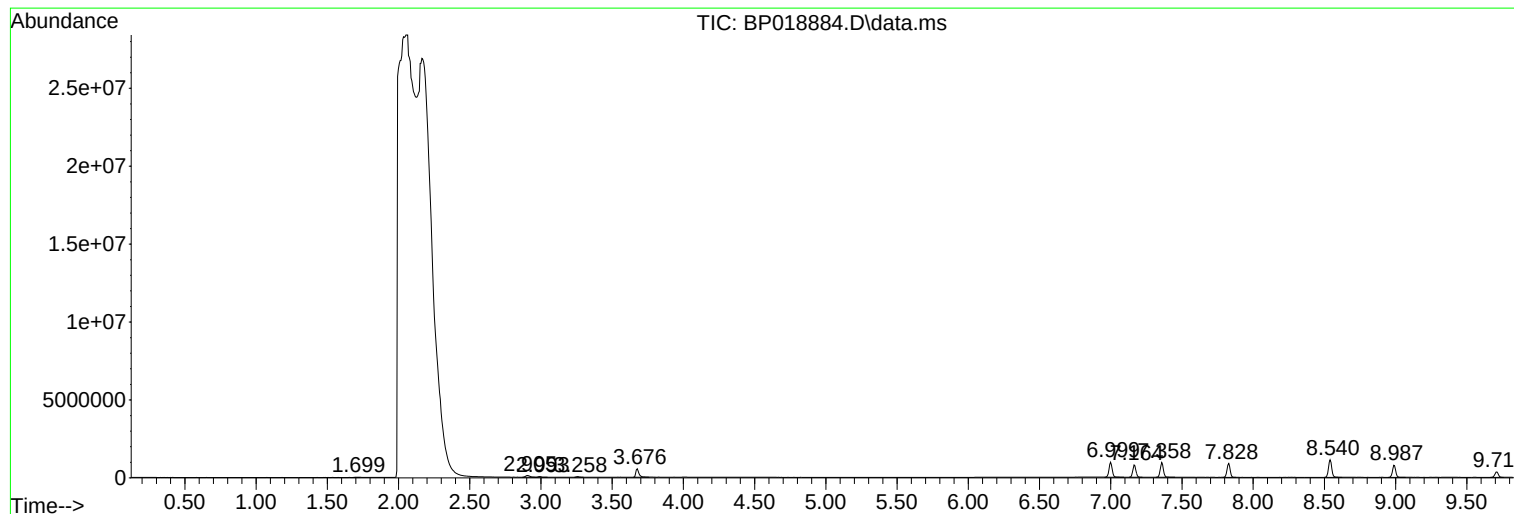

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018884.D
Acq On : 15 Dec 2023 17:46
Operator : MA/JU
Sample : PB157656BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic2.905 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.905	3.30 ng/ul	223464	1,4-Dichlorobenzene-d4	7.828

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexane	84	C6H12	000110-82-7	87
2			Cyclohexane	84	C6H12	000110-82-7	87
3			Cyclohexane	84	C6H12	000110-82-7	87
4			1-Pentene, 2-methyl-	84	C6H12	000763-29-1	80
5			1-Pentene, 2-methyl-	84	C6H12	000763-29-1	72

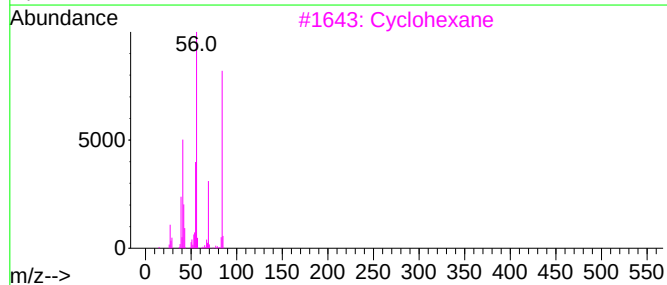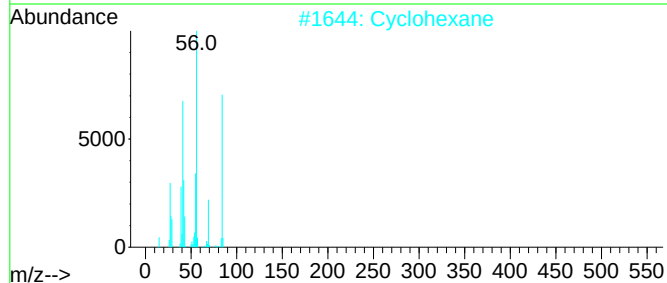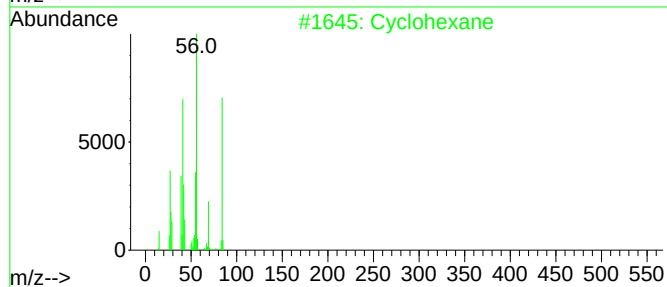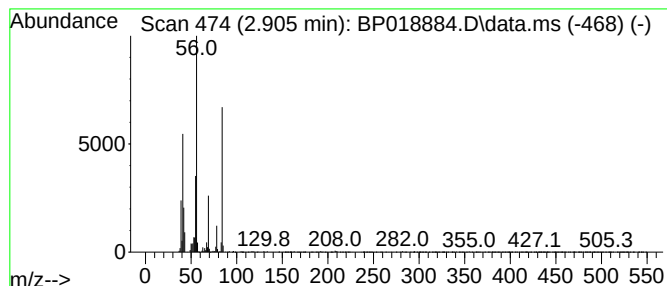

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018884.D
Acq On : 15 Dec 2023 17:46
Operator : MA/JU
Sample : PB157656BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK656

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	2.905	3.3	ng/u1	223464	1	7.828	1353230	20.0