

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018889.D
 Acq On : 15 Dec 2023 20:36
 Operator : MA/JU
 Sample : 05646-19DL 5X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AS6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	97	101	112	rBV	136116	232462	0.76%	0.229%
2	5.140	341	349	363	rBV	6545520	10033007	32.72%	9.870%
3	6.999	660	665	677	rVB2	210524	371900	1.21%	0.366%
4	7.163	687	693	703	rVB	187287	294431	0.96%	0.290%
5	7.357	721	726	740	rVB2	203942	369613	1.21%	0.364%
6	7.716	779	787	795	rBV	706836	1093210	3.57%	1.075%
7	7.869	797	813	824	rBV	16278210	30660497	100.00%	30.161%
8	8.181	858	866	874	rVB	2470408	4024254	13.13%	3.959%
9	8.540	920	927	933	rBV	243645	390963	1.28%	0.385%
10	8.599	933	937	943	rVB	65903	103730	0.34%	0.102%
11	8.987	996	1003	1015	rBV	165077	279609	0.91%	0.275%
12	9.551	1093	1099	1102	rBV2	88530	140280	0.46%	0.138%
13	9.593	1102	1106	1119	rVB	85597	203130	0.66%	0.200%
14	9.710	1119	1126	1131	rBV	102939	172802	0.56%	0.170%
15	9.769	1131	1136	1142	rVB	43733	75316	0.25%	0.074%
16	10.004	1170	1176	1182	rVB	24419	39909	0.13%	0.039%
17	10.246	1211	1217	1224	rBV	234912	393900	1.28%	0.387%
18	10.310	1224	1228	1236	rVB	33962	63410	0.21%	0.062%
19	10.493	1249	1259	1272	rBV	11580925	19910101	64.94%	19.586%
20	10.622	1274	1281	1290	rVB	1412180	2269859	7.40%	2.233%
21	10.763	1298	1305	1317	rBV	217875	394947	1.29%	0.389%
22	11.004	1338	1346	1356	rBV	4104305	6948980	22.66%	6.836%
23	12.187	1542	1547	1557	rVB4	19141	39724	0.13%	0.039%
24	12.363	1572	1577	1584	rBV3	24684	37192	0.12%	0.037%
25	12.616	1614	1620	1621	rBV2	90617	115993	0.38%	0.114%
26	12.651	1621	1626	1632	rVV	320098	534939	1.74%	0.526%
27	13.257	1722	1729	1739	rBV	1373214	2141892	6.99%	2.107%
28	13.875	1824	1834	1846	rBV	441822	628897	2.05%	0.619%
29	14.151	1873	1881	1891	rBV	489514	717903	2.34%	0.706%
30	14.457	1926	1933	1943	rBV	2038745	3008550	9.81%	2.960%
31	14.675	1963	1970	1981	rBV	61299	145974	0.48%	0.144%
32	14.775	1981	1987	1994	rVB	160776	237906	0.78%	0.234%
33	15.451	2095	2102	2115	rBV	661901	1016107	3.31%	1.000%
34	15.569	2117	2122	2132	rVB	67613	108474	0.35%	0.107%
35	17.204	2394	2400	2411	rBV	2428657	3511510	11.45%	3.454%
36	17.304	2411	2417	2429	rVV	699872	982248	3.20%	0.966%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018889.D
Acq On : 15 Dec 2023 20:36
Operator : MA/JU
Sample : 05646-19DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AS6DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.098	2547	2552	2560	rBV	86339	120629	0.39%	0.119%
38	19.333	2759	2762	2767	rBV6	25718	32005	0.10%	0.031%
39	19.539	2792	2797	2803	rBV	895505	1167089	3.81%	1.148%
40	21.298	3091	3096	3104	rBV	2965455	3714717	12.12%	3.654%
41	23.498	3465	3470	3477	rBV2	540646	997669	3.25%	0.981%
42	23.657	3490	3497	3506	rVB	1968764	3930551	12.82%	3.867%




Sum of corrected areas: 101656279

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018889.D
Acq On : 15 Dec 2023 20:36
Operator : MA/JU
Sample : 05646-19DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AS6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

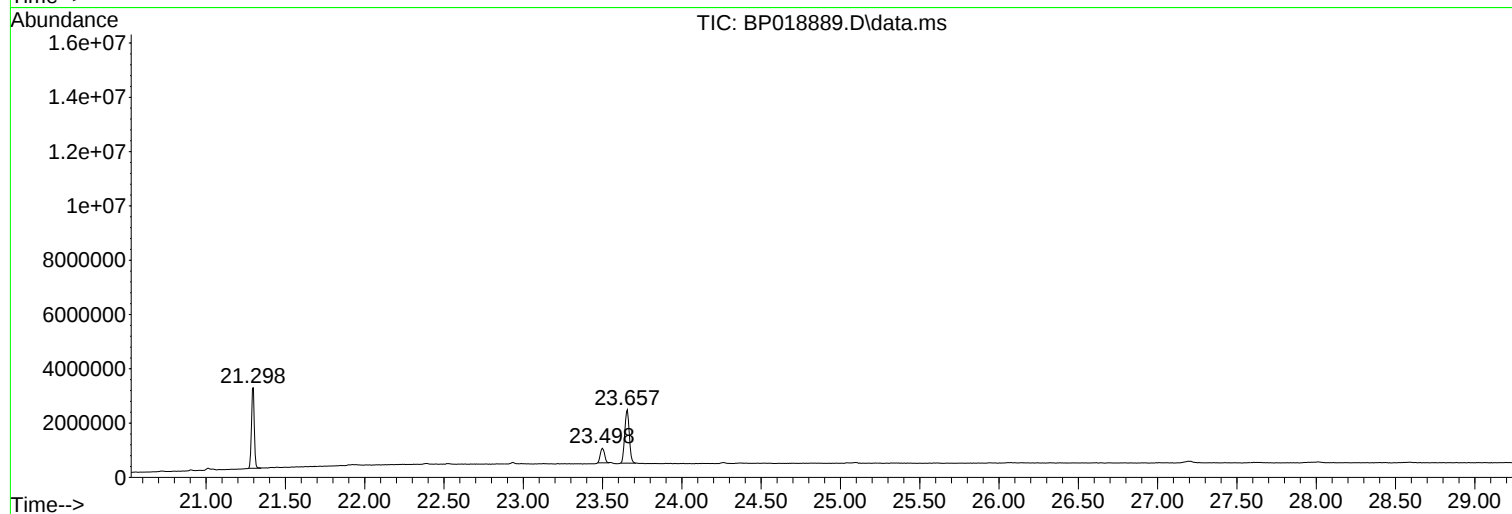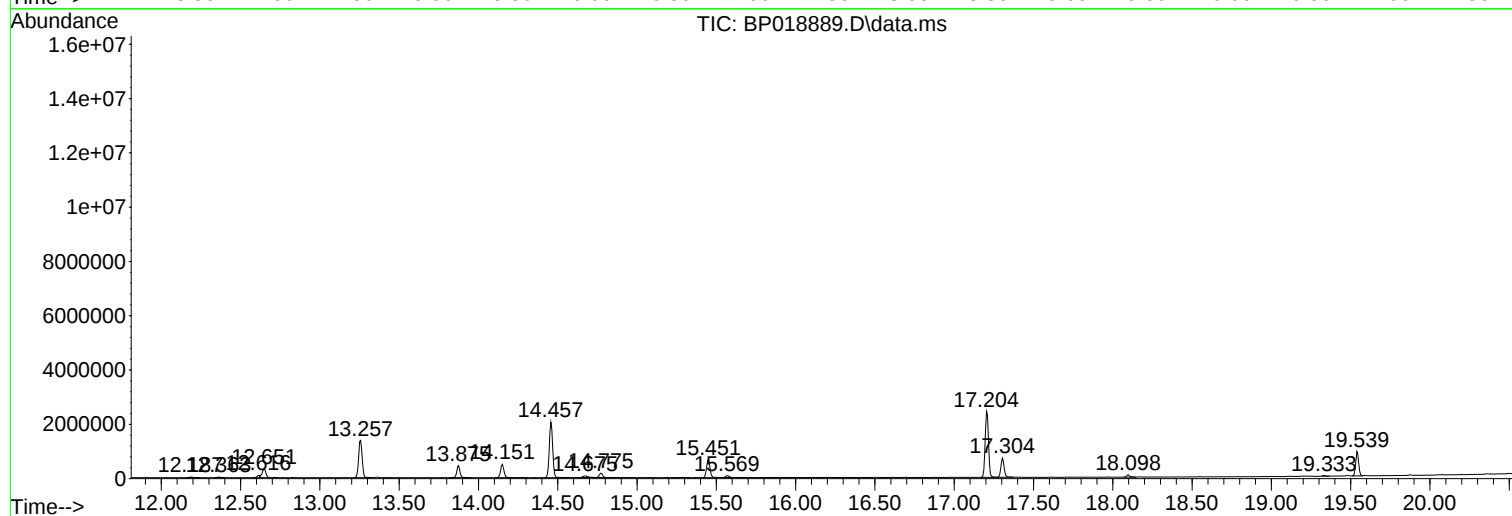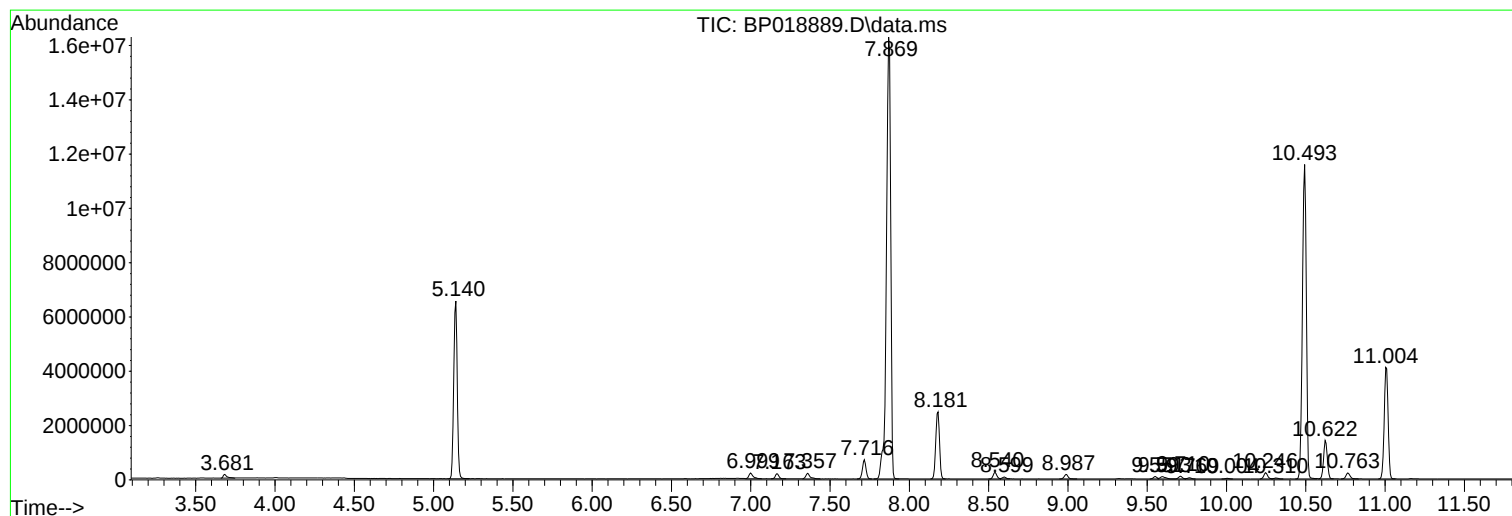

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018889.D
Acq On : 15 Dec 2023 20:36
Operator : MA/JU
Sample : 05646-19DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AS6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018889.D
Acq On : 15 Dec 2023 20:36
Operator : MA/JU
Sample : 05646-19DL 5X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AS6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc