

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018891.D
 Acq On : 15 Dec 2023 21:44
 Operator : MA/JU
 Sample : 05627-14DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	26	29	37	rBV2	16853	24625	0.35%	0.070%
2	3.687	98	102	111	rBV	57586	98984	1.41%	0.281%
3	4.005	152	156	162	rVB2	18023	26635	0.38%	0.076%
4	5.328	377	381	387	rVB5	9240	14098	0.20%	0.040%
5	5.681	436	441	444	rBV7	6221	9170	0.13%	0.026%
6	6.811	627	633	636	rBV5	8502	18986	0.27%	0.054%
7	6.999	660	665	673	rVB	62752	101534	1.44%	0.288%
8	7.164	688	693	700	rBV	237273	377697	5.36%	1.072%
9	7.358	719	726	737	rVB	214955	340925	4.84%	0.968%
10	7.828	795	806	816	rBV	1120273	1854804	26.33%	5.264%
11	7.899	816	818	823	rVB2	14123	16384	0.23%	0.046%
12	8.064	842	846	849	rBV5	4349	7543	0.11%	0.021%
13	8.175	863	865	870	rVB4	7931	11689	0.17%	0.033%
14	8.369	893	898	901	rBV7	4955	9223	0.13%	0.026%
15	8.452	909	912	917	rVB7	4732	8047	0.11%	0.023%
16	8.540	921	927	936	rBV	164414	270084	3.83%	0.767%
17	8.987	997	1003	1013	rBV	213471	354113	5.03%	1.005%
18	9.075	1015	1018	1023	rVV7	6362	9330	0.13%	0.026%
19	9.375	1062	1069	1070	rBV7	5841	9600	0.14%	0.027%
20	9.540	1094	1097	1102	rBV7	5471	9678	0.14%	0.027%
21	9.710	1120	1126	1132	rBV	118507	202026	2.87%	0.573%
22	10.246	1209	1217	1225	rBV	255456	447590	6.35%	1.270%
23	10.405	1238	1244	1247	rBV8	5352	9347	0.13%	0.027%
24	10.487	1252	1258	1264	rBV2	55183	87455	1.24%	0.248%
25	10.622	1273	1281	1289	rBV	1413776	2256187	32.03%	6.403%
26	10.769	1298	1306	1317	rBV	167963	315553	4.48%	0.896%
27	10.940	1328	1335	1339	rBV9	4137	7831	0.11%	0.022%
28	11.005	1339	1346	1352	rBV4	16244	30615	0.43%	0.087%
29	11.281	1389	1393	1398	rVV2	12129	23160	0.33%	0.066%
30	11.540	1429	1437	1438	rBV7	5474	8262	0.12%	0.023%
31	12.046	1518	1523	1527	rBV5	7674	11532	0.16%	0.033%
32	12.210	1547	1551	1557	rBV7	4793	7437	0.11%	0.021%
33	12.399	1577	1583	1590	rBV	38254	70242	1.00%	0.199%
34	12.663	1621	1628	1634	rBV6	17126	33650	0.48%	0.095%
35	12.922	1668	1672	1678	rVB2	12185	19429	0.28%	0.055%
36	13.257	1724	1729	1731	rBV5	5867	7259	0.10%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018891.D
 Acq On : 15 Dec 2023 21:44
 Operator : MA/JU
 Sample : 05627-14DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	13.293	1731	1735	1739	rVB6	7252	10650	0.15%	0.030%
38	13.357	1741	1746	1751	rBV3	20783	33693	0.48%	0.096%
39	13.457	1757	1763	1768	rBV9	9185	15869	0.23%	0.045%
40	13.875	1828	1834	1842	rBV	526408	730977	10.38%	2.075%
41	13.993	1850	1854	1860	rVB7	16427	26409	0.37%	0.075%
42	14.151	1870	1881	1890	rBV	553651	837792	11.89%	2.378%
43	14.457	1926	1933	1944	rBV	1813528	2675935	37.99%	7.594%
44	14.681	1963	1971	1980	rBV5	22236	60685	0.86%	0.172%
45	15.046	2029	2033	2038	rBV7	4098	8745	0.12%	0.025%
46	15.257	2064	2069	2071	rBV6	5010	8389	0.12%	0.024%
47	15.451	2095	2102	2116	rBV	819972	1198489	17.02%	3.401%
48	15.569	2117	2122	2131	rVB	85335	144017	2.04%	0.409%
49	15.869	2168	2173	2176	rBV7	5251	9912	0.14%	0.028%
50	16.228	2230	2234	2239	rBV7	6645	10527	0.15%	0.030%
51	16.692	2309	2313	2317	rBV7	4639	7536	0.11%	0.021%
52	17.016	2359	2368	2376	rBV2	42020	87592	1.24%	0.249%
53	17.204	2394	2400	2411	rBV	2092423	2930572	41.61%	8.317%
54	17.304	2411	2417	2433	rVB	879854	1210906	17.19%	3.437%
55	17.763	2491	2495	2498	rBV6	5451	9021	0.13%	0.026%
56	17.839	2505	2508	2511	rBV	8463	8886	0.13%	0.025%
57	18.039	2539	2542	2545	rBV4	7293	10897	0.15%	0.031%
58	18.092	2547	2551	2559	rVV2	63653	94793	1.35%	0.269%
59	18.169	2559	2564	2577	rVV	5590354	7043583	100.00%	19.990%
60	18.845	2676	2679	2683	rBV	40888	50660	0.72%	0.144%
61	19.198	2735	2739	2745	rBV4	38161	85736	1.22%	0.243%
62	19.328	2755	2761	2766	rBV2	35150	79619	1.13%	0.226%
63	19.475	2784	2786	2790	rVB4	23644	26160	0.37%	0.074%
64	19.539	2792	2797	2803	rBV	1146681	1508321	21.41%	4.281%
65	21.292	3090	3095	3103	rBV	2784102	3556772	50.50%	10.094%
66	23.498	3464	3470	3482	rVB2	845290	1692743	24.03%	4.804%
67	23.651	3489	3496	3506	rVB	1991468	3949039	56.07%	11.208%




Sum of corrected areas: 35235649

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018891.D
Acq On : 15 Dec 2023 21:44
Operator : MA/JU
Sample : 05627-14DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

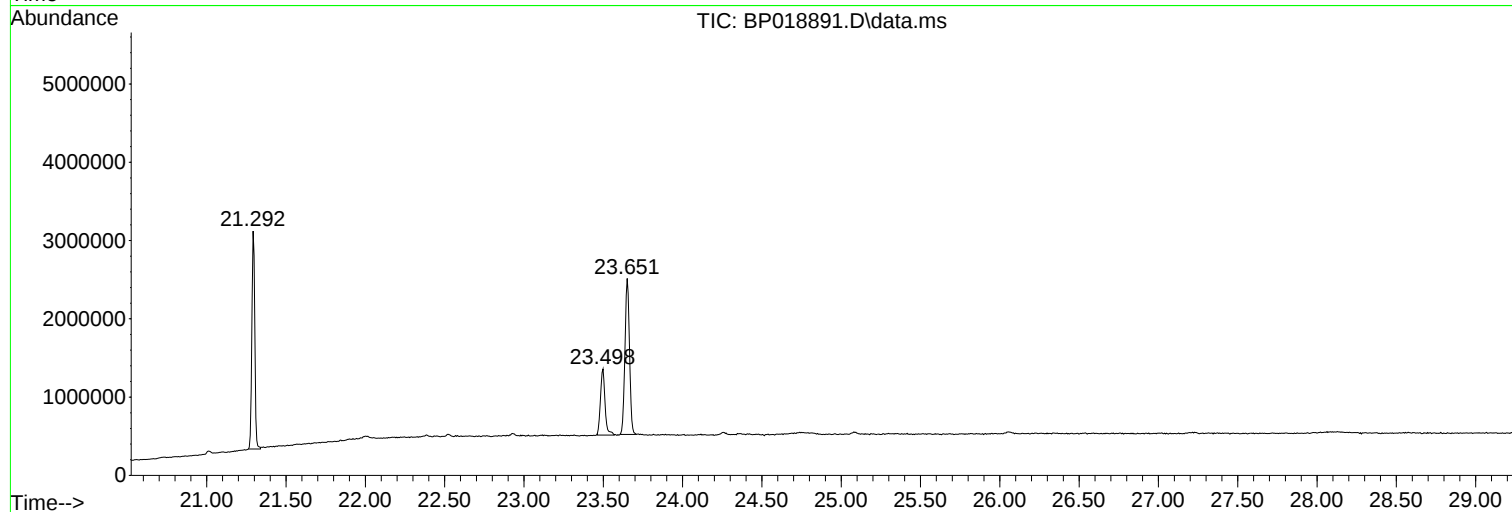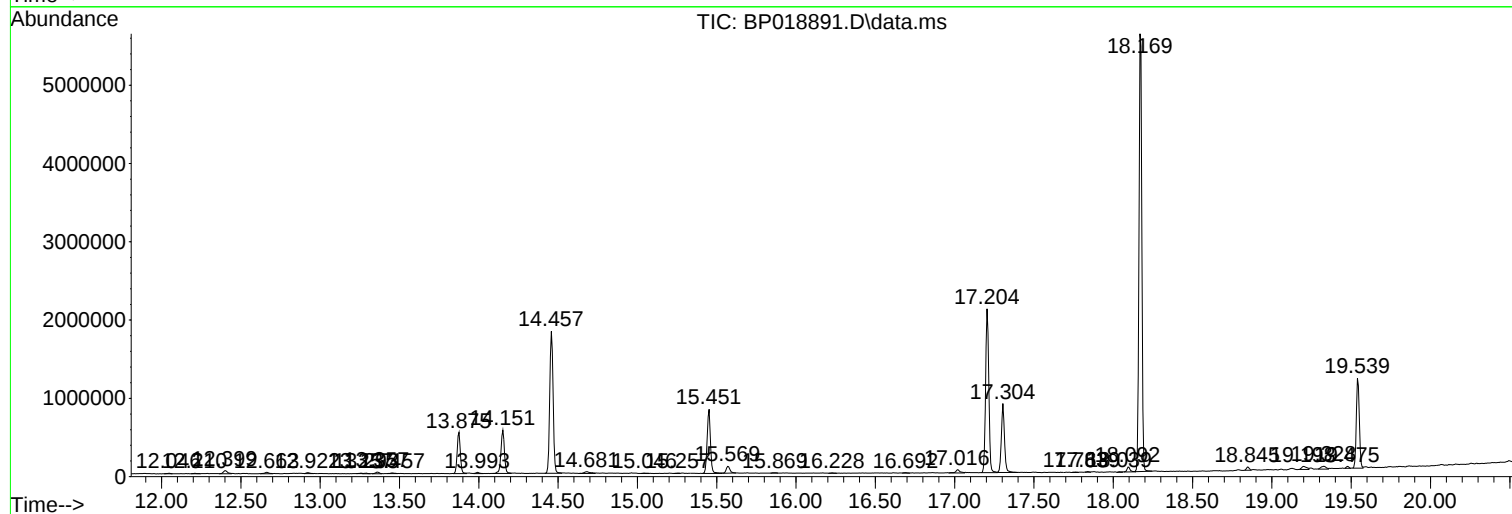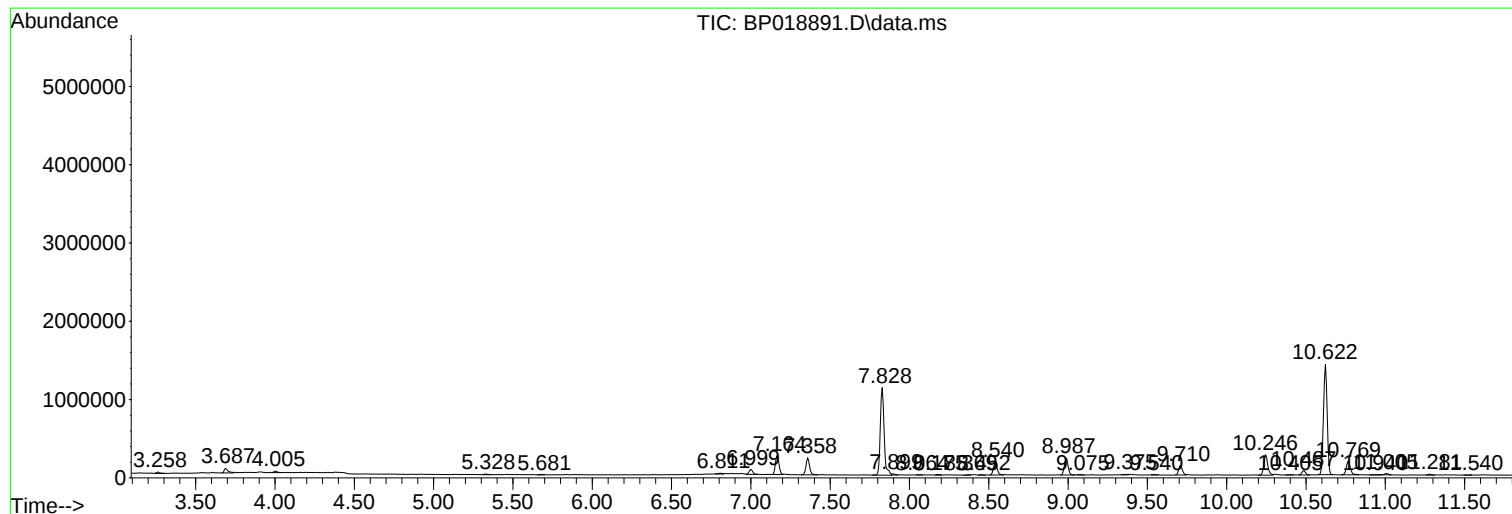

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018891.D
Acq On : 15 Dec 2023 21:44
Operator : MA/JU
Sample : 05627-14DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018891.D
Acq On : 15 Dec 2023 21:44
Operator : MA/JU
Sample : 05627-14DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC6DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc