

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018892.D
 Acq On : 15 Dec 2023 22:18
 Operator : MA/JU
 Sample : 05627-15DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018892.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	27	29	34	rVB2	14941	18307	0.34%	0.056%
2	3.687	99	102	111	rBV	57989	92964	1.73%	0.282%
3	3.999	152	155	160	rBV2	15231	23398	0.44%	0.071%
4	5.464	402	404	410	rVB7	4287	6174	0.11%	0.019%
5	6.999	660	665	672	rVB	54879	86104	1.60%	0.261%
6	7.163	688	693	701	rBV	218202	341840	6.36%	1.036%
7	7.358	720	726	732	rBV	196136	304213	5.66%	0.922%
8	7.828	799	806	814	rBV	992173	1543982	28.74%	4.681%
9	7.899	814	818	826	rVB	27634	46174	0.86%	0.140%
10	8.540	920	927	937	rBV	154112	256958	4.78%	0.779%
11	8.987	996	1003	1011	rVV	192133	321938	5.99%	0.976%
12	9.052	1013	1014	1021	rVB6	3749	5540	0.10%	0.017%
13	9.152	1028	1031	1038	rVB9	3675	5855	0.11%	0.018%
14	9.710	1118	1126	1137	rBV	108162	197428	3.68%	0.599%
15	9.946	1163	1166	1170	rVB6	3762	5560	0.10%	0.017%
16	10.246	1210	1217	1226	rBV	226734	396489	7.38%	1.202%
17	10.481	1253	1257	1262	rBV6	10771	17091	0.32%	0.052%
18	10.622	1274	1281	1289	rVB	1209786	1963927	36.56%	5.955%
19	10.763	1299	1305	1316	rBV	164761	301358	5.61%	0.914%
20	11.281	1388	1393	1397	rBV2	5946	8218	0.15%	0.025%
21	12.046	1519	1523	1531	rVB9	6587	12758	0.24%	0.039%
22	12.410	1580	1585	1595	rBV5	8358	18325	0.34%	0.056%
23	12.822	1651	1655	1660	rBV7	4155	8453	0.16%	0.026%
24	12.922	1668	1672	1678	rVB7	6447	10165	0.19%	0.031%
25	13.287	1731	1734	1738	rVB5	7222	7963	0.15%	0.024%
26	13.363	1741	1747	1752	rBV6	7733	14130	0.26%	0.043%
27	13.875	1827	1834	1842	rBV	459750	647748	12.06%	1.964%
28	13.992	1849	1854	1859	rVB9	12337	18908	0.35%	0.057%
29	14.151	1872	1881	1890	rBV	498567	752678	14.01%	2.282%
30	14.363	1914	1917	1922	rBV7	3075	5709	0.11%	0.017%
31	14.457	1926	1933	1947	rBV	1716720	2436918	45.37%	7.389%
32	14.681	1964	1971	1983	rBV7	23674	64024	1.19%	0.194%
33	14.875	2000	2004	2007	rBV6	4046	6431	0.12%	0.019%
34	15.051	2029	2034	2038	rVB8	5351	8273	0.15%	0.025%
35	15.257	2064	2069	2070	rBV4	4491	6371	0.12%	0.019%
36	15.451	2095	2102	2114	rBV	725066	1083109	20.16%	3.284%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018892.D
 Acq On : 15 Dec 2023 22:18
 Operator : MA/JU
 Sample : 05627-15DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.569	2117	2122	2128	rVV	87383	131981	2.46%	0.400%
38	15.669	2134	2139	2147	rVV7	11526	23511	0.44%	0.071%
39	15.739	2147	2151	2156	rVB6	9518	13933	0.26%	0.042%
40	17.004	2359	2366	2369	rBV5	9519	23479	0.44%	0.071%
41	17.204	2393	2400	2411	rBV	2151709	3043909	56.67%	9.229%
42	17.304	2411	2417	2428	rVB	855489	1256399	23.39%	3.809%
43	17.763	2490	2495	2497	rBV4	6907	10560	0.20%	0.032%
44	17.839	2505	2508	2511	rBV2	6433	7752	0.14%	0.024%
45	17.881	2512	2515	2517	rVB3	6382	5999	0.11%	0.018%
46	18.092	2547	2551	2559	rBV2	62570	90181	1.68%	0.273%
47	18.169	2559	2564	2578	rVV	4679496	5371327	100.00%	16.286%
48	18.633	2641	2643	2647	rBV4	6327	6343	0.12%	0.019%
49	18.851	2676	2680	2685	rBV2	18479	27422	0.51%	0.083%
50	19.057	2713	2715	2718	rVB2	11042	10476	0.20%	0.032%
51	19.128	2723	2727	2733	rVB7	19367	32547	0.61%	0.099%
52	19.198	2735	2739	2745	rBV2	53403	103098	1.92%	0.313%
53	19.327	2756	2761	2766	rBV3	26427	50296	0.94%	0.153%
54	19.480	2784	2787	2792	rVB4	26844	30497	0.57%	0.092%
55	19.539	2792	2797	2803	rBV	1276084	1706084	31.76%	5.173%
56	21.292	3090	3095	3104	rBV	2984595	3928660	73.14%	11.912%
57	23.498	3464	3470	3484	rVB2	913369	1823705	33.95%	5.530%
58	23.651	3490	3496	3511	rVB	2104239	4237077	78.88%	12.847%




Sum of corrected areas: 32980717

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018892.D
Acq On : 15 Dec 2023 22:18
Operator : MA/JU
Sample : 05627-15DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

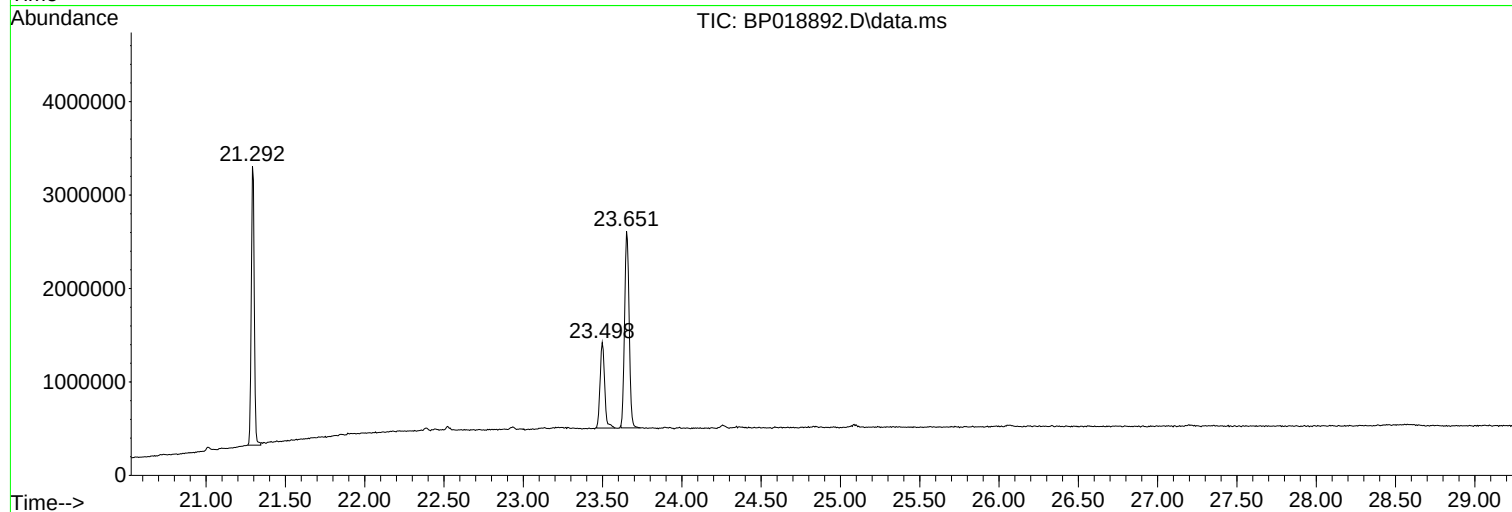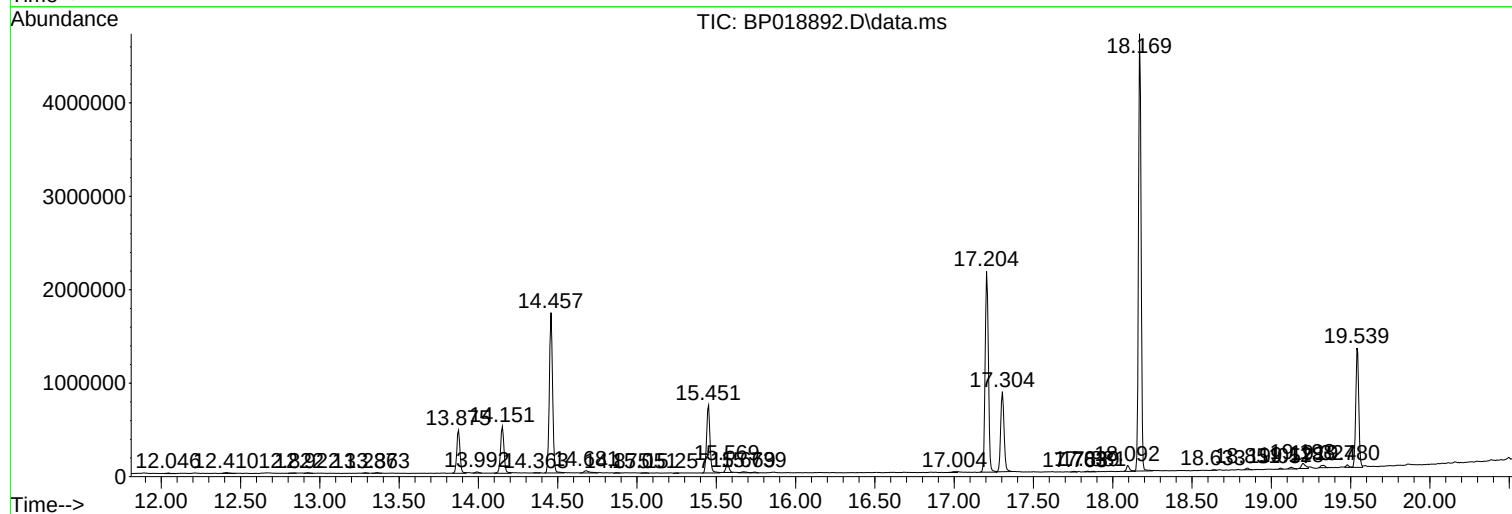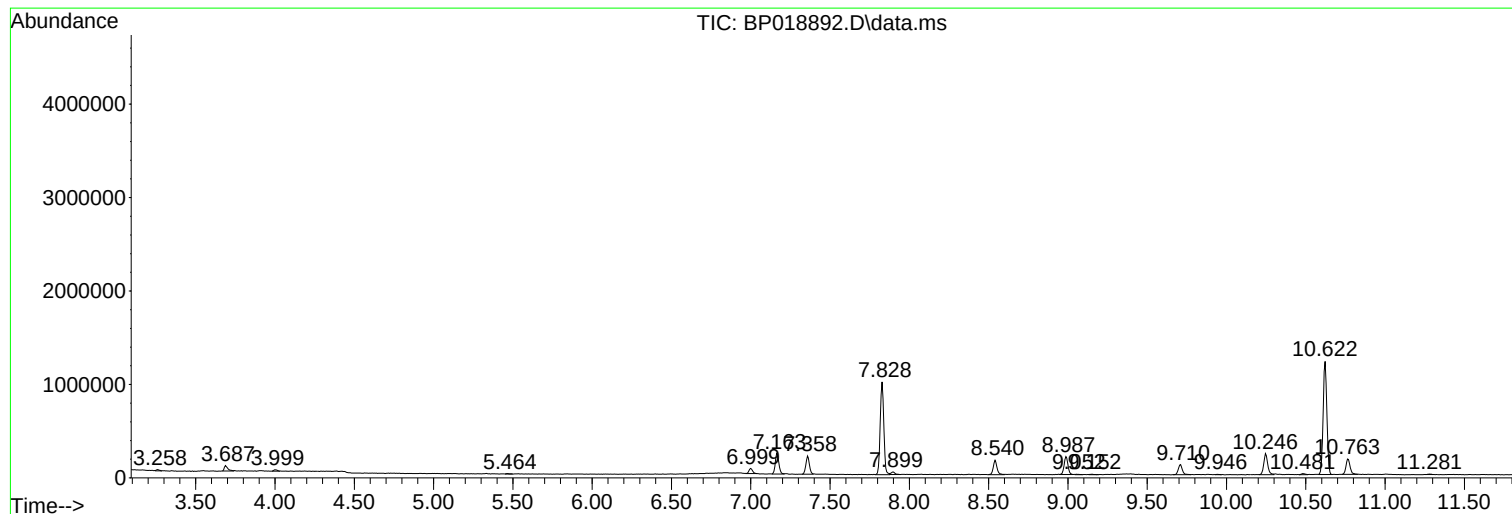

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018892.D
Acq On : 15 Dec 2023 22:18
Operator : MA/JU
Sample : 05627-15DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018892.D
Acq On : 15 Dec 2023 22:18
Operator : MA/JU
Sample : 05627-15DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC7DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc