

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018893.D
 Acq On : 15 Dec 2023 22:52
 Operator : MA/JU
 Sample : 05627-16DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.693	99	103	109	rBV	35278	59541	1.18%	0.184%
2	4.005	152	156	160	rVB3	15587	22880	0.45%	0.071%
3	5.334	377	382	387	rBV2	12916	20926	0.41%	0.065%
4	5.464	399	404	407	rBV2	25063	40832	0.81%	0.126%
5	5.834	462	467	473	rVB	24456	36537	0.72%	0.113%
6	5.917	479	481	486	rBV6	4271	6073	0.12%	0.019%
7	6.505	577	581	589	rBV3	11252	18296	0.36%	0.057%
8	6.999	661	665	671	rVB2	50904	77415	1.53%	0.239%
9	7.164	687	693	704	rVB	210710	331356	6.54%	1.025%
10	7.358	720	726	737	rBV	175792	290709	5.74%	0.899%
11	7.828	798	806	815	rBV	1010016	1565318	30.90%	4.841%
12	7.905	815	819	824	rVB6	11408	19784	0.39%	0.061%
13	8.540	921	927	936	rBV2	121409	203818	4.02%	0.630%
14	8.987	997	1003	1011	rBV	194717	320131	6.32%	0.990%
15	9.152	1029	1031	1037	rVB6	3153	5455	0.11%	0.017%
16	9.710	1115	1126	1136	rBV	98391	180129	3.56%	0.557%
17	10.246	1210	1217	1226	rBV	197412	352906	6.97%	1.091%
18	10.399	1240	1243	1249	rVB8	3356	5562	0.11%	0.017%
19	10.487	1252	1258	1262	rVV9	6117	10184	0.20%	0.031%
20	10.622	1273	1281	1290	rBV	1200721	1992137	39.33%	6.161%
21	10.763	1300	1305	1319	rVB	151643	284724	5.62%	0.881%
22	11.275	1388	1392	1399	rVB6	5778	11839	0.23%	0.037%
23	11.422	1413	1417	1423	rBV9	5308	10876	0.21%	0.034%
24	12.216	1546	1552	1555	rVB8	6032	10056	0.20%	0.031%
25	12.410	1578	1585	1595	rBV6	9816	23428	0.46%	0.072%
26	12.757	1638	1644	1647	rVB8	3070	6218	0.12%	0.019%
27	13.357	1741	1746	1751	rBV6	12226	21377	0.42%	0.066%
28	13.875	1828	1834	1840	rBV	465090	644895	12.73%	1.994%
29	13.993	1850	1854	1858	rVB7	8642	13457	0.27%	0.042%
30	14.151	1871	1881	1891	rBV	489812	738950	14.59%	2.285%
31	14.457	1926	1933	1945	rBV	1696333	2438797	48.15%	7.543%
32	14.681	1965	1971	1979	rBV4	23473	56036	1.11%	0.173%
33	14.881	2002	2005	2011	rVB7	4928	7747	0.15%	0.024%
34	15.210	2057	2061	2065	rBV7	3485	5705	0.11%	0.018%
35	15.451	2095	2102	2111	rBV	733357	1078774	21.30%	3.336%
36	15.569	2117	2122	2130	rBV	87844	135806	2.68%	0.420%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
 Data File : BP018893.D
 Acq On : 15 Dec 2023 22:52
 Operator : MA/JU
 Sample : 05627-16DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCLC8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.687	2140	2142	2148	rVB7	5564	9796	0.19%	0.030%
38	16.610	2295	2299	2303	rBV6	8164	10333	0.20%	0.032%
39	16.687	2308	2312	2314	rBV5	6170	8444	0.17%	0.026%
40	16.863	2338	2342	2348	rBV9	5290	8963	0.18%	0.028%
41	17.204	2391	2400	2411	rBV	2251492	3073255	60.67%	9.505%
42	17.304	2411	2417	2428	rVV	911663	1266808	25.01%	3.918%
43	17.839	2505	2508	2512	rBV3	7208	10701	0.21%	0.033%
44	17.969	2528	2530	2536	rVB7	12497	19884	0.39%	0.061%
45	18.092	2547	2551	2559	rBV2	64723	97581	1.93%	0.302%
46	18.169	2559	2564	2573	rVV	4269591	5065514	100.00%	15.666%
47	18.845	2676	2679	2685	rBV3	19767	27688	0.55%	0.086%
48	19.192	2734	2738	2739	rBV2	21808	26184	0.52%	0.081%
49	19.475	2783	2786	2790	rVB2	26202	29615	0.58%	0.092%
50	19.539	2792	2797	2803	rBV	1352402	1720191	33.96%	5.320%
51	21.292	3090	3095	3104	rBV	3092639	3927045	77.53%	12.145%
52	23.498	3464	3470	3477	rBV2	930468	1741420	34.38%	5.386%
53	23.657	3490	3497	3509	rVB	2096758	4241653	83.74%	13.118%




Sum of corrected areas: 32333749

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018893.D
Acq On : 15 Dec 2023 22:52
Operator : MA/JU
Sample : 05627-16DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

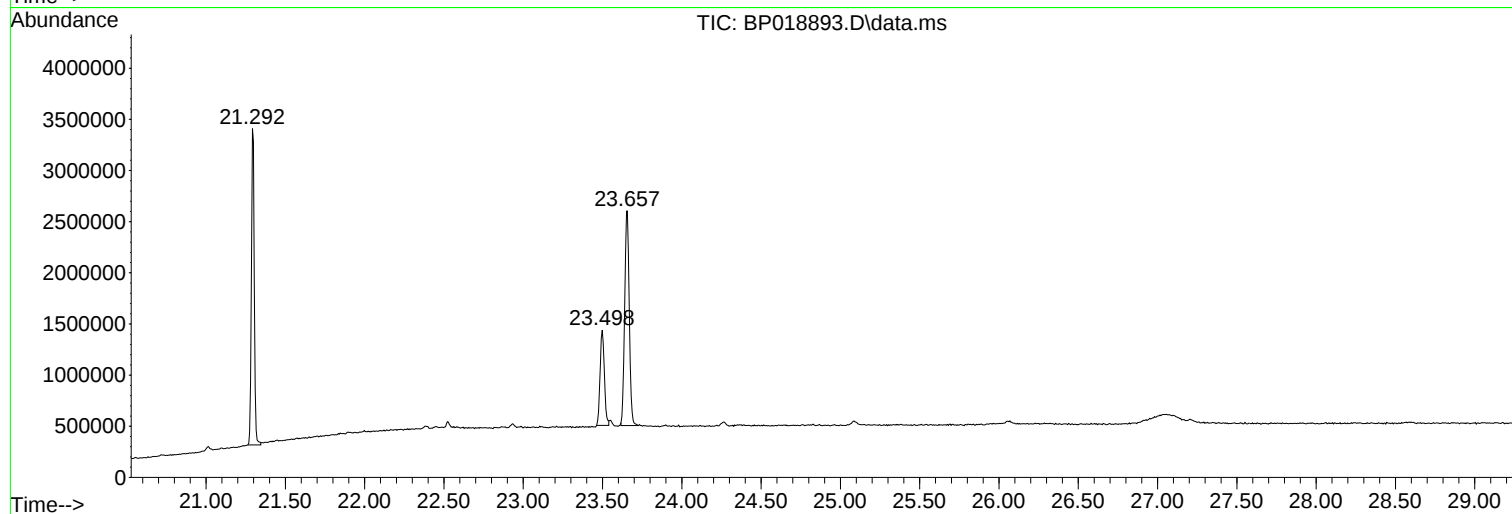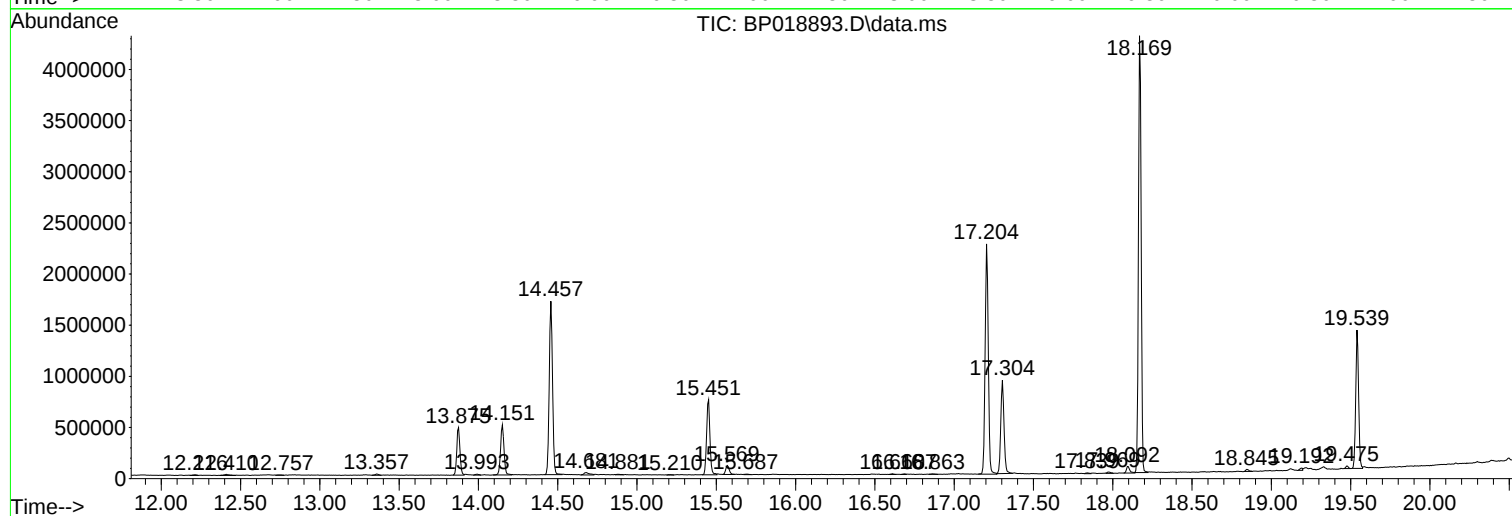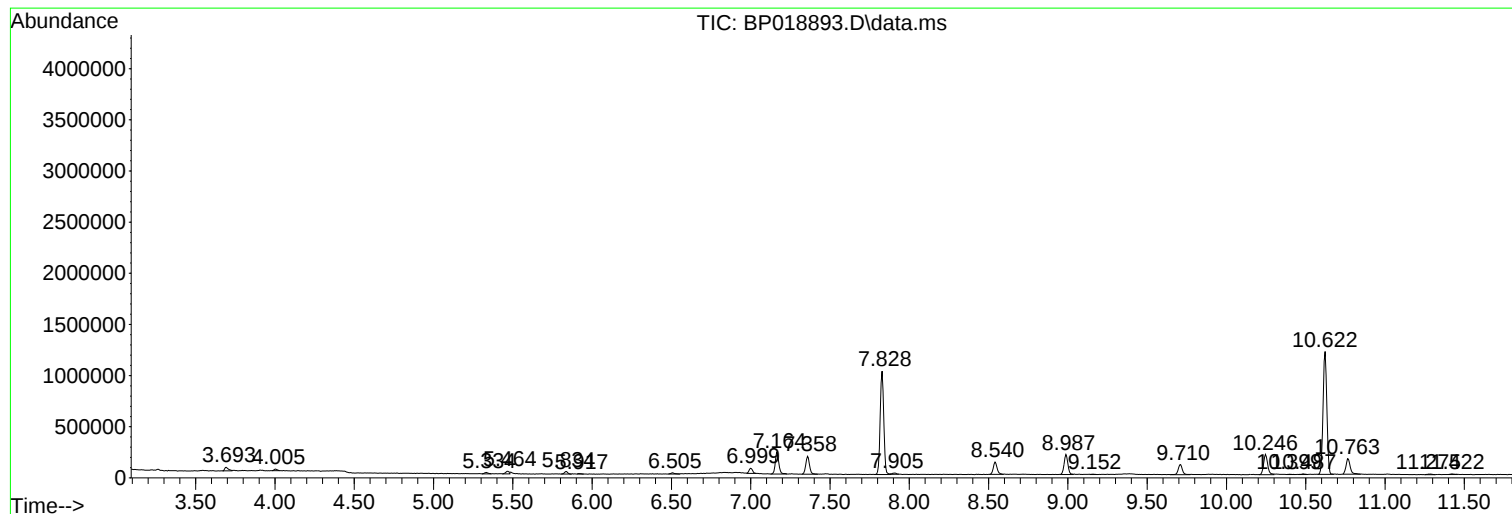

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018893.D
Acq On : 15 Dec 2023 22:52
Operator : MA/JU
Sample : 05627-16DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP121523\
Data File : BP018893.D
Acq On : 15 Dec 2023 22:52
Operator : MA/JU
Sample : 05627-16DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCLC8DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------